

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031422\
 Data File : PL073315.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2022 09:37
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 13:02:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.644	5.489	6710966	32532460	20.953	19.822
28)	SA Decachlor...	10.419	11.328	10741452	34703403	21.124	19.407
Target Compounds							
2)	A alpha-BHC	5.370f	0.000	78745	0	0.191	N.D. #
6)	B beta-BHC	0.000	6.681	0	440260	N.D.	0.422 #
7)	B delta-BHC	0.000	6.932	0	1718034	N.D.	0.798 #
10)	B gamma-Chl...	0.000	8.194	0	798920	N.D.	0.391 #
11)	B alpha-Chl...	0.000	8.296f	0	104268	N.D.	0.052 #
15)	B Endosulfa...	8.352f	9.049f	45286	52428	0.116	0.034 #
16)	A 4,4'-DDD	0.000	8.995	0	152134	N.D.	0.104 #
19)	B Endosulfa...	0.000	9.456f	0	89369	N.D.	0.057 #
25)	Chlordane-3	0.000	8.194	0	798920	N.D.	2.947 #
26)	Chlordane-4	0.000	8.296	0	104268	N.D.	0.315 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031422\
Data File : PL073315.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2022 09:37
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 13:02:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

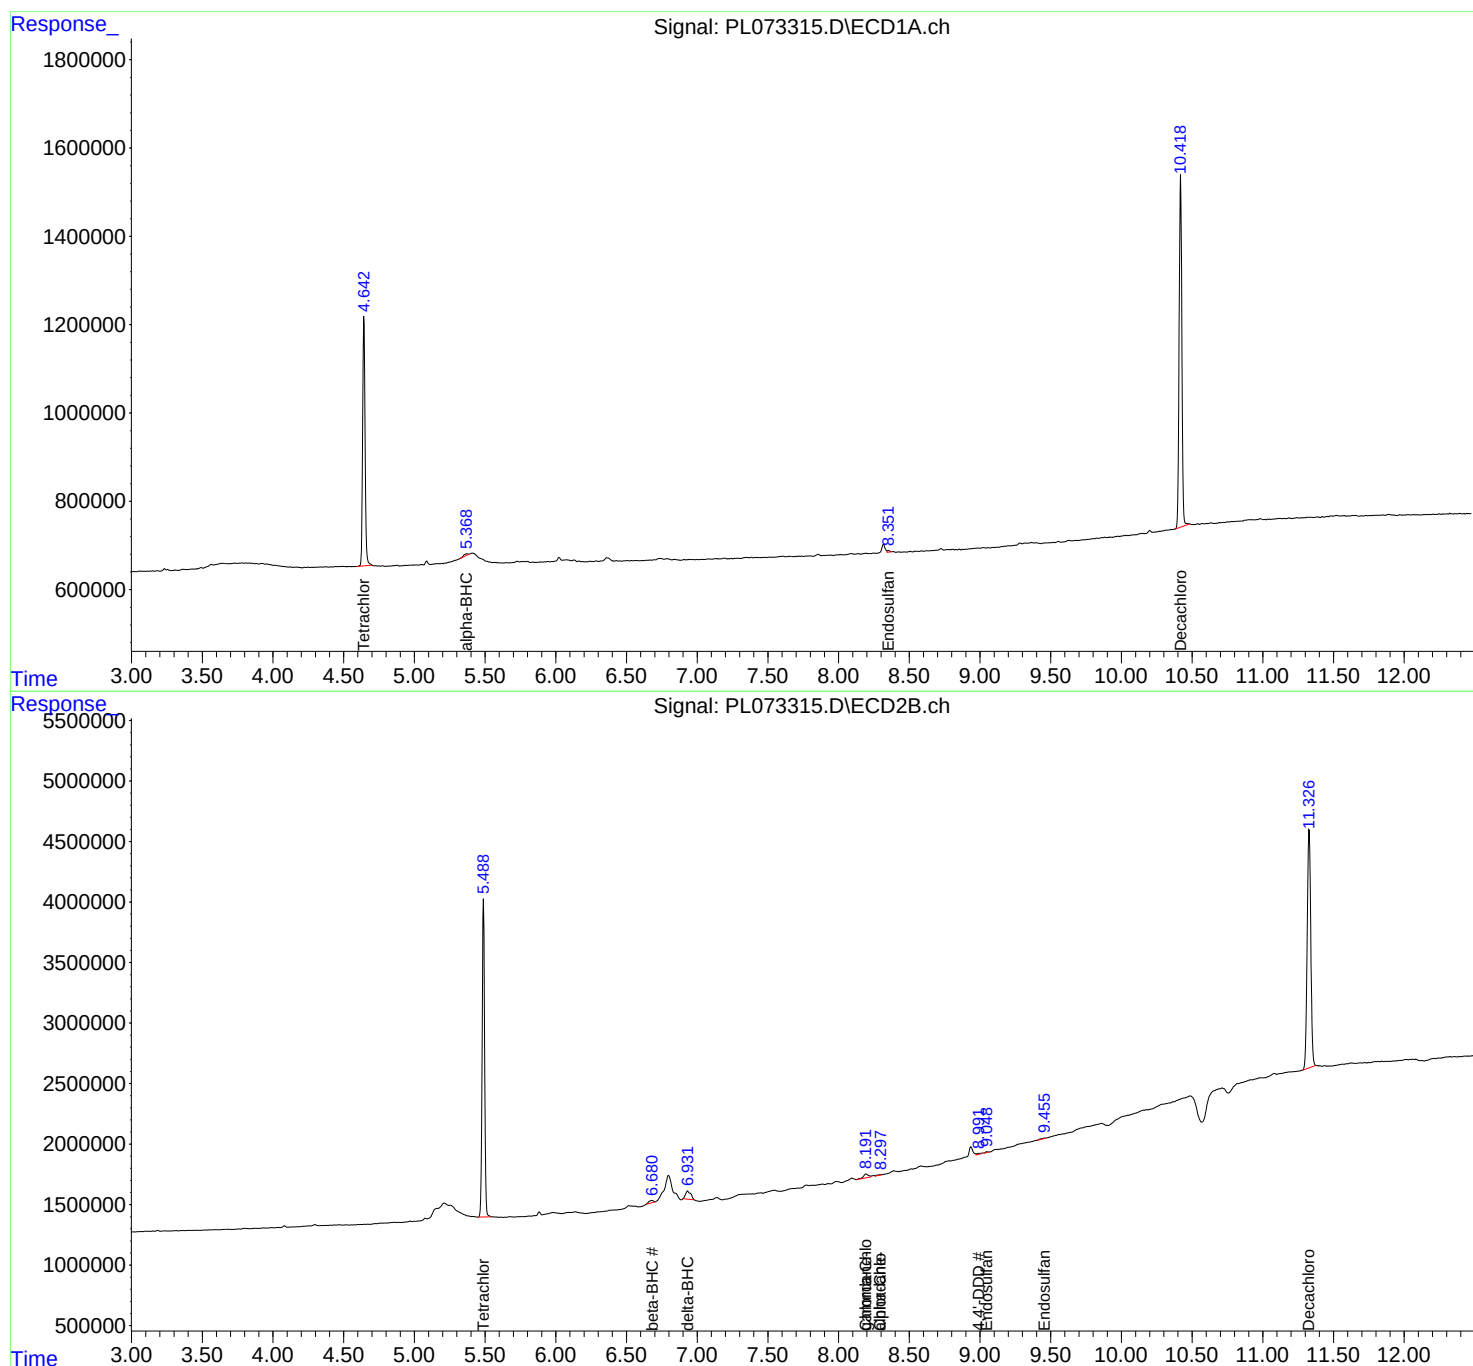


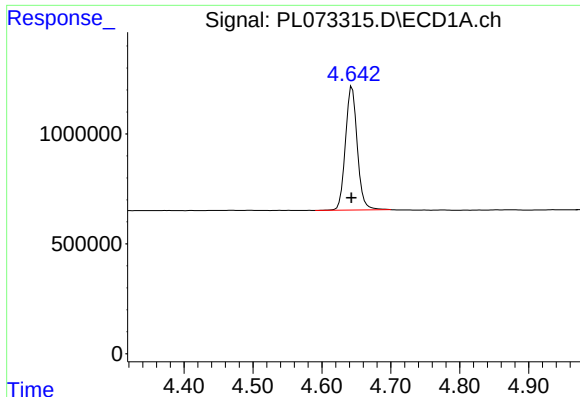

#1 Tetrachloro-m-xylene


R.T.: 4.644 min
Delta R.T.: 0.000 min
Response: 6710966
Conc: 20.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

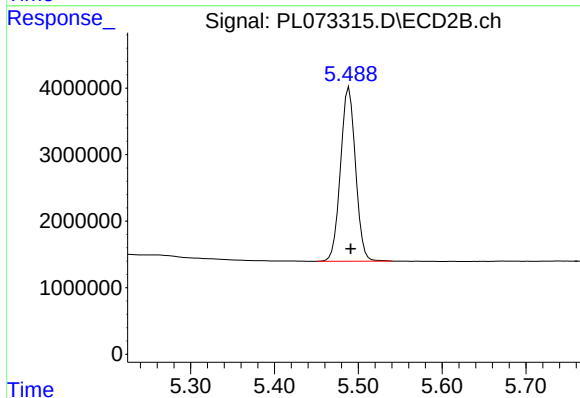


#1 Tetrachloro-m-xylene

R.T.: 5.489 min
Delta R.T.: -0.002 min
Response: 32532460
Conc: 19.82 ng/ml

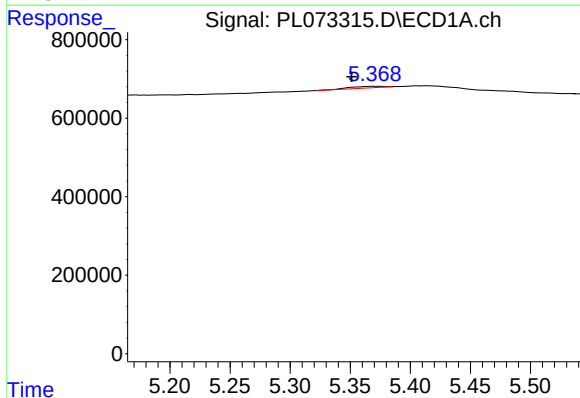


#2 alpha-BHC

R.T.: 5.370 min
Delta R.T.: 0.018 min
Response: 78745
Conc: 0.19 ng/ml

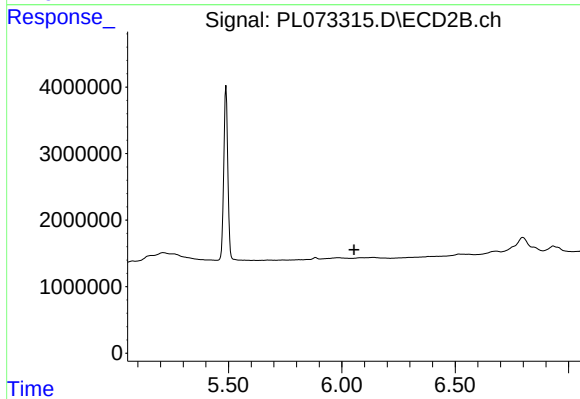

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 6.054 min
Response: 0
Conc: N.D.

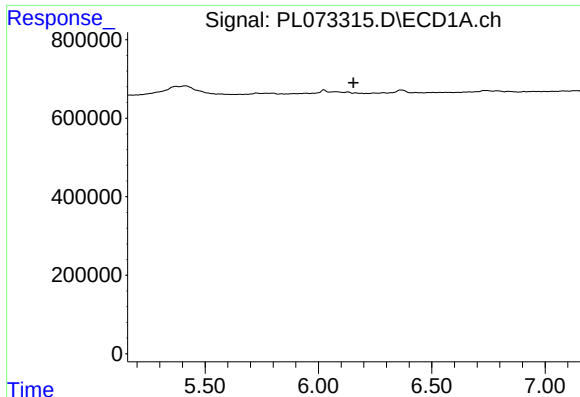

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.155 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

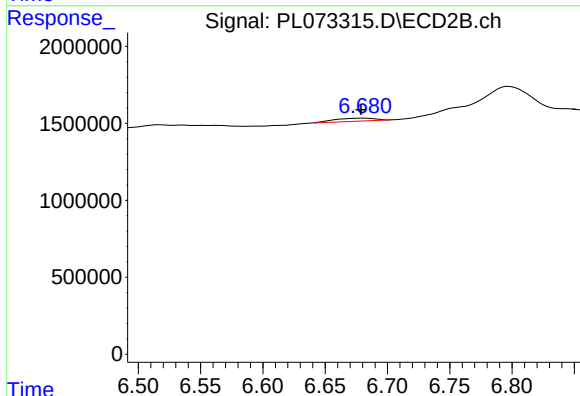


#6 beta-BHC

R.T.: 6.681 min
Delta R.T.: 0.002 min
Response: 440260
Conc: 0.42 ng/ml

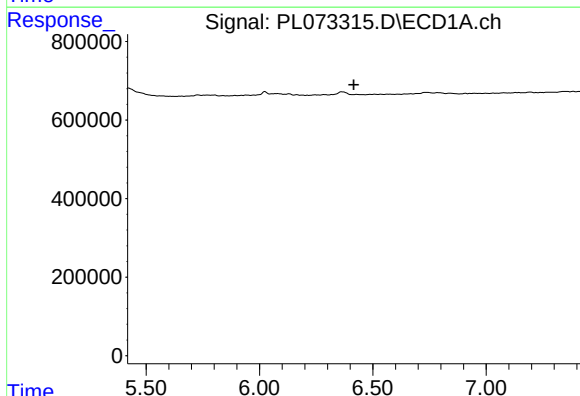


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 6.416 min
Response: 0
Conc: N.D.

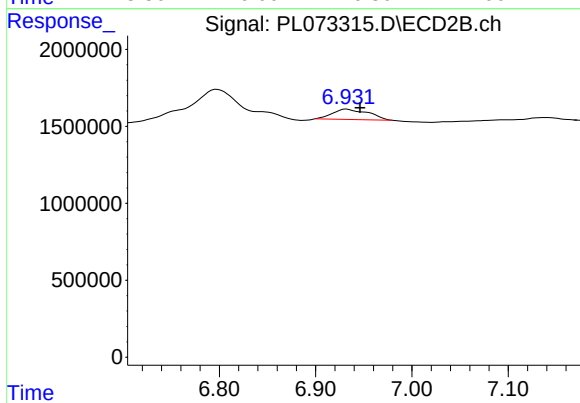

#7 delta-BHC


R.T.: 6.932 min
Delta R.T.: -0.014 min
Response: 1718034
Conc: 0.80 ng/ml

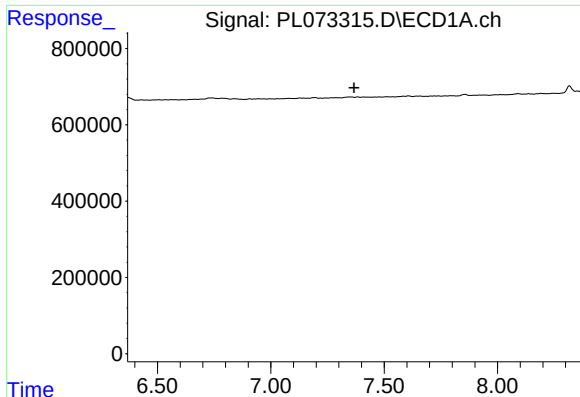

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

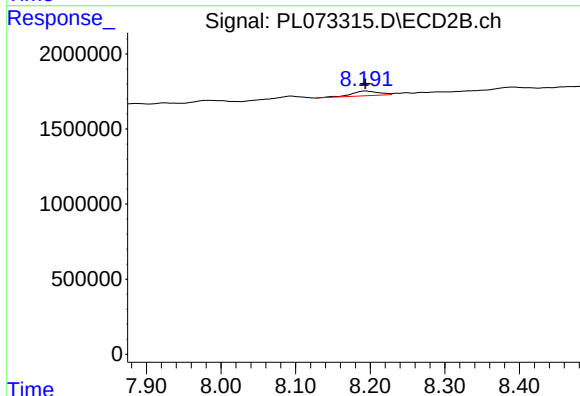


#10 gamma-Chlordane

R.T.: 8.194 min
Delta R.T.: 0.000 min
Response: 798920
Conc: 0.39 ng/ml

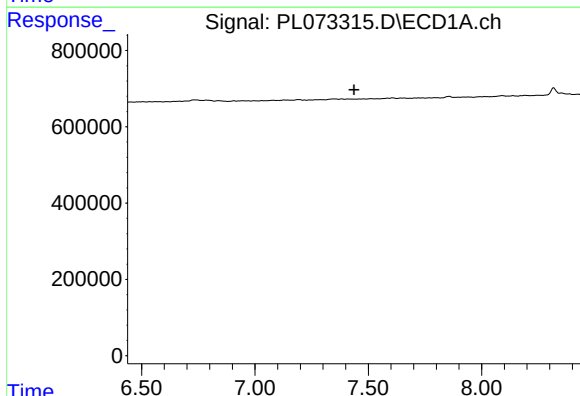


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.437 min
Response: 0
Conc: N.D.

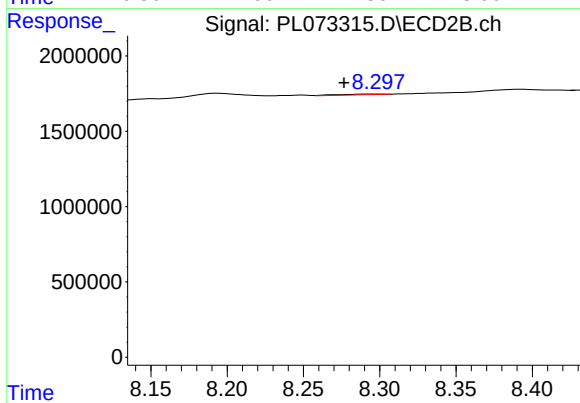

#11 alpha-Chlordane


R.T.: 8.296 min
Delta R.T.: 0.019 min
Response: 104268
Conc: 0.05 ng/ml

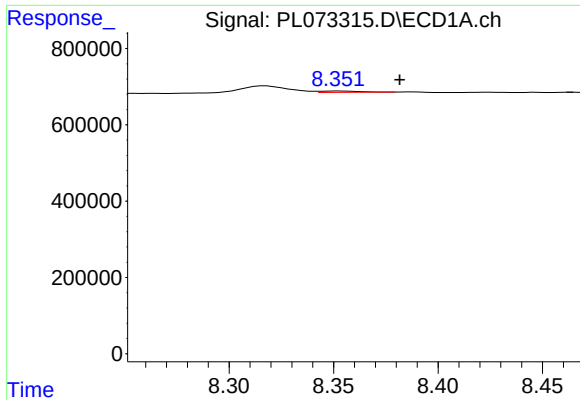

#15 Endosulfan II


R.T.: 8.352 min
Delta R.T.: -0.029 min
Response: 45286
Conc: 0.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

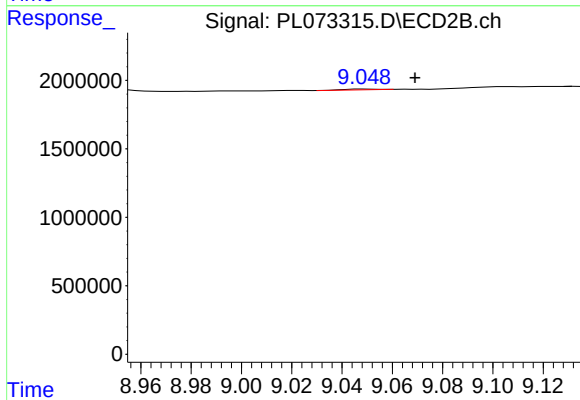


#15 Endosulfan II

R.T.: 9.049 min
Delta R.T.: -0.020 min
Response: 52428
Conc: 0.03 ng/ml

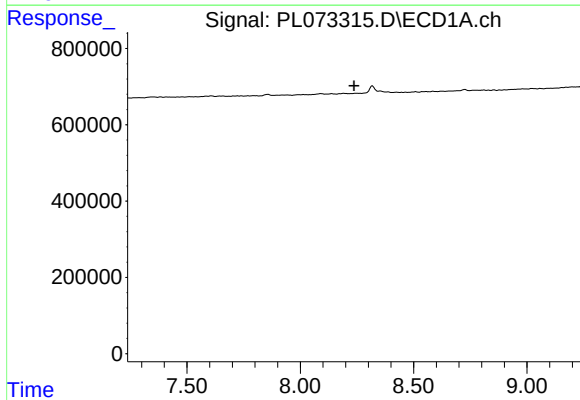


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.237 min
Response: 0
Conc: N.D.

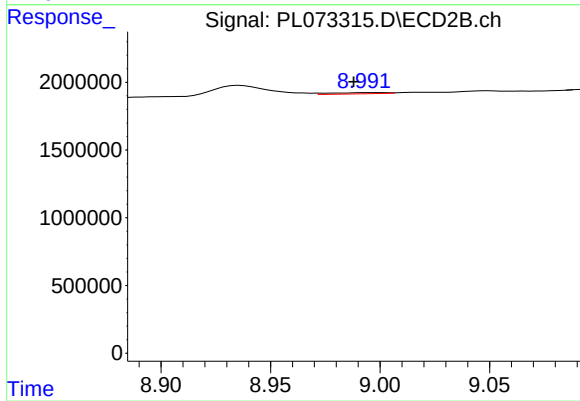

#16 4,4'-DDD


R.T.: 8.995 min
Delta R.T.: 0.007 min
Response: 152134
Conc: 0.10 ng/ml

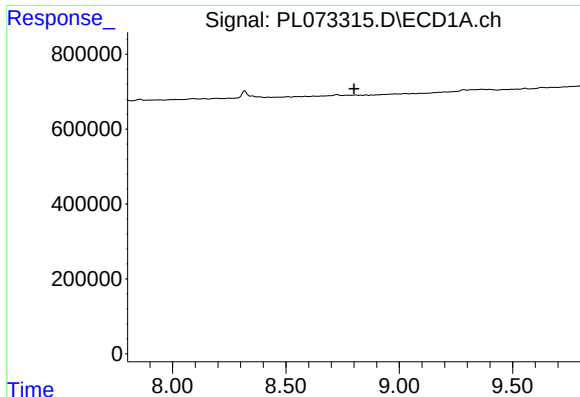

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 8.801 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

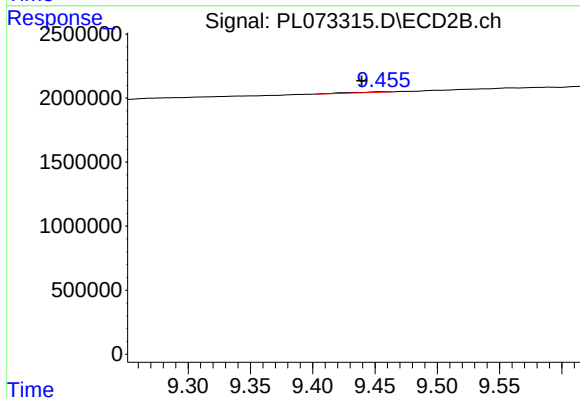


#19 Endosulfan Sulfate

R.T.: 9.456 min
Delta R.T.: 0.017 min
Response: 89369
Conc: 0.06 ng/ml

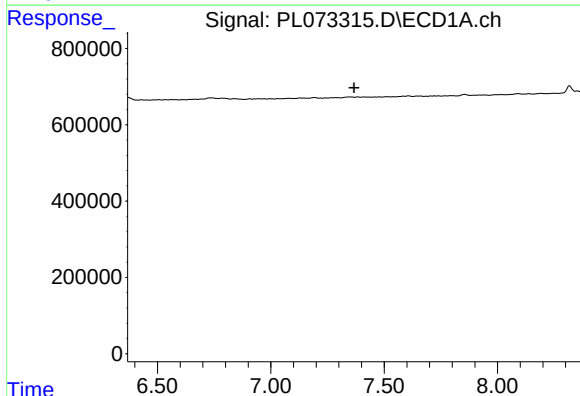


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

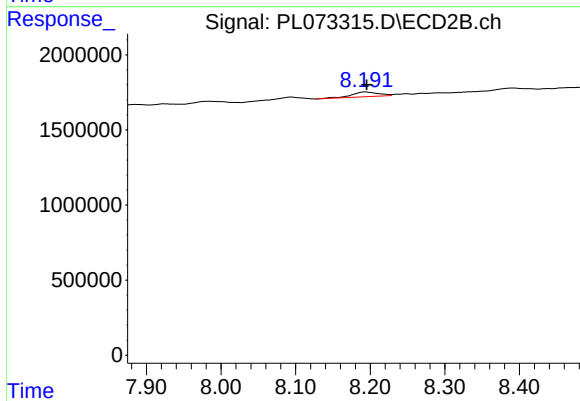

#25 Chlordane-3


R.T.: 8.194 min
Delta R.T.: -0.002 min
Response: 798920
Conc: 2.95 ng/ml

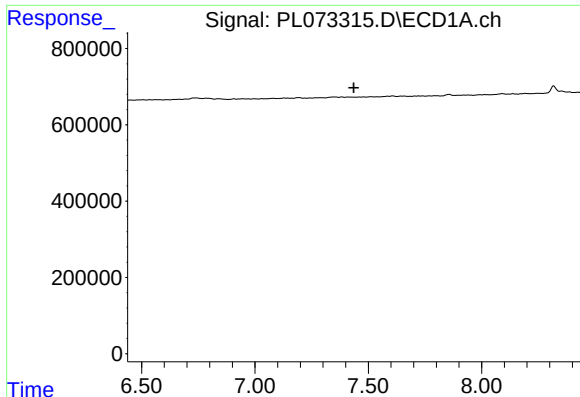

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.437 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

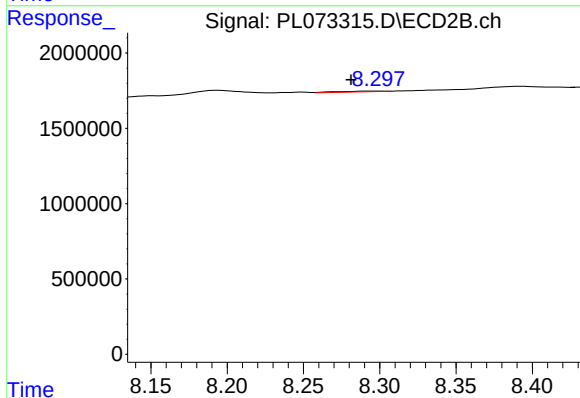


#26 Chlordane-4

R.T.: 8.296 min
Delta R.T.: 0.015 min
Response: 104268
Conc: 0.31 ng/ml

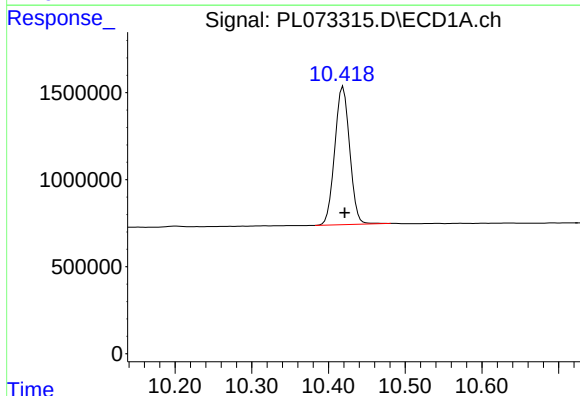

#28 Decachlorobiphenyl

R.T.: 10.419 min
Delta R.T.: -0.002 min
Response: 10741452
Conc: 21.12 ng/ml

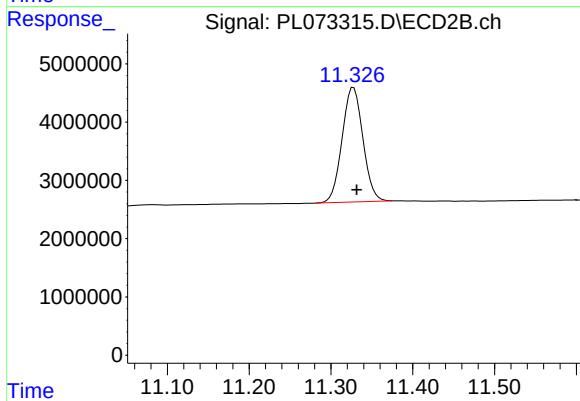

#28 Decachlorobiphenyl

R.T.: 11.328 min
Delta R.T.: -0.004 min
Response: 34703403
Conc: 19.41 ng/ml