

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031422\
 Data File : PL073316.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2022 09:54
 Operator : AR\AJ
 Sample : PEM
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 13:02:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.644	5.490	6199504	30142101	19.356	18.365
28)	SA Decachlor...	10.419	11.328	10160993	33327596	19.982	18.638
Target Compounds							
2)	A alpha-BHC	5.352	6.052	3754428	18347616	9.108	8.156
3)	MA gamma-BHC...	5.775	6.441	3782241	17906472	9.067	8.387
5)	MB Aldrin	6.537f	0.000	34275	0	0.083	N.D. #
6)	B beta-BHC	6.156	6.677	2259788	10266156	10.975	9.849
7)	B delta-BHC	0.000	6.933	0	1747900	N.D.	0.812 #
9)	A Endosulfan I	0.000	8.332	0	34749	N.D.	0.019 #
10)	B gamma-Chl...	0.000	8.194	0	1040096	N.D.	0.509 #
11)	B alpha-Chl...	0.000	8.297f	0	356838	N.D.	0.178 #
12)	B 4,4'-DDE	7.652	8.460	77365	245312	0.216	0.137 #
14)	MA Endrin	8.070	8.844	18173391	70047678	46.838	45.503
15)	B Endosulfa...	8.368	0.000	18191	0	0.047	N.D. #
16)	A 4,4'-DDD	8.237	8.986	228832	982412	0.705	0.673
17)	MA 4,4'-DDT	8.498	9.305	35924130	146.7E6	94.991	89.750
18)	B Endrin al...	8.574	9.201	414392	314696	1.310	0.257 #
19)	B Endosulfa...	0.000	9.437	0	61750	N.D.	0.039 #
20)	A Methoxychlor	9.094	9.784	53374540	192.0E6	208.060	213.095
21)	B Endrin ke...	9.318	9.924	662077	1226614	1.353	0.743 #
25)	Chlordane-3	0.000	8.194	0	1040096	N.D.	3.836 #
26)	Chlordane-4	0.000	8.297f	0	356838	N.D.	1.077 #
27)	Chlordane-5	8.368f	0.000	18191	0	1.111	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031422\
 Data File : PL073316.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2022 09:54
 Operator : AR\AJ
 Sample : PEM
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 13:02:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

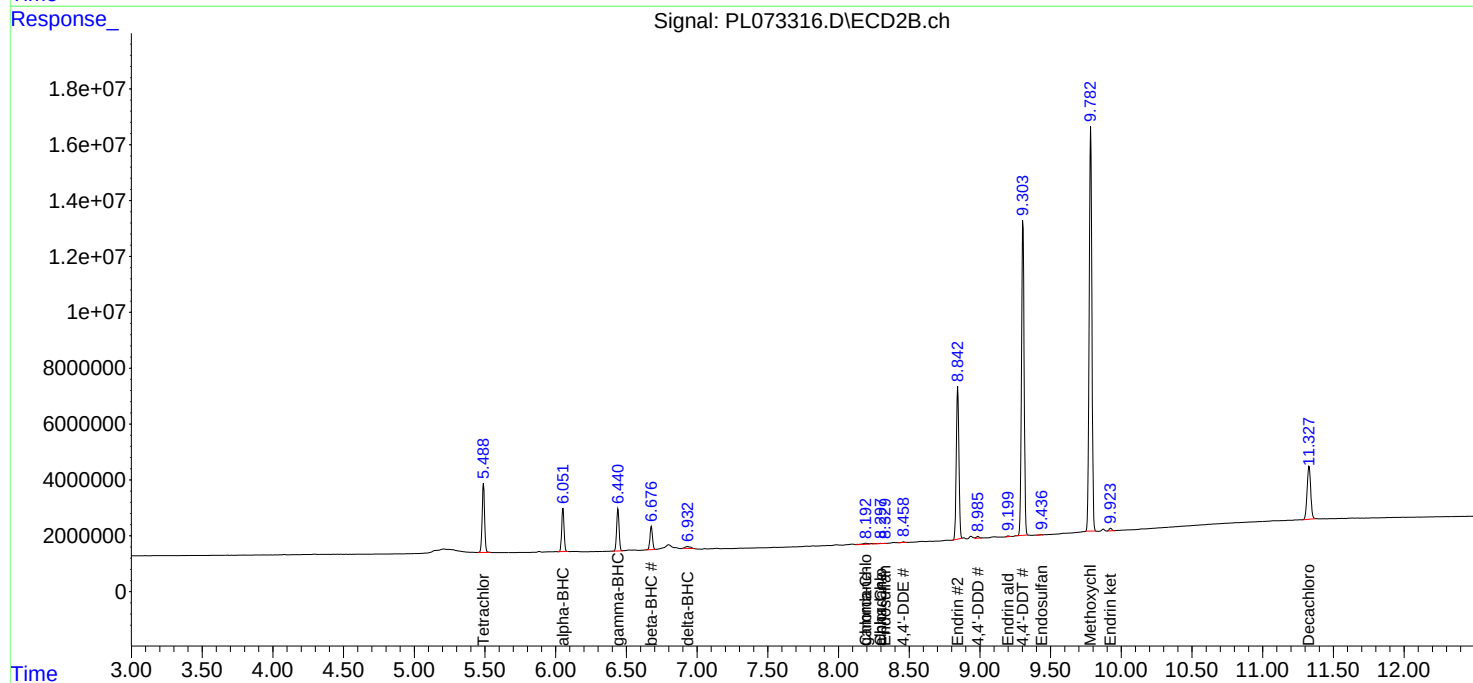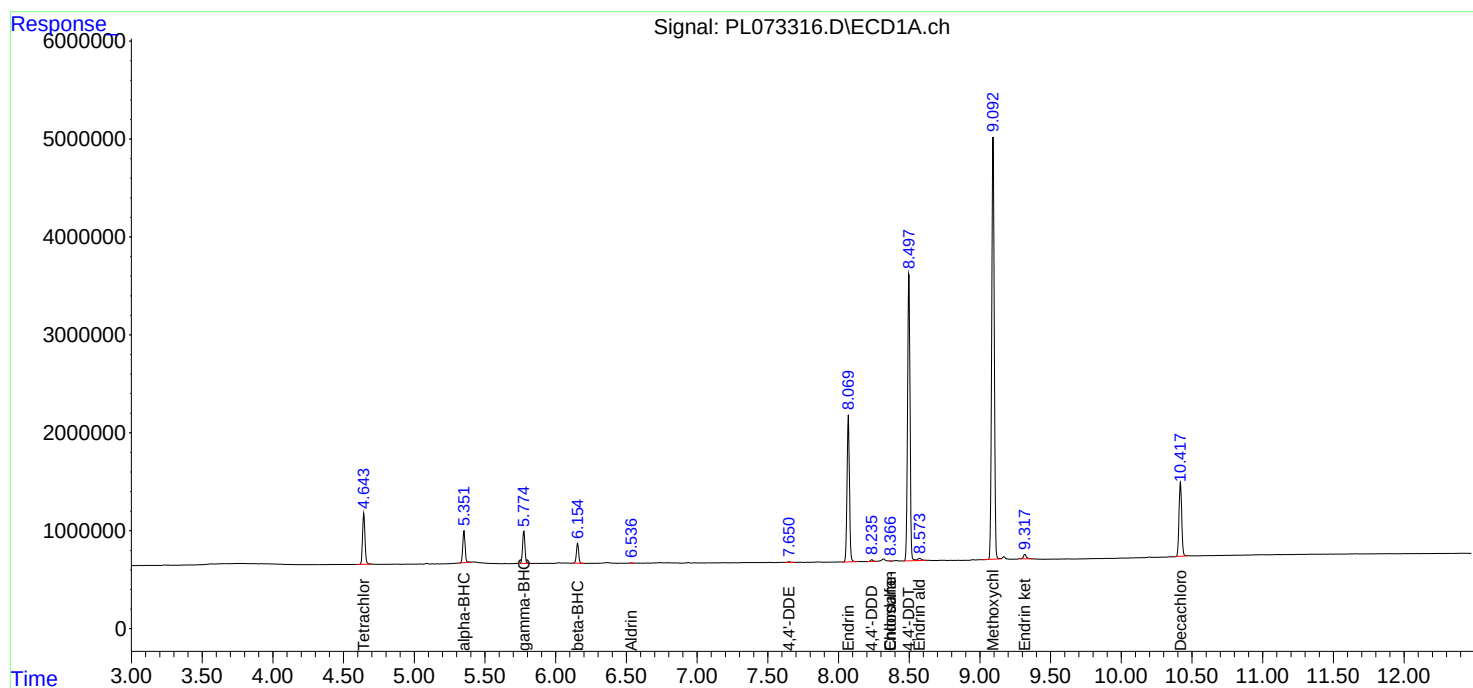


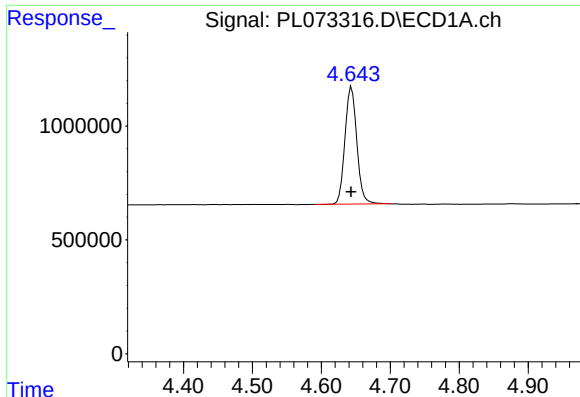

#1 Tetrachloro-m-xylene


R.T.: 4.644 min
Delta R.T.: 0.000 min
Response: 6199504
Conc: 19.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

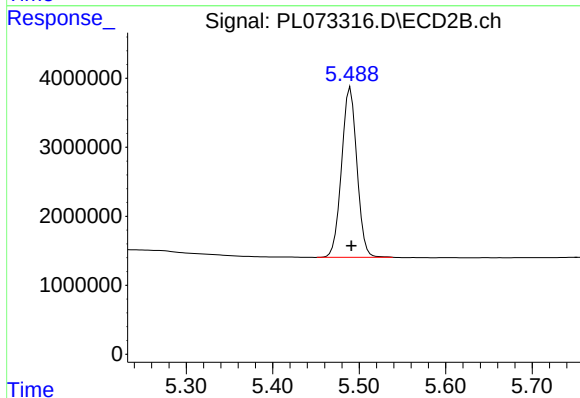


#1 Tetrachloro-m-xylene

R.T.: 5.490 min
Delta R.T.: -0.001 min
Response: 30142101
Conc: 18.37 ng/ml

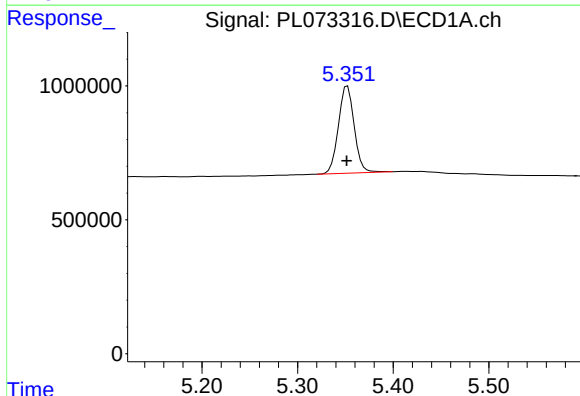


#2 alpha-BHC

R.T.: 5.352 min
Delta R.T.: 0.000 min
Response: 3754428
Conc: 9.11 ng/ml

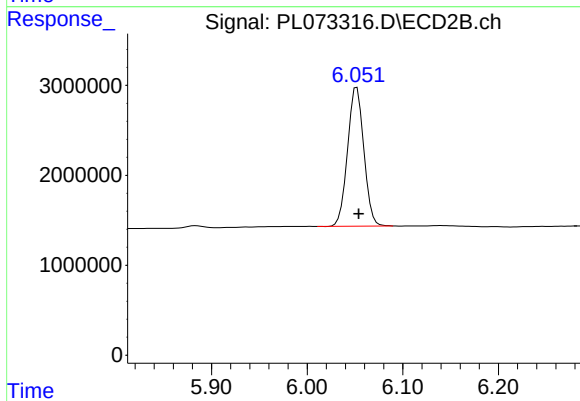

#2 alpha-BHC


R.T.: 6.052 min
Delta R.T.: -0.002 min
Response: 18347616
Conc: 8.16 ng/ml

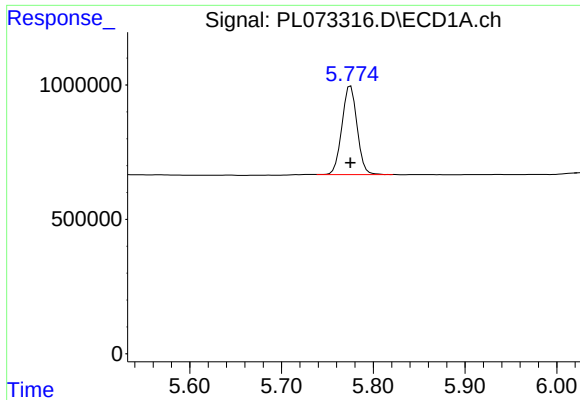

#3 gamma-BHC (Lindane)


R.T.: 5.775 min
Delta R.T.: 0.000 min
Response: 3782241
Conc: 9.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

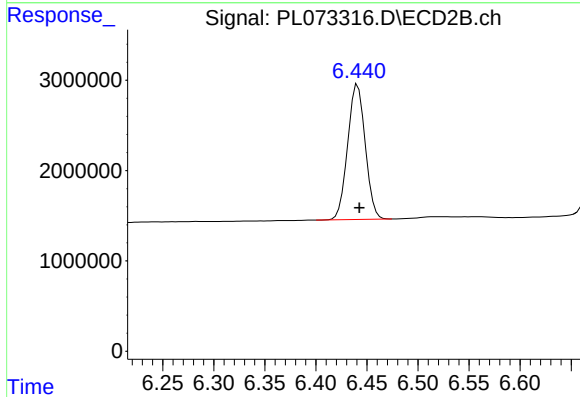


#3 gamma-BHC (Lindane)

R.T.: 6.441 min
Delta R.T.: -0.002 min
Response: 17906472
Conc: 8.39 ng/ml

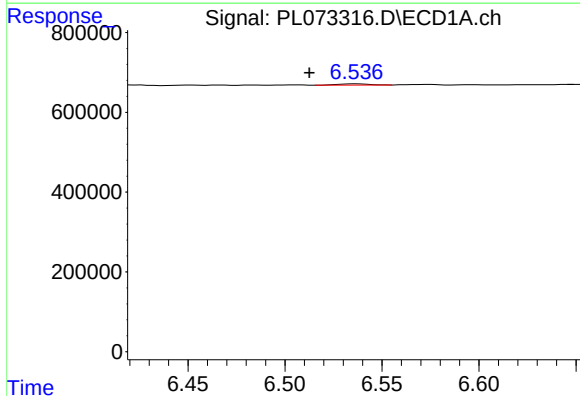


#5 Aldrin

R.T.: 6.537 min
Delta R.T.: 0.024 min
Response: 34275
Conc: 0.08 ng/ml

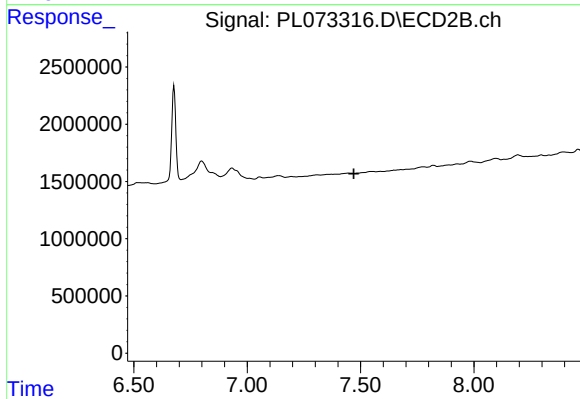

#5 Aldrin


R.T.: 0.000 min
Exp R.T. : 7.470 min
Response: 0
Conc: N.D.

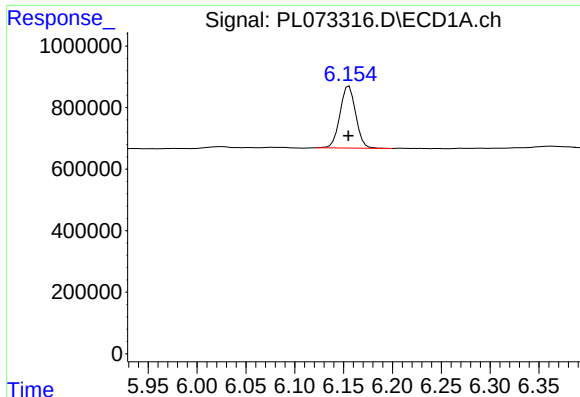

#6 beta-BHC


R.T.: 6.156 min
Delta R.T.: 0.000 min
Response: 2259788
Conc: 10.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

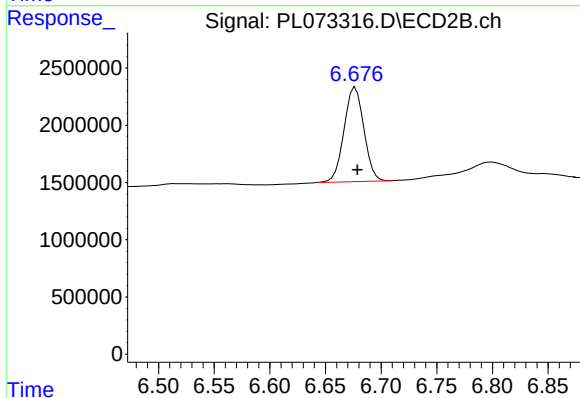


#6 beta-BHC

R.T.: 6.677 min
Delta R.T.: -0.002 min
Response: 10266156
Conc: 9.85 ng/ml

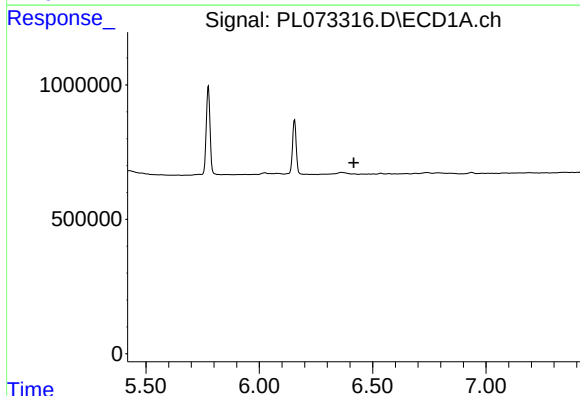


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.416 min
Response: 0
Conc: N.D.

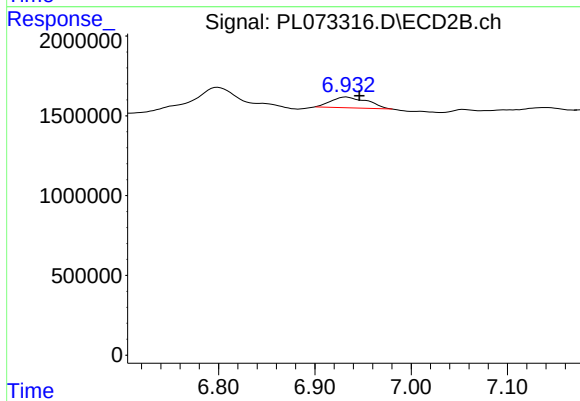

#7 delta-BHC


R.T.: 6.933 min
Delta R.T.: -0.013 min
Response: 1747900
Conc: 0.81 ng/ml

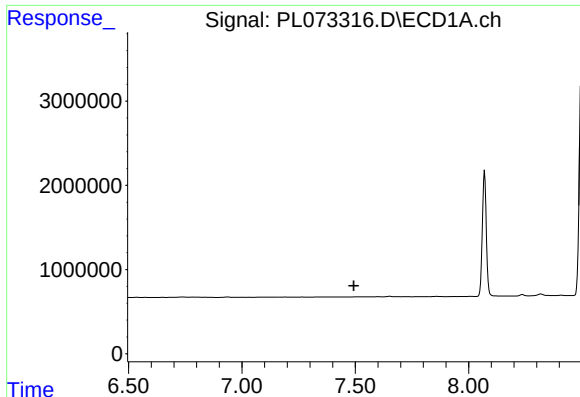

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.493 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

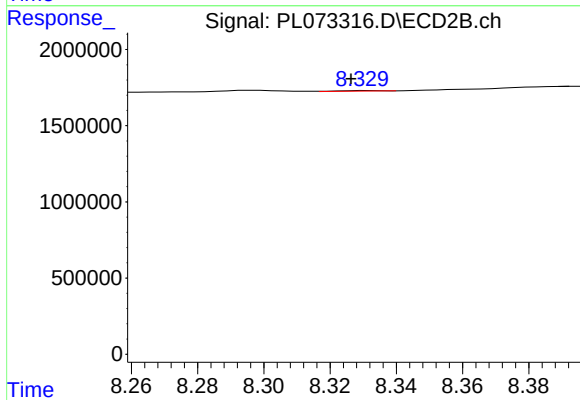


#9 Endosulfan I

R.T.: 8.332 min
Delta R.T.: 0.005 min
Response: 34749
Conc: 0.02 ng/ml

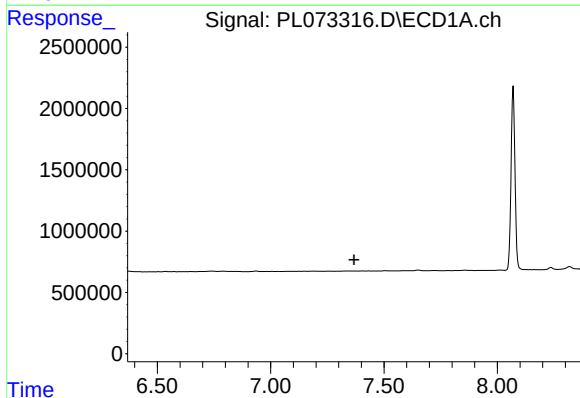


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

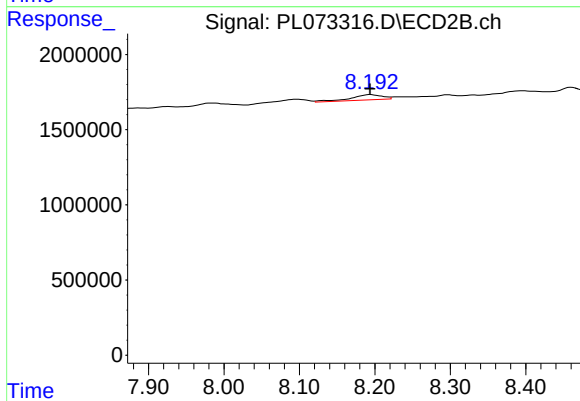

#10 gamma-Chlordane


R.T.: 8.194 min
Delta R.T.: 0.000 min
Response: 1040096
Conc: 0.51 ng/ml

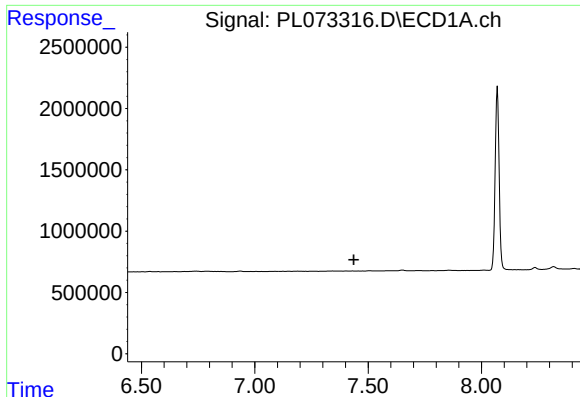

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.437 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

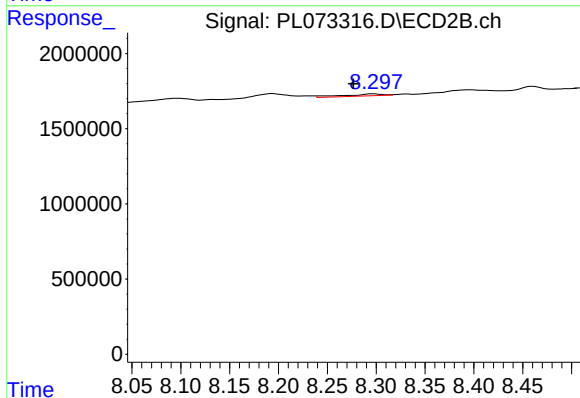


#11 alpha-Chlordane

R.T.: 8.297 min
Delta R.T.: 0.021 min
Response: 356838
Conc: 0.18 ng/ml

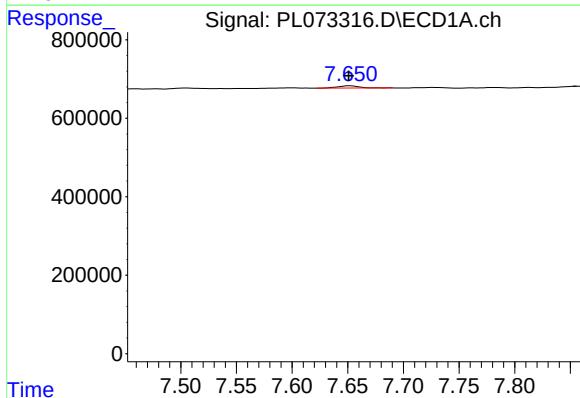


#12 4,4'-DDE

R.T.: 7.652 min
Delta R.T.: 0.000 min
Response: 77365
Conc: 0.22 ng/ml

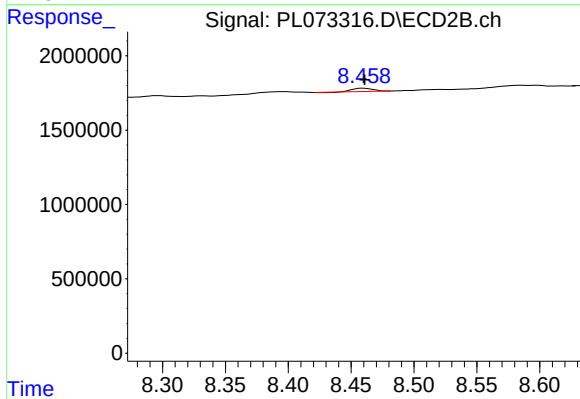

#12 4,4'-DDE


R.T.: 8.460 min
Delta R.T.: 0.000 min
Response: 245312
Conc: 0.14 ng/ml

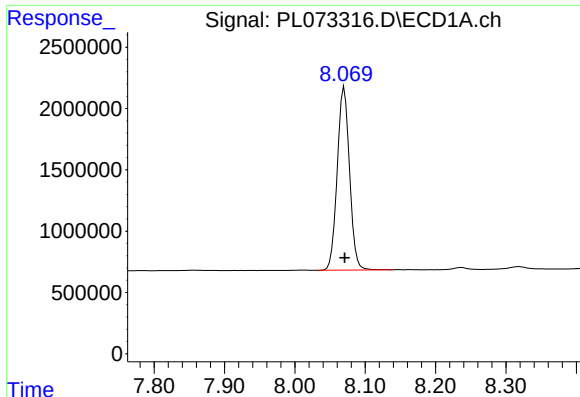

#14 Endrin


R.T.: 8.070 min
Delta R.T.: 0.000 min
Response: 18173391
Conc: 46.84 ng/ml

Instrument :
ECD_L
ClientSampleId :

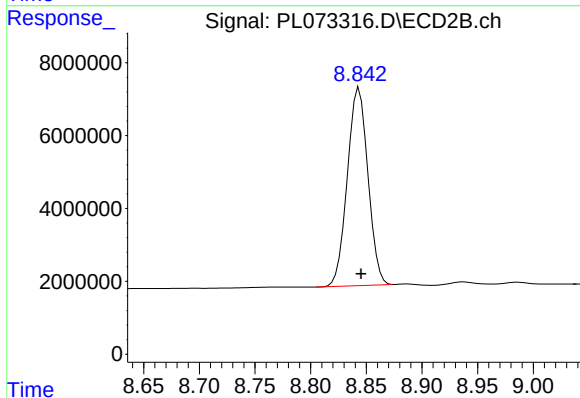


#14 Endrin

R.T.: 8.844 min
Delta R.T.: -0.002 min
Response: 70047678
Conc: 45.50 ng/ml

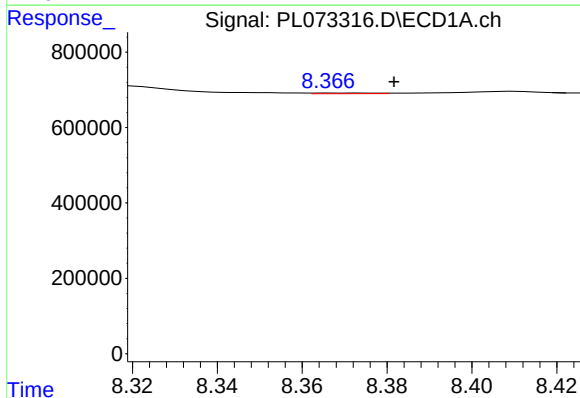


#15 Endosulfan II

R.T.: 8.368 min
Delta R.T.: -0.014 min
Response: 18191
Conc: 0.05 ng/ml

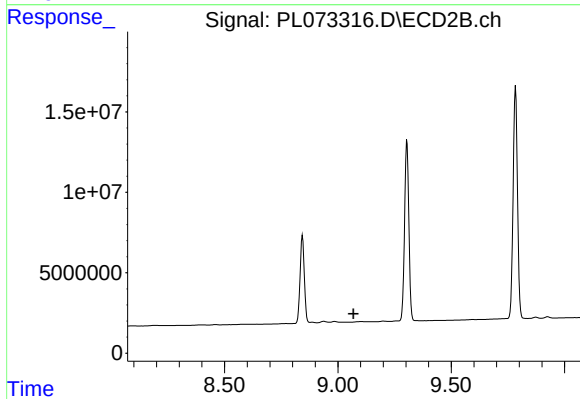

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 9.069 min
Response: 0
Conc: N.D.

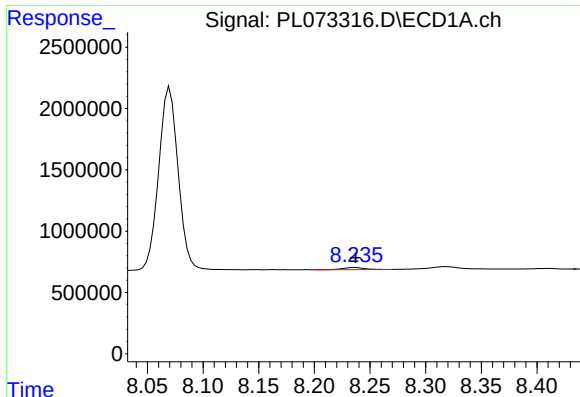

#16 4,4'-DDD


R.T.: 8.237 min
Delta R.T.: 0.000 min
Response: 228832
Conc: 0.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

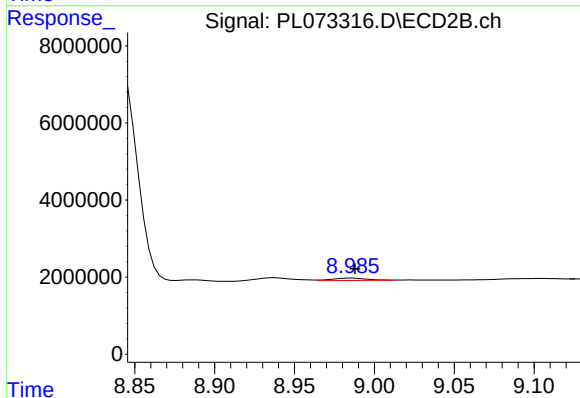


#16 4,4'-DDD

R.T.: 8.986 min
Delta R.T.: -0.002 min
Response: 982412
Conc: 0.67 ng/ml

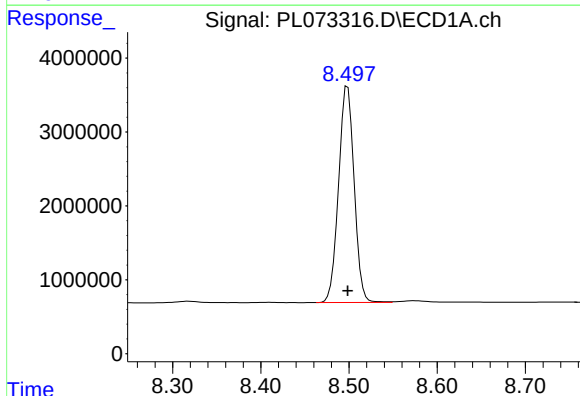


#17 4,4'-DDT

R.T.: 8.498 min
Delta R.T.: 0.000 min
Response: 35924130
Conc: 94.99 ng/ml

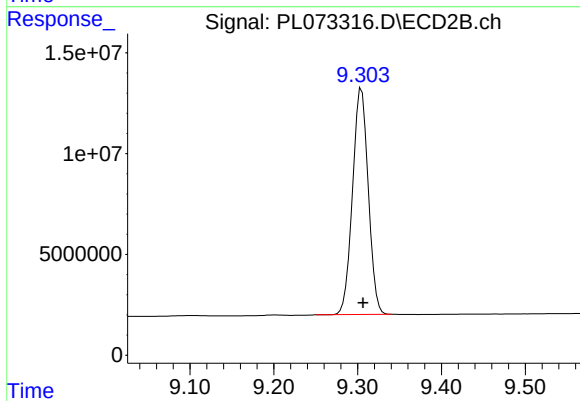

#17 4,4'-DDT


R.T.: 9.305 min
Delta R.T.: -0.002 min
Response: 146699602
Conc: 89.75 ng/ml

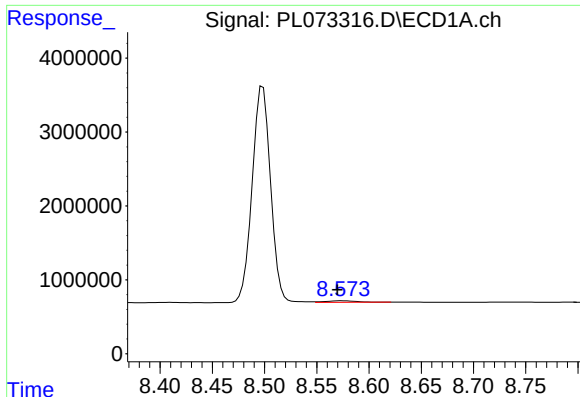

#18 Endrin aldehyde


R.T.: 8.574 min
Delta R.T.: 0.004 min
Response: 414392
Conc: 1.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

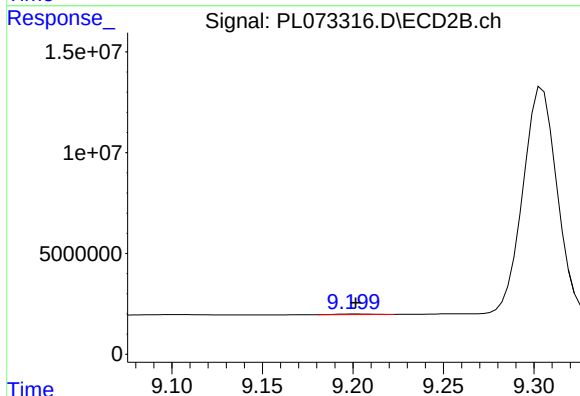


#18 Endrin aldehyde

R.T.: 9.201 min
Delta R.T.: 0.000 min
Response: 314696
Conc: 0.26 ng/ml

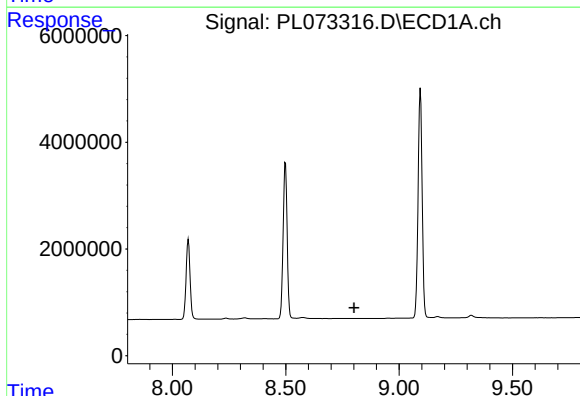


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 8.801 min
Response: 0
Conc: N.D.

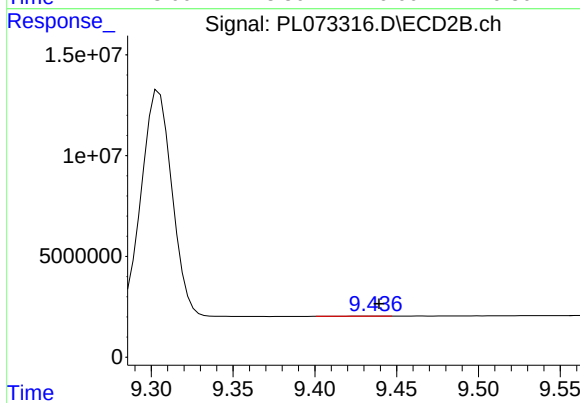

#19 Endosulfan Sulfate


R.T.: 9.437 min
Delta R.T.: -0.002 min
Response: 61750
Conc: 0.04 ng/ml

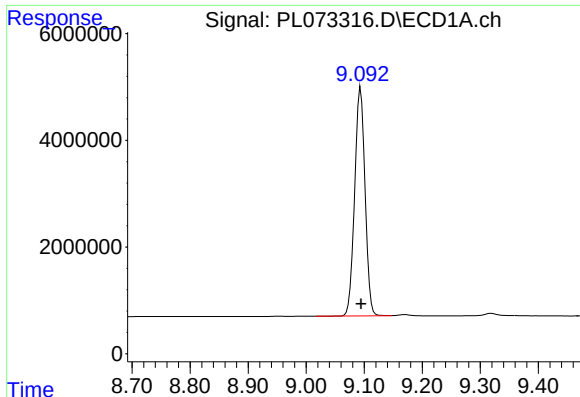

#20 Methoxychlor


R.T.: 9.094 min
Delta R.T.: 0.000 min
Response: 53374540
Conc: 208.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

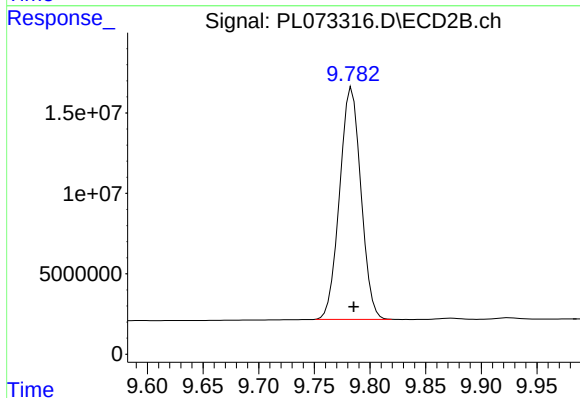


#20 Methoxychlor

R.T.: 9.784 min
Delta R.T.: -0.002 min
Response: 192014269
Conc: 213.09 ng/ml

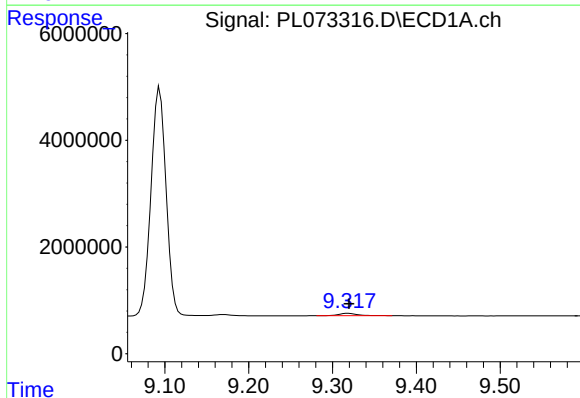


#21 Endrin ketone

R.T.: 9.318 min
Delta R.T.: -0.002 min
Response: 662077
Conc: 1.35 ng/ml

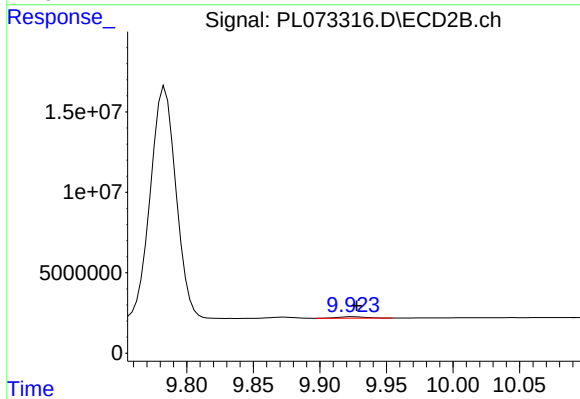

#21 Endrin ketone


R.T.: 9.924 min
Delta R.T.: -0.003 min
Response: 1226614
Conc: 0.74 ng/ml

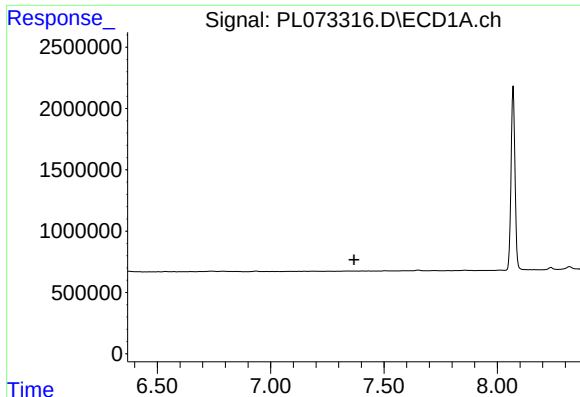

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

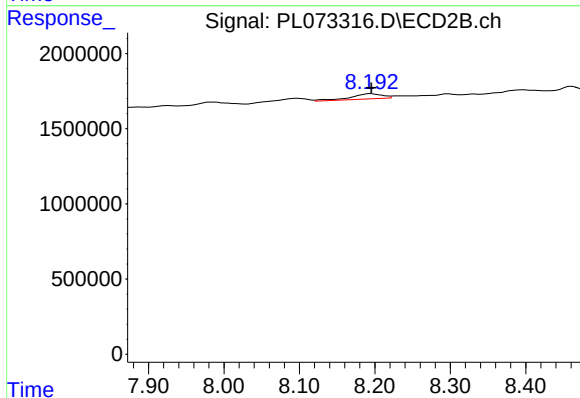


#25 Chlordane-3

R.T.: 8.194 min
Delta R.T.: -0.001 min
Response: 1040096
Conc: 3.84 ng/ml

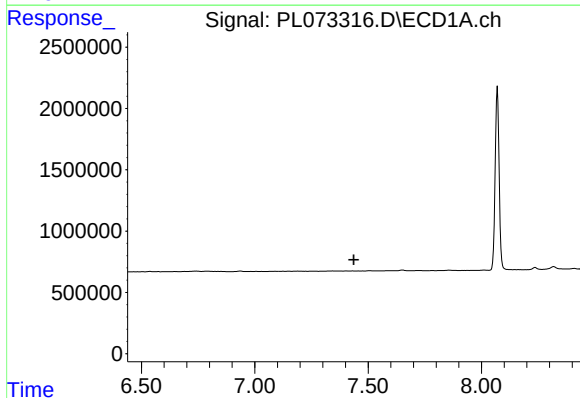


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.437 min
Response: 0
Conc: N.D.

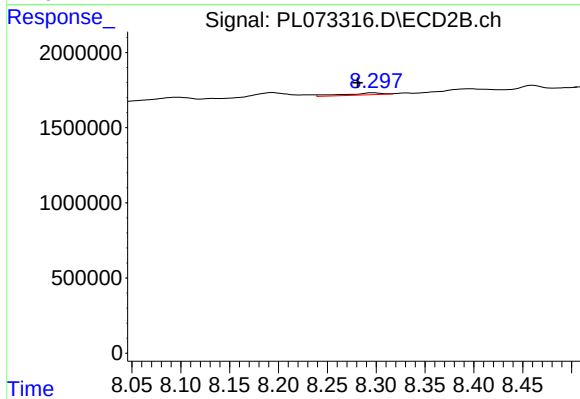

#26 Chlordane-4


R.T.: 8.297 min
Delta R.T.: 0.016 min
Response: 356838
Conc: 1.08 ng/ml

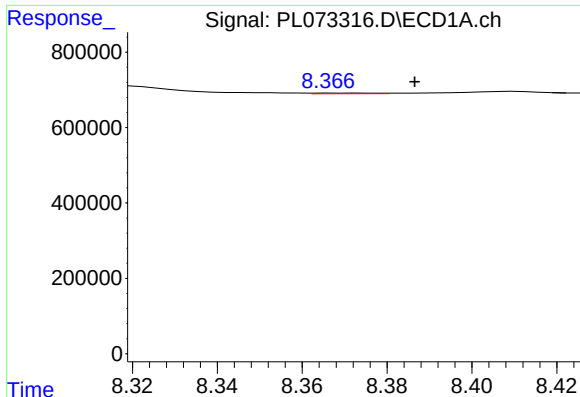

#27 Chlordane-5


R.T.: 8.368 min
Delta R.T.: -0.019 min
Response: 18191
Conc: 1.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

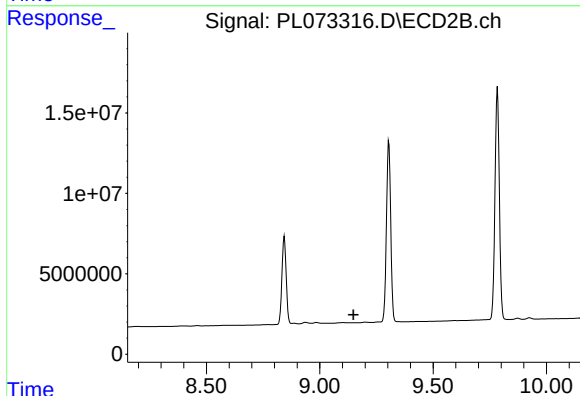


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.149 min
Response: 0
Conc: N.D.

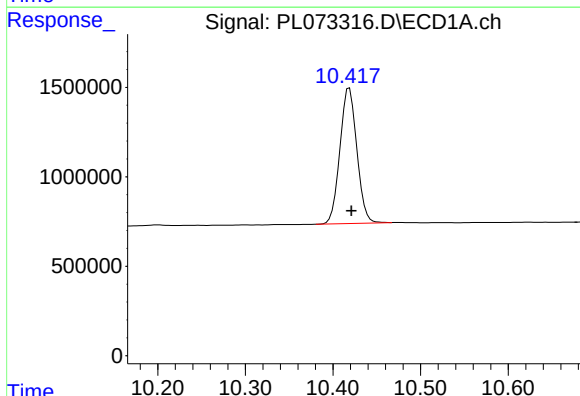

#28 Decachlorobiphenyl

R.T.: 10.419 min
Delta R.T.: -0.002 min
Response: 10160993
Conc: 19.98 ng/ml

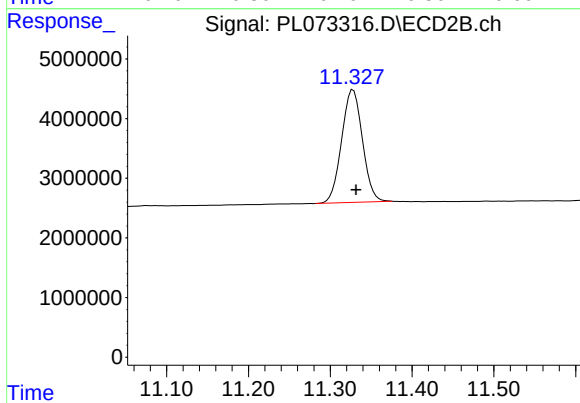

#28 Decachlorobiphenyl

R.T.: 11.328 min
Delta R.T.: -0.003 min
Response: 33327596
Conc: 18.64 ng/ml