

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031422\
 Data File : PL073349.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2022 20:18
 Operator : AR\AJ
 Sample : PB143285TB
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB143285TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 05:08:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.643	5.489	5895971	29763075	18.408	18.134
28)	SA Decachlor...	10.418	11.328	9964853	35266514	19.597	19.722
Target Compounds							
2)	A alpha-BHC	5.360	0.000	37627	0	0.091	N.D. #
6)	B beta-BHC	6.129f	6.678	1593	680664	0.008	0.653 #
7)	B delta-BHC	6.429	6.958	52844	2634891	0.132	1.224 #
10)	B gamma-Chl...	7.346f	8.196	13216	526133	0.030	0.258 #
16)	A 4,4'-DDD	0.000	9.006f	0	354175	N.D.	0.243 #
17)	MA 4,4'-DDT	0.000	9.293	0	69760	N.D.	0.043 #
19)	B Endosulfa...	0.000	9.429	0	37782	N.D.	0.024 #
25)	Chlordane-3	7.346f	8.196	13216	526133	0.324	1.941 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031422\
Data File : PL073349.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2022 20:18
Operator : AR\AJ
Sample : PB143285TB
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB143285TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 05:08:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

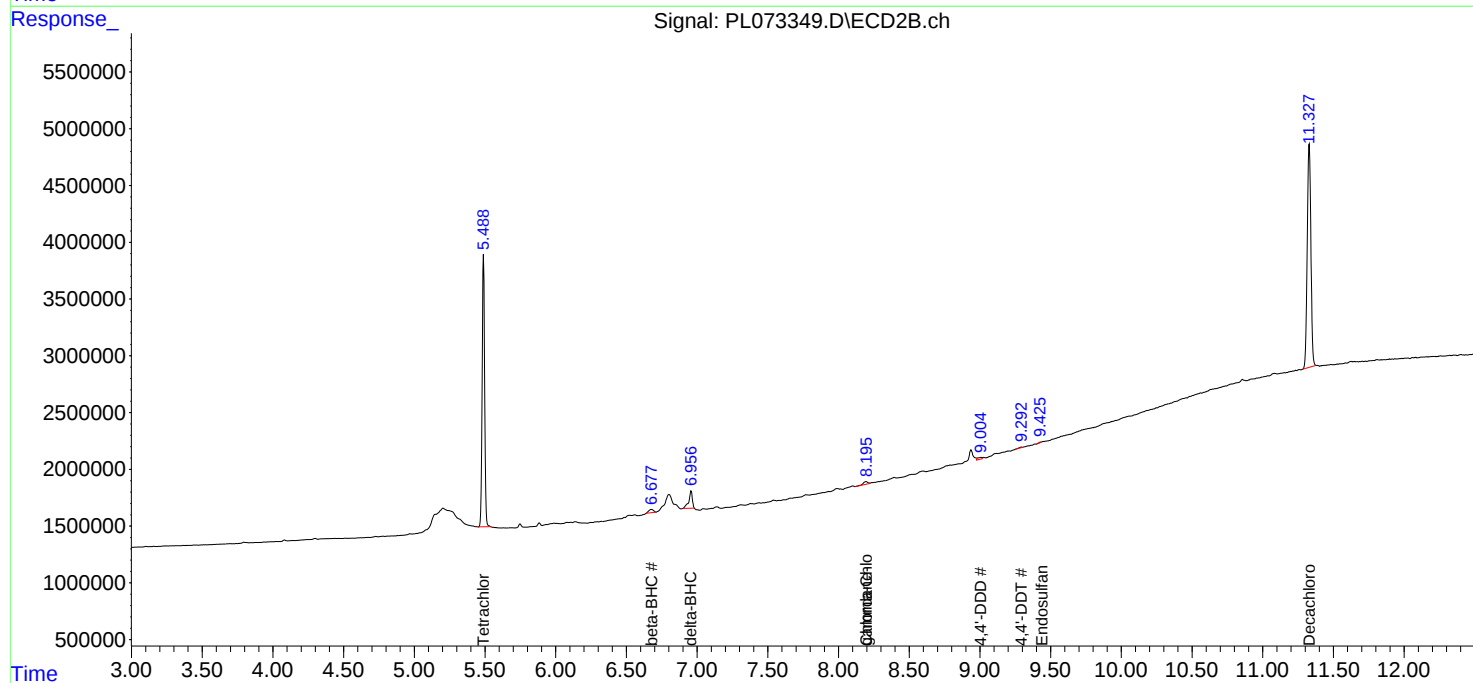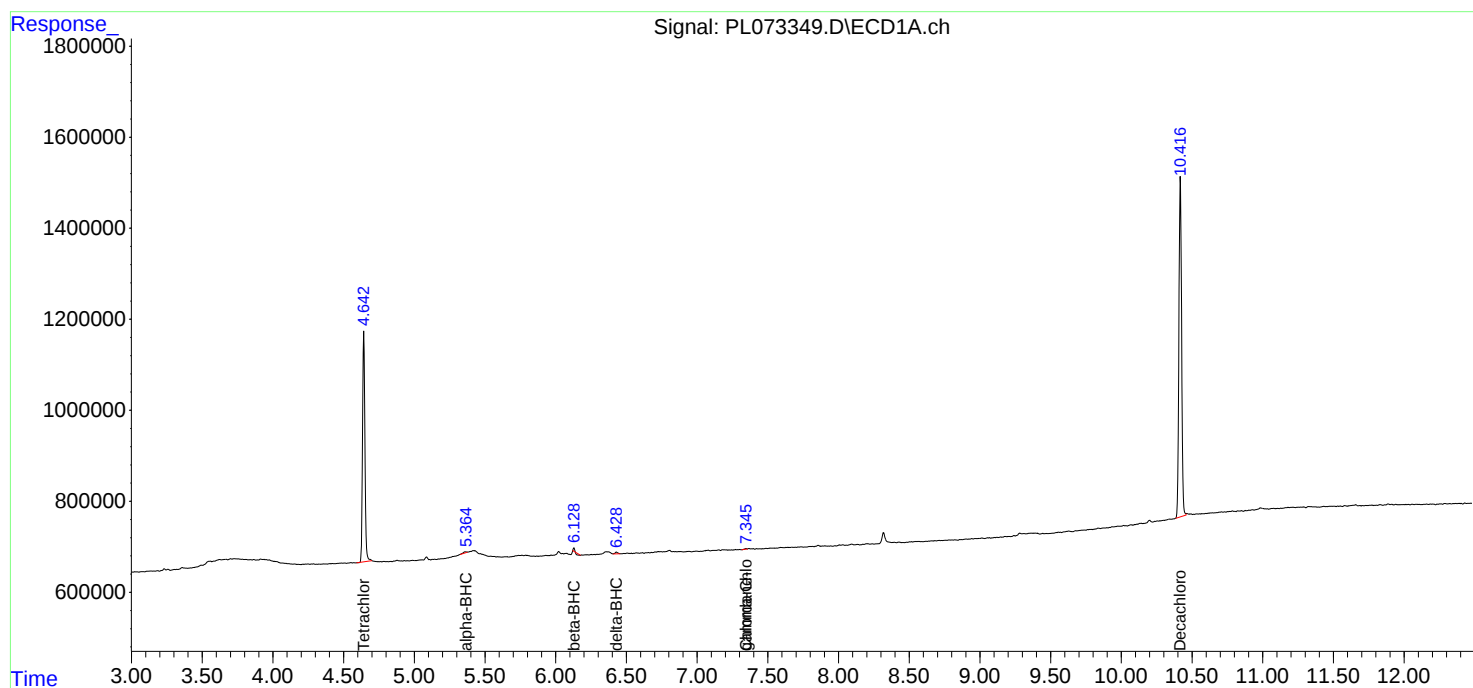


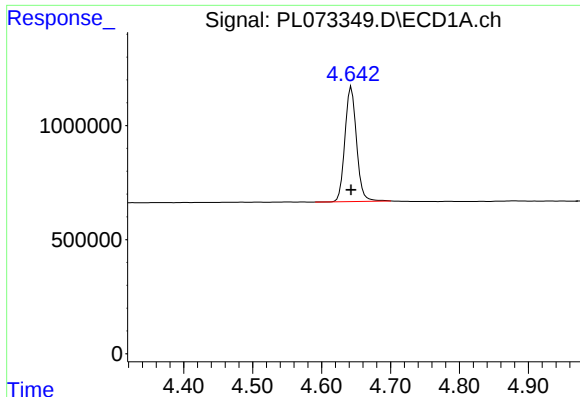

#1 Tetrachloro-m-xylene


R.T.: 4.643 min
Delta R.T.: 0.000 min
Response: 5895971
Conc: 18.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB143285TB

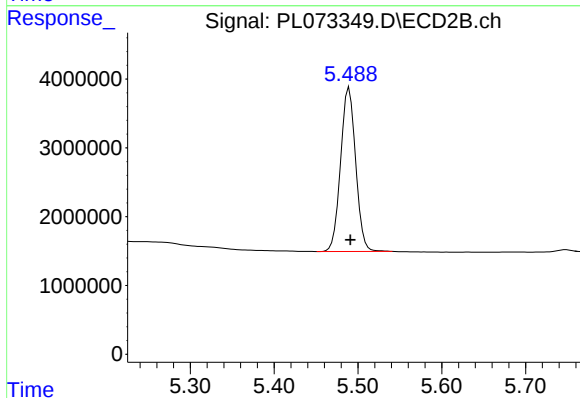


#1 Tetrachloro-m-xylene

R.T.: 5.489 min
Delta R.T.: -0.002 min
Response: 29763075
Conc: 18.13 ng/ml

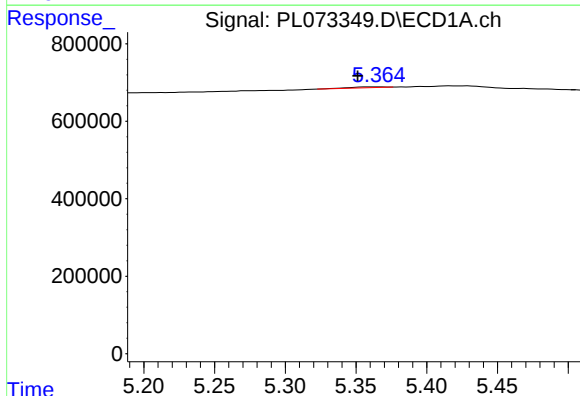


#2 alpha-BHC

R.T.: 5.360 min
Delta R.T.: 0.009 min
Response: 37627
Conc: 0.09 ng/ml

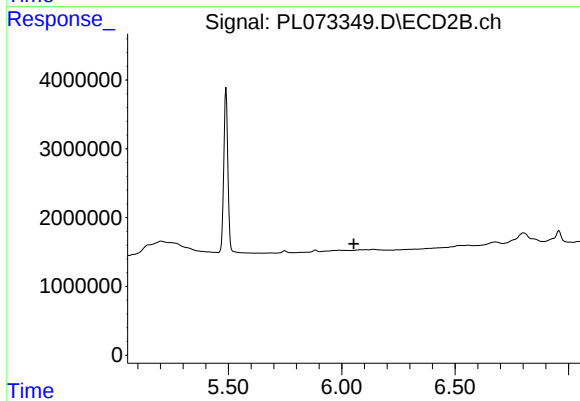

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.054 min
Response: 0
Conc: N.D.

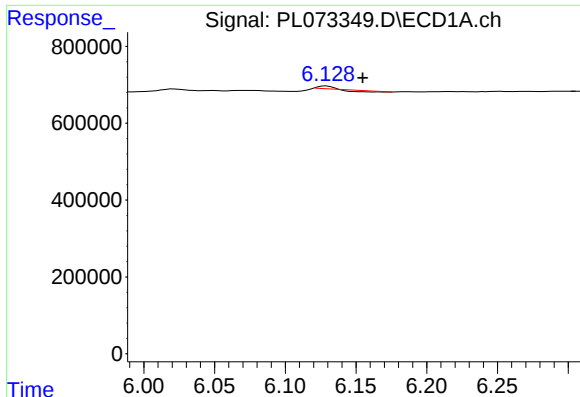

#6 beta-BHC


R.T.: 6.129 min
Delta R.T.: -0.026 min
Response: 1593
Conc: 0.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB143285TB

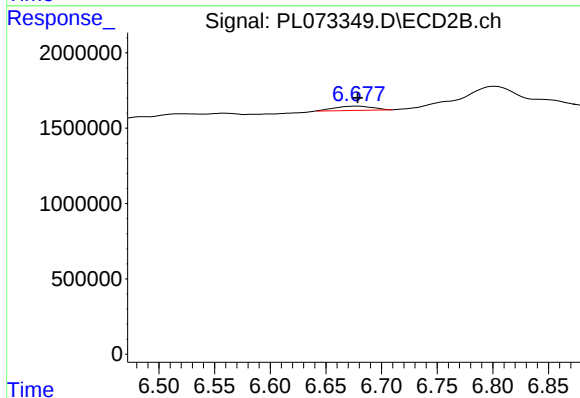


#6 beta-BHC

R.T.: 6.678 min
Delta R.T.: 0.000 min
Response: 680664
Conc: 0.65 ng/ml

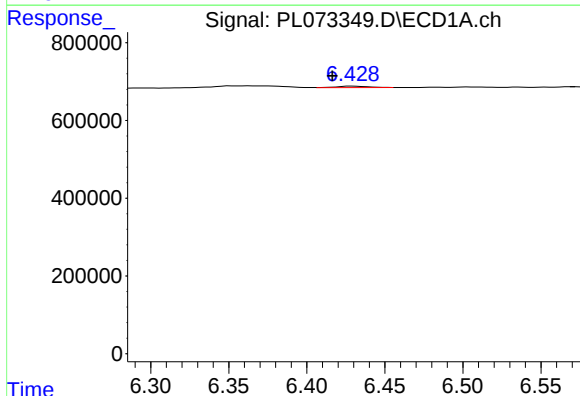


#7 delta-BHC

R.T.: 6.429 min
Delta R.T.: 0.013 min
Response: 52844
Conc: 0.13 ng/ml

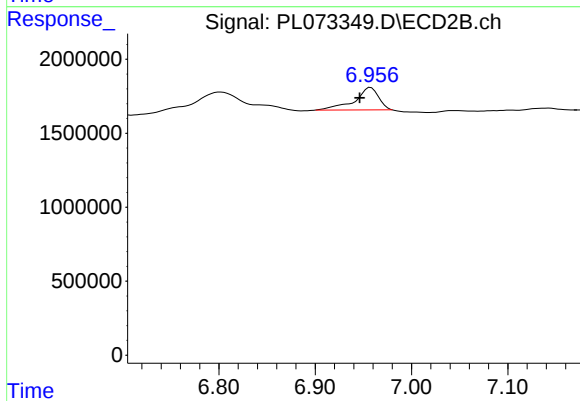

#7 delta-BHC


R.T.: 6.958 min
Delta R.T.: 0.011 min
Response: 2634891
Conc: 1.22 ng/ml

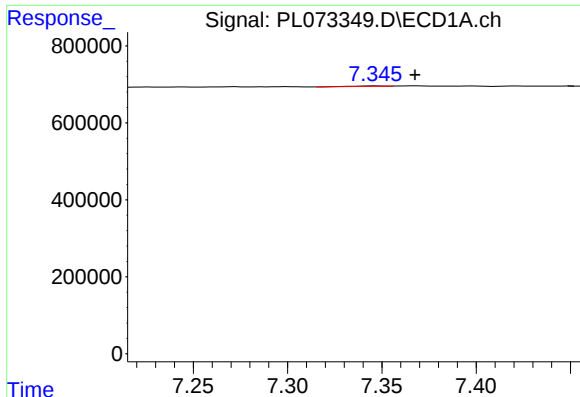

#10 gamma-Chlordane


R.T.: 7.346 min
Delta R.T.: -0.021 min
Response: 13216
Conc: 0.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB143285TB

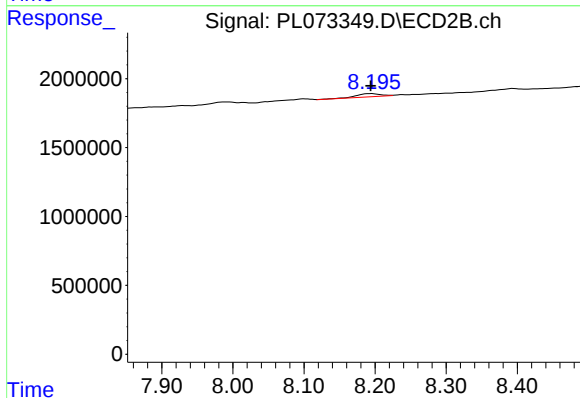


#10 gamma-Chlordane

R.T.: 8.196 min
Delta R.T.: 0.002 min
Response: 526133
Conc: 0.26 ng/ml

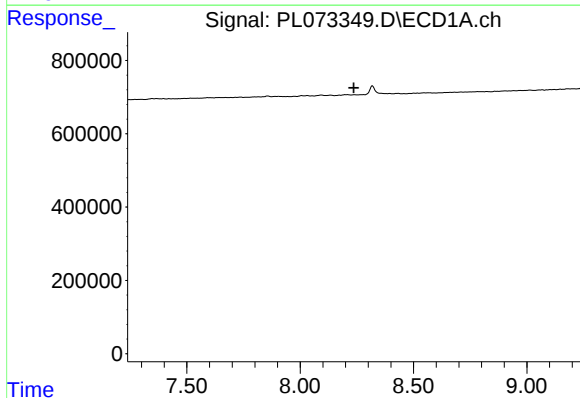


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.237 min
Response: 0
Conc: N.D.

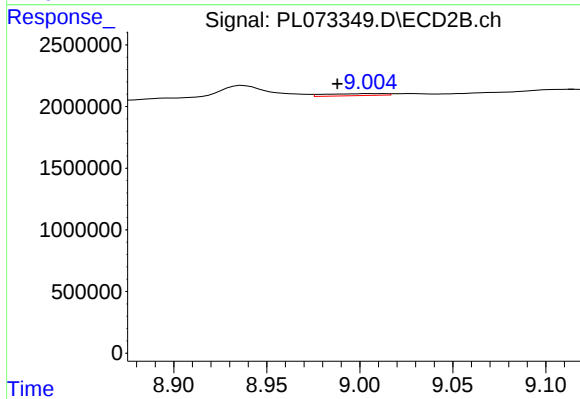

#16 4,4'-DDD


R.T.: 9.006 min
Delta R.T.: 0.018 min
Response: 354175
Conc: 0.24 ng/ml

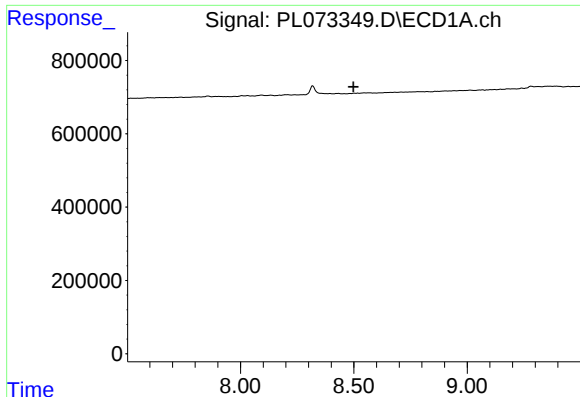

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.499 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB143285TB

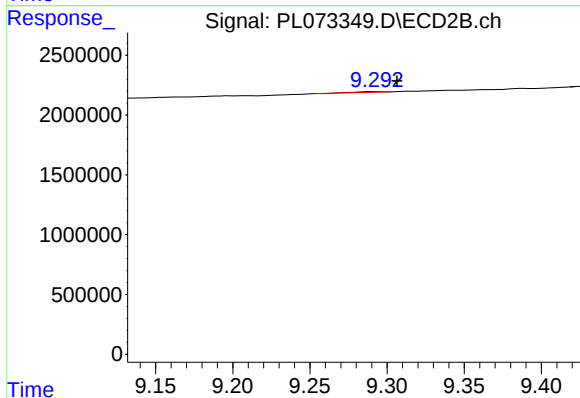


#17 4,4'-DDT

R.T.: 9.293 min
Delta R.T.: -0.013 min
Response: 69760
Conc: 0.04 ng/ml

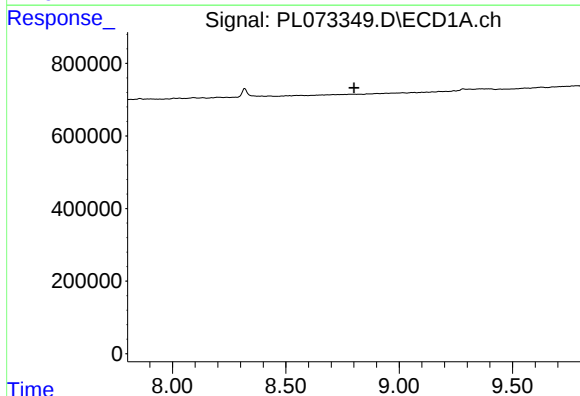


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 8.801 min
Response: 0
Conc: N.D.

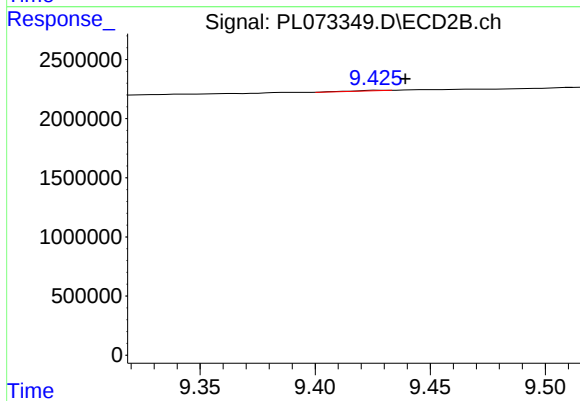

#19 Endosulfan Sulfate


R.T.: 9.429 min
Delta R.T.: -0.011 min
Response: 37782
Conc: 0.02 ng/ml

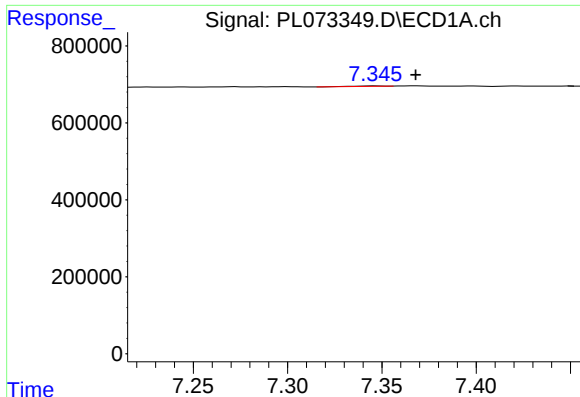

#25 Chlordane-3


R.T.: 7.346 min
Delta R.T.: -0.022 min
Response: 13216
Conc: 0.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB143285TB

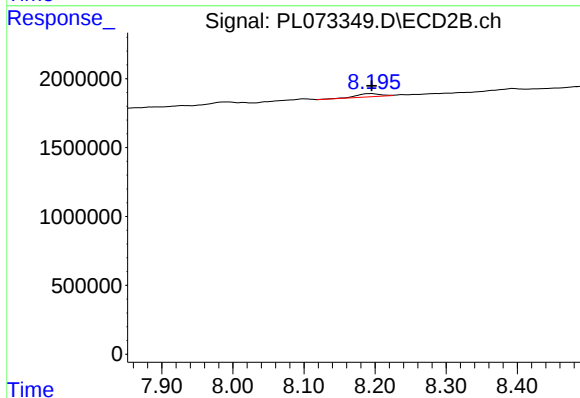


#25 Chlordane-3

R.T.: 8.196 min
Delta R.T.: 0.000 min
Response: 526133
Conc: 1.94 ng/ml

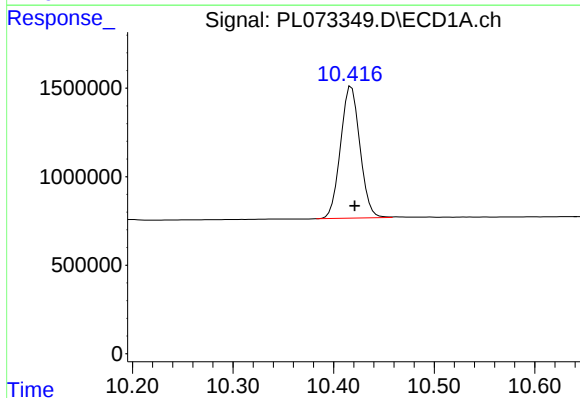

#28 Decachlorobiphenyl

R.T.: 10.418 min
Delta R.T.: -0.003 min
Response: 9964853
Conc: 19.60 ng/ml

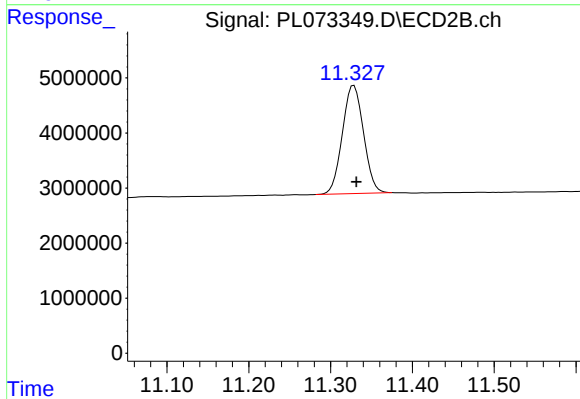

#28 Decachlorobiphenyl

R.T.: 11.328 min
Delta R.T.: -0.003 min
Response: 35266514
Conc: 19.72 ng/ml