

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031422\
 Data File : PL073350.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2022 20:35
 Operator : AR\AJ
 Sample : N1918-02
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 AVENUE-X-GROUT-SAMPLE-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 05:08:49 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
28) SA Decachlor...	0.000	11.358f	0	52079	N.D.	0.029 #
Target Compounds						
6) B beta-BHC	0.000	6.679	0	658849	N.D.	0.632 #
7) B delta-BHC	0.000	6.937	0	793085	N.D.	0.368 #
10) B gamma-Chl...	0.000	8.207	0	326415	N.D.	0.160 #
11) B alpha-Chl...	0.000	8.254f	0	150718	N.D.	0.075 #
15) B Endosulfa...	0.000	9.066	0	165229	N.D.	0.108 #
23) Chlordane-1	0.000	6.854	0	879131	N.D.	12.869 #
25) Chlordane-3	0.000	8.207	0	326415	N.D.	1.204 #
26) Chlordane-4	0.000	8.254f	0	150718	N.D.	0.455 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031422\
Data File : PL073350.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2022 20:35
Operator : AR\AJ
Sample : N1918-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
AVENUE-X-GROUT-SAMPLE-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 05:08:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

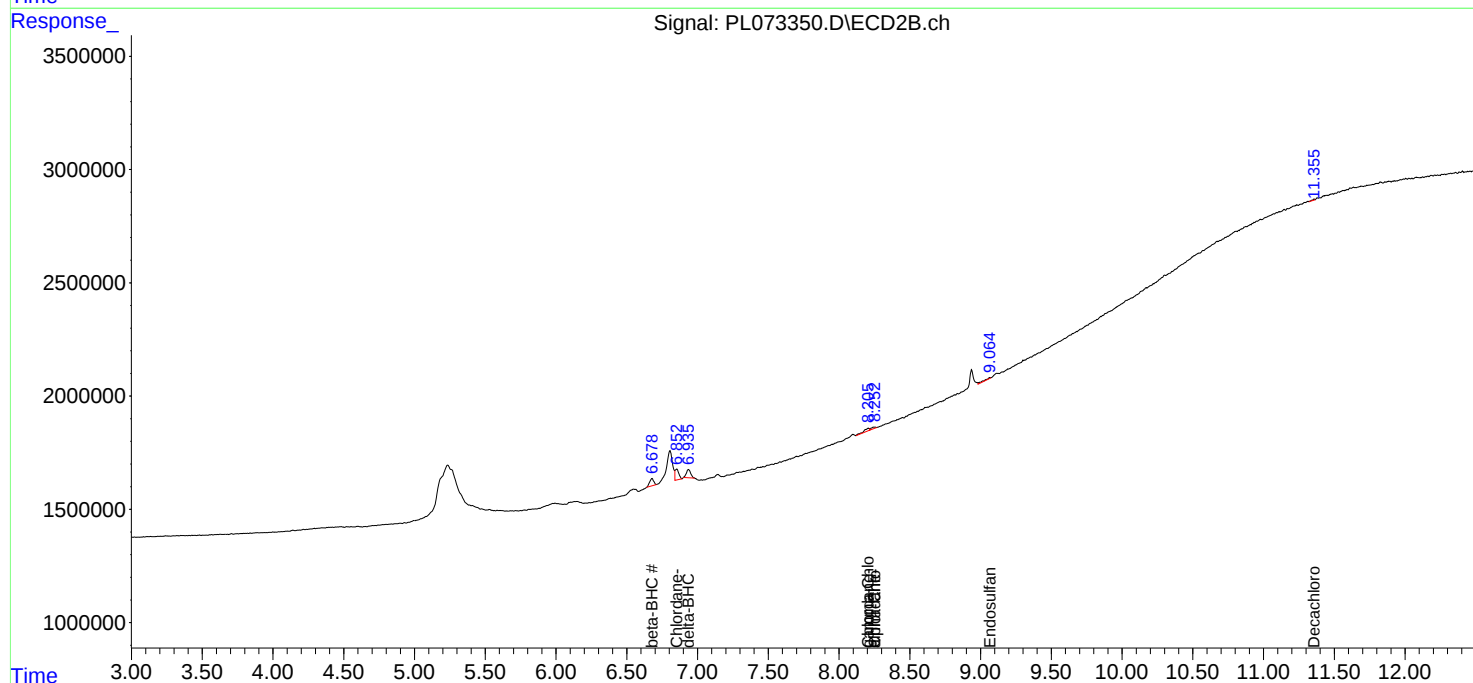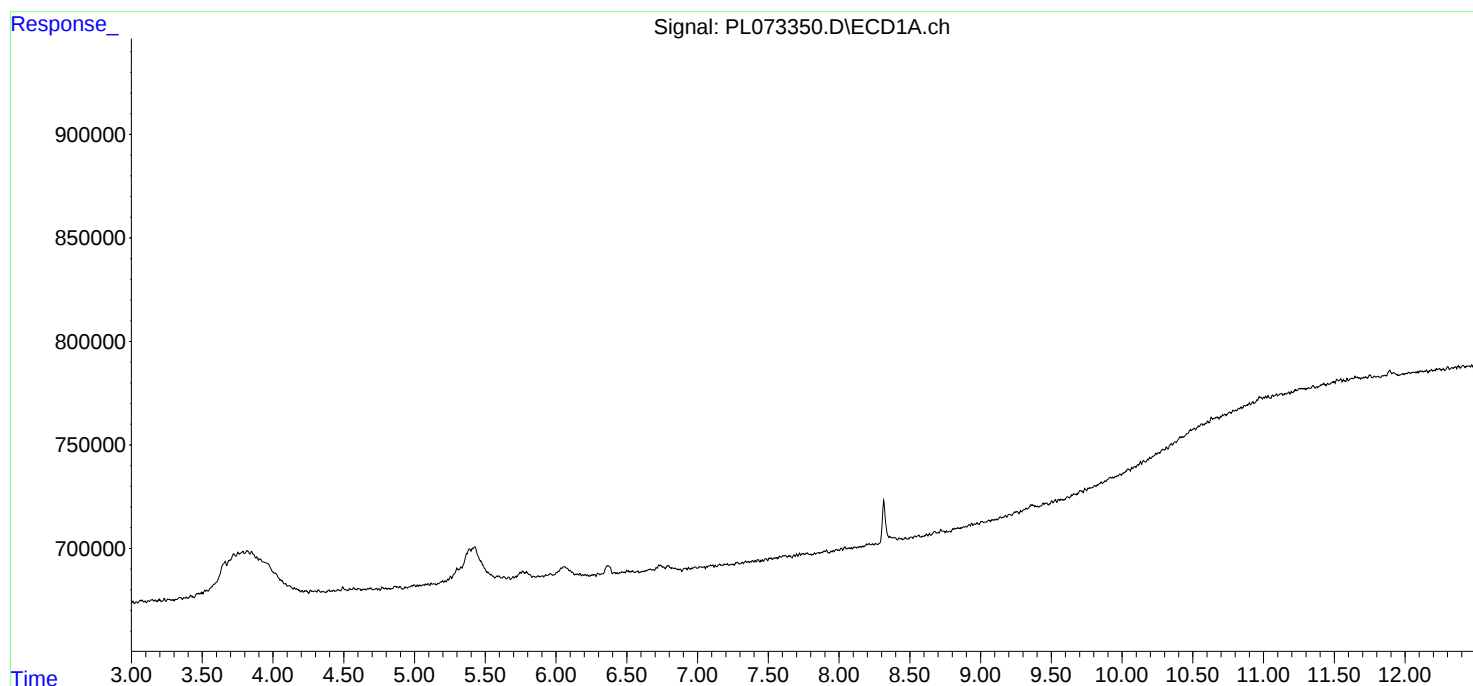


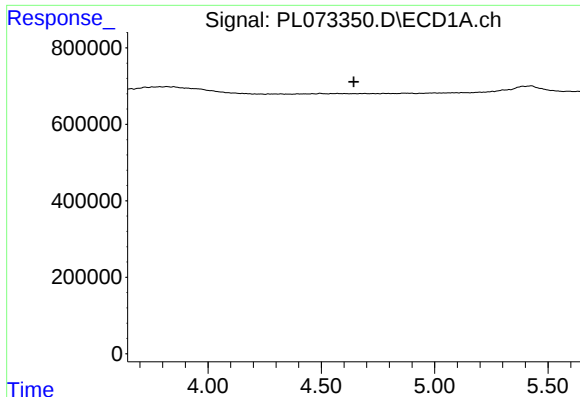

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.643 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
AVENUE-X-GROUT-SAMPLE-A

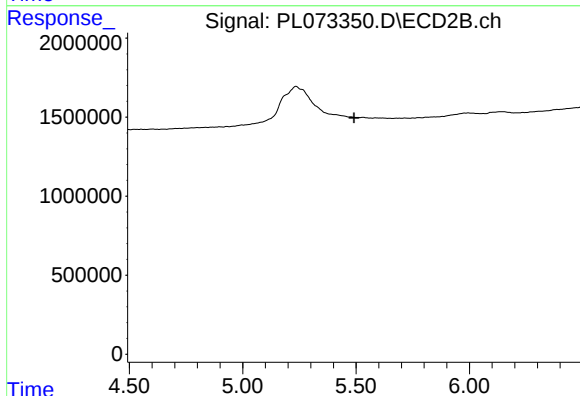


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 5.491 min
Response: 0
Conc: N.D.

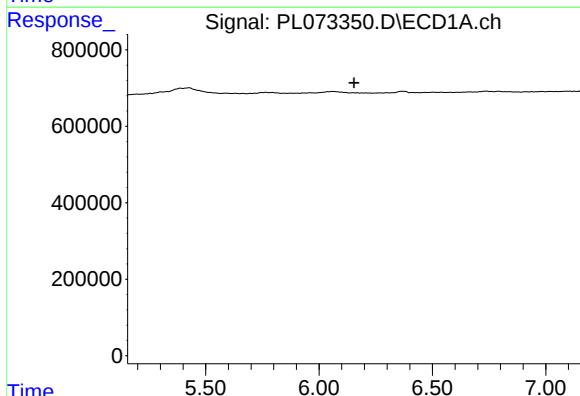


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.155 min
Response: 0
Conc: N.D.

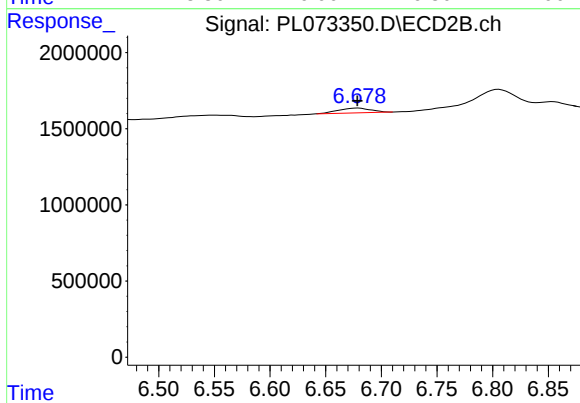

#6 beta-BHC


R.T.: 6.679 min
Delta R.T.: 0.000 min
Response: 658849
Conc: 0.63 ng/ml

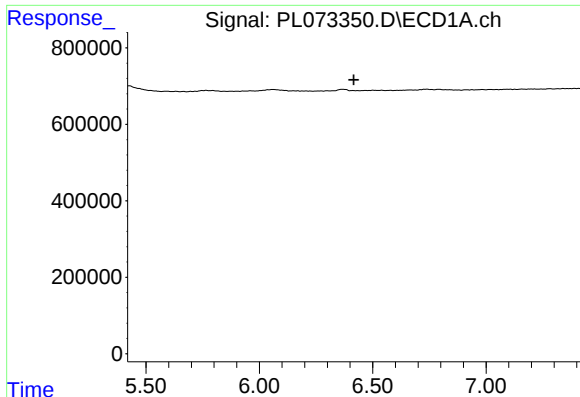

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.416 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
AVENUE-X-GROUT-SAMPLE-A

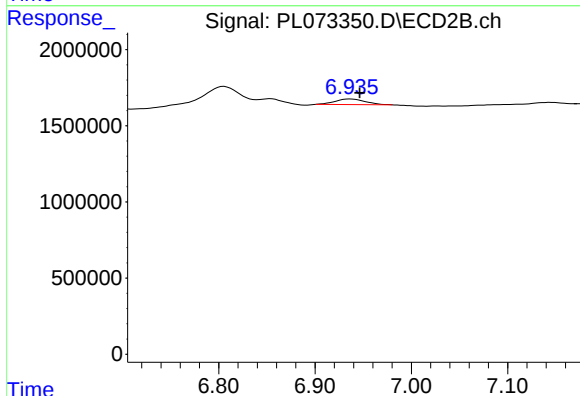


#7 delta-BHC

R.T.: 6.937 min
Delta R.T.: -0.010 min
Response: 793085
Conc: 0.37 ng/ml

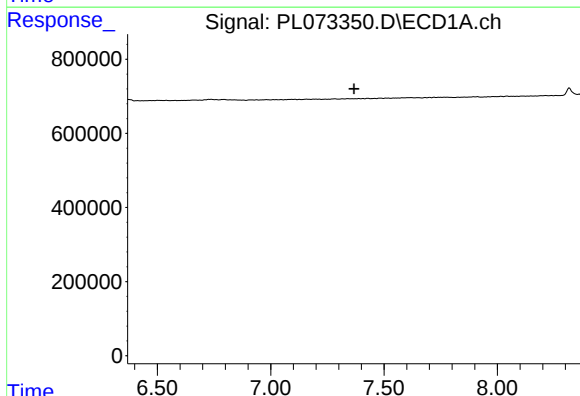


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 7.368 min
Response: 0
Conc: N.D.

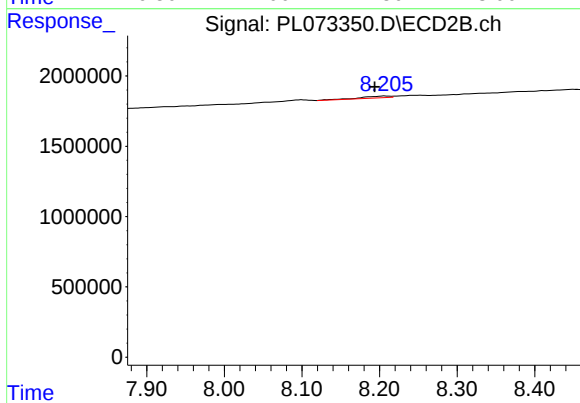

#10 gamma-Chlordane


R.T.: 8.207 min
Delta R.T.: 0.013 min
Response: 326415
Conc: 0.16 ng/ml

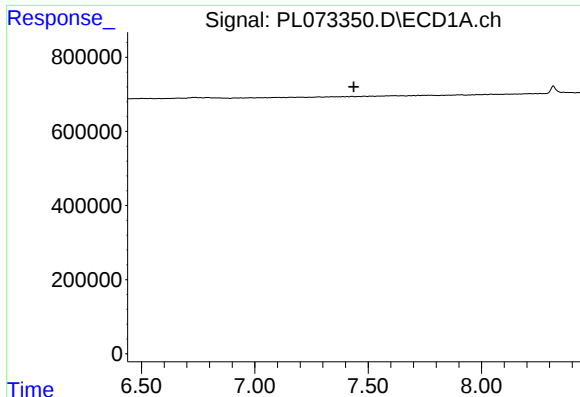

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.437 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
AVENUE-X-GROUT-SAMPLE-A

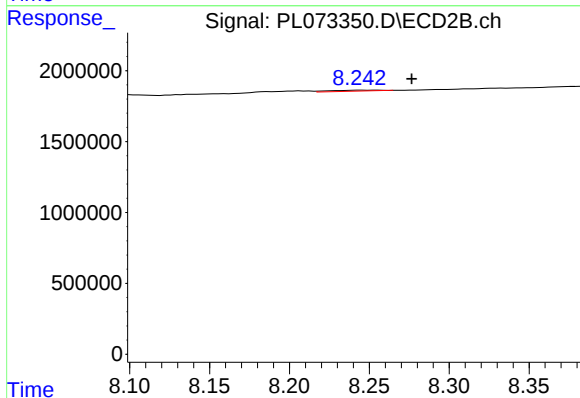


#11 alpha-Chlordane

R.T.: 8.254 min
Delta R.T.: -0.022 min
Response: 150718
Conc: 0.08 ng/ml

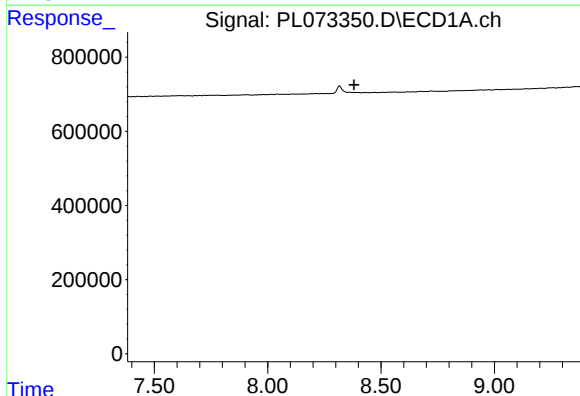


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.382 min
Response: 0
Conc: N.D.

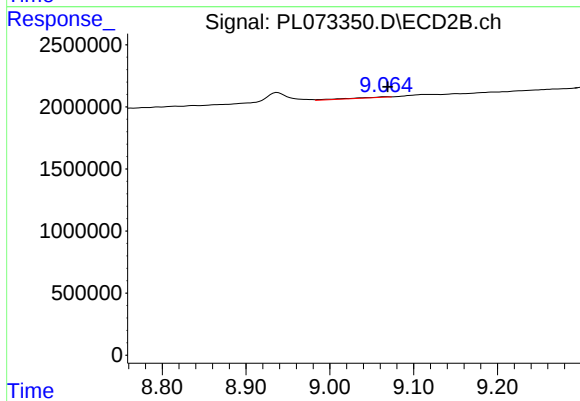

#15 Endosulfan II


R.T.: 9.066 min
Delta R.T.: -0.003 min
Response: 165229
Conc: 0.11 ng/ml

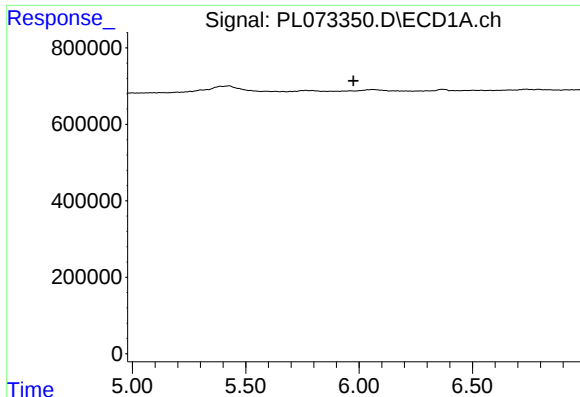

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.976 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
AVENUE-X-GROUT-SAMPLE-A

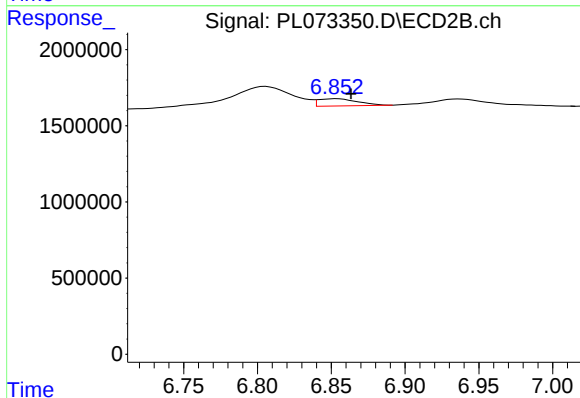


#23 Chlordane-1

R.T.: 6.854 min
Delta R.T.: -0.009 min
Response: 879131
Conc: 12.87 ng/ml

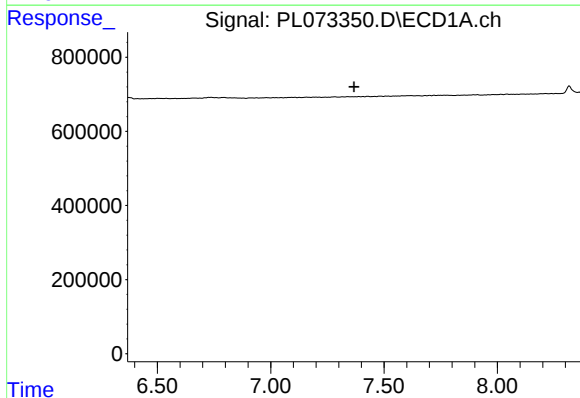


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

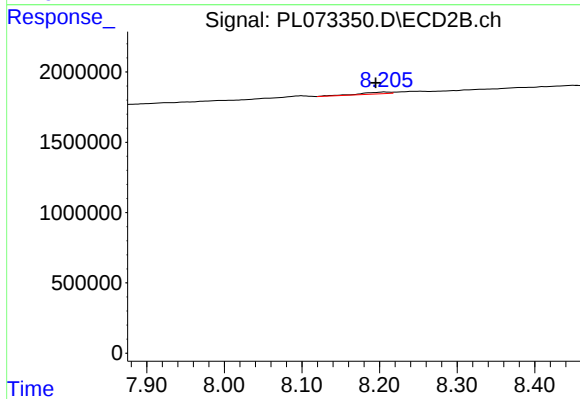

#25 Chlordane-3


R.T.: 8.207 min
Delta R.T.: 0.011 min
Response: 326415
Conc: 1.20 ng/ml

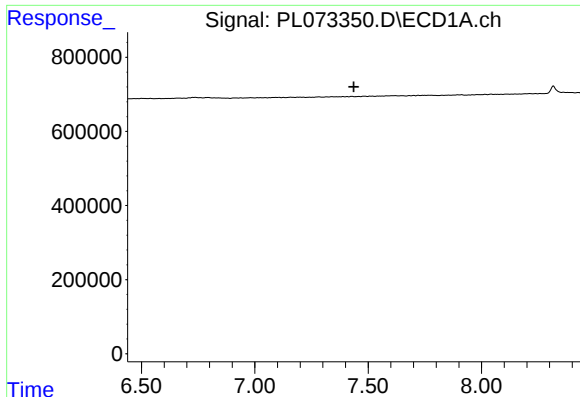

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.437 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
AVENUE-X-GROUT-SAMPLE-A

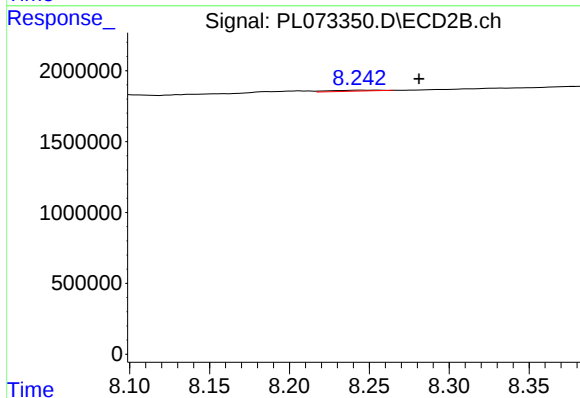


#26 Chlordane-4

R.T.: 8.254 min
Delta R.T.: -0.027 min
Response: 150718
Conc: 0.45 ng/ml

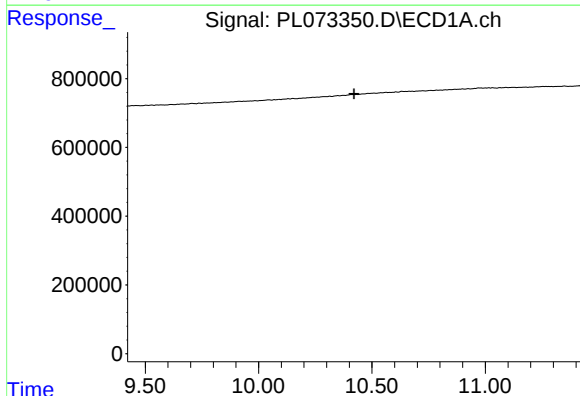

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 10.421 min
Response: 0
Conc: N.D.

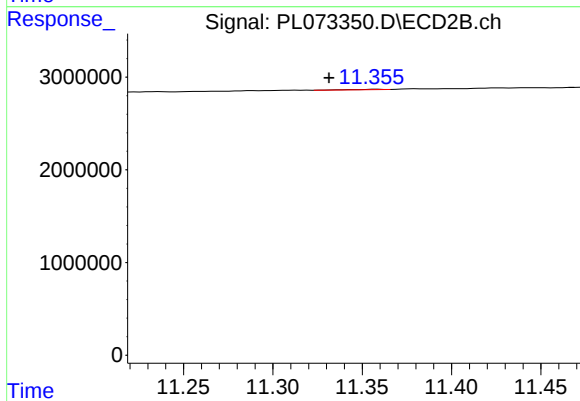

#28 Decachlorobiphenyl

R.T.: 11.358 min
Delta R.T.: 0.026 min
Response: 52079
Conc: 0.03 ng/ml