

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031422\
 Data File : PL073354.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2022 21:41
 Operator : AR\AJ
 Sample : PB143309BL
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB143309BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 05:11:49 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.643	5.489	6130740	31380453	19.141	19.120
28)	SA Decachlor...	10.417	11.328	10305864	36661829	20.267	20.502
Target Compounds							
6)	B beta-BHC	0.000	6.672	0	626555	N.D.	0.601 #
7)	B delta-BHC	0.000	6.956	0	1073449	N.D.	0.498 #
9)	A Endosulfan I	0.000	8.328	0	42416	N.D.	0.023 #
10)	B gamma-Chl...	0.000	8.196	0	510781	N.D.	0.250 #
11)	B alpha-Chl...	0.000	8.302f	0	288734	N.D.	0.144 #
15)	B Endosulfa...	8.354f	9.052f	112370	397452	0.287	0.259
23)	Chlordane-1	0.000	6.848f	0	939888	N.D.	13.759 #
25)	Chlordane-3	0.000	8.196	0	510781	N.D.	1.884 #
26)	Chlordane-4	0.000	8.302f	0	288734	N.D.	0.872 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031422\
Data File : PL073354.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2022 21:41
Operator : AR\AJ
Sample : PB143309BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB143309BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 05:11:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

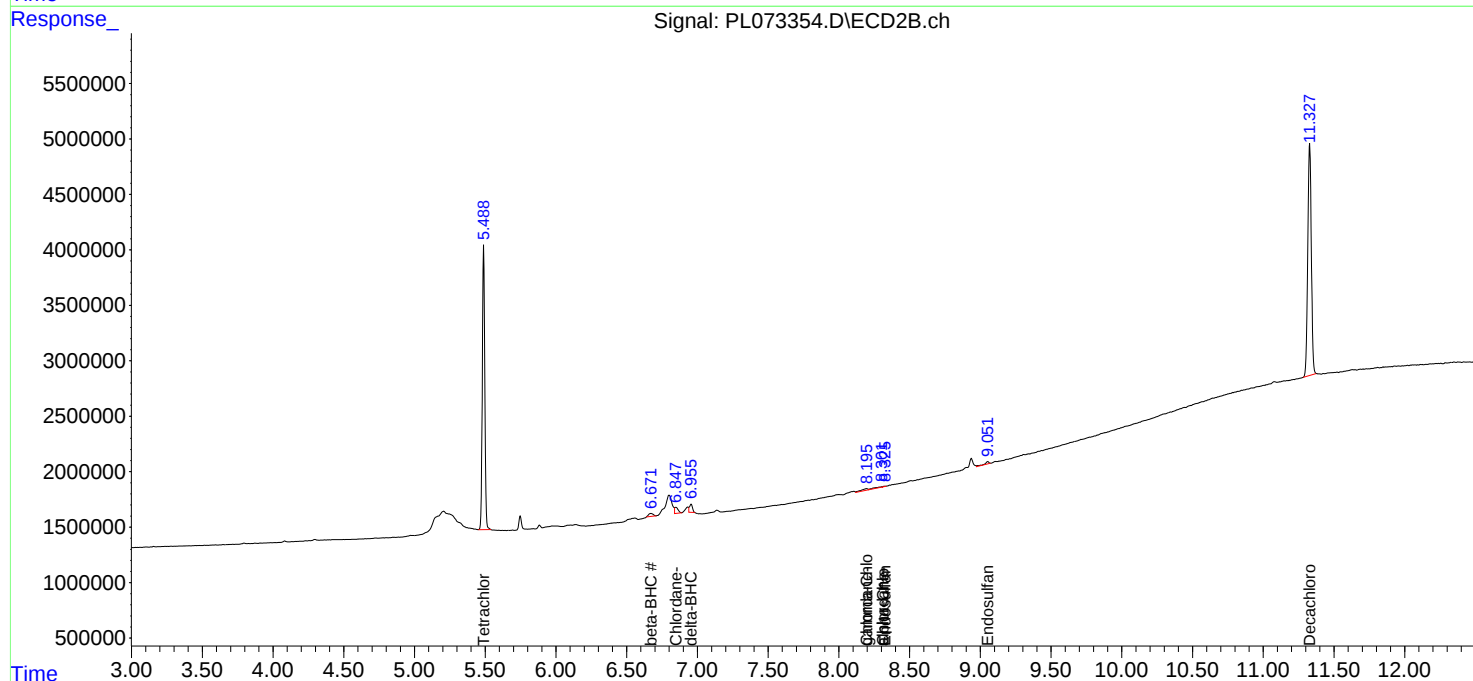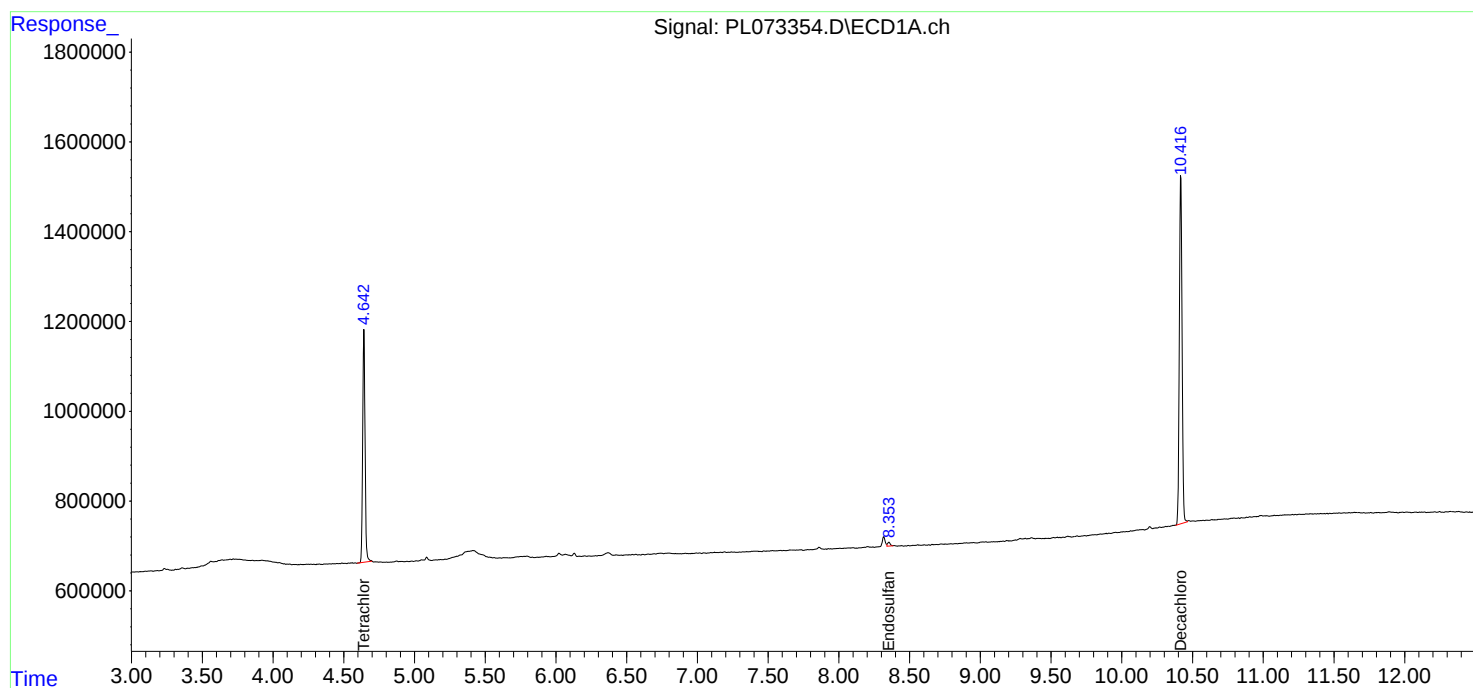


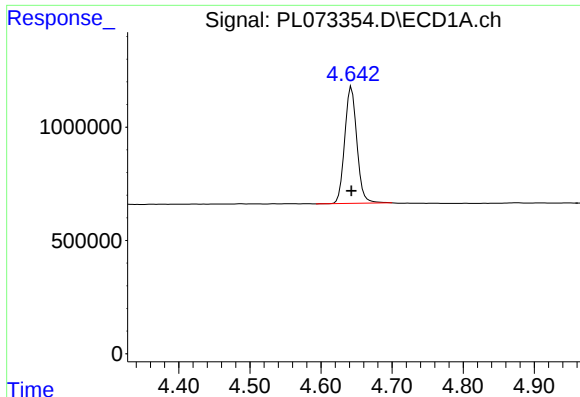

#1 Tetrachloro-m-xylene


R.T.: 4.643 min
Delta R.T.: 0.000 min
Response: 6130740
Conc: 19.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB143309BL

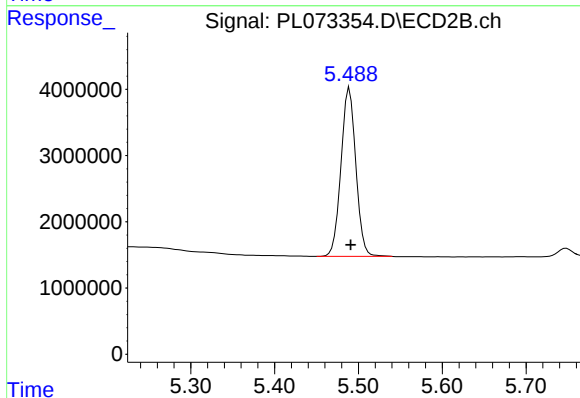


#1 Tetrachloro-m-xylene

R.T.: 5.489 min
Delta R.T.: -0.002 min
Response: 31380453
Conc: 19.12 ng/ml

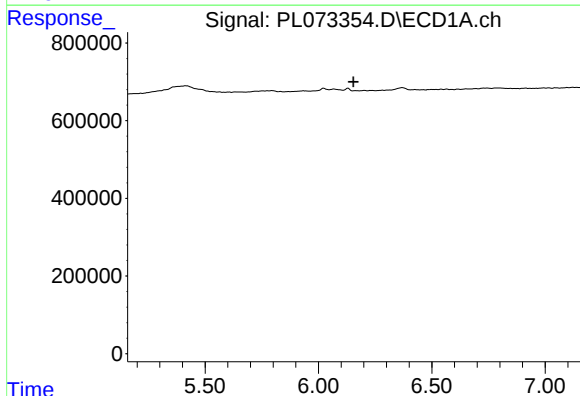


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.155 min
Response: 0
Conc: N.D.

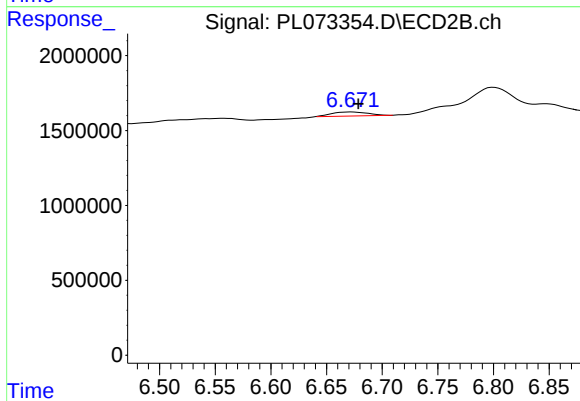

#6 beta-BHC


R.T.: 6.672 min
Delta R.T.: -0.006 min
Response: 626555
Conc: 0.60 ng/ml

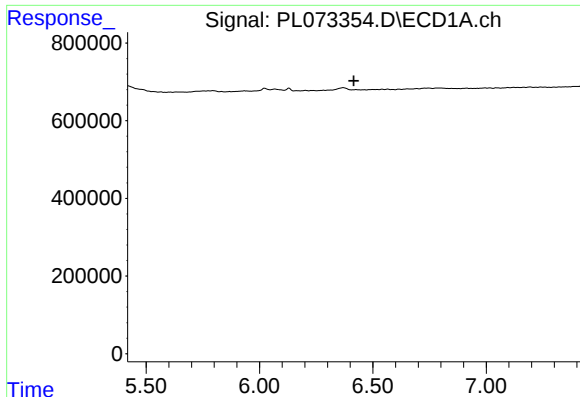

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.416 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB143309BL

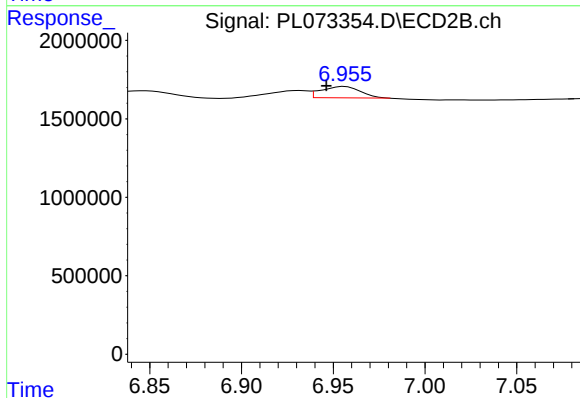


#7 delta-BHC

R.T.: 6.956 min
Delta R.T.: 0.010 min
Response: 1073449
Conc: 0.50 ng/ml

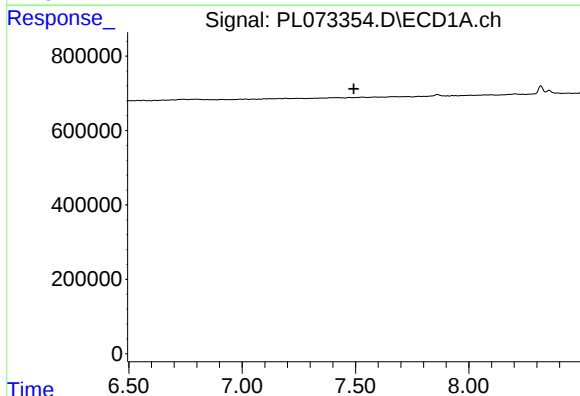


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.493 min
Response: 0
Conc: N.D.

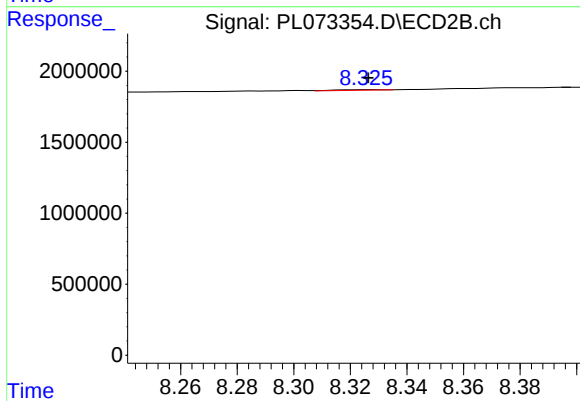

#9 Endosulfan I


R.T.: 8.328 min
Delta R.T.: 0.001 min
Response: 42416
Conc: 0.02 ng/ml

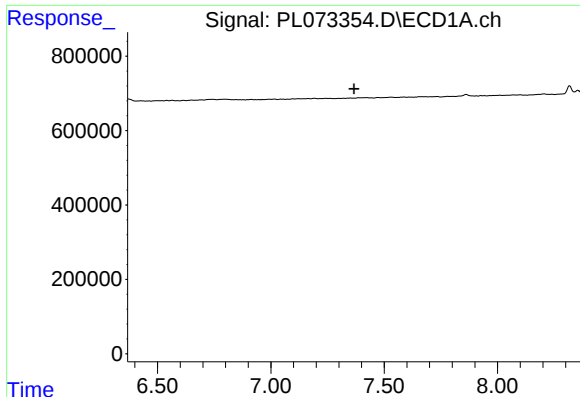

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB143309BL

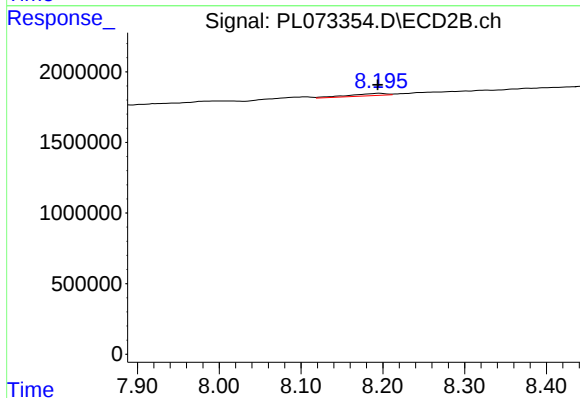


#10 gamma-Chlordane

R.T.: 8.196 min
Delta R.T.: 0.003 min
Response: 510781
Conc: 0.25 ng/ml

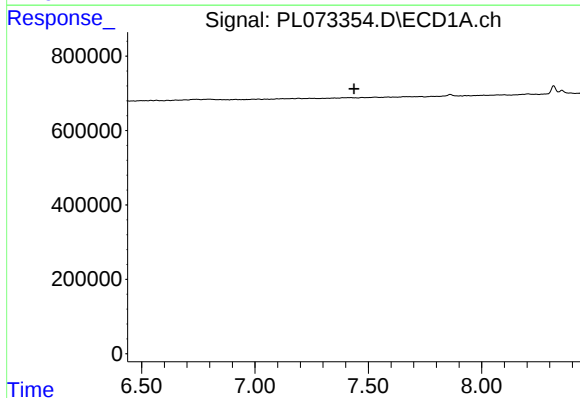


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.437 min
Response: 0
Conc: N.D.

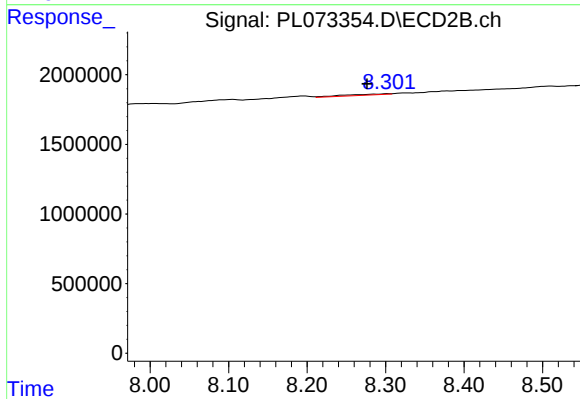

#11 alpha-Chlordane


R.T.: 8.302 min
Delta R.T.: 0.026 min
Response: 288734
Conc: 0.14 ng/ml

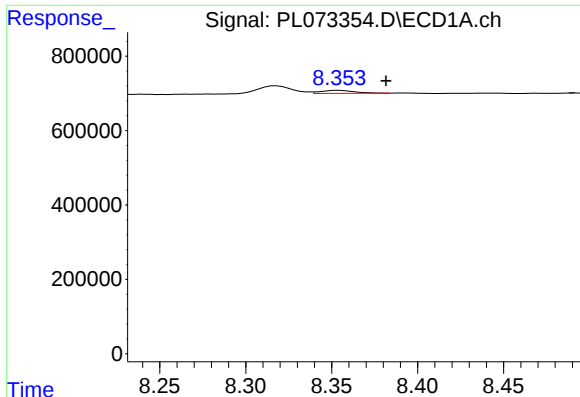

#15 Endosulfan II


R.T.: 8.354 min
Delta R.T.: -0.027 min
Response: 112370
Conc: 0.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB143309BL

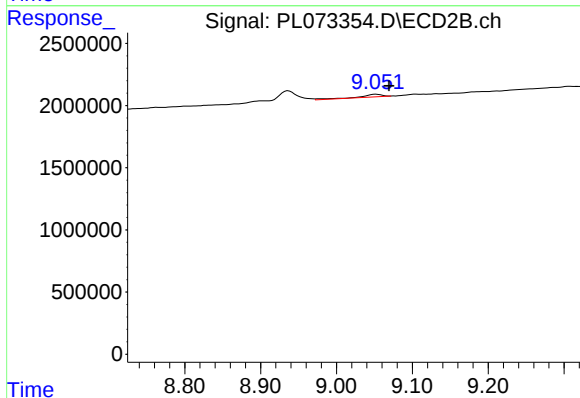


#15 Endosulfan II

R.T.: 9.052 min
Delta R.T.: -0.017 min
Response: 397452
Conc: 0.26 ng/ml

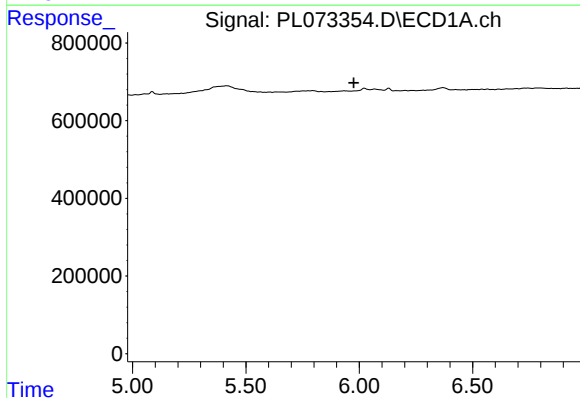


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.976 min
Response: 0
Conc: N.D.

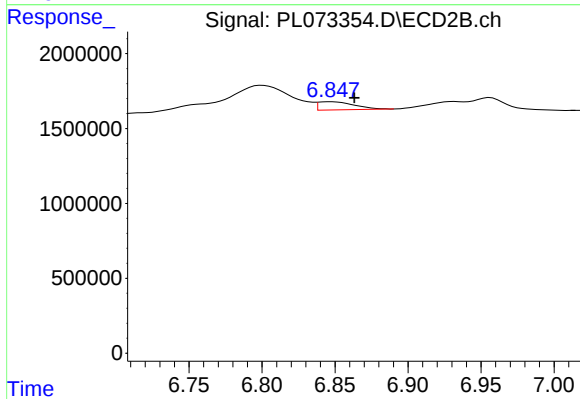

#23 Chlordane-1


R.T.: 6.848 min
Delta R.T.: -0.015 min
Response: 939888
Conc: 13.76 ng/ml

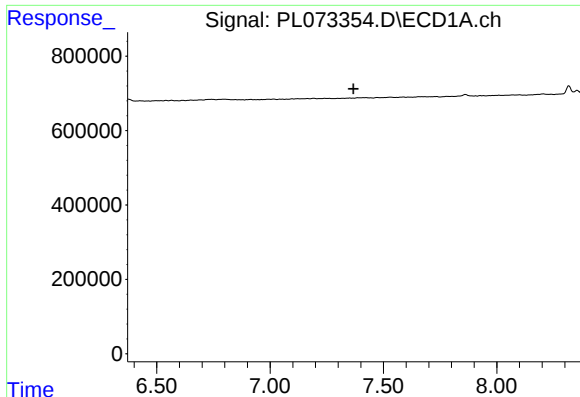

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB143309BL

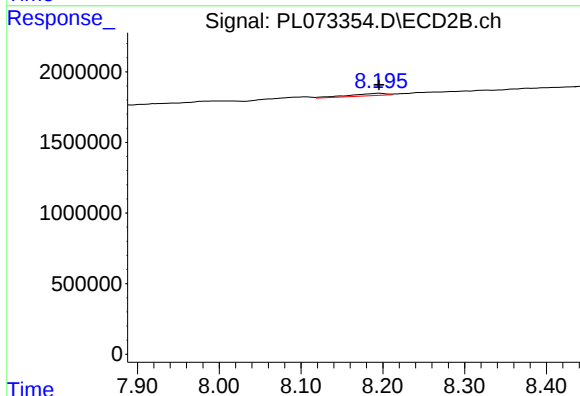


#25 Chlordane-3

R.T.: 8.196 min
Delta R.T.: 0.001 min
Response: 510781
Conc: 1.88 ng/ml

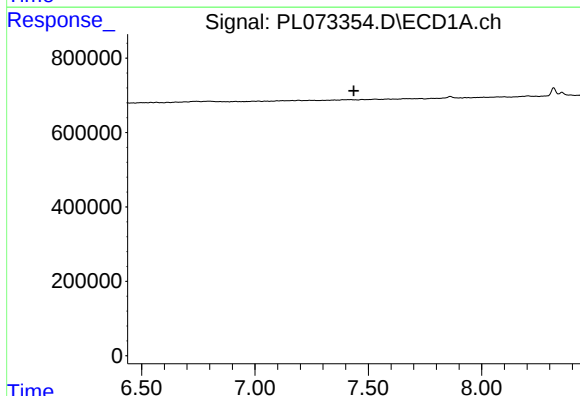


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.437 min
Response: 0
Conc: N.D.

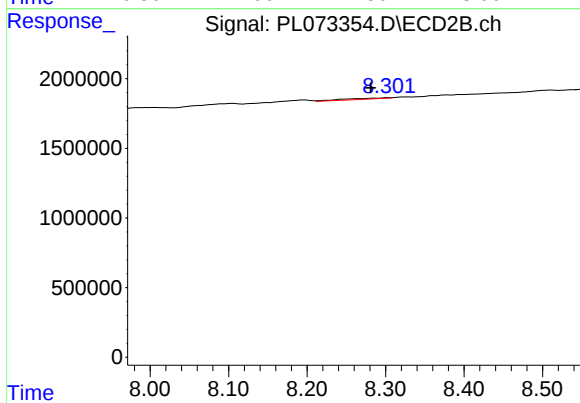

#26 Chlordane-4


R.T.: 8.302 min
Delta R.T.: 0.021 min
Response: 288734
Conc: 0.87 ng/ml

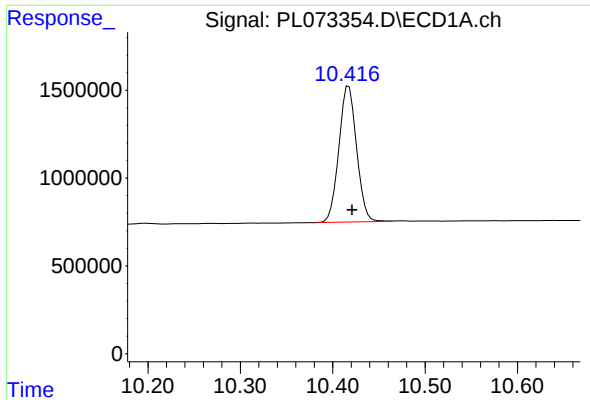

#28 Decachlorobiphenyl

R.T.: 10.417 min
Delta R.T.: -0.004 min
Response: 10305864
Conc: 20.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB143309BL

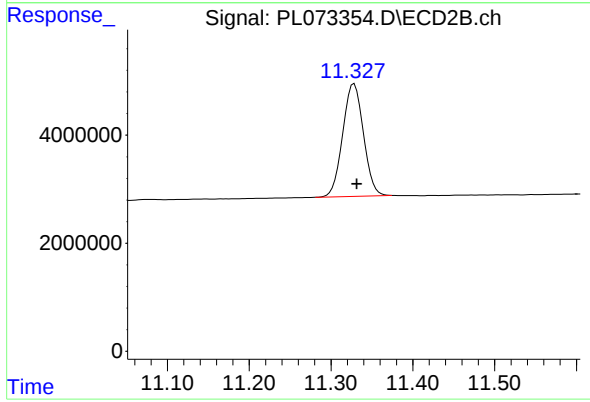

#28 Decachlorobiphenyl

R.T.: 11.328 min
Delta R.T.: -0.003 min
Response: 36661829
Conc: 20.50 ng/ml