

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031422\
 Data File : PL073345.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2022 19:12
 Operator : AR\AJ
 Sample : PB143301BS
 Misc : CHLOR BS
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB143301BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 05:05:49 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.641	5.489	7969230	33266720	24.882	20.269
28)	SA Decachlor...	10.416	11.327	10675639	37201665	20.994	20.804
Target Compounds							
23)	Chlordane-1	5.973	6.861	2458672	13270584	207.395	194.261
24)	Chlordane-2	6.663	7.443	3417754	14477297	209.512	201.427
25)	Chlordane-3	7.365	8.193	7835135	51475324	191.877	189.853
26)	Chlordane-4	7.433	8.279	8631316	63747290	194.746	192.443
27)	Chlordane-5	8.383	9.147	3274654	10294657	199.975	189.667



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031422\
Data File : PL073345.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2022 19:12
Operator : AR\AJ
Sample : PB143301BS
Misc : CHLOR BS
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB143301BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 05:05:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

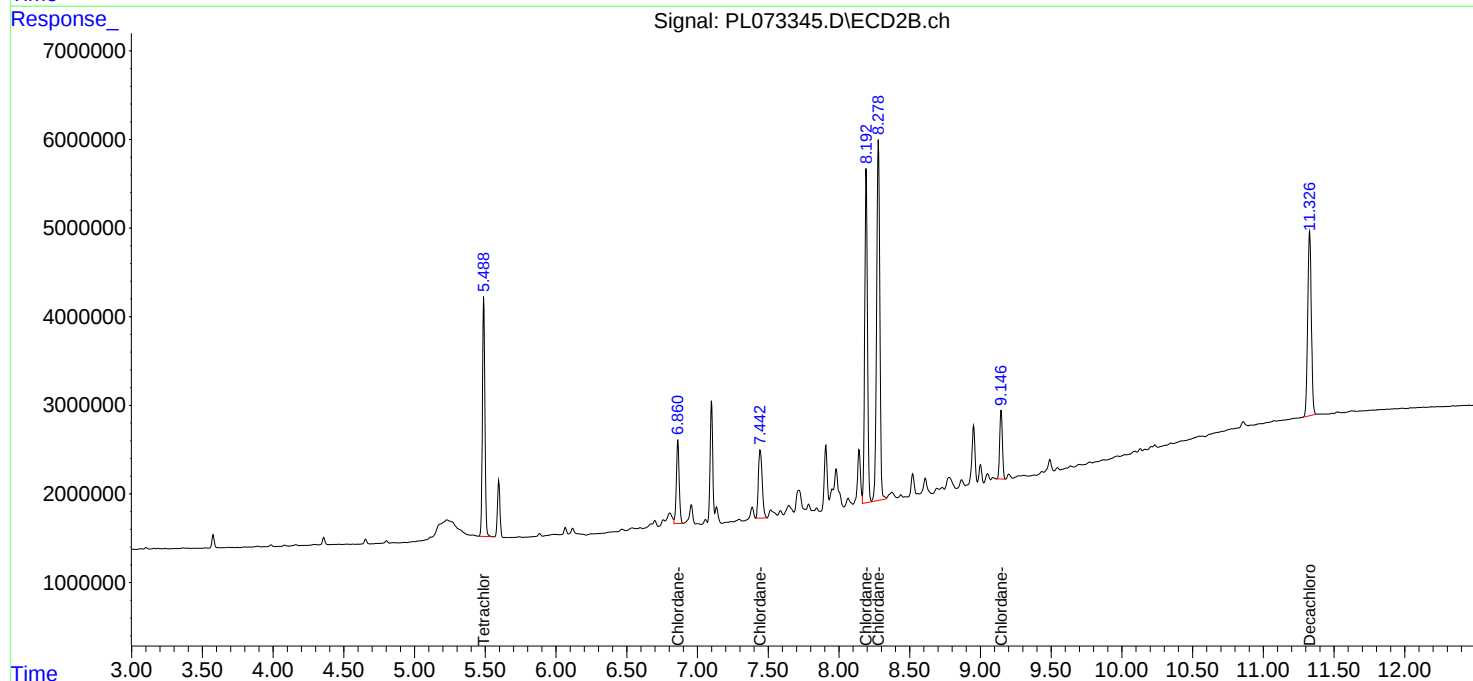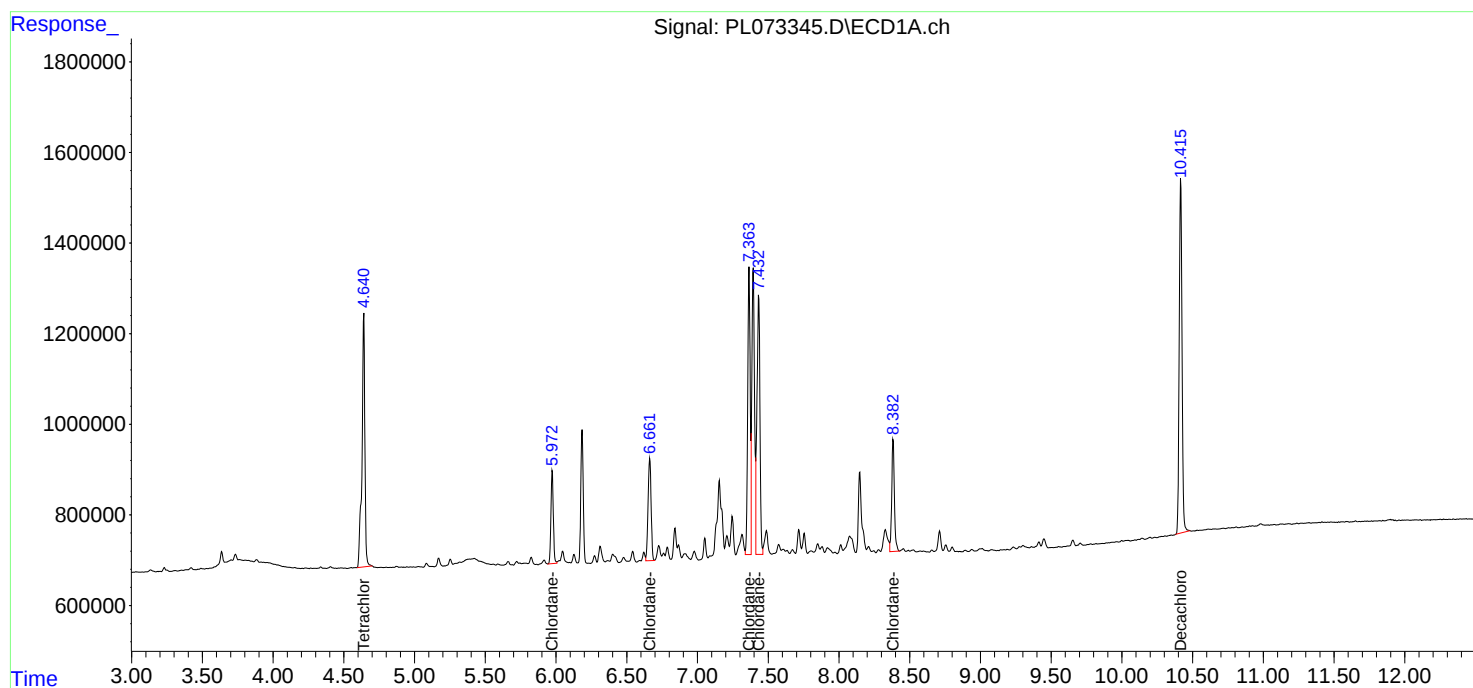


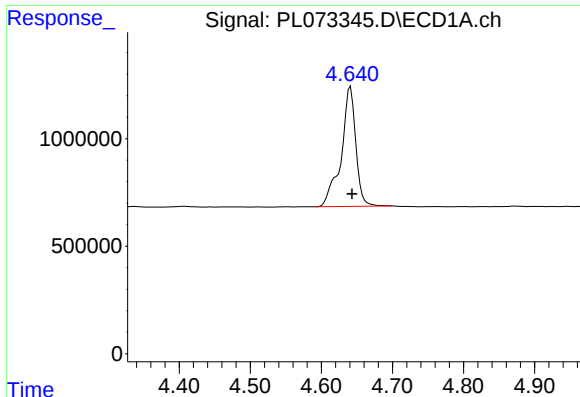

#1 Tetrachloro-m-xylene


R.T.: 4.641 min
Delta R.T.: -0.002 min
Response: 7969230
Conc: 24.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB143301BS

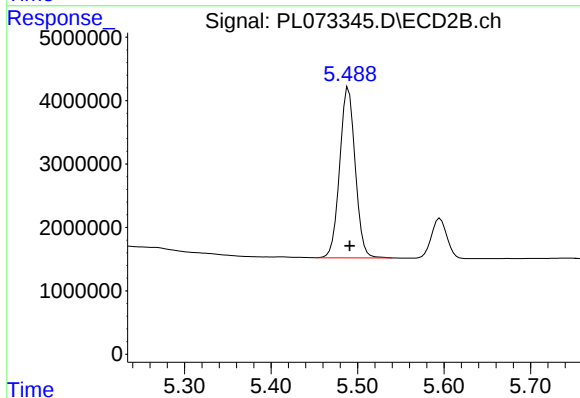


#1 Tetrachloro-m-xylene

R.T.: 5.489 min
Delta R.T.: -0.002 min
Response: 33266720
Conc: 20.27 ng/ml

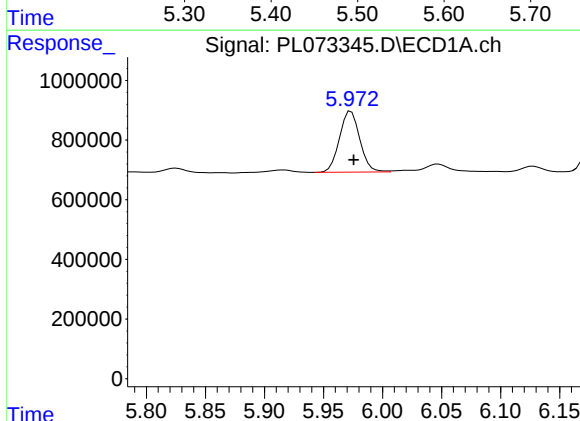


#23 Chlordane-1

R.T.: 5.973 min
Delta R.T.: -0.002 min
Response: 2458672
Conc: 207.40 ng/ml

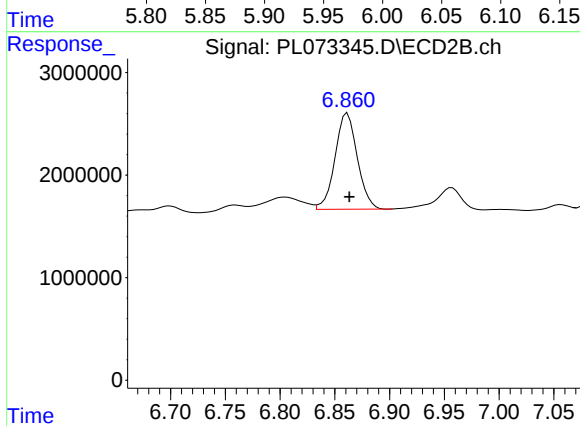

#23 Chlordane-1


R.T.: 6.861 min
Delta R.T.: -0.002 min
Response: 13270584
Conc: 194.26 ng/ml

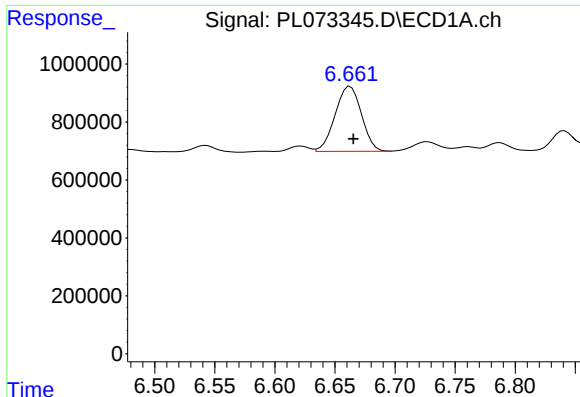

#24 Chlordane-2


R.T.: 6.663 min
Delta R.T.: -0.003 min
Response: 3417754
Conc: 209.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB143301BS

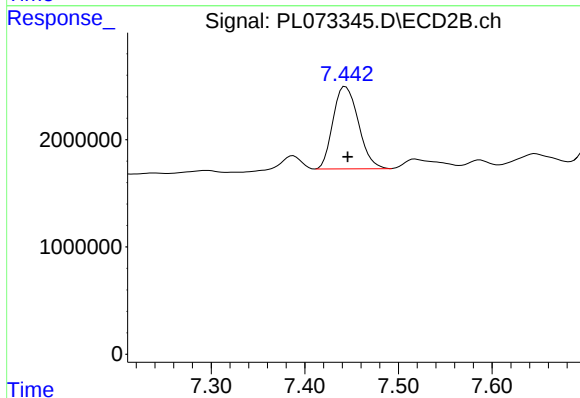


#24 Chlordane-2

R.T.: 7.443 min
Delta R.T.: -0.002 min
Response: 14477297
Conc: 201.43 ng/ml

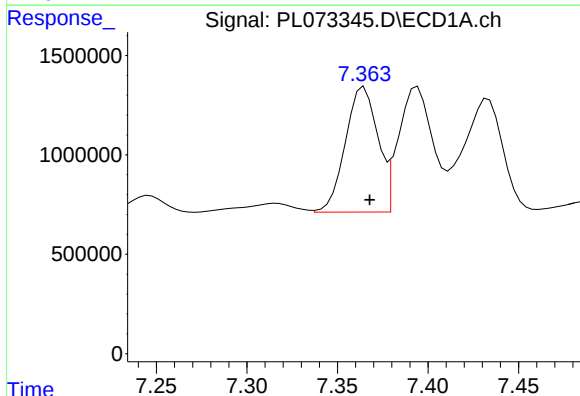


#25 Chlordane-3

R.T.: 7.365 min
Delta R.T.: -0.003 min
Response: 7835135
Conc: 191.88 ng/ml

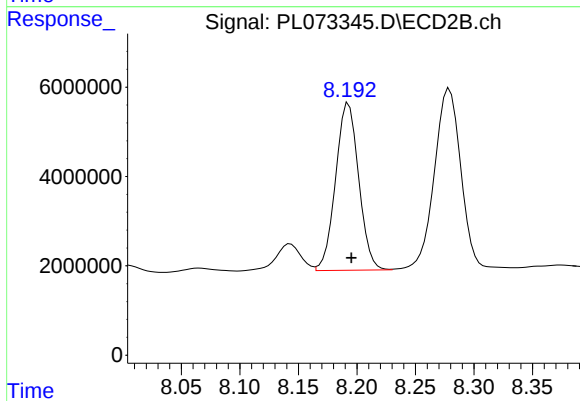

#25 Chlordane-3


R.T.: 8.193 min
Delta R.T.: -0.002 min
Response: 51475324
Conc: 189.85 ng/ml

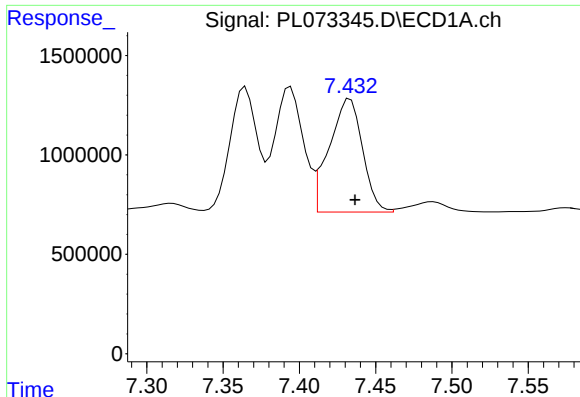

#26 Chlordane-4


R.T.: 7.433 min
Delta R.T.: -0.003 min
Response: 8631316
Conc: 194.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB143301BS

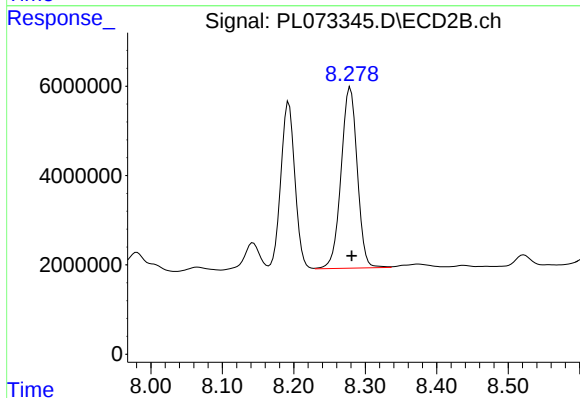


#26 Chlordane-4

R.T.: 8.279 min
Delta R.T.: -0.002 min
Response: 63747290
Conc: 192.44 ng/ml

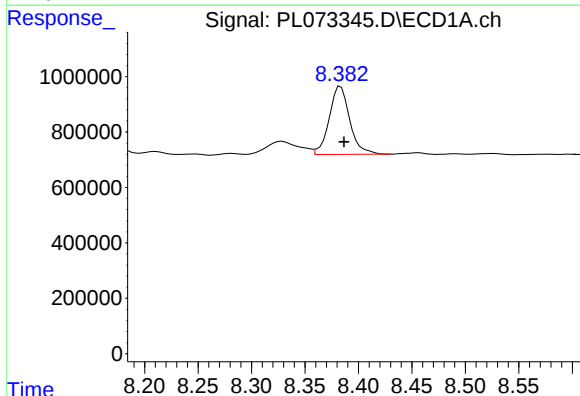


#27 Chlordane-5

R.T.: 8.383 min
Delta R.T.: -0.003 min
Response: 3274654
Conc: 199.98 ng/ml

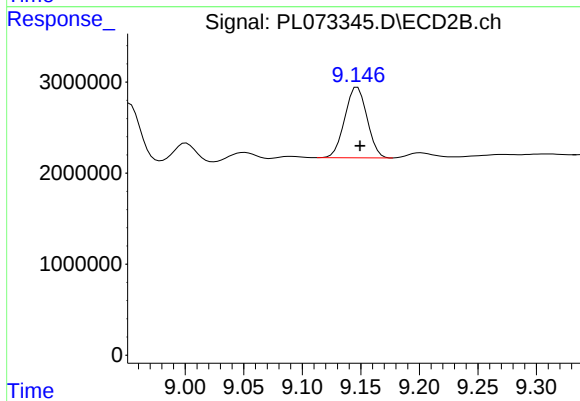

#27 Chlordane-5


R.T.: 9.147 min
Delta R.T.: -0.002 min
Response: 10294657
Conc: 189.67 ng/ml

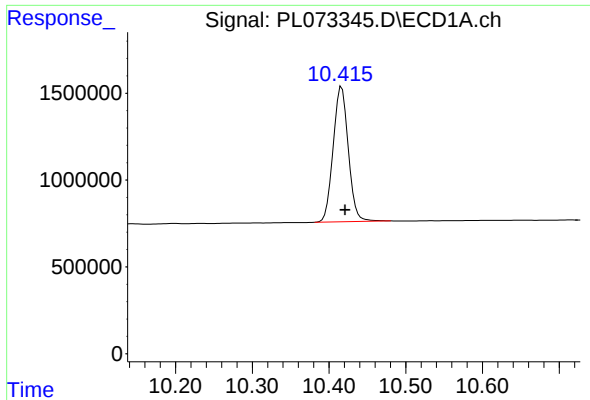

#28 Decachlorobiphenyl

R.T.: 10.416 min
Delta R.T.: -0.005 min
Response: 10675639
Conc: 20.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB143301BS

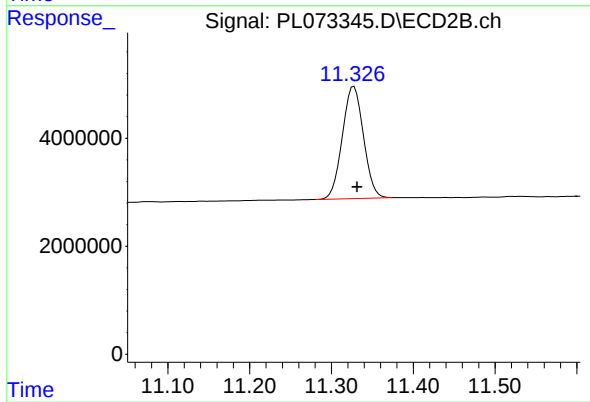

#28 Decachlorobiphenyl

R.T.: 11.327 min
Delta R.T.: -0.004 min
Response: 37201665
Conc: 20.80 ng/ml