

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031422\
 Data File : PL073366.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2022 01:05
 Operator : AR\AJ
 Sample : N1905-11
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WC-14A-1C

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/15/2022
 Supervised By : Ankita Jodhani 03/15/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 05:19:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.644	5.490	3737191	14658290	11.668	8.931
28) SA Decachlor...	10.417	11.327	5982065	20045466	11.764m	11.210m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031422\
Data File : PL073366.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2022 01:05
Operator : AR\AJ
Sample : N1905-11
Misc :
ALS Vial : 35 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
WC-14A-1C


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/15/2022
Supervised By : Ankita Jodhani 03/15/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 05:19:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

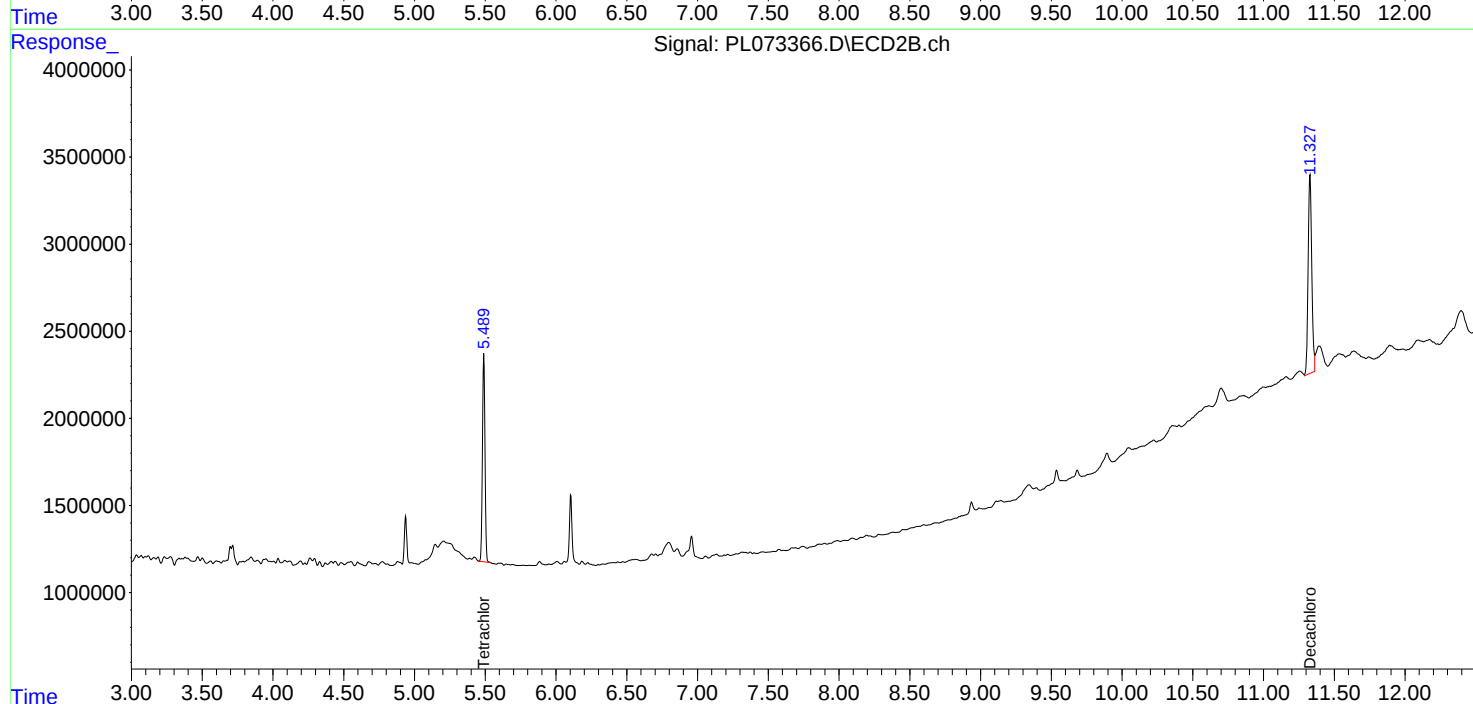

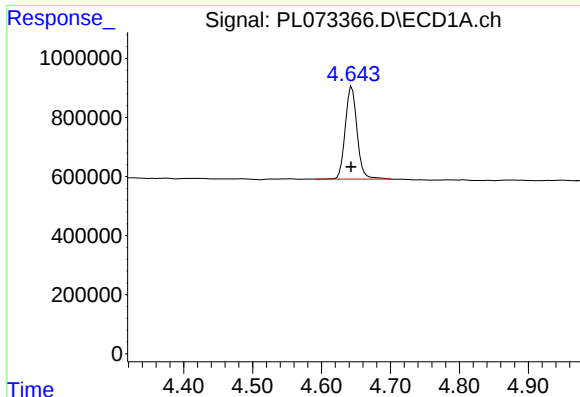


#1 Tetrachloro-m-xylene

R.T.: 4.644 min
Delta R.T.: 0.001 min
Response: 3737191
Conc: 11.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
WC-14A-1C


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/15/2022
Supervised By :Ankita Jodhani 03/15/2022

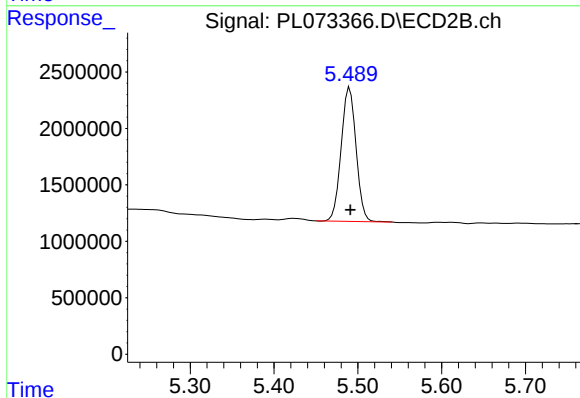


#1 Tetrachloro-m-xylene

R.T.: 5.490 min
Delta R.T.: 0.000 min
Response: 14658290
Conc: 8.93 ng/ml

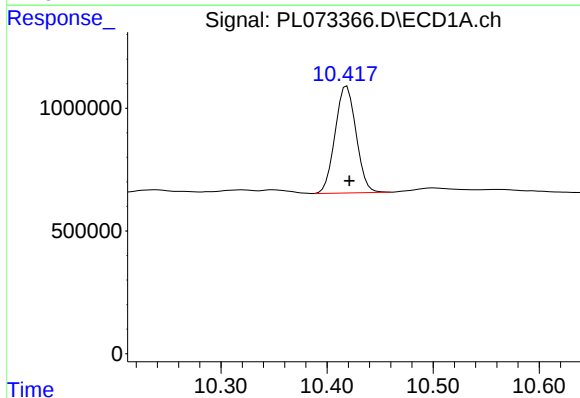

#28 Decachlorobiphenyl

R.T.: 10.417 min
Delta R.T.: -0.004 min
Response: 5982065
Conc: 11.76 ng/ml m

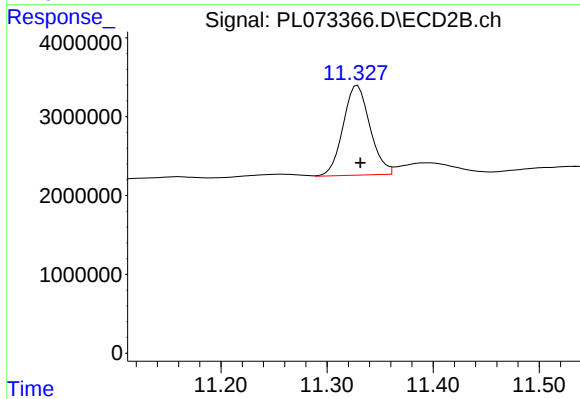

#28 Decachlorobiphenyl

R.T.: 11.327 min
Delta R.T.: -0.004 min
Response: 20045466
Conc: 11.21 ng/ml m