

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031424\
 Data File : PL088557.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2024 12:44
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 15:37:49 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 13 15:37:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.634	2.852	281.9E6	174.0E6	103.994	105.075
28)	SA Decachlor...	9.303	8.082	241.3E6	135.6E6	100.589	98.917
Target Compounds							
23)	Chlordane-1	4.819	3.874	119.6E6	50006194	1034.666	1043.620
24)	Chlordane-2	5.356	4.462	125.9E6	58869323	986.883	987.644
25)	Chlordane-3	6.076	5.103	516.7E6	179.5E6	1052.193	1052.589
26)	Chlordane-4	6.159	5.167	612.2E6	165.7E6	1034.555	1041.832
27)	Chlordane-5	7.020	5.843	105.9E6	50744780	1017.873	1012.924



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031424\
Data File : PL088557.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2024 12:44
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 15:37:49 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
Quant Title : GC Extractables
QLast Update : Wed Mar 13 15:37:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

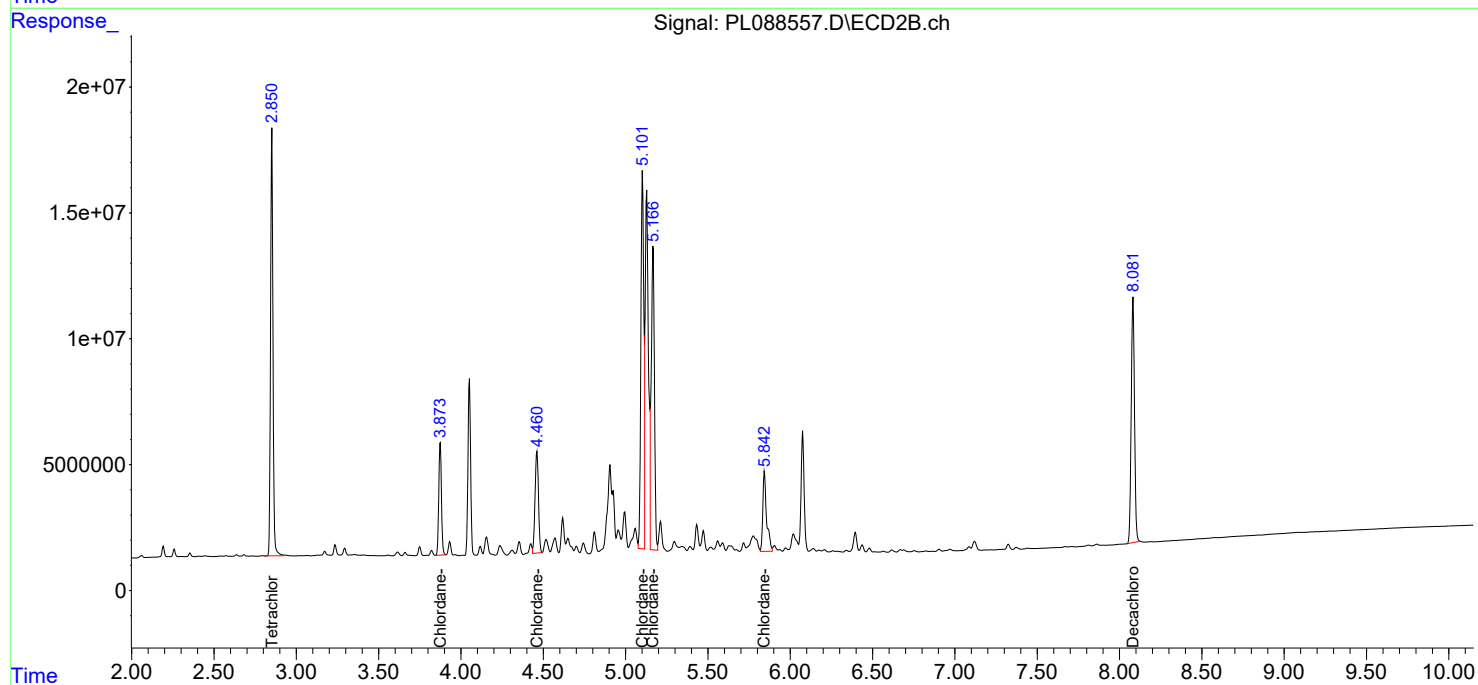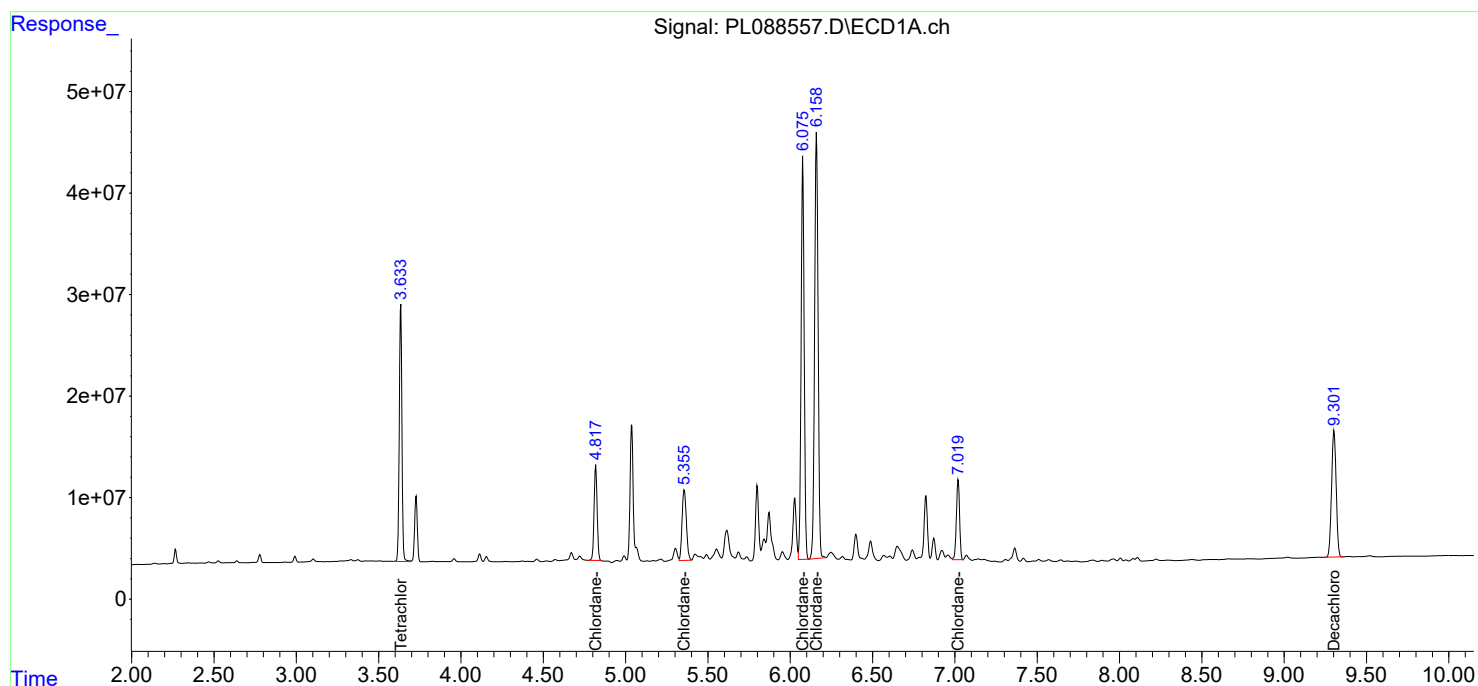


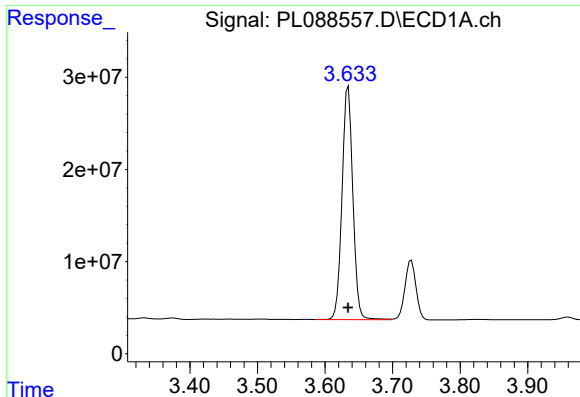

#1 Tetrachloro-m-xylene


R.T.: 3.634 min
Delta R.T.: 0.000 min
Response: 281875907
Conc: 103.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

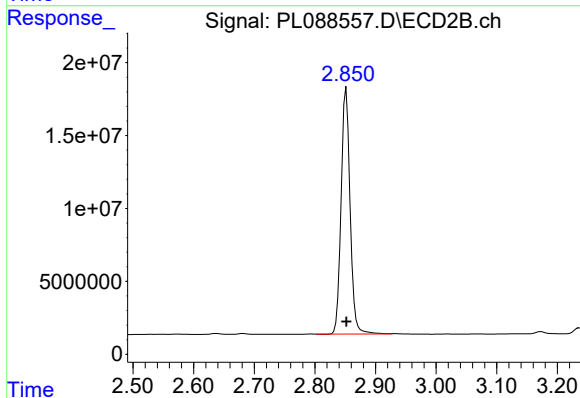


#1 Tetrachloro-m-xylene

R.T.: 2.852 min
Delta R.T.: 0.000 min
Response: 173972385
Conc: 105.07 ng/ml

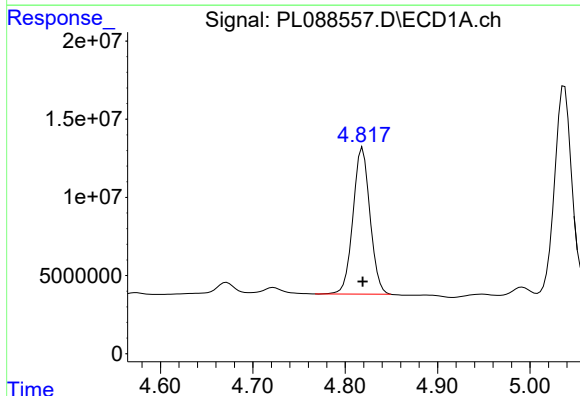


#23 Chlordane-1

R.T.: 4.819 min
Delta R.T.: 0.000 min
Response: 119610353
Conc: 1034.67 ng/ml

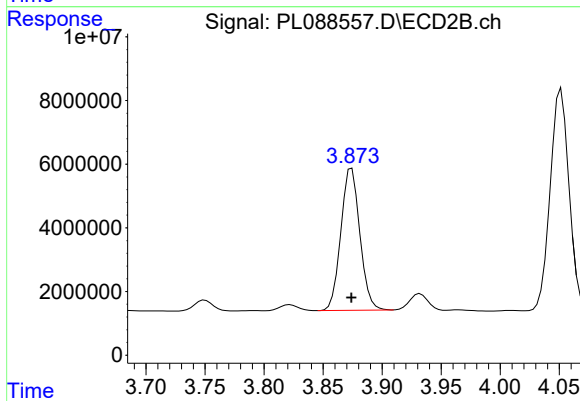

#23 Chlordane-1


R.T.: 3.874 min
Delta R.T.: 0.000 min
Response: 50006194
Conc: 1043.62 ng/ml

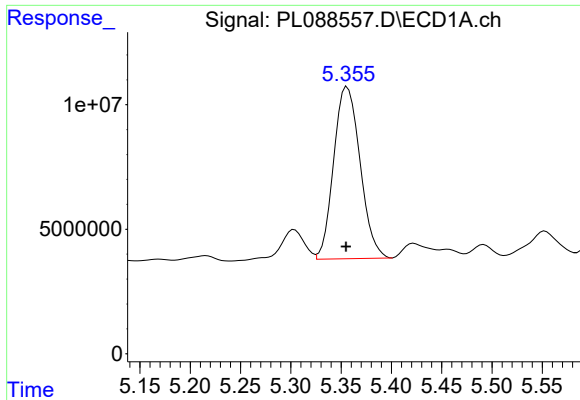

#24 Chlordane-2


R.T.: 5.356 min
Delta R.T.: 0.001 min
Response: 125930098
Conc: 986.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

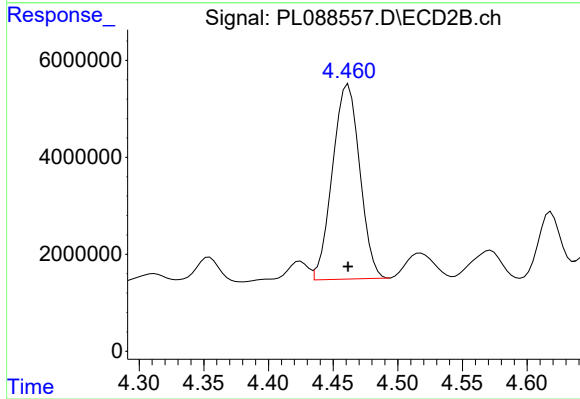


#24 Chlordane-2

R.T.: 4.462 min
Delta R.T.: 0.000 min
Response: 58869323
Conc: 987.64 ng/ml

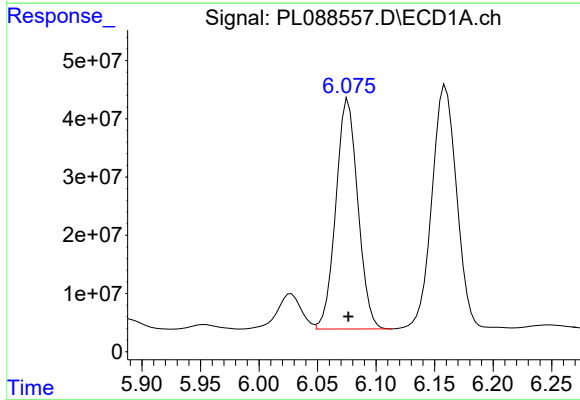


#25 Chlordane-3

R.T.: 6.076 min
Delta R.T.: 0.000 min
Response: 516656182
Conc: 1052.19 ng/ml

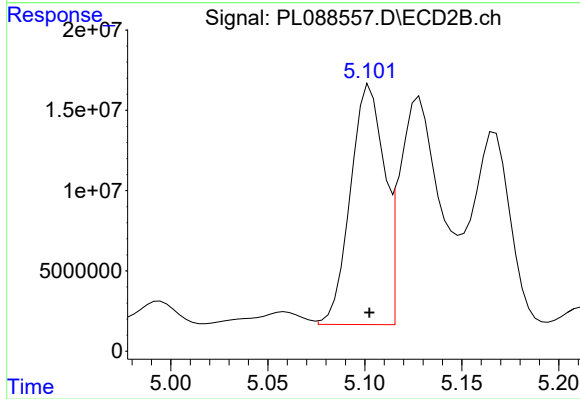

#25 Chlordane-3


R.T.: 5.103 min
Delta R.T.: 0.000 min
Response: 179539516
Conc: 1052.59 ng/ml

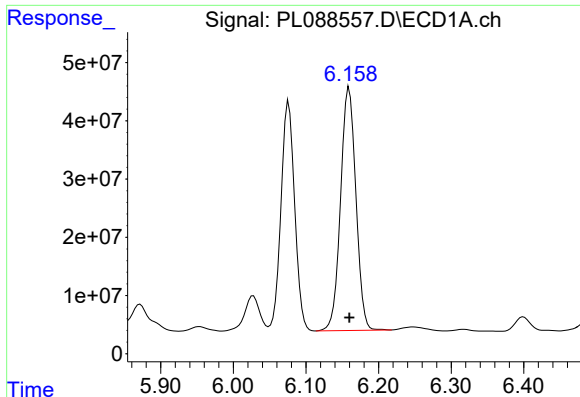

#26 Chlordane-4


R.T.: 6.159 min
Delta R.T.: 0.000 min
Response: 612221388
Conc: 1034.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

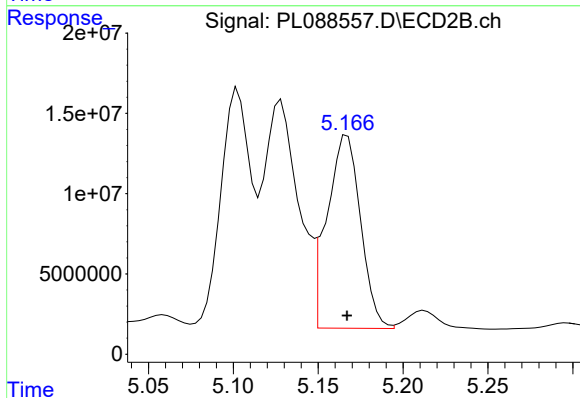


#26 Chlordane-4

R.T.: 5.167 min
Delta R.T.: 0.000 min
Response: 165669559
Conc: 1041.83 ng/ml

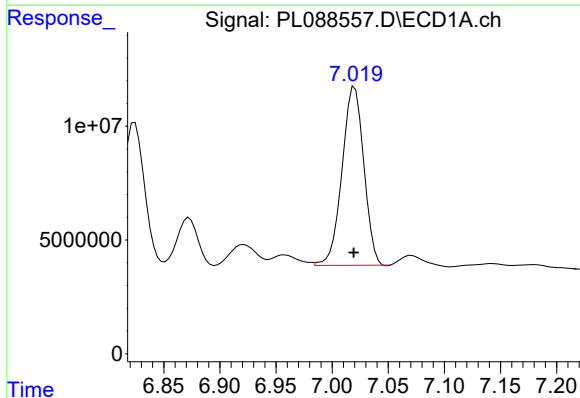


#27 Chlordane-5

R.T.: 7.020 min
Delta R.T.: 0.000 min
Response: 105931075
Conc: 1017.87 ng/ml

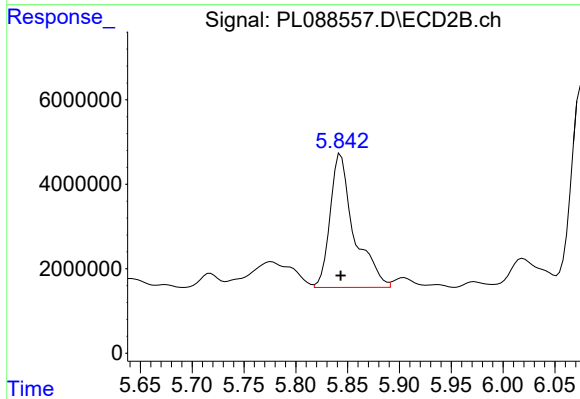

#27 Chlordane-5


R.T.: 5.843 min
Delta R.T.: 0.000 min
Response: 50744780
Conc: 1012.92 ng/ml

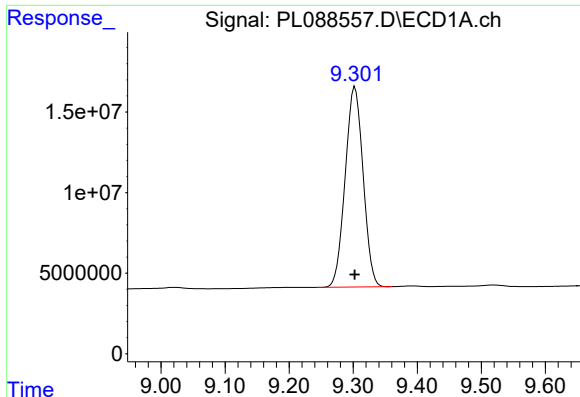

#28 Decachlorobiphenyl

R.T.: 9.303 min
Delta R.T.: 0.000 min
Response: 241339816
Conc: 100.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

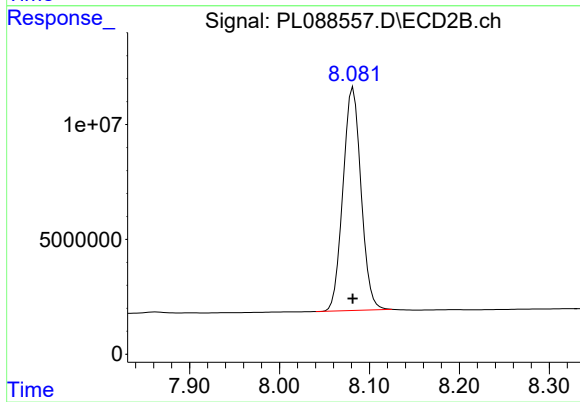

#28 Decachlorobiphenyl

R.T.: 8.082 min
Delta R.T.: 0.000 min
Response: 135646636
Conc: 98.92 ng/ml