

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031424\
 Data File : PL088559.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2024 13:12
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 15:38:18 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 13 15:37:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.634	2.852	135.5E6	82785125	50.000	50.000
28)	SA Decachlor...	9.302	8.081	120.0E6	68565645	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.819	3.874	57801407	23958054	500.000	500.000
24)	Chlordane-2	5.355	4.462	63801940	29802915	500.000	500.000
25)	Chlordane-3	6.076	5.102	245.5E6	85284750	500.000	500.000
26)	Chlordane-4	6.160	5.167	295.9E6	79508777	500.000	500.000
27)	Chlordane-5	7.019	5.843	52035485	25048666	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031424\
Data File : PL088559.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2024 13:12
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 15:38:18 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
Quant Title : GC Extractables
QLast Update : Wed Mar 13 15:37:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

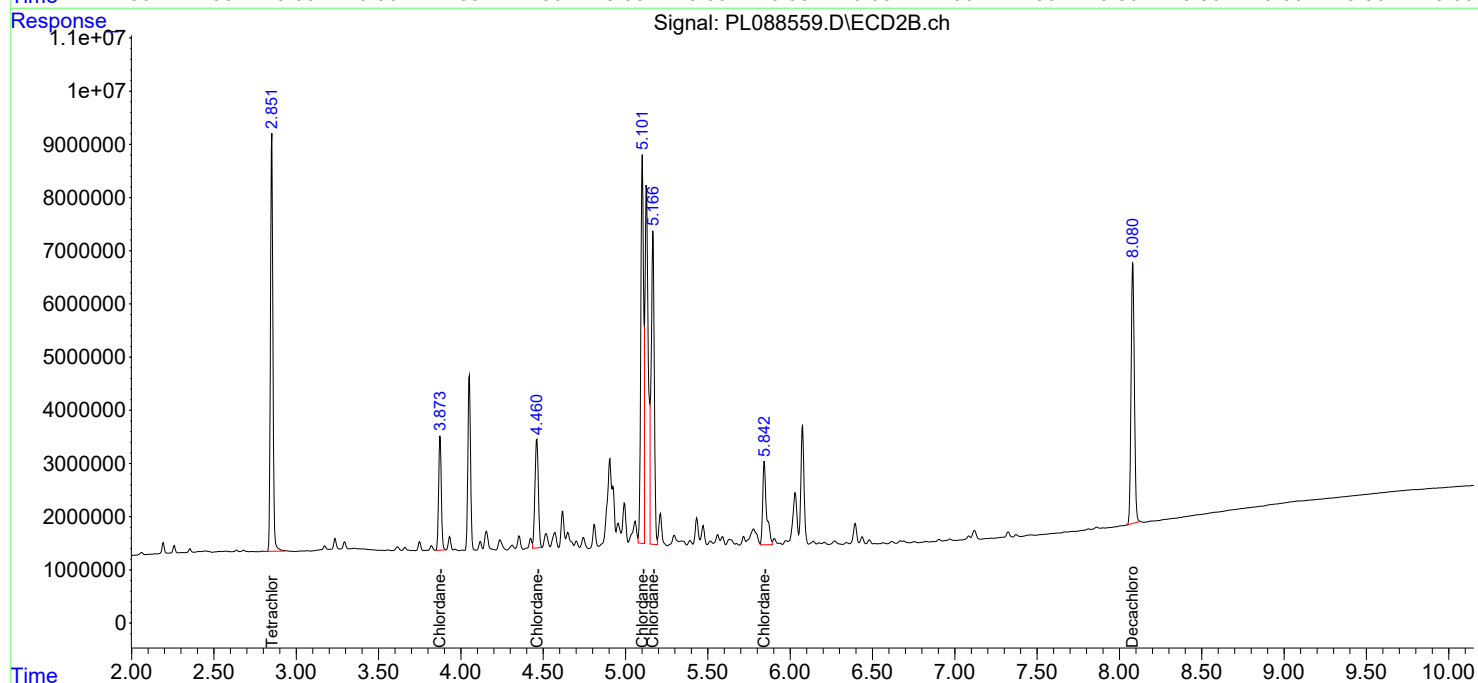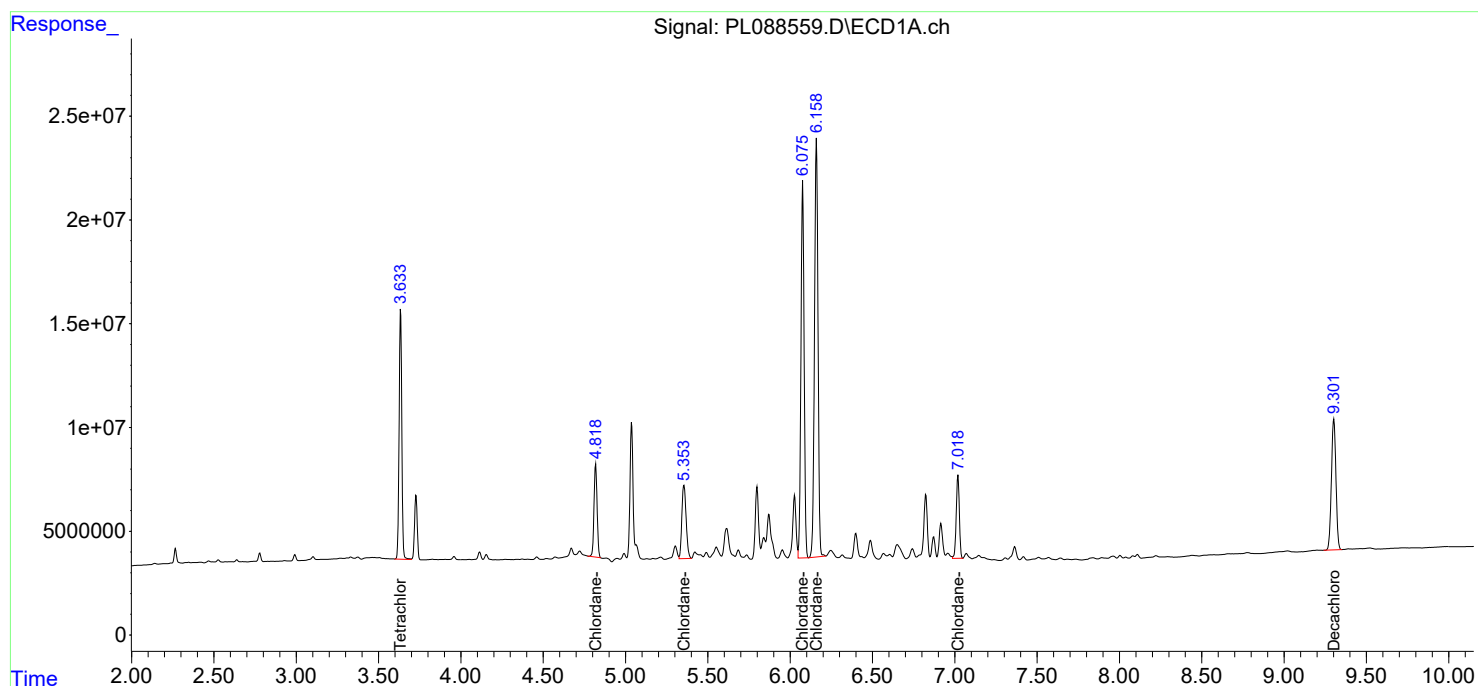


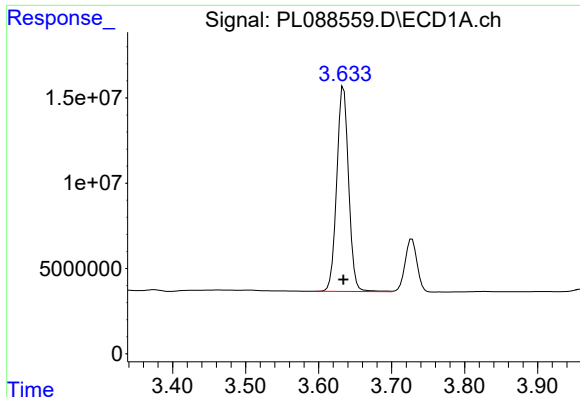

#1 Tetrachloro-m-xylene


R.T.: 3.634 min
Delta R.T.: 0.000 min
Response: 135525658
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

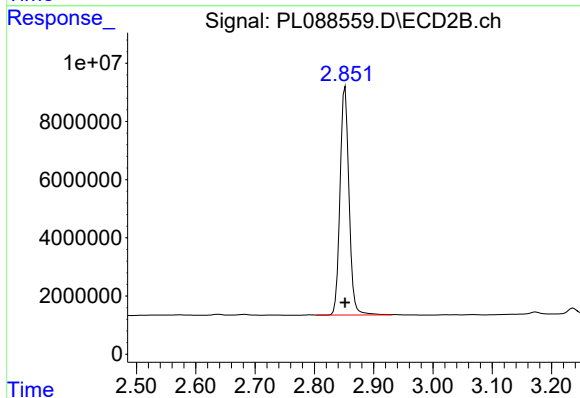


#1 Tetrachloro-m-xylene

R.T.: 2.852 min
Delta R.T.: 0.000 min
Response: 82785125
Conc: 50.00 ng/ml

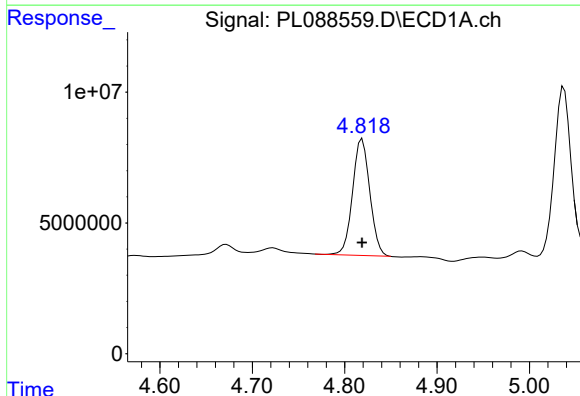


#23 Chlordane-1

R.T.: 4.819 min
Delta R.T.: 0.000 min
Response: 57801407
Conc: 500.00 ng/ml

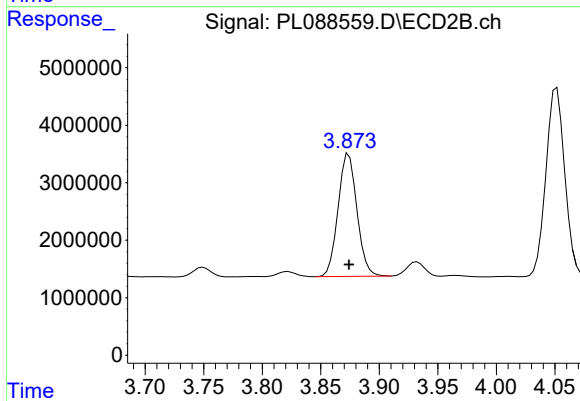

#23 Chlordane-1


R.T.: 3.874 min
Delta R.T.: 0.000 min
Response: 23958054
Conc: 500.00 ng/ml

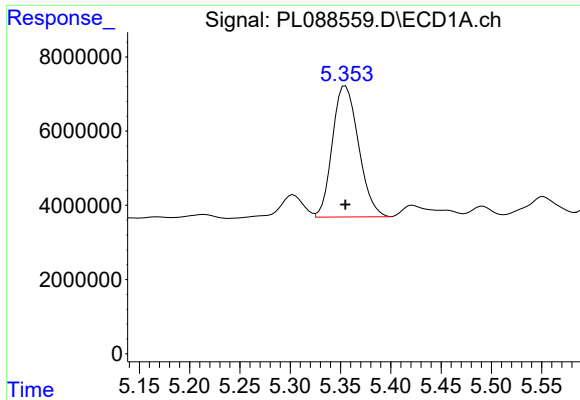

#24 Chlordane-2


R.T.: 5.355 min
Delta R.T.: 0.000 min
Response: 63801940
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

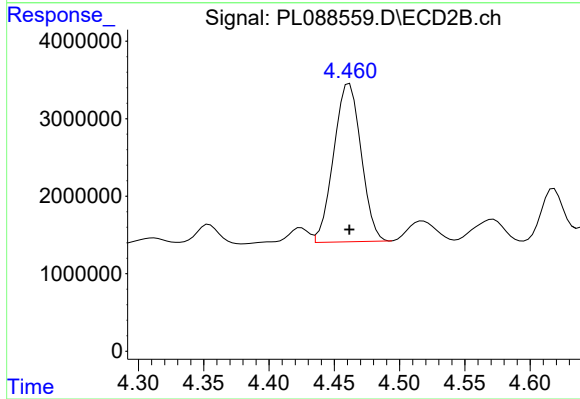


#24 Chlordane-2

R.T.: 4.462 min
Delta R.T.: 0.000 min
Response: 29802915
Conc: 500.00 ng/ml

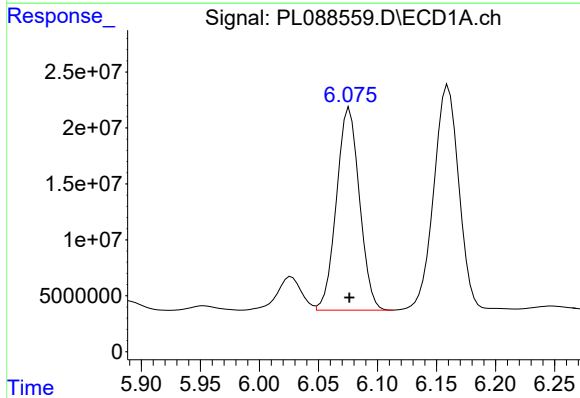


#25 Chlordane-3

R.T.: 6.076 min
Delta R.T.: 0.000 min
Response: 245514035
Conc: 500.00 ng/ml

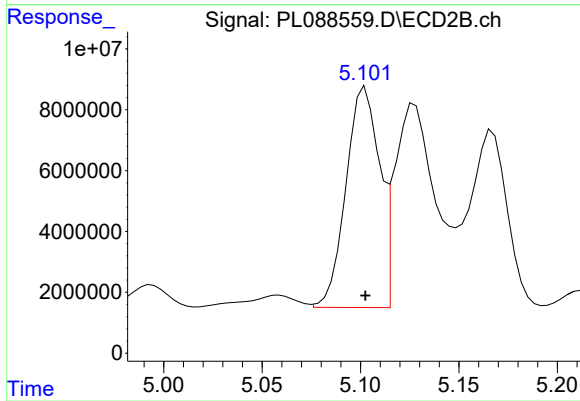

#25 Chlordane-3


R.T.: 5.102 min
Delta R.T.: 0.000 min
Response: 85284750
Conc: 500.00 ng/ml

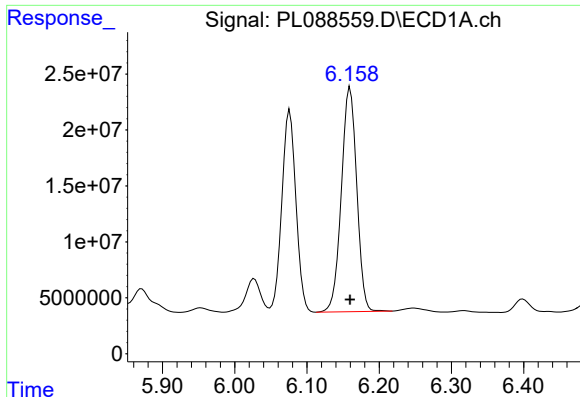

#26 Chlordane-4


R.T.: 6.160 min
Delta R.T.: 0.000 min
Response: 295886444
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

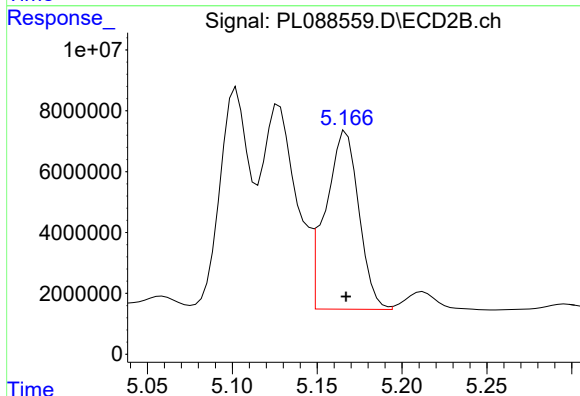


#26 Chlordane-4

R.T.: 5.167 min
Delta R.T.: 0.000 min
Response: 79508777
Conc: 500.00 ng/ml

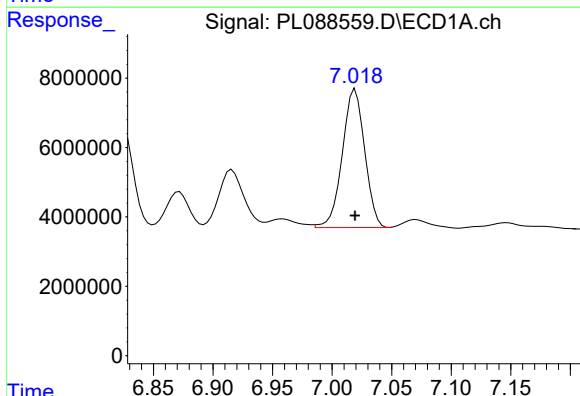


#27 Chlordane-5

R.T.: 7.019 min
Delta R.T.: 0.000 min
Response: 52035485
Conc: 500.00 ng/ml

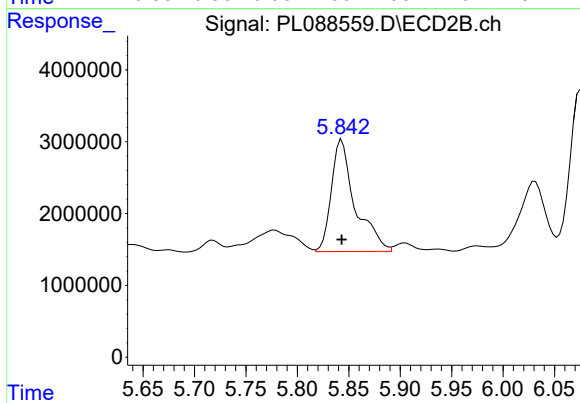

#27 Chlordane-5


R.T.: 5.843 min
Delta R.T.: 0.000 min
Response: 25048666
Conc: 500.00 ng/ml

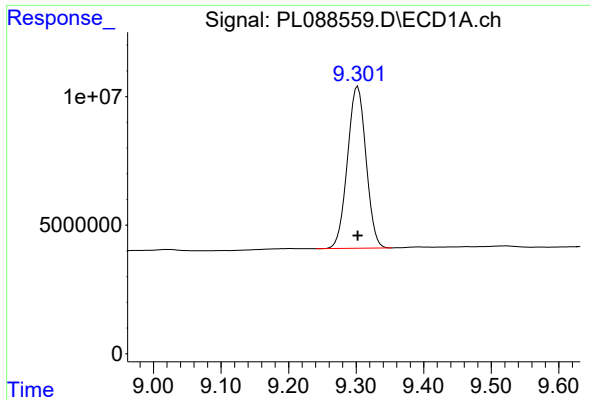

#28 Decachlorobiphenyl

R.T.: 9.302 min
Delta R.T.: 0.000 min
Response: 119963682
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

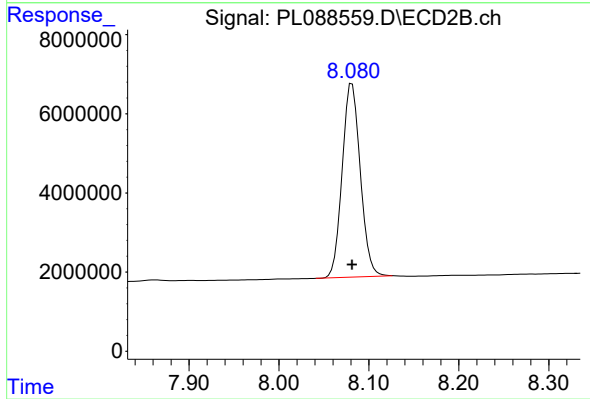

#28 Decachlorobiphenyl

R.T.: 8.081 min
Delta R.T.: 0.000 min
Response: 68565645
Conc: 50.00 ng/ml