

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031424\
 Data File : PL088560.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2024 13:26
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 15:38:32 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 13 15:37:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.634	2.851	68983991	41660591	25.451	25.162
28)	SA Decachlor...	9.302	8.081	63123156	35049650	26.309	25.559
Target Compounds							
23)	Chlordane-1	4.819	3.874	28972480	12110100	250.621	252.735
24)	Chlordane-2	5.355	4.461	33345068	15634994	261.317	262.306
25)	Chlordane-3	6.076	5.102	121.3E6	40945962	246.957	240.054
26)	Chlordane-4	6.160	5.167	147.4E6	38558496	249.147	242.479
27)	Chlordane-5	7.020	5.843	26285676	12730359	252.575	254.113



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031424\
Data File : PL088560.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2024 13:26
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 15:38:32 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
Quant Title : GC Extractables
QLast Update : Wed Mar 13 15:37:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

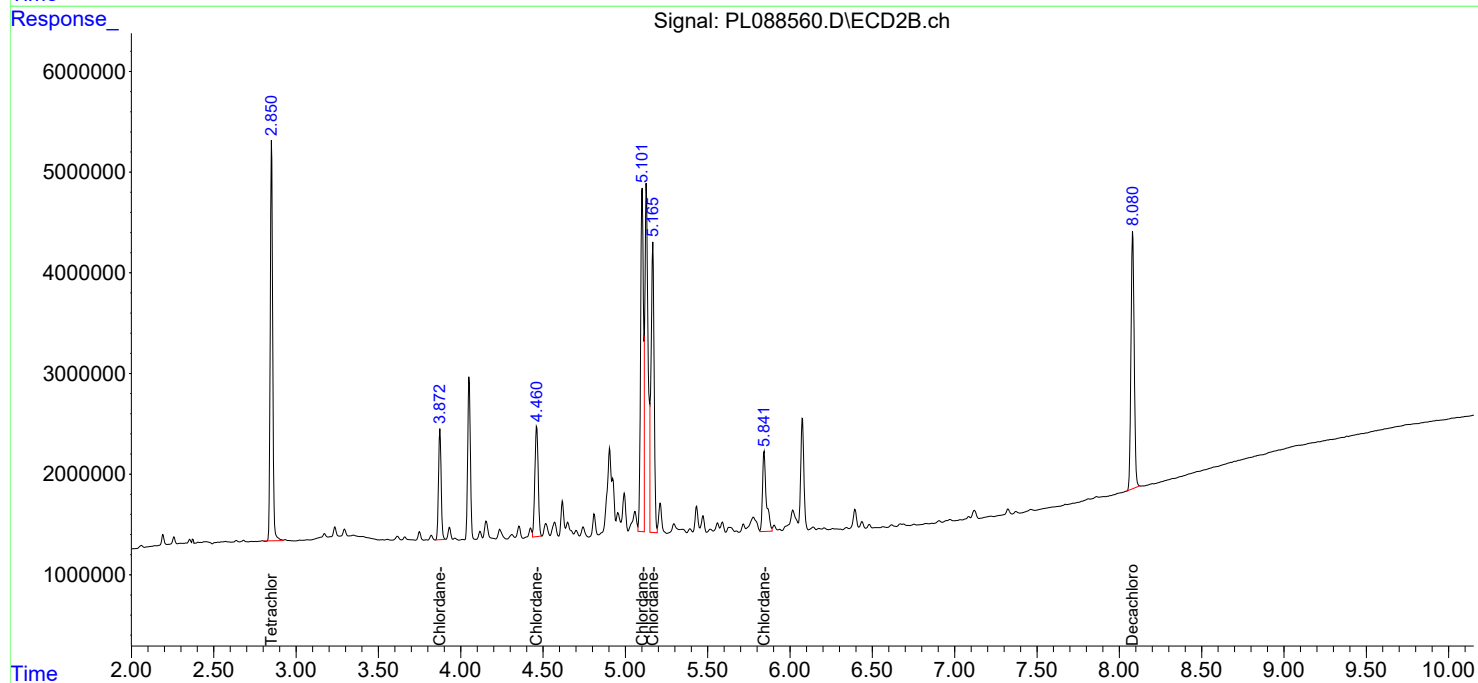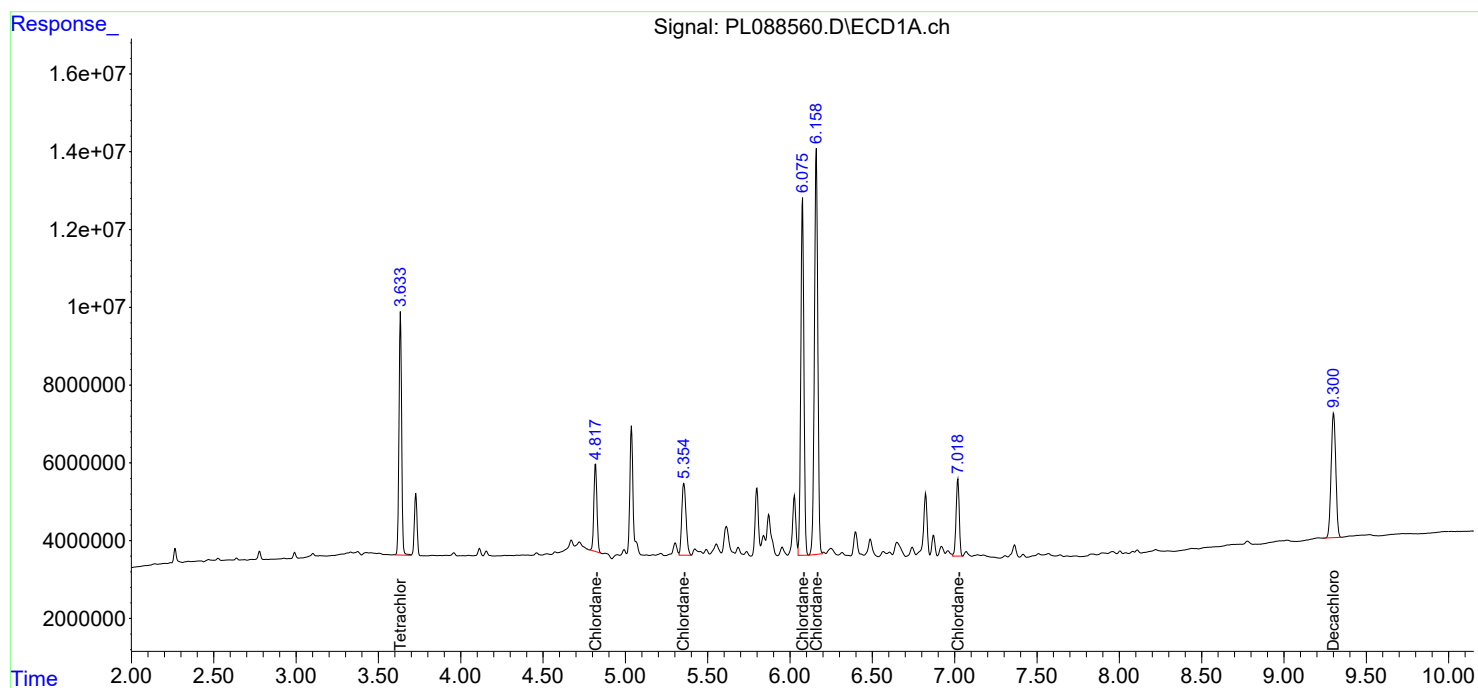


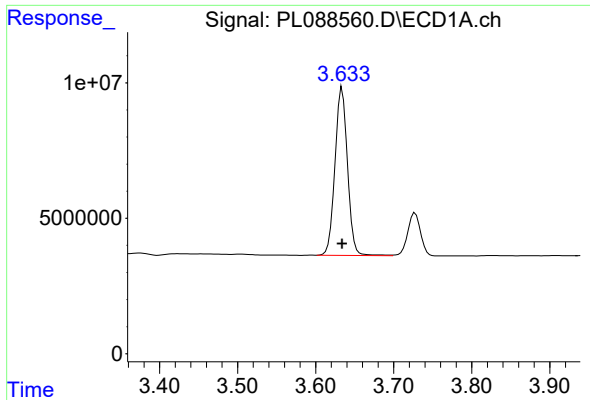

#1 Tetrachloro-m-xylene


R.T.: 3.634 min
Delta R.T.: 0.000 min
Response: 68983991
Conc: 25.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

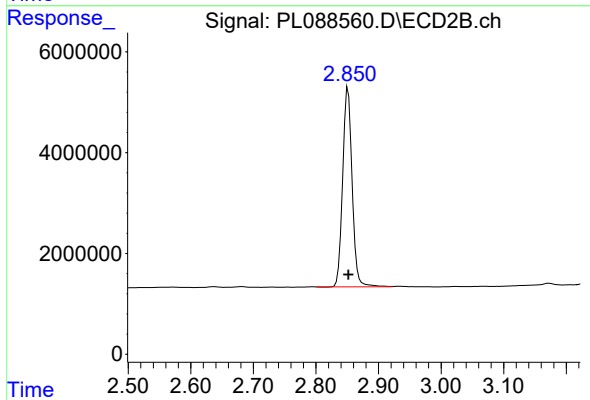


#1 Tetrachloro-m-xylene

R.T.: 2.851 min
Delta R.T.: 0.000 min
Response: 41660591
Conc: 25.16 ng/ml

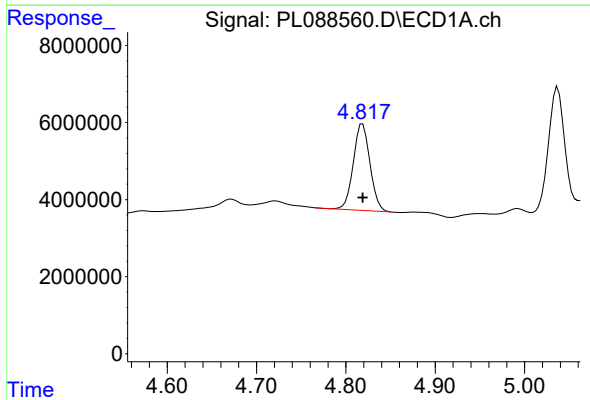


#23 Chlordane-1

R.T.: 4.819 min
Delta R.T.: 0.000 min
Response: 28972480
Conc: 250.62 ng/ml

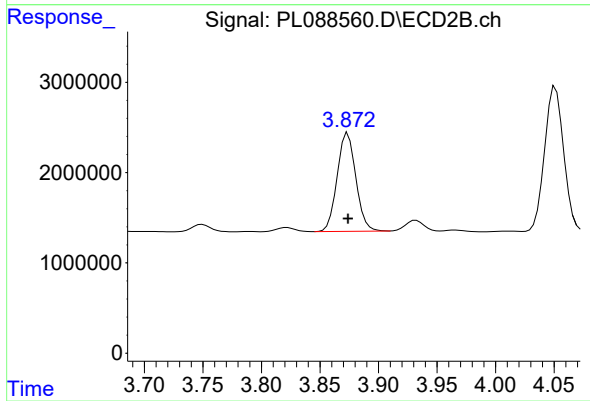

#23 Chlordane-1


R.T.: 3.874 min
Delta R.T.: 0.000 min
Response: 12110100
Conc: 252.74 ng/ml

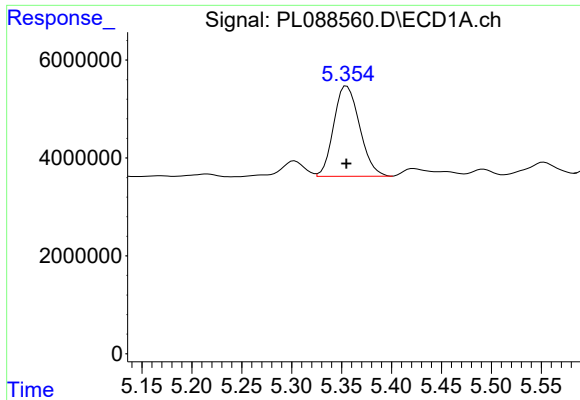

#24 Chlordane-2


R.T.: 5.355 min
Delta R.T.: 0.000 min
Response: 33345068
Conc: 261.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

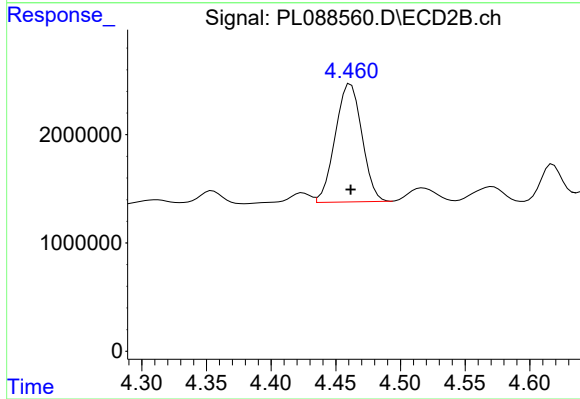


#24 Chlordane-2

R.T.: 4.461 min
Delta R.T.: 0.000 min
Response: 15634994
Conc: 262.31 ng/ml

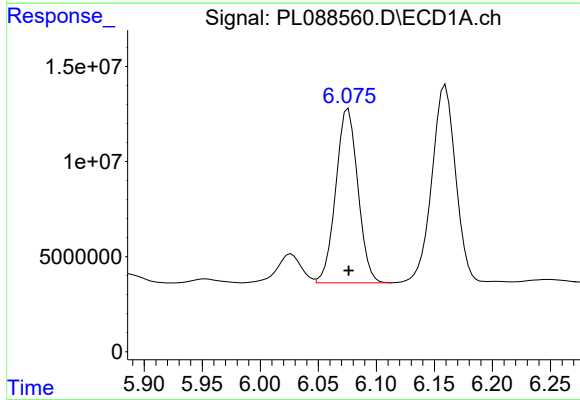


#25 Chlordane-3

R.T.: 6.076 min
Delta R.T.: 0.000 min
Response: 121262621
Conc: 246.96 ng/ml

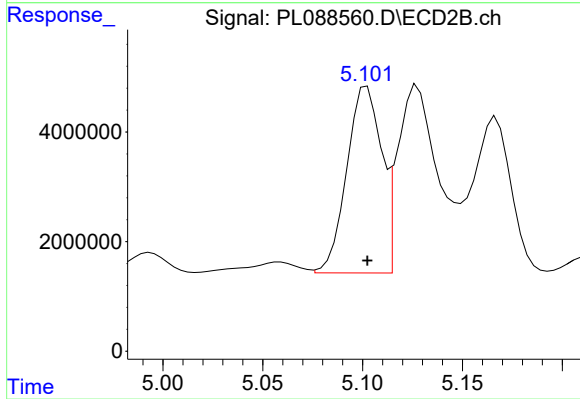

#25 Chlordane-3


R.T.: 5.102 min
Delta R.T.: 0.000 min
Response: 40945962
Conc: 240.05 ng/ml

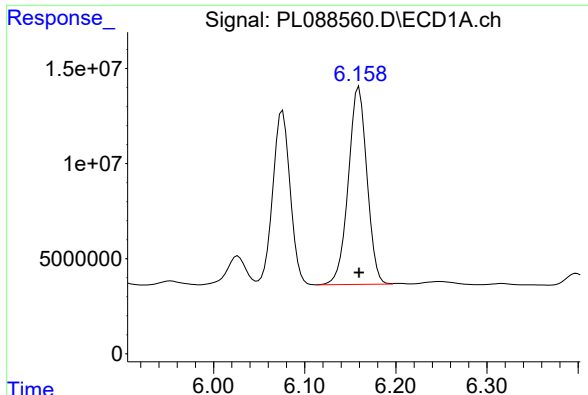

#26 Chlordane-4


R.T.: 6.160 min
Delta R.T.: 0.000 min
Response: 147438478
Conc: 249.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

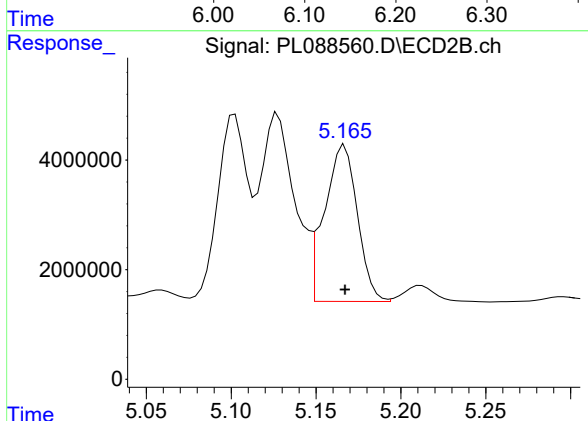


#26 Chlordane-4

R.T.: 5.167 min
Delta R.T.: 0.000 min
Response: 38558496
Conc: 242.48 ng/ml

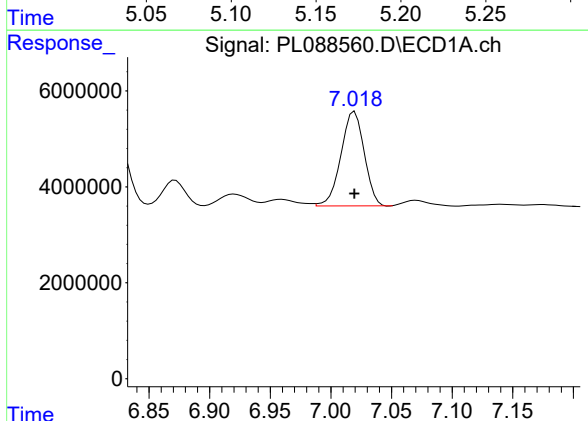


#27 Chlordane-5

R.T.: 7.020 min
Delta R.T.: 0.000 min
Response: 26285676
Conc: 252.57 ng/ml

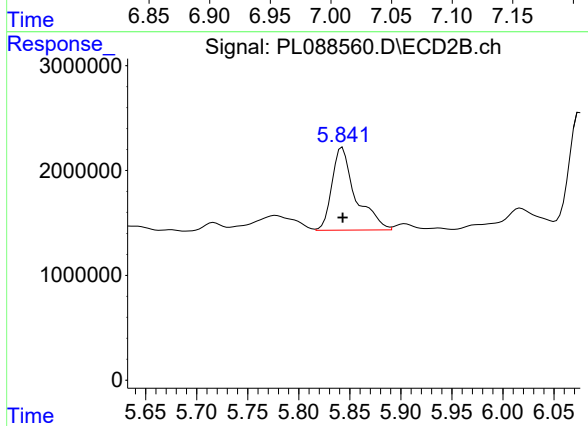

#27 Chlordane-5


R.T.: 5.843 min
Delta R.T.: 0.000 min
Response: 12730359
Conc: 254.11 ng/ml

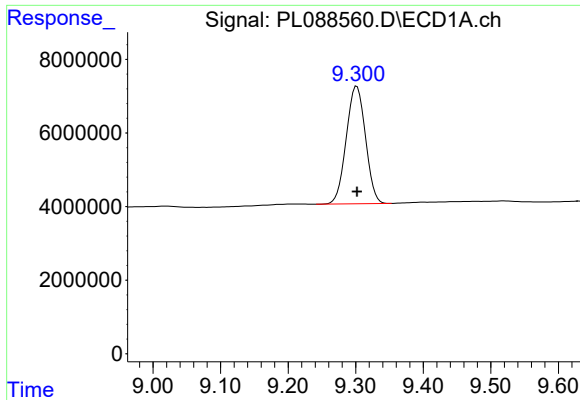

#28 Decachlorobiphenyl

R.T.: 9.302 min
Delta R.T.: 0.000 min
Response: 63123156
Conc: 26.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

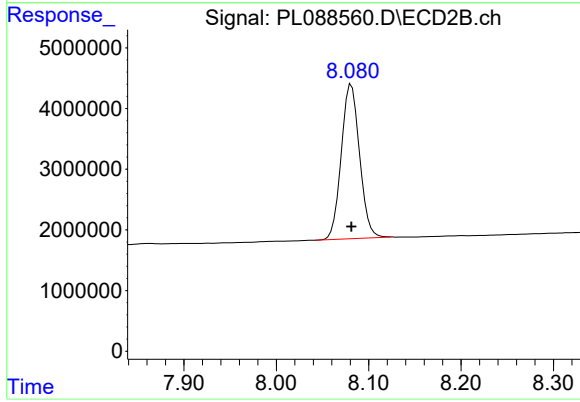

#28 Decachlorobiphenyl

R.T.: 8.081 min
Delta R.T.: 0.000 min
Response: 35049650
Conc: 25.56 ng/ml