

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031424\
 Data File : PL088568.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2024 15:16
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL031424CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 15:44:12 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 13 15:37:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.634	2.851	141.7E6	85598130	51.481	50.629
28)	SA Decachlor...	9.304	8.081	124.1E6	68254860	50.169	48.818
Target Compounds							
23)	Chlordane-1	4.819	3.874	59876372	24489591	514.918	504.365
24)	Chlordane-2	5.355	4.461	66371156	30368054	504.845	500.171
25)	Chlordane-3	6.076	5.103	255.5E6	85871706	513.853	503.143
26)	Chlordane-4	6.160	5.167	306.9E6	80138084	511.596	502.308
27)	Chlordane-5	7.020	5.843	54096038	25261739	511.769	498.108



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031424\
Data File : PL088568.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2024 15:16
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL031424CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 15:44:12 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
Quant Title : GC Extractables
QLast Update : Wed Mar 13 15:37:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

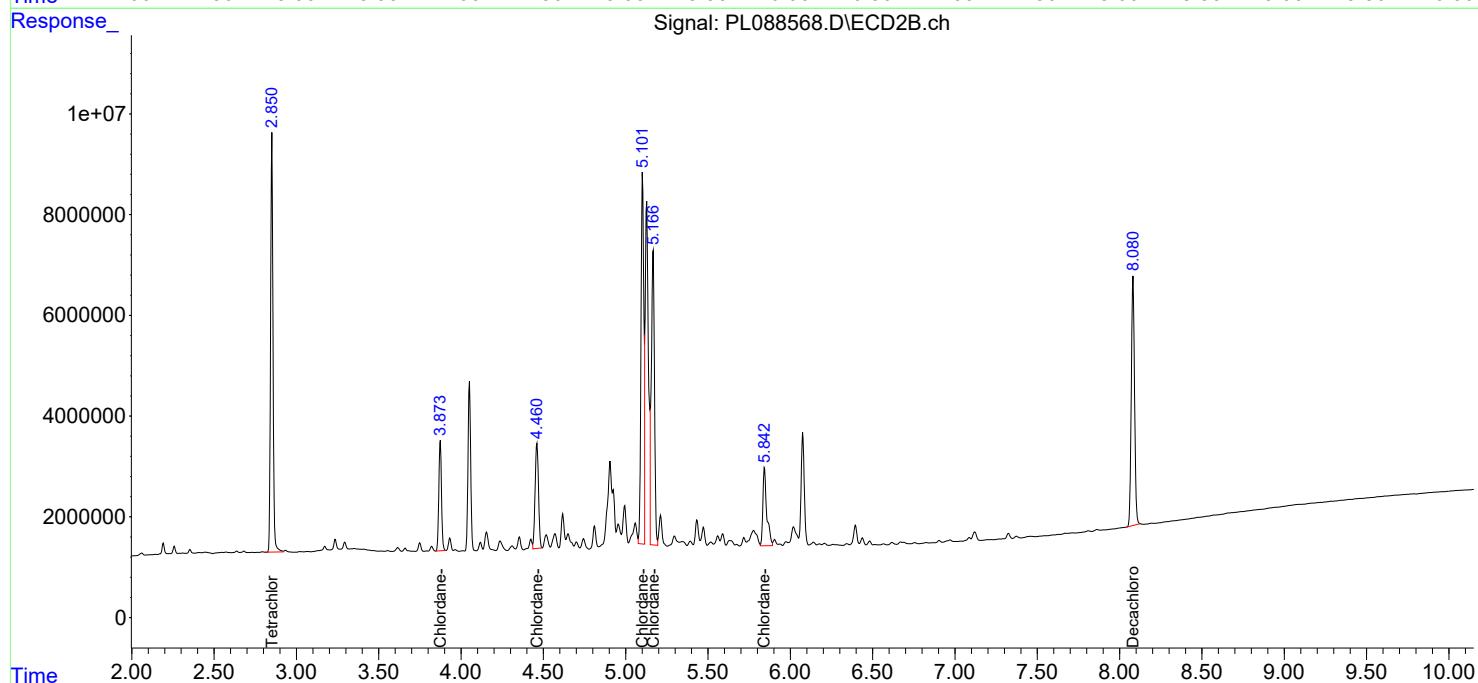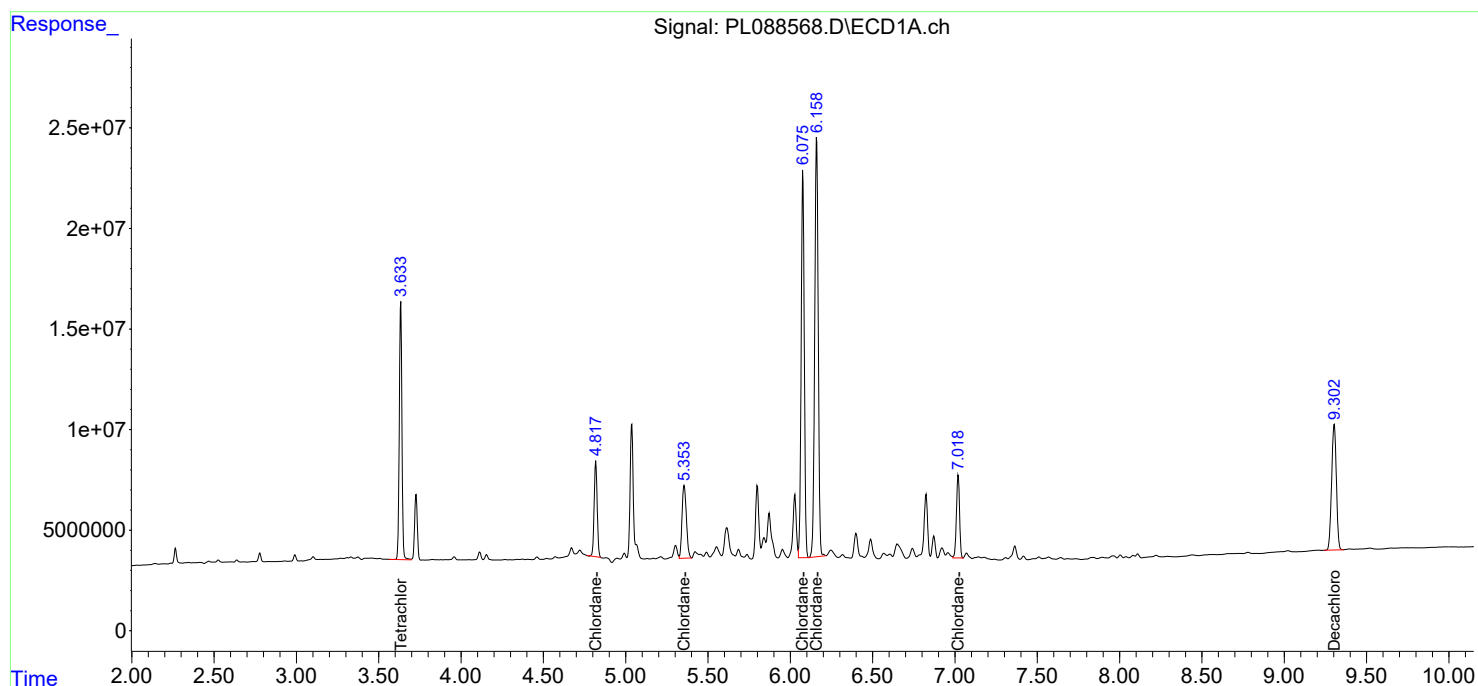


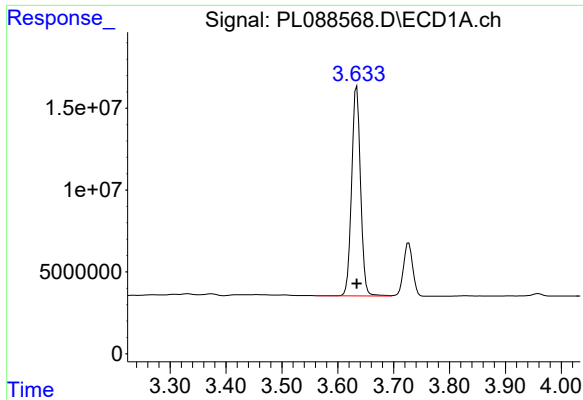

#1 Tetrachloro-m-xylene


R.T.: 3.634 min
Delta R.T.: 0.000 min
Response: 141698345
Conc: 51.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL031424CHLOR

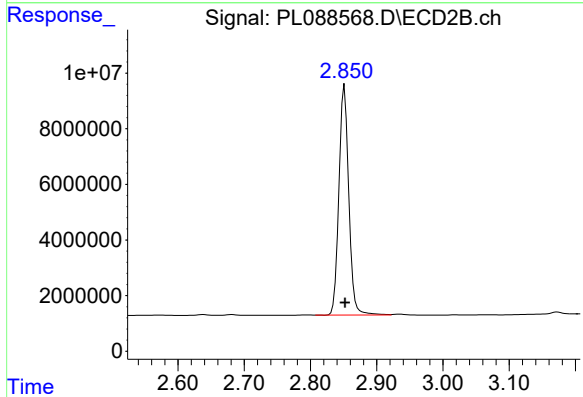


#1 Tetrachloro-m-xylene

R.T.: 2.851 min
Delta R.T.: 0.000 min
Response: 85598130
Conc: 50.63 ng/ml

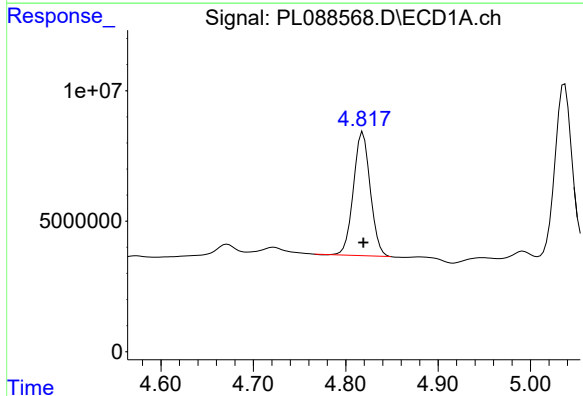


#23 Chlordane-1

R.T.: 4.819 min
Delta R.T.: 0.000 min
Response: 59876372
Conc: 514.92 ng/ml

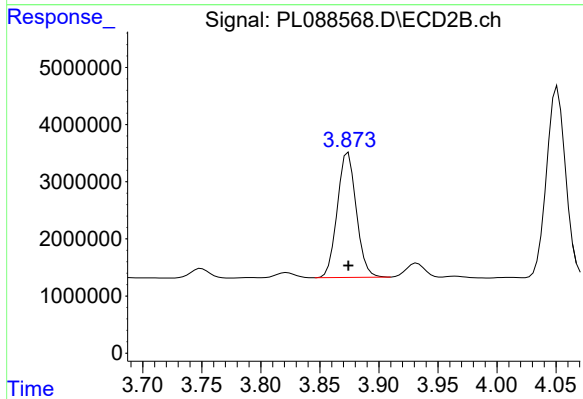

#23 Chlordane-1


R.T.: 3.874 min
Delta R.T.: 0.000 min
Response: 24489591
Conc: 504.36 ng/ml

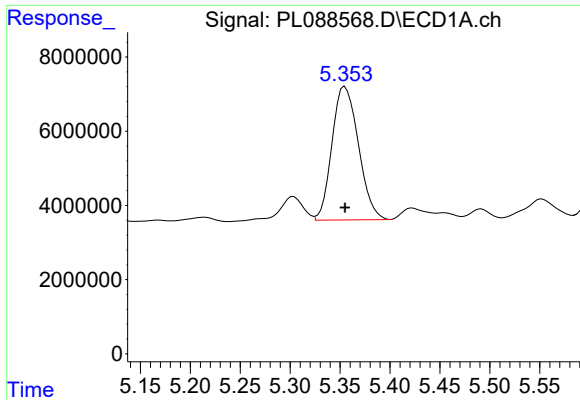

#24 Chlordane-2


R.T.: 5.355 min
Delta R.T.: 0.000 min
Response: 66371156
Conc: 504.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL031424CHLOR

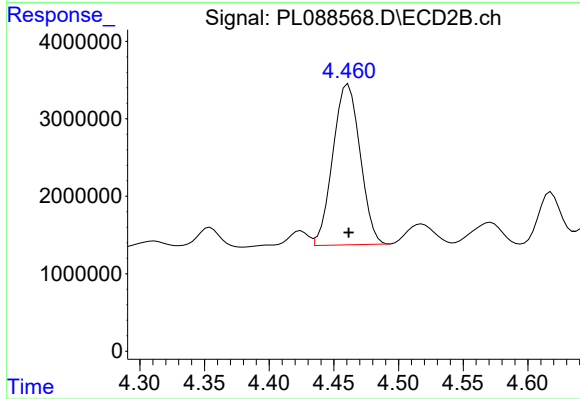


#24 Chlordane-2

R.T.: 4.461 min
Delta R.T.: 0.000 min
Response: 30368054
Conc: 500.17 ng/ml

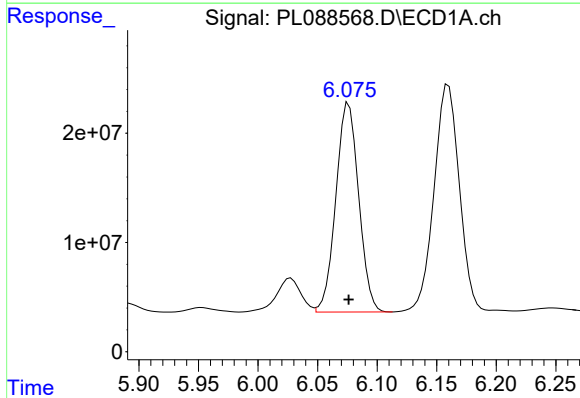


#25 Chlordane-3

R.T.: 6.076 min
Delta R.T.: 0.000 min
Response: 255506096
Conc: 513.85 ng/ml

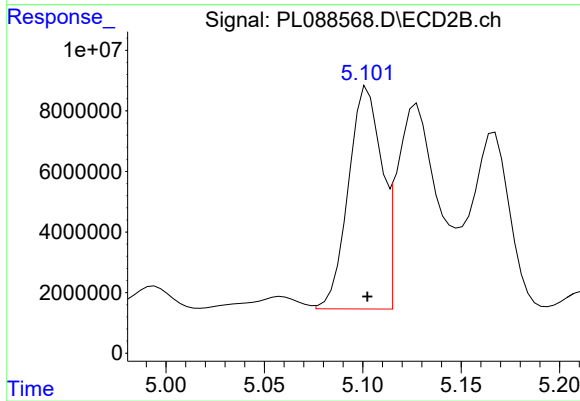

#25 Chlordane-3


R.T.: 5.103 min
Delta R.T.: 0.000 min
Response: 85871706
Conc: 503.14 ng/ml

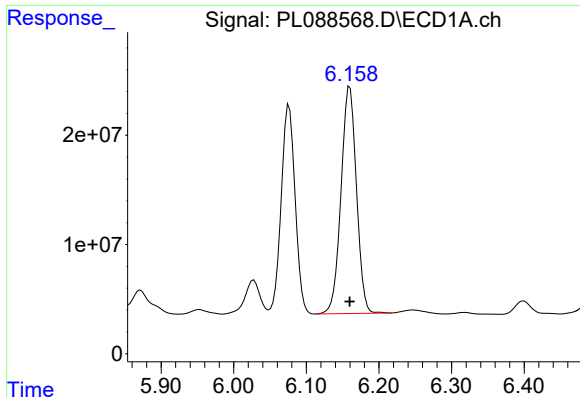

#26 Chlordane-4


R.T.: 6.160 min
Delta R.T.: 0.000 min
Response: 306889744
Conc: 511.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL031424CHLOR

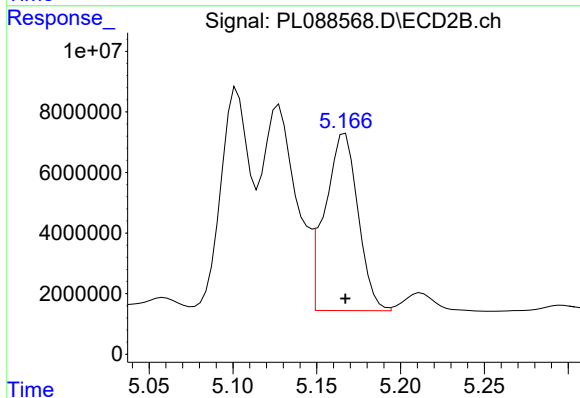


#26 Chlordane-4

R.T.: 5.167 min
Delta R.T.: 0.000 min
Response: 80138084
Conc: 502.31 ng/ml

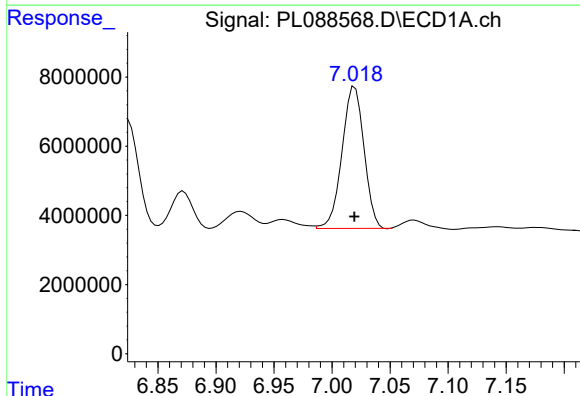


#27 Chlordane-5

R.T.: 7.020 min
Delta R.T.: 0.000 min
Response: 54096038
Conc: 511.77 ng/ml

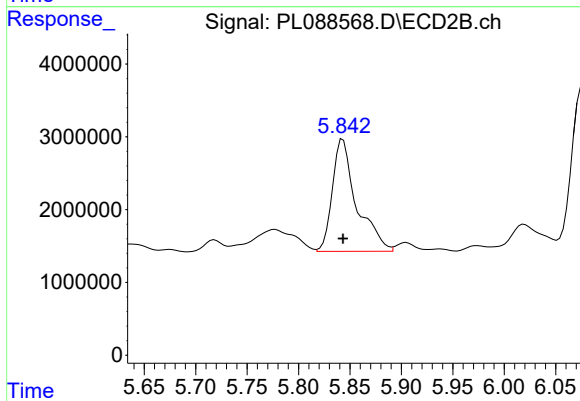

#27 Chlordane-5


R.T.: 5.843 min
Delta R.T.: 0.000 min
Response: 25261739
Conc: 498.11 ng/ml

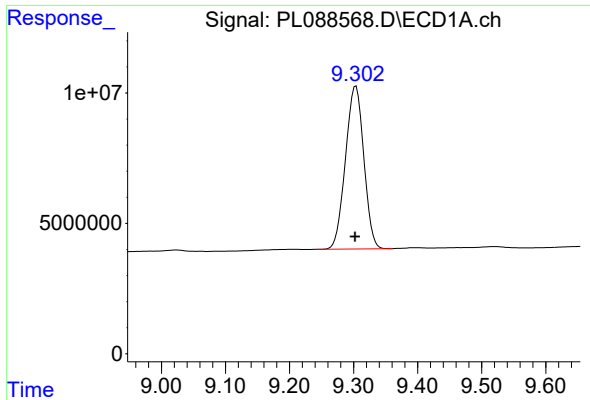

#28 Decachlorobiphenyl

R.T.: 9.304 min
Delta R.T.: 0.001 min
Response: 124076778
Conc: 50.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL031424CHLOR

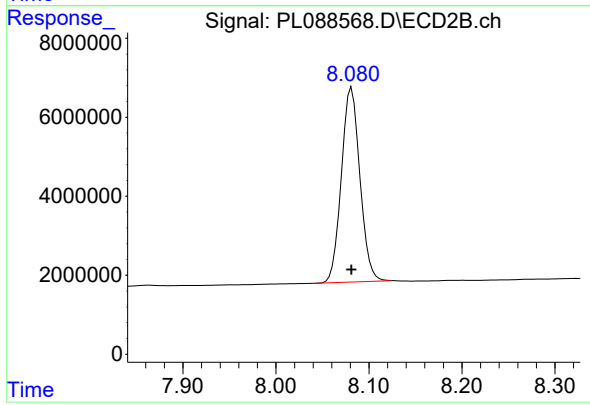

#28 Decachlorobiphenyl

R.T.: 8.081 min
Delta R.T.: 0.000 min
Response: 68254860
Conc: 48.82 ng/ml