

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031424\
 Data File : PL088558.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2024 12:58
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 15:38:04 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 13 15:37:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.634	2.851	206.5E6	126.9E6	76.177	76.629
28)	SA Decachlor...	9.301	8.081	178.8E6	100.9E6	74.524	73.593
Target Compounds							
23)	Chlordane-1	4.818	3.874	87981827	36437991	761.070	760.454
24)	Chlordane-2	5.356	4.461	94609984	43913755	741.435	736.736
25)	Chlordane-3	6.076	5.102	377.3E6	131.3E6	768.487	769.645
26)	Chlordane-4	6.159	5.166	450.1E6	120.9E6	760.642	760.151
27)	Chlordane-5	7.019	5.843	78108434	37489463	750.530	748.333



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031424\
Data File : PL088558.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2024 12:58
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 15:38:04 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
Quant Title : GC Extractables
QLast Update : Wed Mar 13 15:37:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

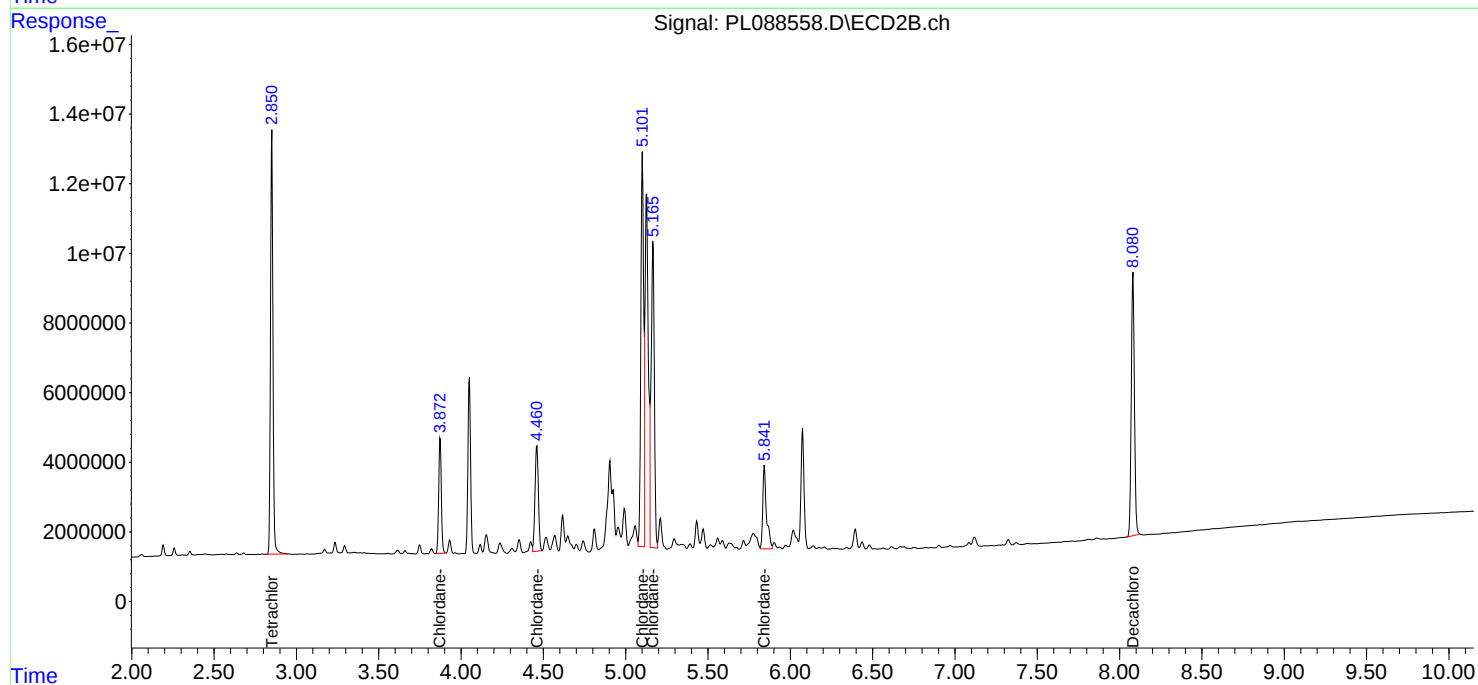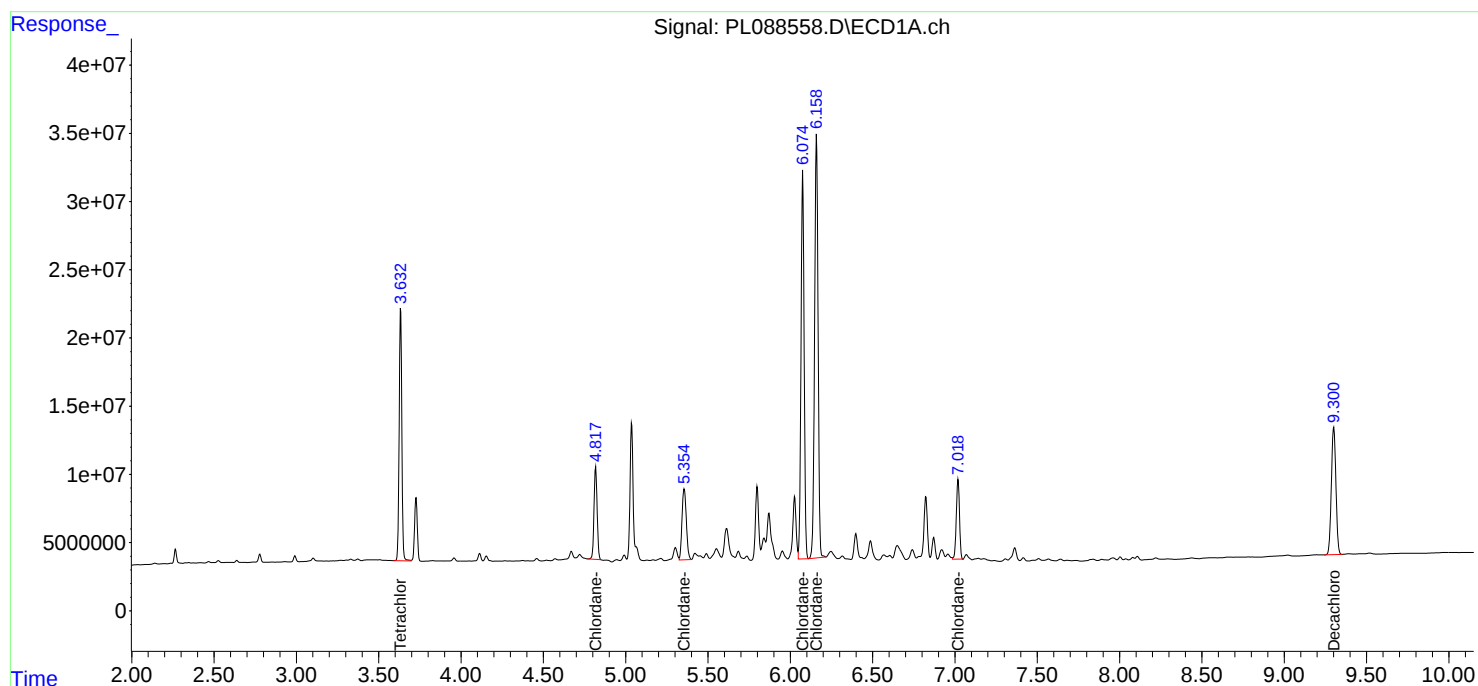


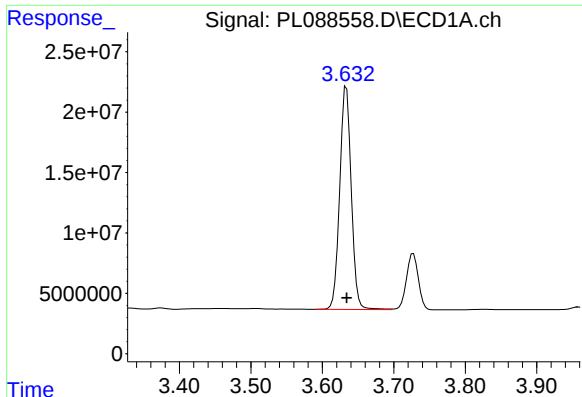

#1 Tetrachloro-m-xylene


R.T.: 3.634 min
Delta R.T.: 0.000 min
Response: 206479097
Conc: 76.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

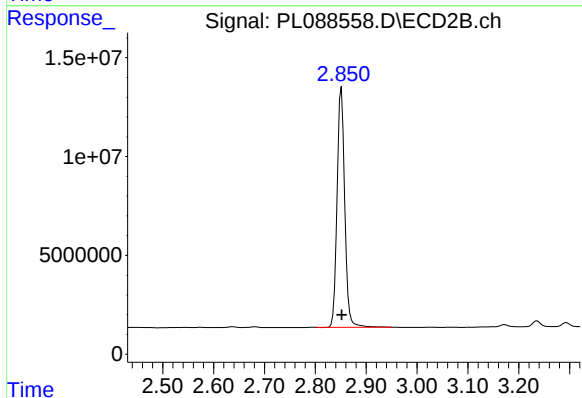


#1 Tetrachloro-m-xylene

R.T.: 2.851 min
Delta R.T.: 0.000 min
Response: 126875564
Conc: 76.63 ng/ml

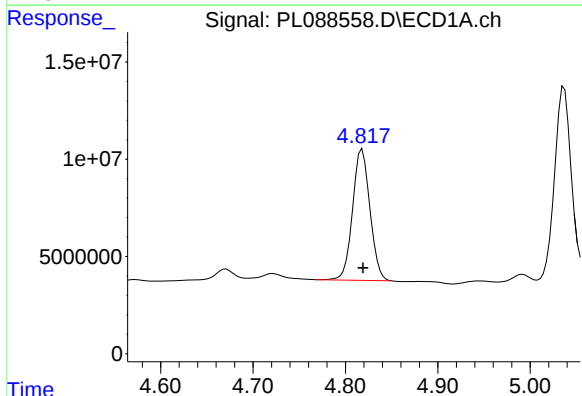


#23 Chlordane-1

R.T.: 4.818 min
Delta R.T.: 0.000 min
Response: 87981827
Conc: 761.07 ng/ml

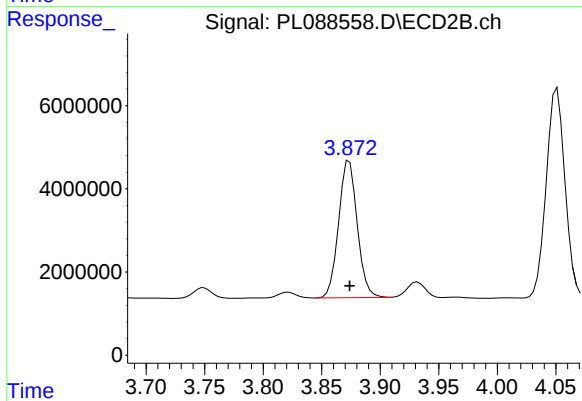

#23 Chlordane-1


R.T.: 3.874 min
Delta R.T.: 0.000 min
Response: 36437991
Conc: 760.45 ng/ml

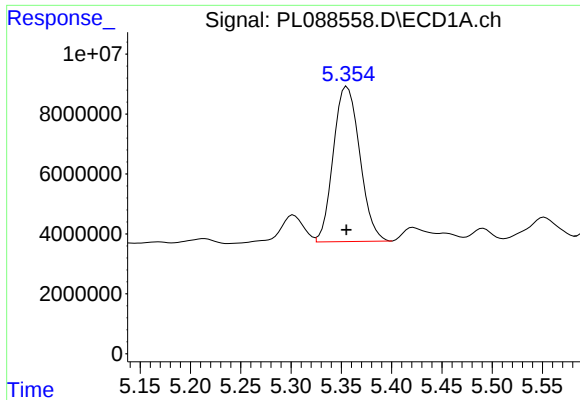

#24 Chlordane-2


R.T.: 5.356 min
Delta R.T.: 0.000 min
Response: 94609984
Conc: 741.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

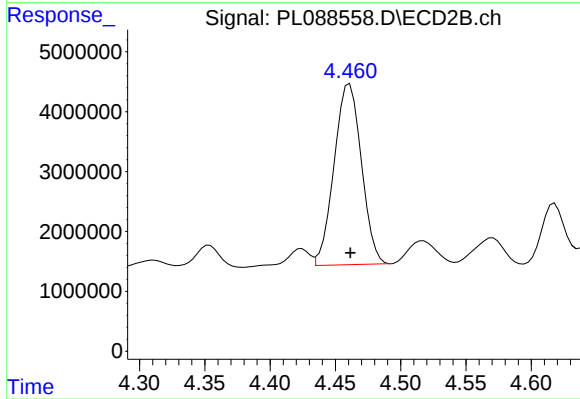


#24 Chlordane-2

R.T.: 4.461 min
Delta R.T.: 0.000 min
Response: 43913755
Conc: 736.74 ng/ml

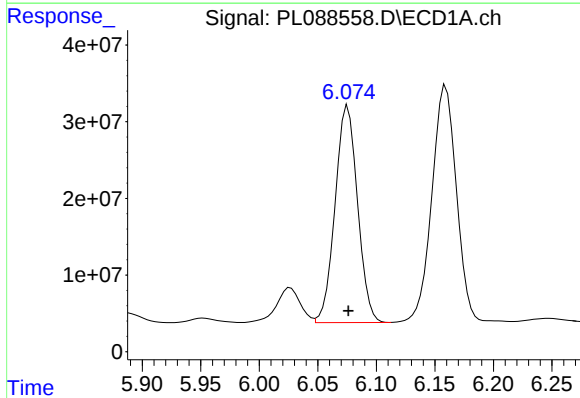


#25 Chlordane-3

R.T.: 6.076 min
Delta R.T.: 0.000 min
Response: 377348581
Conc: 768.49 ng/ml

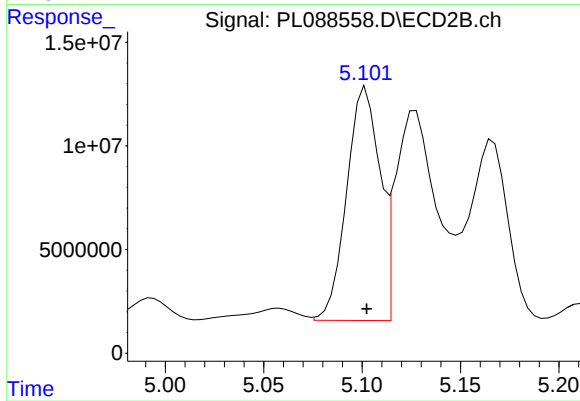

#25 Chlordane-3


R.T.: 5.102 min
Delta R.T.: 0.000 min
Response: 131277983
Conc: 769.65 ng/ml

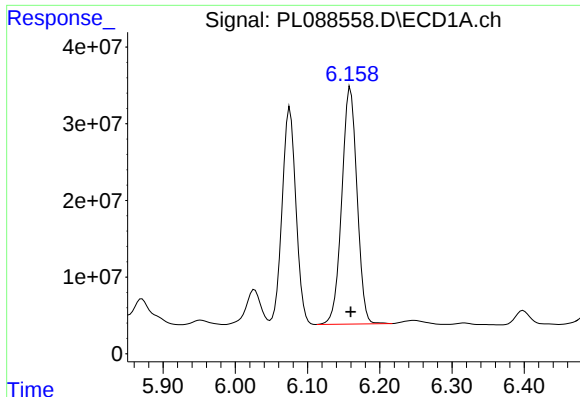

#26 Chlordane-4


R.T.: 6.159 min
Delta R.T.: 0.000 min
Response: 450127025
Conc: 760.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

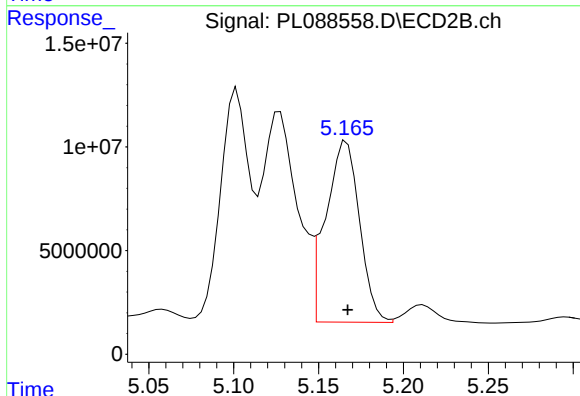


#26 Chlordane-4

R.T.: 5.166 min
Delta R.T.: 0.000 min
Response: 120877296
Conc: 760.15 ng/ml

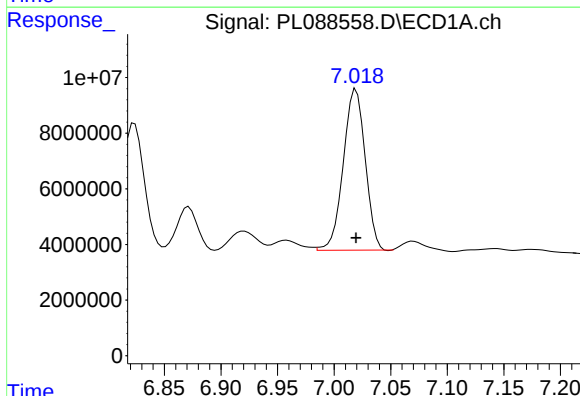


#27 Chlordane-5

R.T.: 7.019 min
Delta R.T.: 0.000 min
Response: 78108434
Conc: 750.53 ng/ml

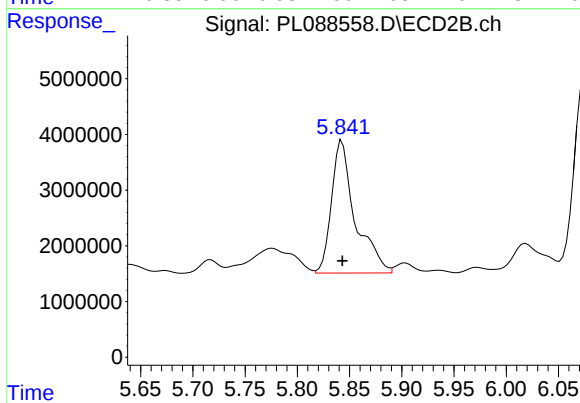

#27 Chlordane-5


R.T.: 5.843 min
Delta R.T.: 0.000 min
Response: 37489463
Conc: 748.33 ng/ml

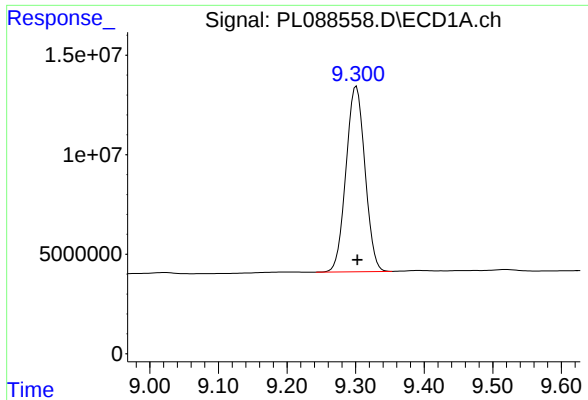

#28 Decachlorobiphenyl

R.T.: 9.301 min
Delta R.T.: -0.001 min
Response: 178804416
Conc: 74.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

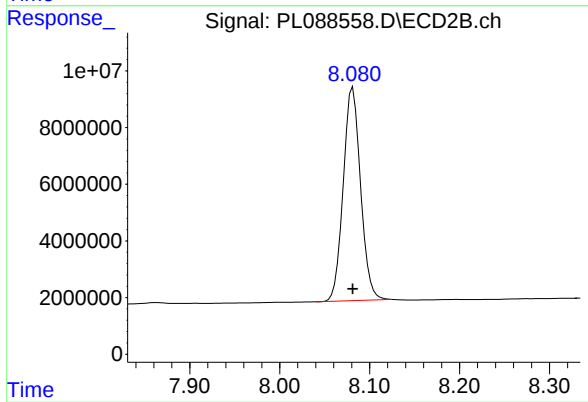

#28 Decachlorobiphenyl

R.T.: 8.081 min
Delta R.T.: 0.000 min
Response: 100919662
Conc: 73.59 ng/ml