

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031424\
 Data File : PL088561.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Mar 2024 13:39
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 13 15:38:45 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 13 15:37:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.633	2.851	13602953	8499767	5.019	5.134
28)	SA Decachlor...	9.301	8.082	13220667	7576974	5.510	5.525
Target Compounds							
23)	Chlordane-1	4.818	3.873	5650247	2391501	48.876	49.910
24)	Chlordane-2	5.354	4.461	7214050	3200501	56.535	53.694
25)	Chlordane-3	6.076	5.102	24515658	8221160	49.927	48.198
26)	Chlordane-4	6.160	5.167	30270860	7880418	51.153	49.557
27)	Chlordane-5	7.020	5.843	5461555	2591372	52.479	51.727



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031424\
Data File : PL088561.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Mar 2024 13:39
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 13 15:38:45 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
Quant Title : GC Extractables
QLast Update : Wed Mar 13 15:37:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

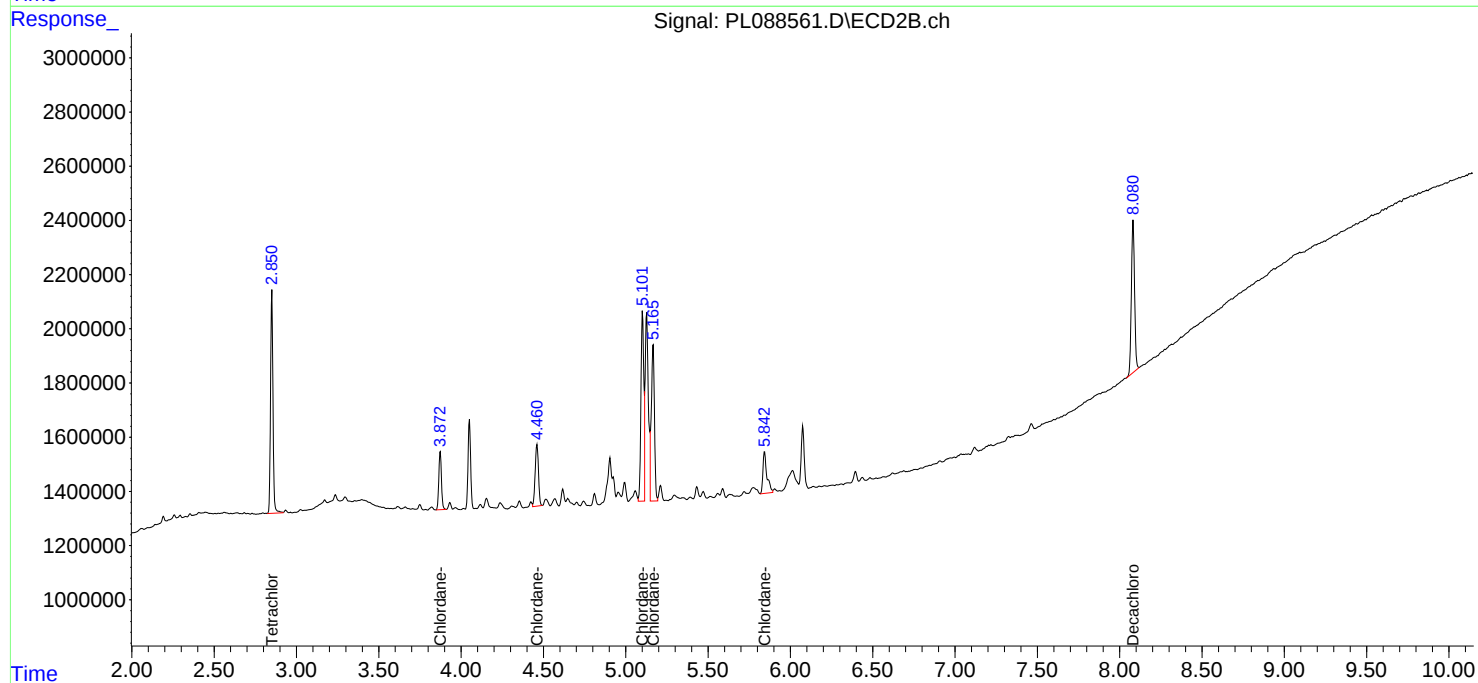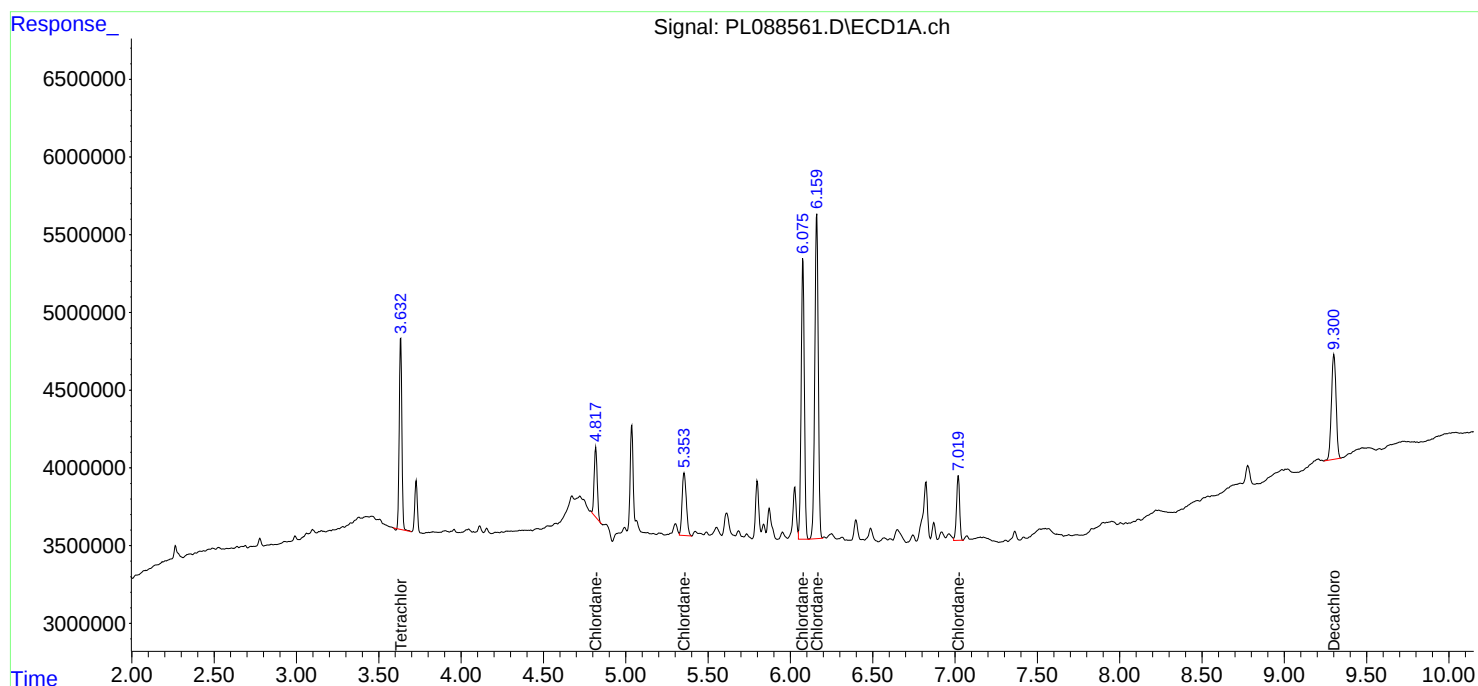


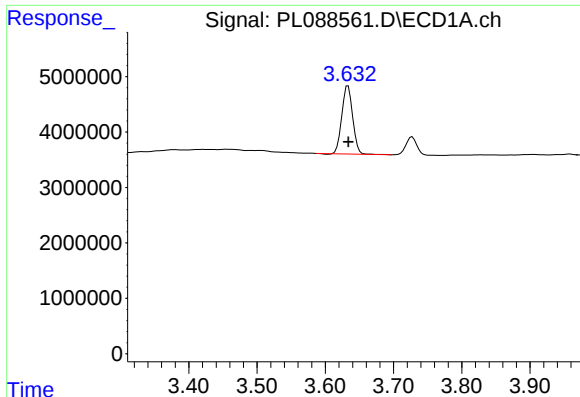

#1 Tetrachloro-m-xylene


R.T.: 3.633 min
Delta R.T.: 0.000 min
Response: 13602953
Conc: 5.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

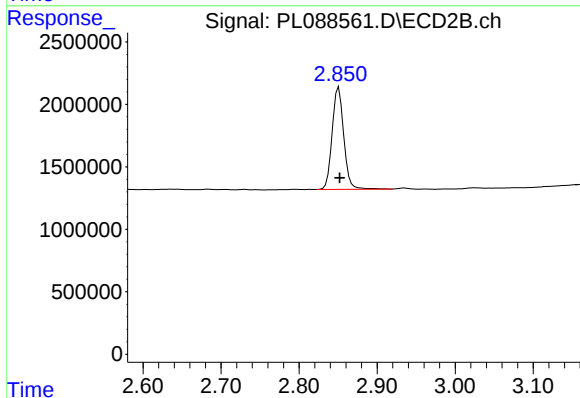


#1 Tetrachloro-m-xylene

R.T.: 2.851 min
Delta R.T.: 0.000 min
Response: 8499767
Conc: 5.13 ng/ml

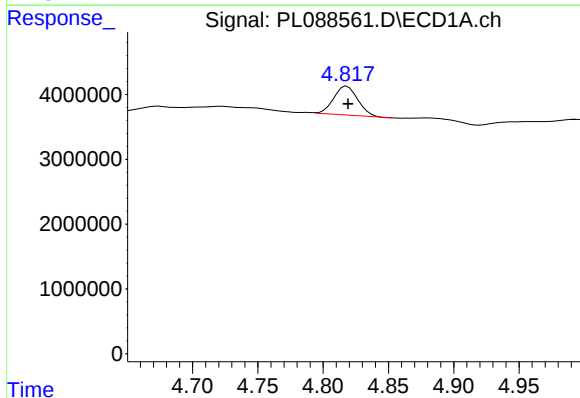


#23 Chlordane-1

R.T.: 4.818 min
Delta R.T.: 0.000 min
Response: 5650247
Conc: 48.88 ng/ml

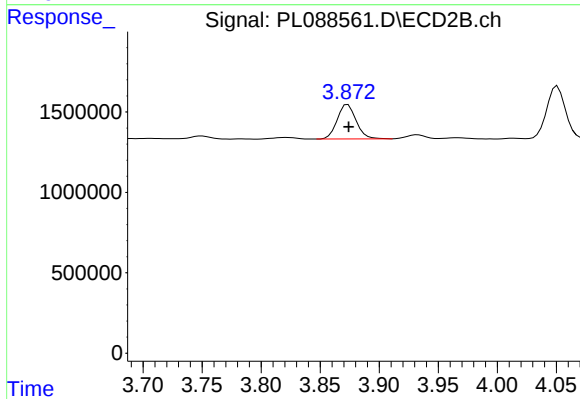

#23 Chlordane-1


R.T.: 3.873 min
Delta R.T.: 0.000 min
Response: 2391501
Conc: 49.91 ng/ml

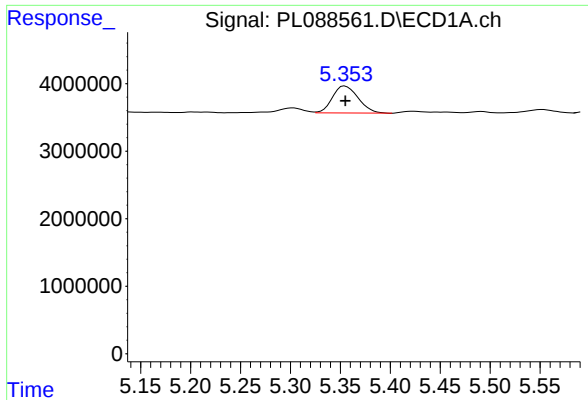

#24 Chlordane-2


R.T.: 5.354 min
Delta R.T.: 0.000 min
Response: 7214050
Conc: 56.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

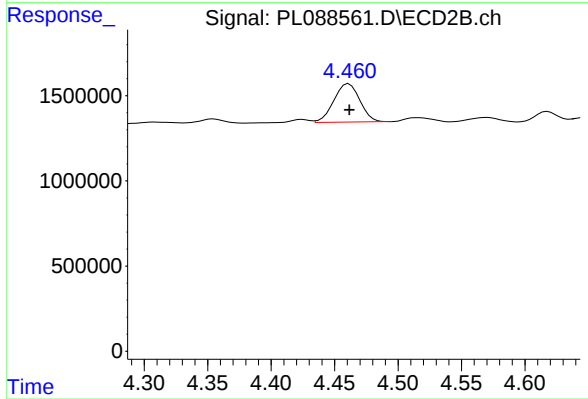


#24 Chlordane-2

R.T.: 4.461 min
Delta R.T.: 0.000 min
Response: 3200501
Conc: 53.69 ng/ml

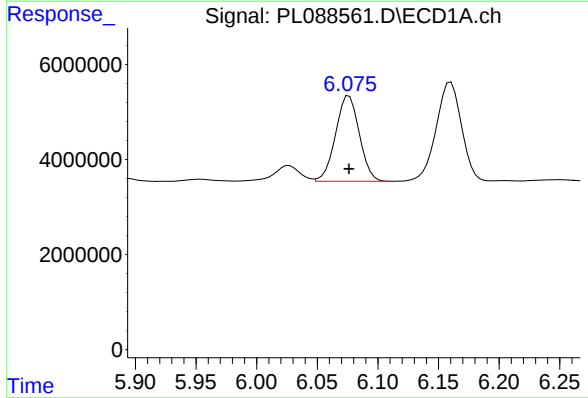


#25 Chlordane-3

R.T.: 6.076 min
Delta R.T.: 0.000 min
Response: 24515658
Conc: 49.93 ng/ml

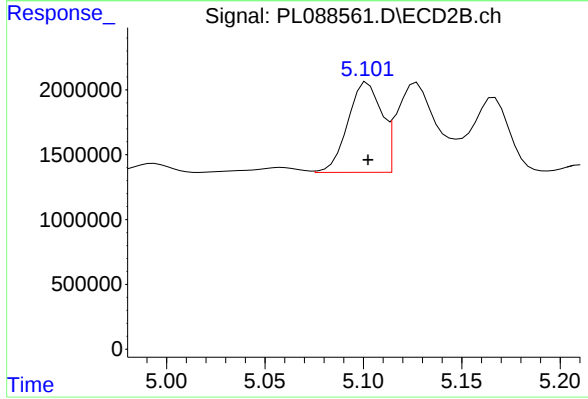

#25 Chlordane-3


R.T.: 5.102 min
Delta R.T.: 0.000 min
Response: 8221160
Conc: 48.20 ng/ml

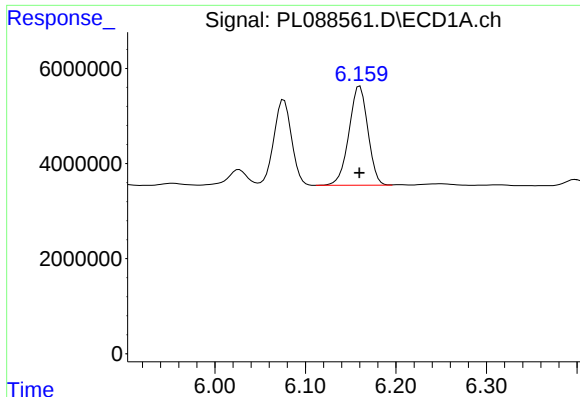

#26 Chlordane-4


R.T.: 6.160 min
Delta R.T.: 0.000 min
Response: 30270860
Conc: 51.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

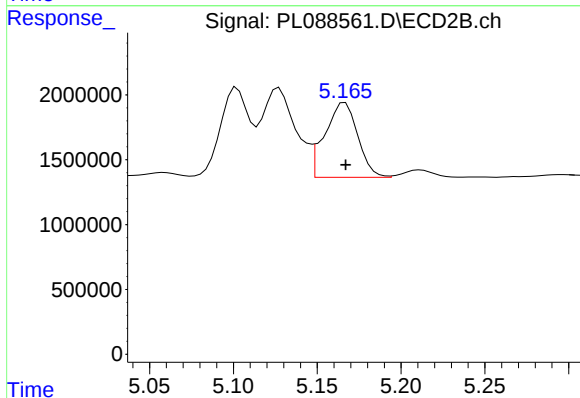


#26 Chlordane-4

R.T.: 5.167 min
Delta R.T.: 0.000 min
Response: 7880418
Conc: 49.56 ng/ml

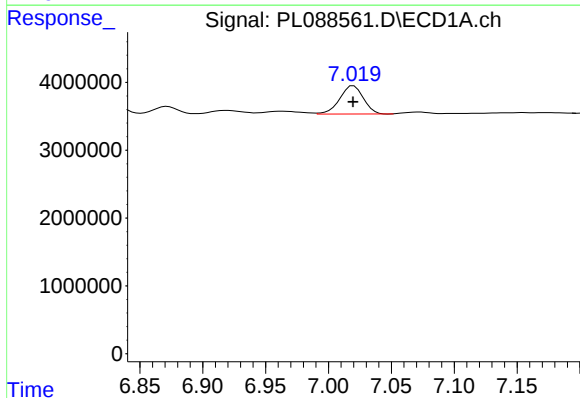


#27 Chlordane-5

R.T.: 7.020 min
Delta R.T.: 0.000 min
Response: 5461555
Conc: 52.48 ng/ml

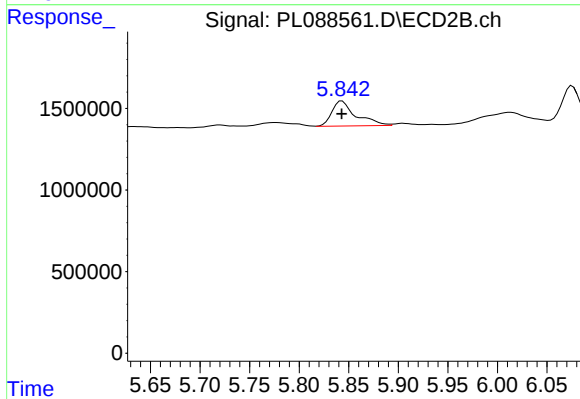

#27 Chlordane-5


R.T.: 5.843 min
Delta R.T.: 0.000 min
Response: 2591372
Conc: 51.73 ng/ml

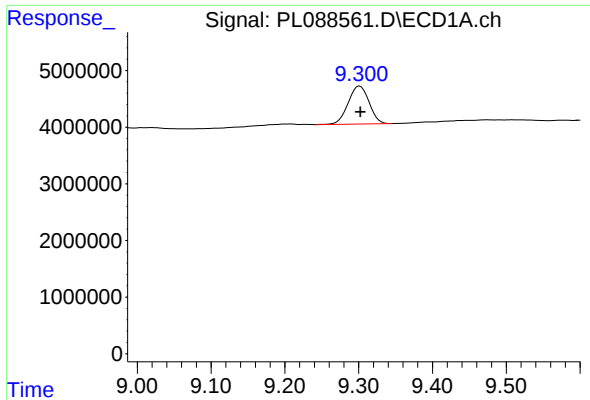

#28 Decachlorobiphenyl

R.T.: 9.301 min
Delta R.T.: 0.000 min
Response: 13220667
Conc: 5.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC050

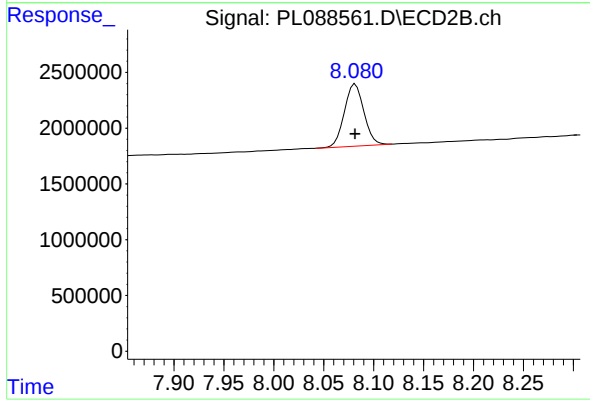

#28 Decachlorobiphenyl

R.T.: 8.082 min
Delta R.T.: 0.000 min
Response: 7576974
Conc: 5.53 ng/ml