

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031519\
 Data File : PL045974.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2019 11:16
 Operator : AJ\SJ
 Sample : K1807-44DL 2X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-22DL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 23:02:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.365	3.981	44354782	13780177	6.448	6.435
28)	SA Decachlor...	8.047	9.041	53047534	14157360	6.340	6.196
Target Compounds							
12)	B 4,4'-DDE	5.486	6.320	325.4E6	84863504	37.064	36.330
13)	MA Dieldrin	5.611	6.468	53247687	14408865	5.571	5.607
14)	MA Endrin	5.868	6.714f	57038910	-1599285	6.334	N.D. #
15)	B Endosulfa...	0.000	6.896	0	2015076	N.D.	0.857 #
16)	A 4,4'-DDD	5.997	6.809	19672458	6251156	2.687	3.251
17)	MA 4,4'-DDT	6.233	7.108	550.3E6	140.7E6	73.370	71.313
18)	B Endrin a...	6.291	0.000	8162368	0	1.117	N.D. #
19)	B Endosulfa...	6.517	7.242	7767064	2187998	0.956	0.973



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031519\
Data File : PL045974.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2019 11:16
Operator : AJ\SJ
Sample : K1807-44DL 2X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
TP-22DL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 23:02:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

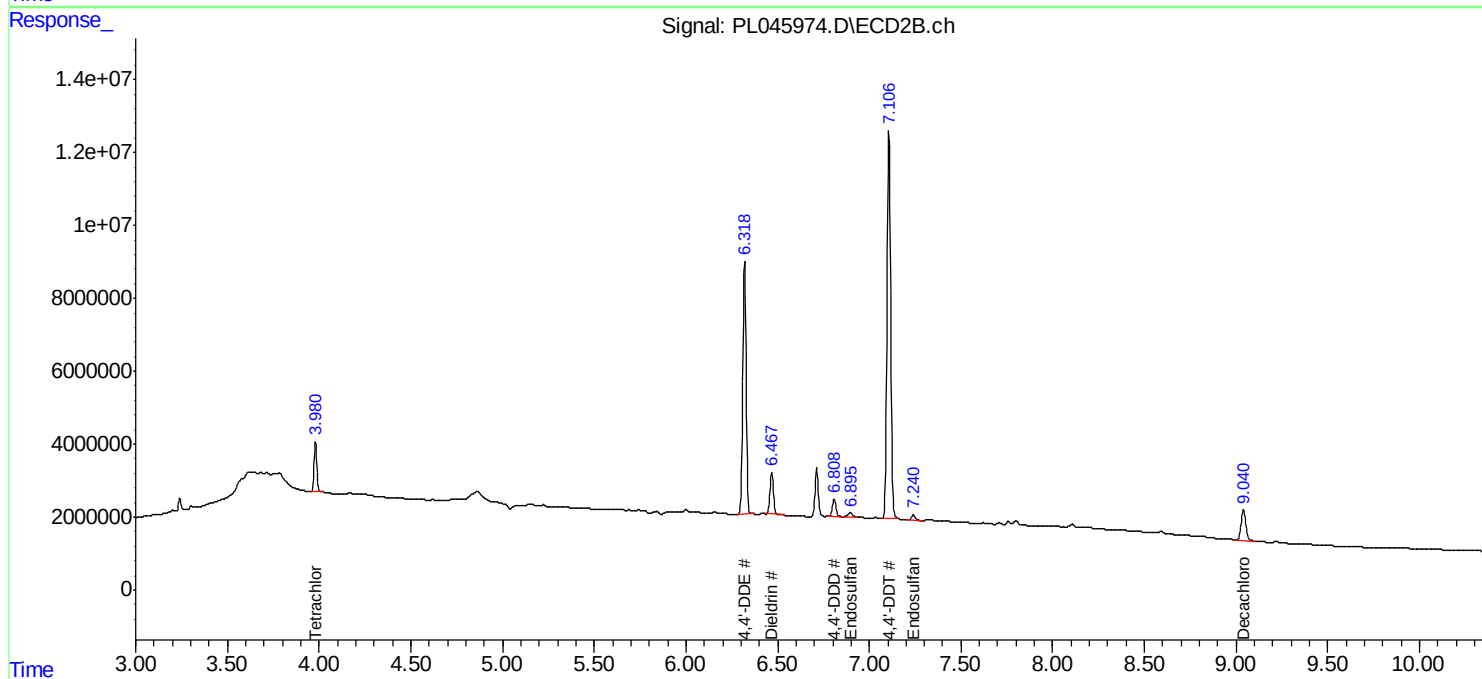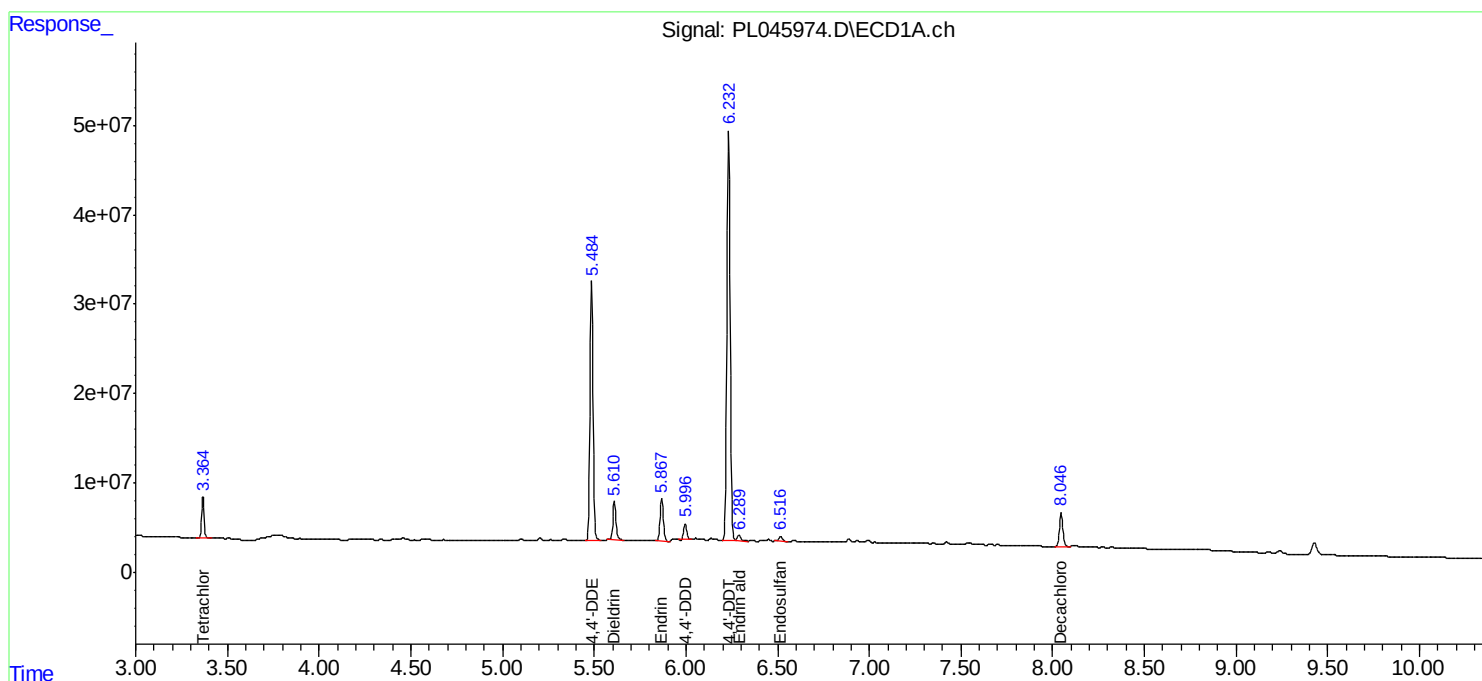


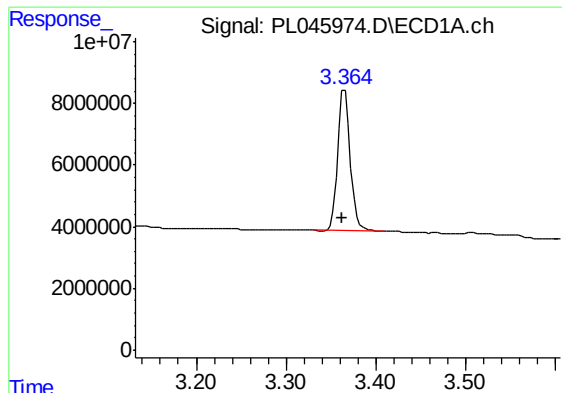

#1 Tetrachloro-m-xylene


R.T.: 3.365 min
Delta R.T.: 0.002 min
Response: 44354782
Conc: 6.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-22DL

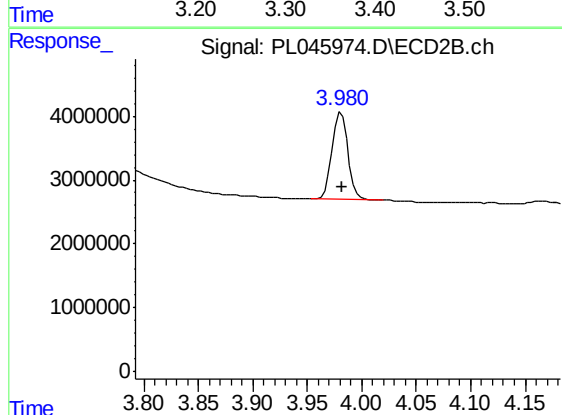


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 13780177
Conc: 6.43 ng/ml

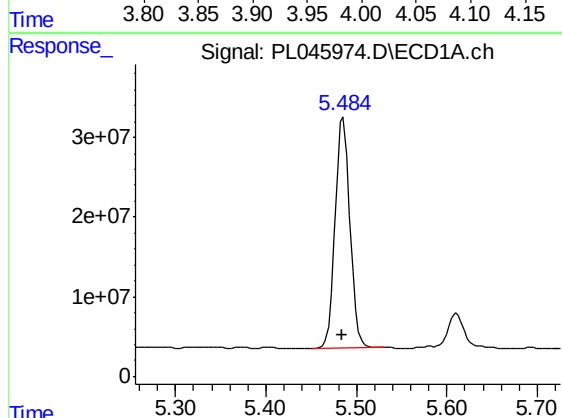


#12 4,4'-DDE

R.T.: 5.486 min
Delta R.T.: 0.002 min
Response: 325351912
Conc: 37.06 ng/ml

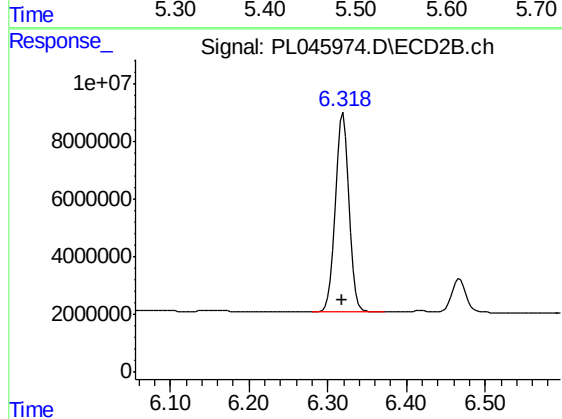

#12 4,4'-DDE


R.T.: 6.320 min
Delta R.T.: 0.001 min
Response: 84863504
Conc: 36.33 ng/ml

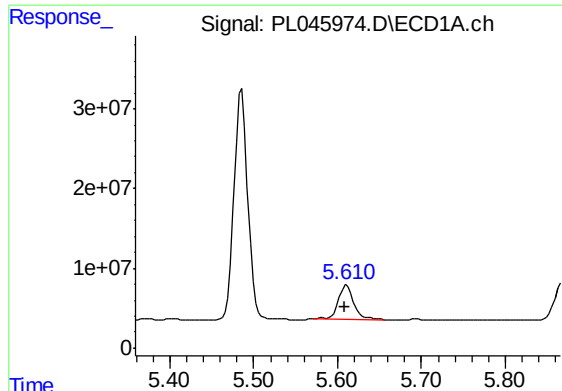

#13 Dieldrin


R.T.: 5.611 min
Delta R.T.: 0.002 min
Response: 53247687
Conc: 5.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-22DL

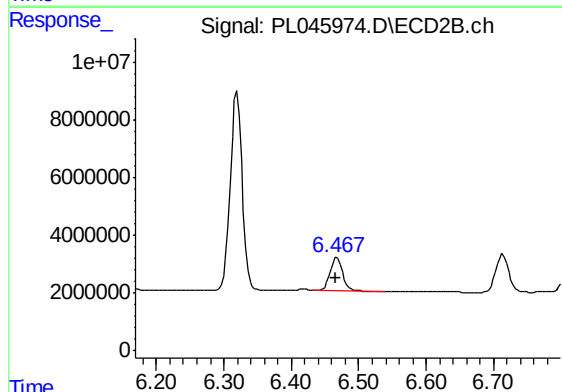


#13 Dieldrin

R.T.: 6.468 min
Delta R.T.: 0.001 min
Response: 14408865
Conc: 5.61 ng/ml

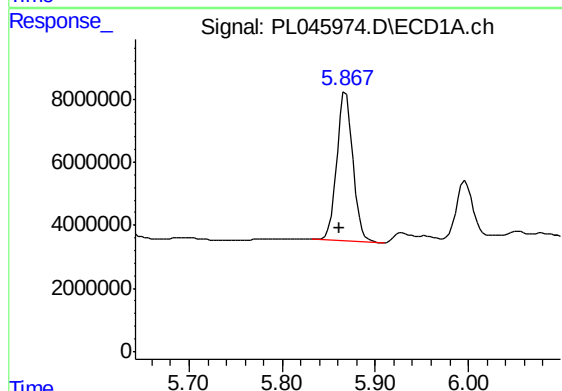


#14 Endrin

R.T.: 5.868 min
Delta R.T.: 0.006 min
Response: 57038910
Conc: 6.33 ng/ml

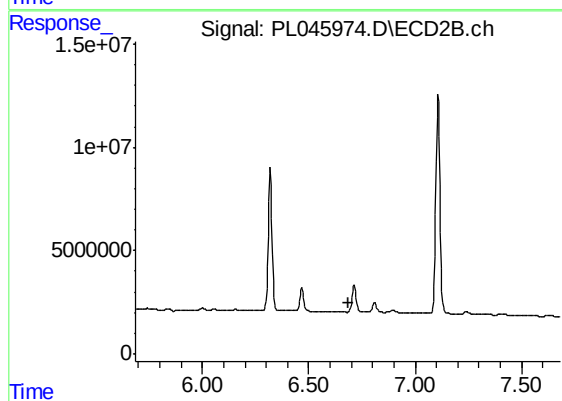

#14 Endrin


R.T.: 6.714 min
Delta R.T.: 0.030 min
Response: -1599285
Conc: N.D.

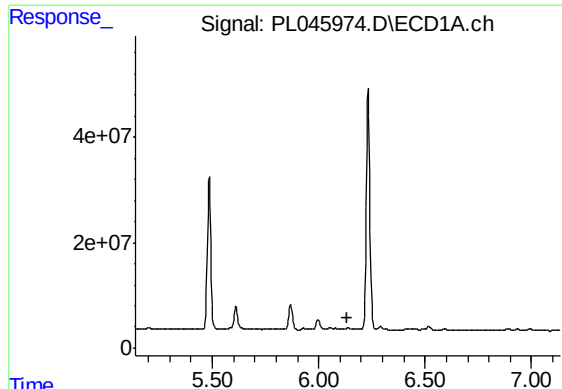

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.137 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-22DL

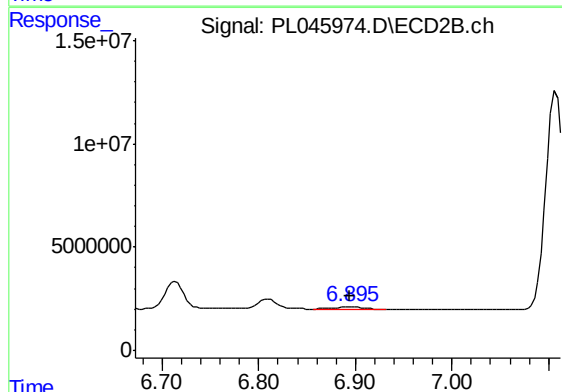


#15 Endosulfan II

R.T.: 6.896 min
Delta R.T.: 0.002 min
Response: 2015076
Conc: 0.86 ng/ml

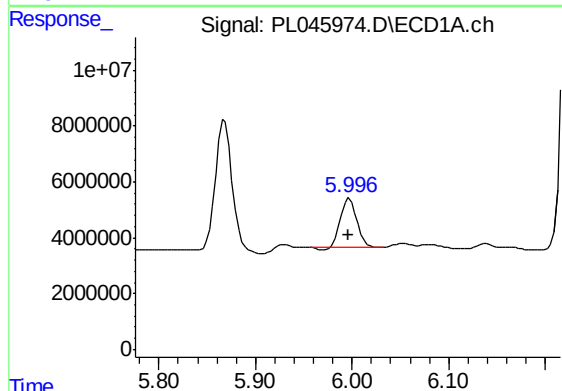


#16 4,4'-DDD

R.T.: 5.997 min
Delta R.T.: 0.001 min
Response: 19672458
Conc: 2.69 ng/ml

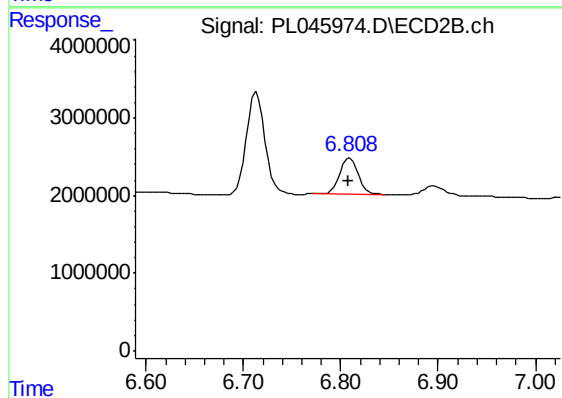

#16 4,4'-DDD


R.T.: 6.809 min
Delta R.T.: 0.002 min
Response: 6251156
Conc: 3.25 ng/ml

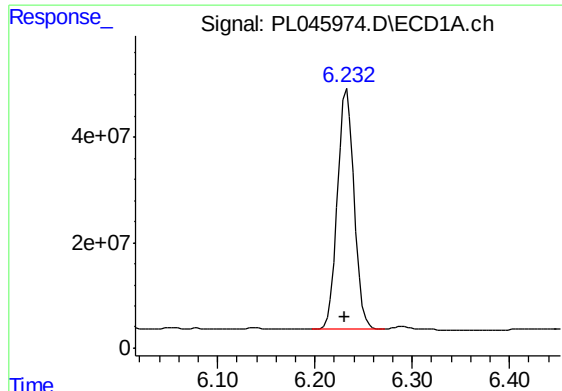

#17 4,4'-DDT


R.T.: 6.233 min
Delta R.T.: 0.002 min
Response: 550286177
Conc: 73.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-22DL

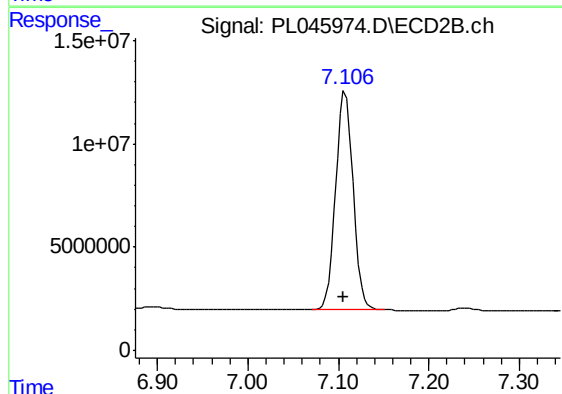


#17 4,4'-DDT

R.T.: 7.108 min
Delta R.T.: 0.002 min
Response: 140731692
Conc: 71.31 ng/ml

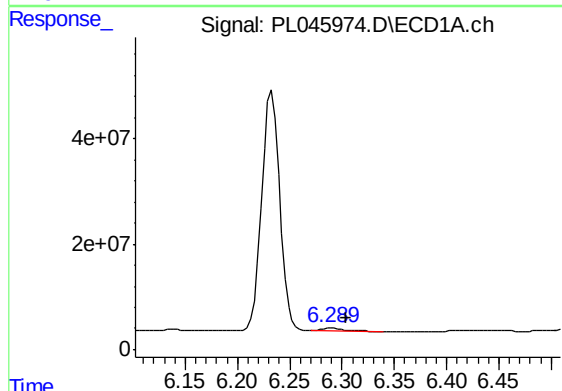


#18 Endrin aldehyde

R.T.: 6.291 min
Delta R.T.: -0.013 min
Response: 8162368
Conc: 1.12 ng/ml

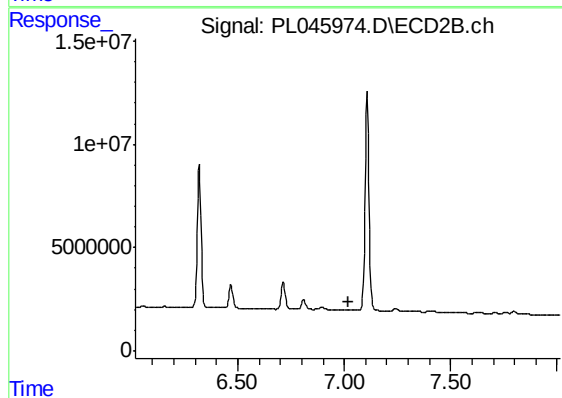

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 7.017 min
Response: 0
Conc: N.D.

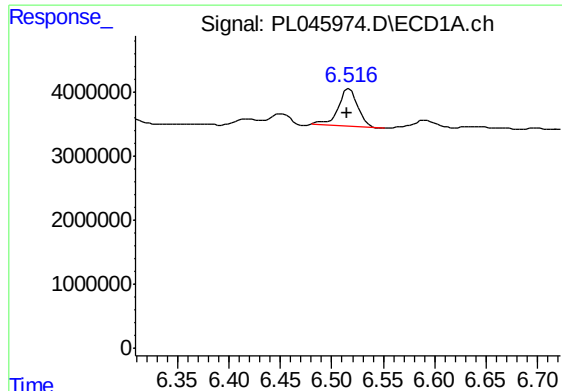

#19 Endosulfan Sulfate


R.T.: 6.517 min
Delta R.T.: 0.002 min
Response: 7767064
Conc: 0.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-22DL

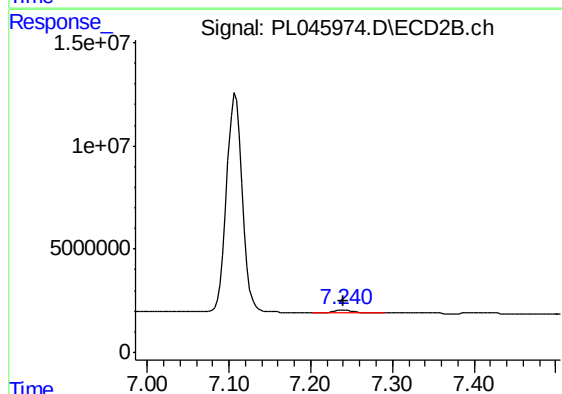


#19 Endosulfan Sulfate

R.T.: 7.242 min
Delta R.T.: 0.001 min
Response: 2187998
Conc: 0.97 ng/ml

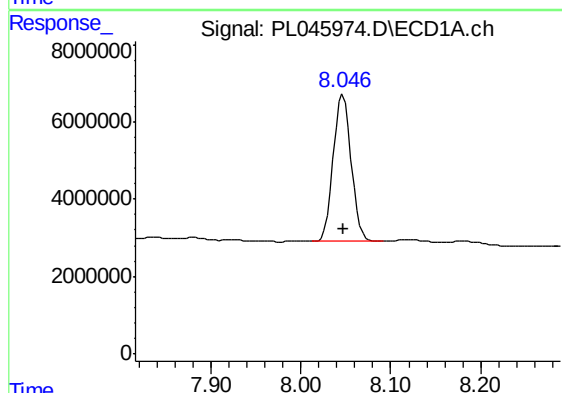

#28 Decachlorobiphenyl

R.T.: 8.047 min
Delta R.T.: 0.000 min
Response: 53047534
Conc: 6.34 ng/ml

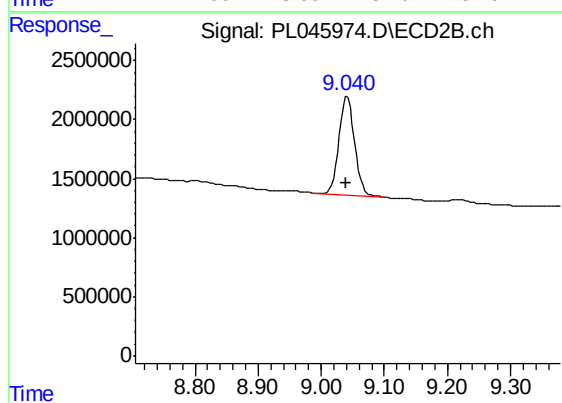

#28 Decachlorobiphenyl

R.T.: 9.041 min
Delta R.T.: 0.003 min
Response: 14157360
Conc: 6.20 ng/ml