

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031519\
 Data File : PL045976.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2019 11:44
 Operator : AJ\SJ
 Sample : K1897-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 23:02:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.362	3.981	55536794	17234128	8.073	8.048
28)	SA Decachlor...	8.044	9.039	74020004	20314554	8.846	8.891
Target Compounds							
10)	B gamma-Chl...	0.000	6.060f	0	1649299	N.D.	0.615 #
12)	B 4,4'-DDE	5.482	6.318	946.5E6	246.1E6	107.820	105.375
14)	MA Endrin	5.864	6.713f	43146717	-322717	4.791	N.D. #
16)	A 4,4'-DDD	5.993	6.810	16321163	8099888	2.229	4.212 #
17)	MA 4,4'-DDT	6.228	7.106	177.1E6	42641782	23.610	21.608
19)	B Endosulfa...	6.506	0.000	9851252	0	1.212	N.D. #
20)	A Methoxychlor	6.753f	0.000	11757314	0	2.677	N.D. #
21)	B Endrin ke...	7.023f	0.000	4649809	0	0.505	N.D. #
25)	Chlordane-3	0.000	6.060f	0	1649299	N.D.	4.233 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031519\
Data File : PL045976.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2019 11:44
Operator : AJ\SJ
Sample : K1897-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
TP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 23:02:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

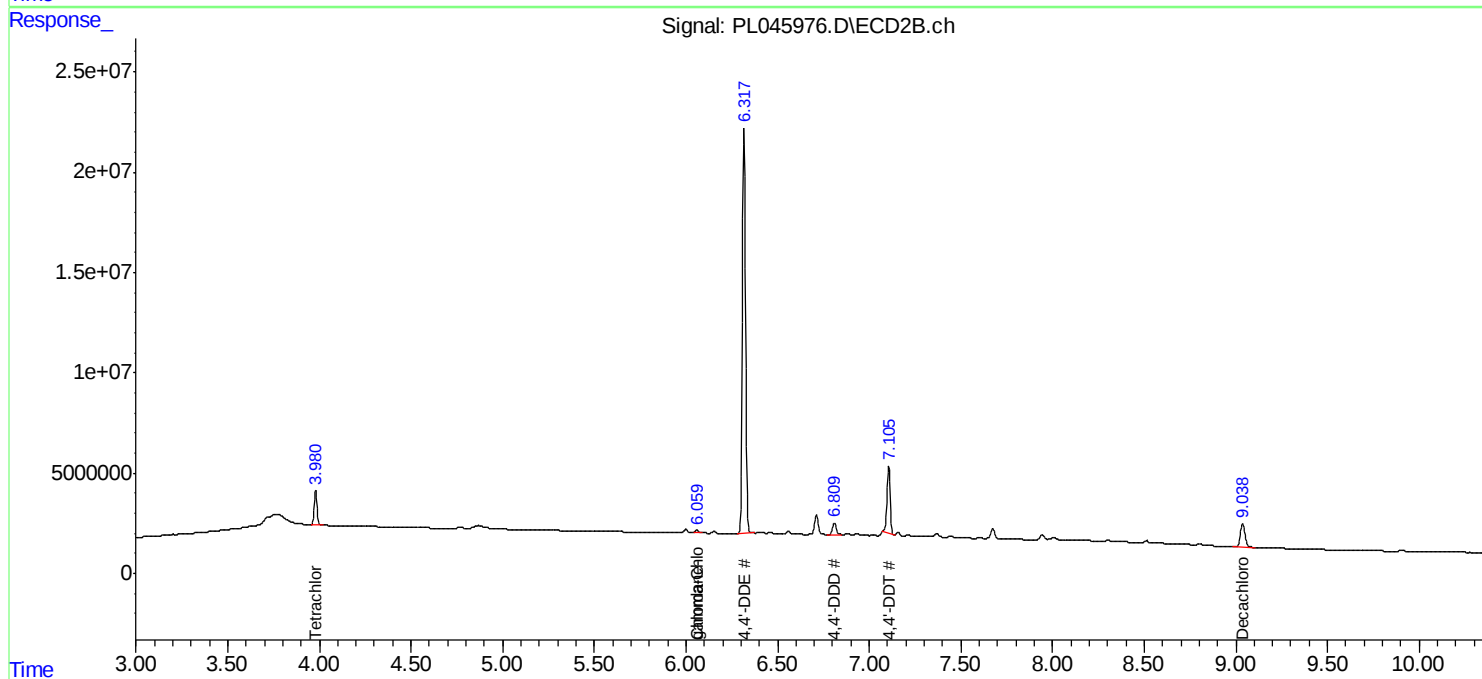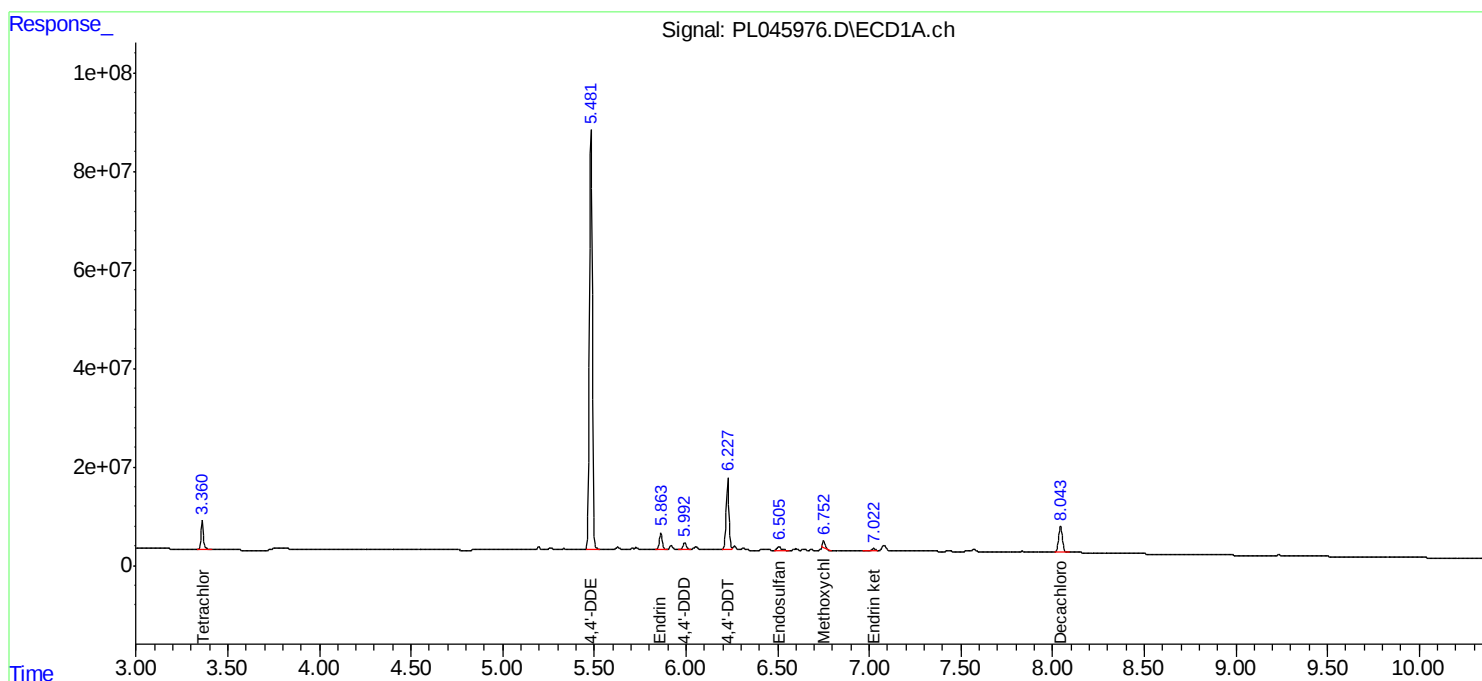


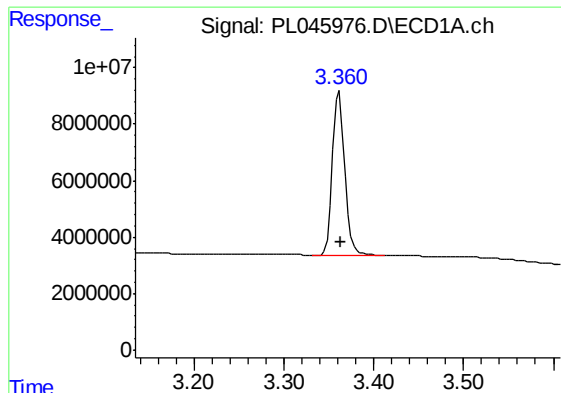

#1 Tetrachloro-m-xylene


R.T.: 3.362 min
Delta R.T.: -0.001 min
Response: 55536794
Conc: 8.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

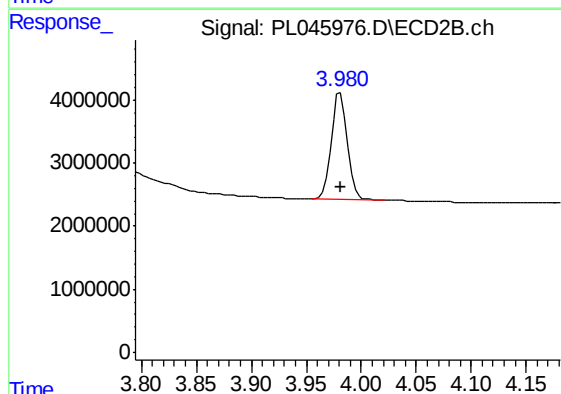


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 17234128
Conc: 8.05 ng/ml

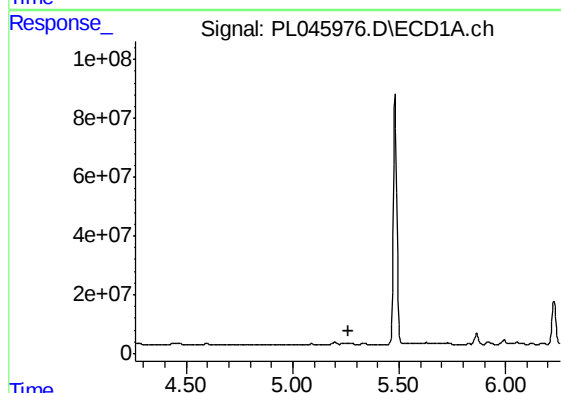


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.261 min
Response: 0
Conc: N.D.

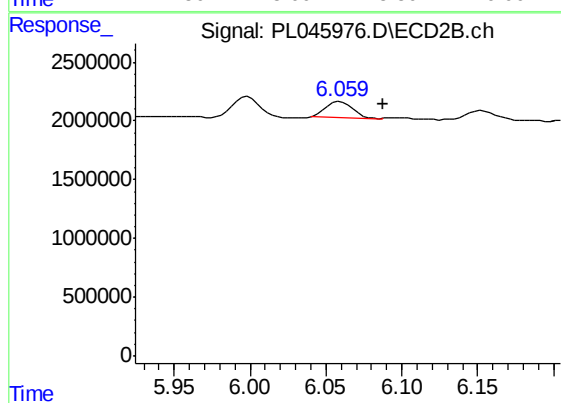

#10 gamma-Chlordane


R.T.: 6.060 min
Delta R.T.: -0.028 min
Response: 1649299
Conc: 0.61 ng/ml

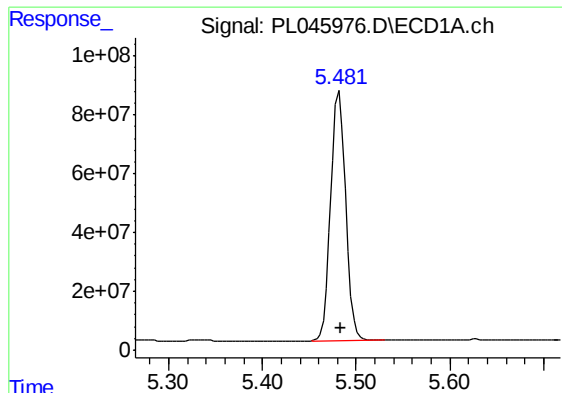

#12 4,4'-DDE


R.T.: 5.482 min
Delta R.T.: -0.002 min
Response: 946467994
Conc: 107.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

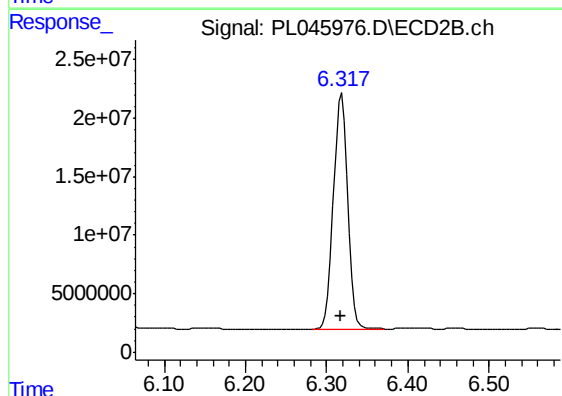


#12 4,4'-DDE

R.T.: 6.318 min
Delta R.T.: 0.000 min
Response: 246145101
Conc: 105.37 ng/ml

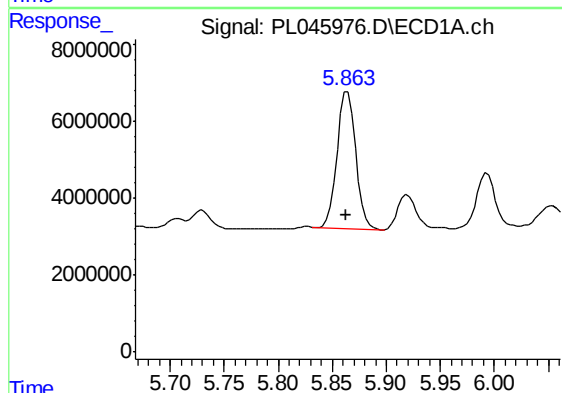


#14 Endrin

R.T.: 5.864 min
Delta R.T.: 0.002 min
Response: 43146717
Conc: 4.79 ng/ml

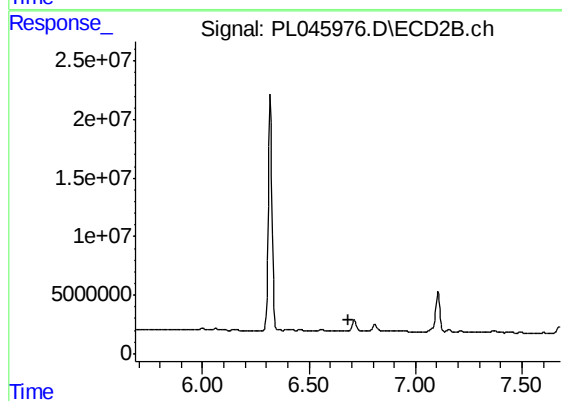

#14 Endrin


R.T.: 6.713 min
Delta R.T.: 0.029 min
Response: -322717
Conc: N.D.

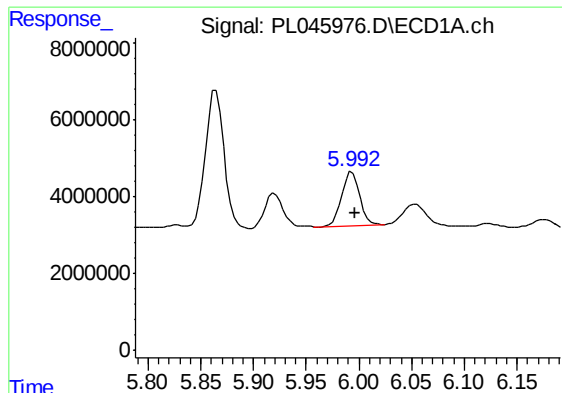

#16 4,4'-DDD


R.T.: 5.993 min
Delta R.T.: -0.002 min
Response: 16321163
Conc: 2.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

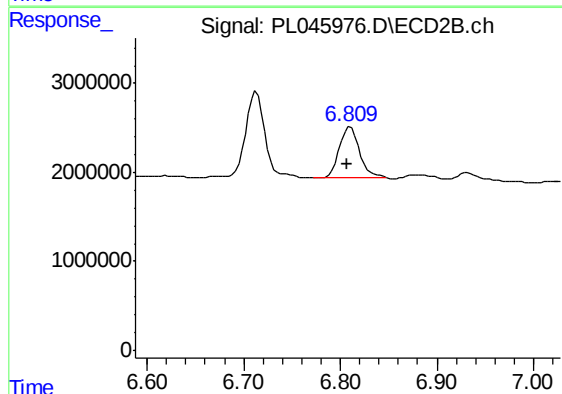


#16 4,4'-DDD

R.T.: 6.810 min
Delta R.T.: 0.002 min
Response: 8099888
Conc: 4.21 ng/ml

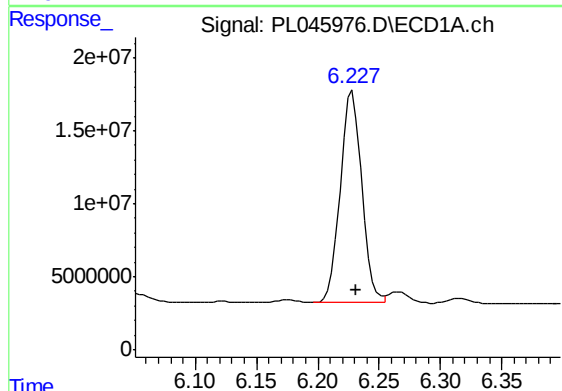


#17 4,4'-DDT

R.T.: 6.228 min
Delta R.T.: -0.003 min
Response: 177077730
Conc: 23.61 ng/ml

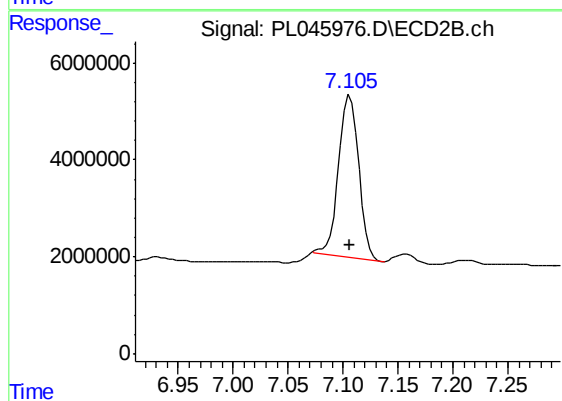

#17 4,4'-DDT


R.T.: 7.106 min
Delta R.T.: 0.000 min
Response: 42641782
Conc: 21.61 ng/ml

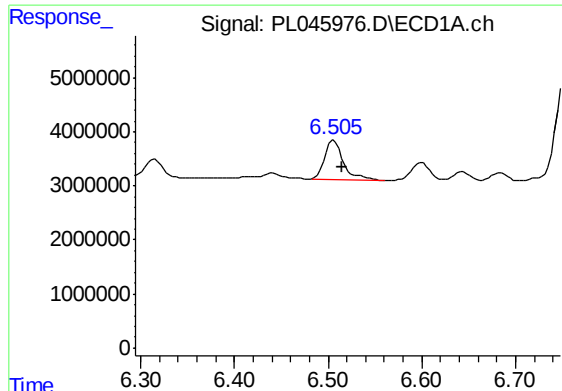

#19 Endosulfan Sulfate


R.T.: 6.506 min
Delta R.T.: -0.009 min
Response: 9851252
Conc: 1.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

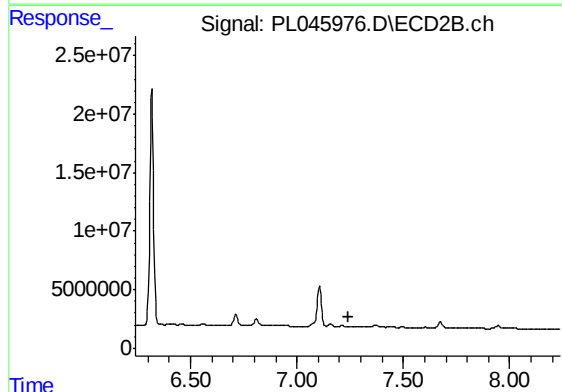


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.241 min
Response: 0
Conc: N.D.

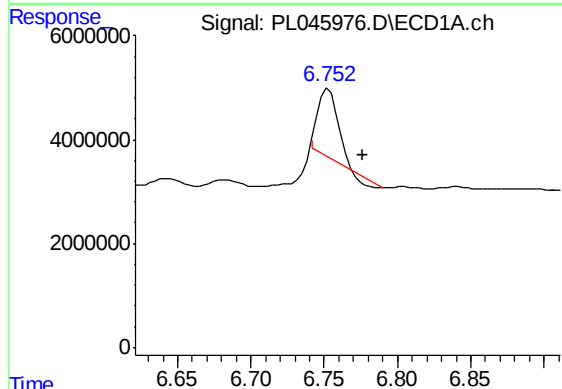


#20 Methoxychlor

R.T.: 6.753 min
Delta R.T.: -0.023 min
Response: 11757314
Conc: 2.68 ng/ml

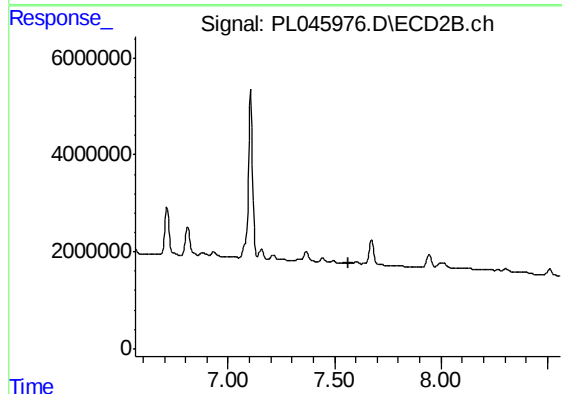

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.564 min
Response: 0
Conc: N.D.

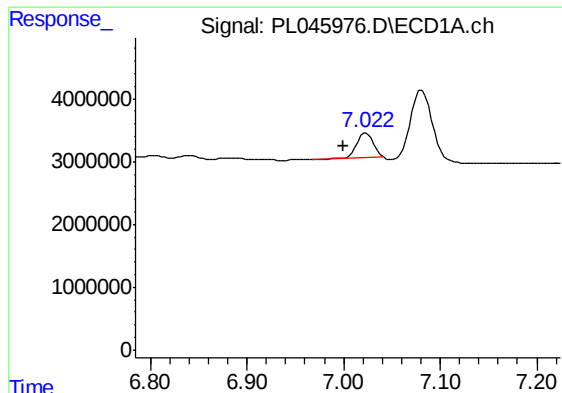

#21 Endrin ketone


R.T.: 7.023 min
Delta R.T.: 0.024 min
Response: 4649809
Conc: 0.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

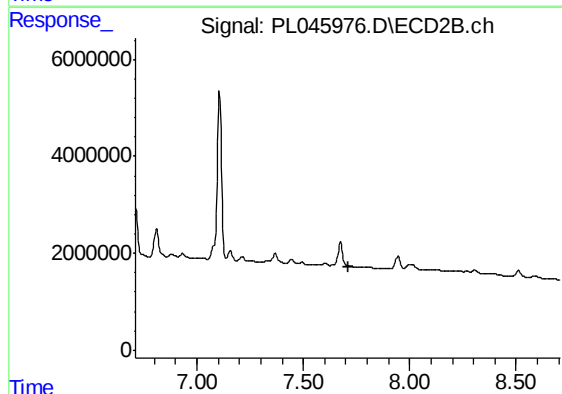


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.710 min
Response: 0
Conc: N.D.

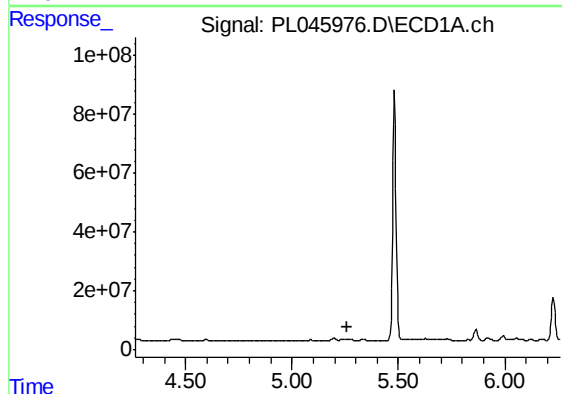


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.262 min
Response: 0
Conc: N.D.

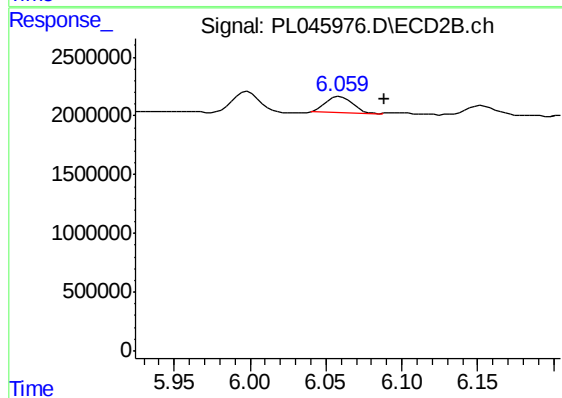

#25 Chlordane-3


R.T.: 6.060 min
Delta R.T.: -0.029 min
Response: 1649299
Conc: 4.23 ng/ml

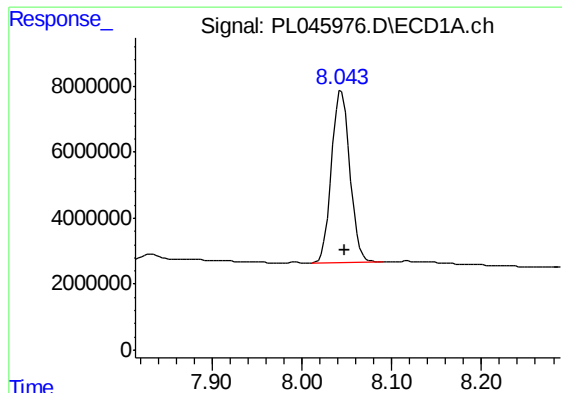

#28 Decachlorobiphenyl

R.T.: 8.044 min
Delta R.T.: -0.003 min
Response: 74020004
Conc: 8.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

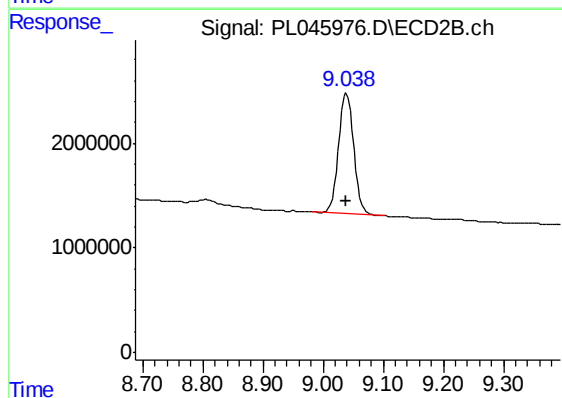

#28 Decachlorobiphenyl

R.T.: 9.039 min
Delta R.T.: 0.000 min
Response: 20314554
Conc: 8.89 ng/ml