

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031519\
 Data File : PL045988.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2019 16:01
 Operator : AJ\SJ
 Sample : K1685-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 AU-05-031419-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 23:05:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.362	3.981	62748784	19571166	9.121	9.139
28)	SA Decachlor...	8.045	9.040	78950577	23425949	9.435	10.252
Target Compounds							
5)	MB Aldrin	0.000	5.467	0	3566008	N.D.	1.320 #
10)	B gamma-Chl...	5.278f	0.000	6820623	0	0.697	N.D. #
11)	B alpha-Chl...	0.000	6.162	0	3322263	N.D.	1.232 #
12)	B 4,4'-DDE	5.481	6.318	10183772	3857120	1.160	1.651 #
23)	Chlordane-1	4.208	4.973	6863956	2141454	20.371	18.991
24)	Chlordane-2	4.702	5.442	7693752	2835620	19.890	23.468
25)	Chlordane-3	5.278f	0.000	6820623	0	5.946	N.D. #
26)	Chlordane-4	0.000	6.162	0	3322263	N.D.	7.102 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031519\
Data File : PL045988.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2019 16:01
Operator : AJ\SJ
Sample : K1685-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
AU-05-031419-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 23:05:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

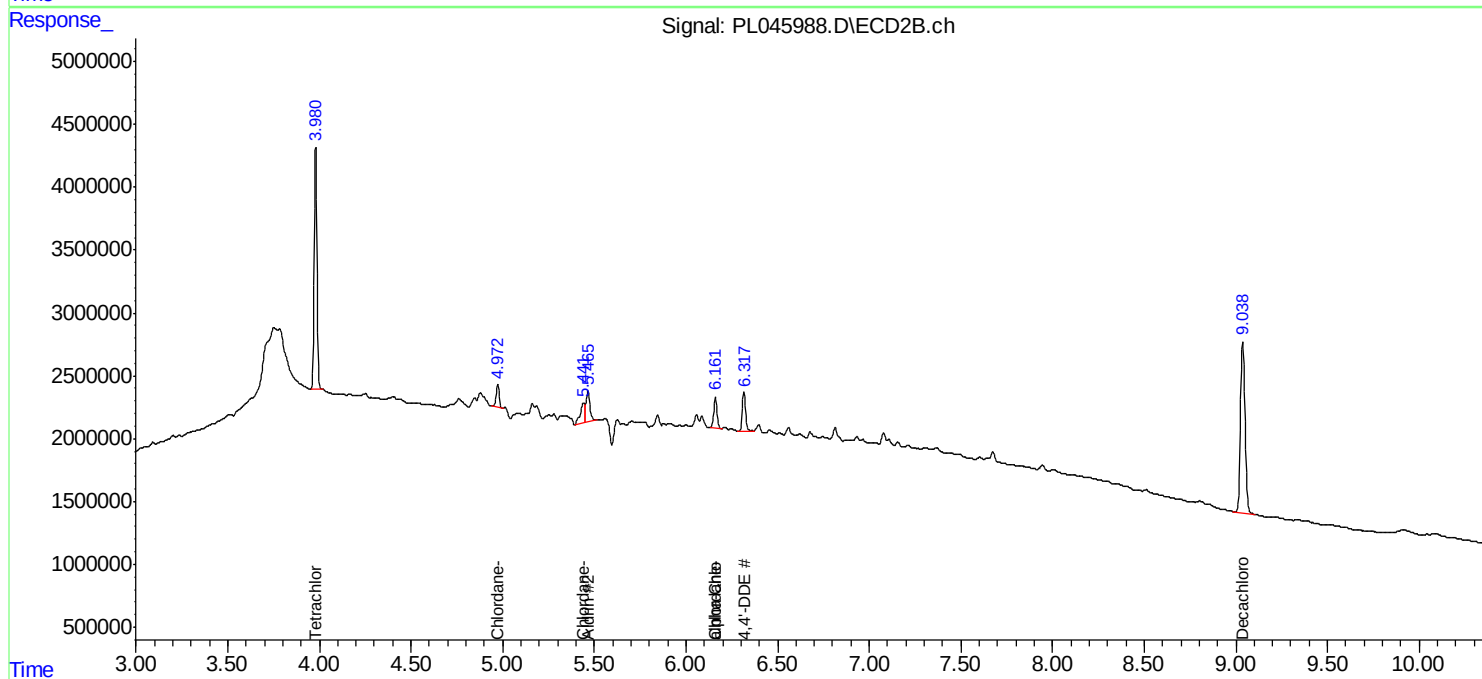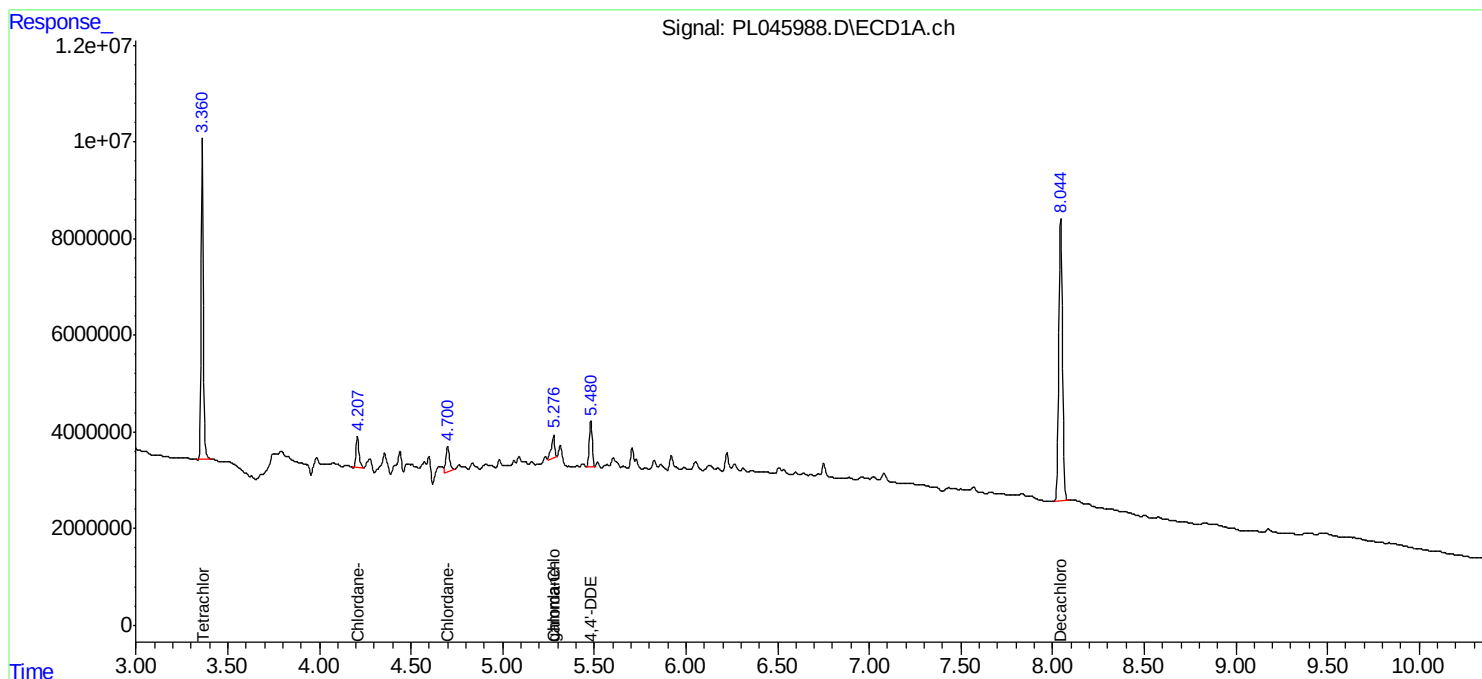


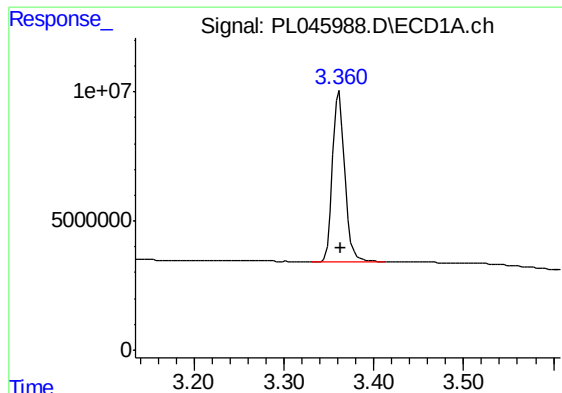

#1 Tetrachloro-m-xylene


R.T.: 3.362 min
Delta R.T.: -0.001 min
Response: 62748784
Conc: 9.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-05-031419-A

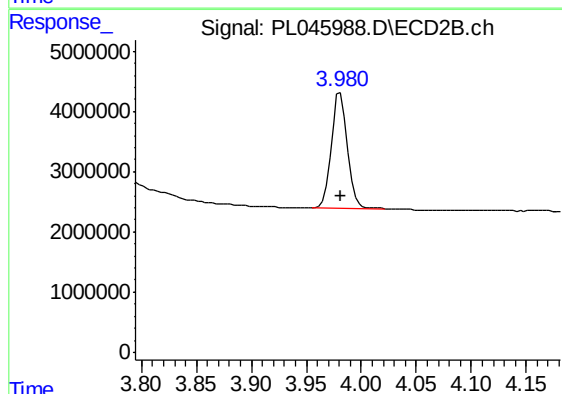


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 19571166
Conc: 9.14 ng/ml

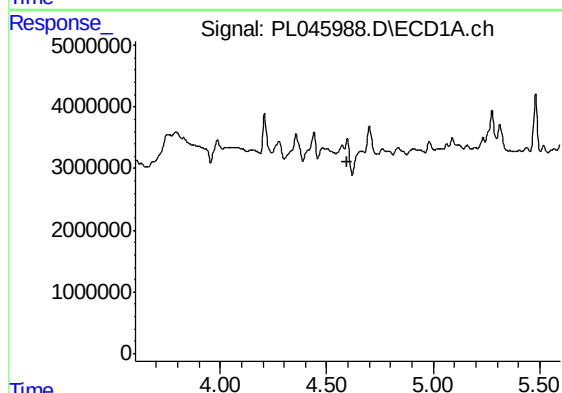


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.599 min
Response: 0
Conc: N.D.

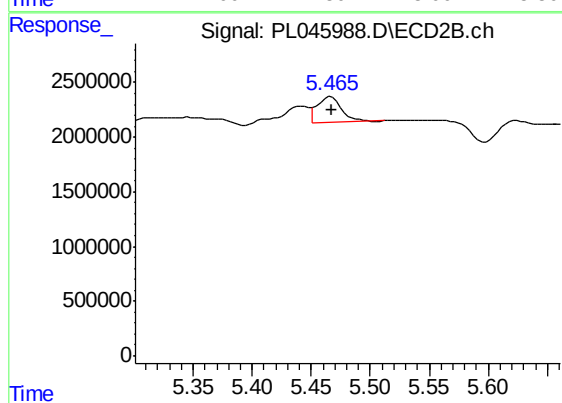

#5 Aldrin


R.T.: 5.467 min
Delta R.T.: 0.000 min
Response: 3566008
Conc: 1.32 ng/ml

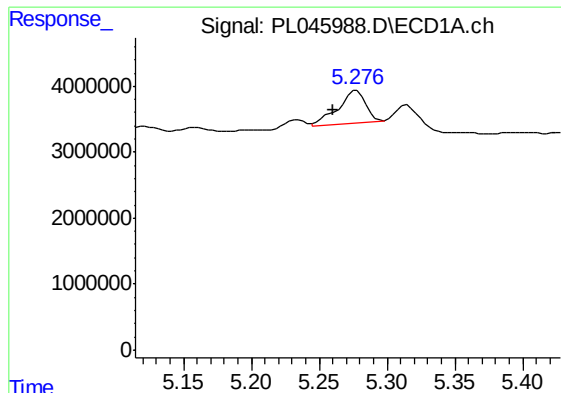

#10 gamma-Chlordane


R.T.: 5.278 min
Delta R.T.: 0.017 min
Response: 6820623
Conc: 0.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-05-031419-A

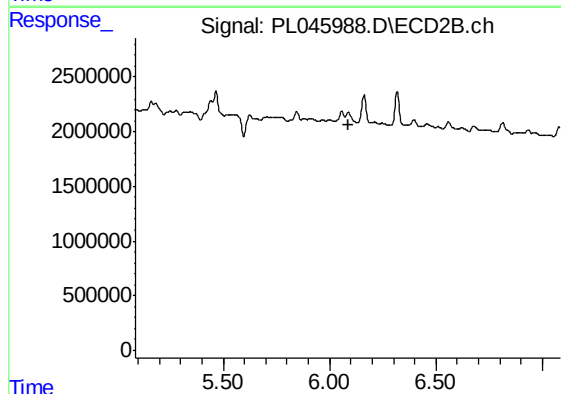


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.088 min
Response: 0
Conc: N.D.

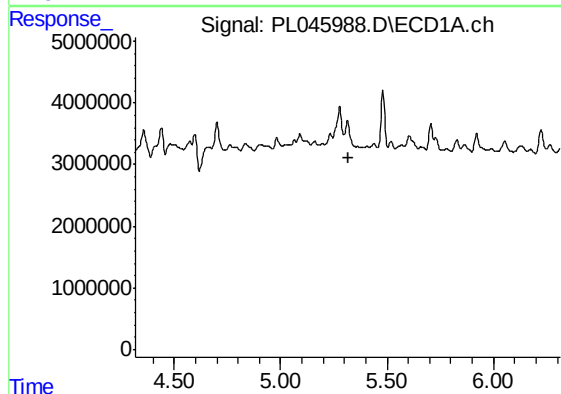


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.317 min
Response: 0
Conc: N.D.

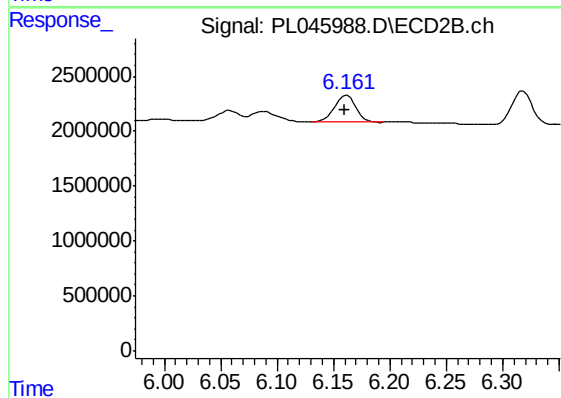

#11 alpha-Chlordane


R.T.: 6.162 min
Delta R.T.: 0.002 min
Response: 3322263
Conc: 1.23 ng/ml

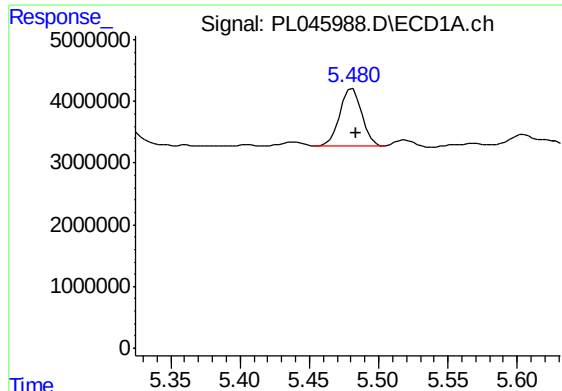

#12 4,4'-DDE


R.T.: 5.481 min
Delta R.T.: -0.003 min
Response: 10183772
Conc: 1.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-05-031419-A

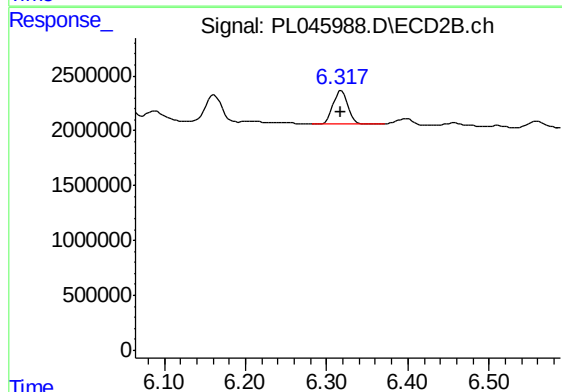


#12 4,4'-DDE

R.T.: 6.318 min
Delta R.T.: 0.000 min
Response: 3857120
Conc: 1.65 ng/ml

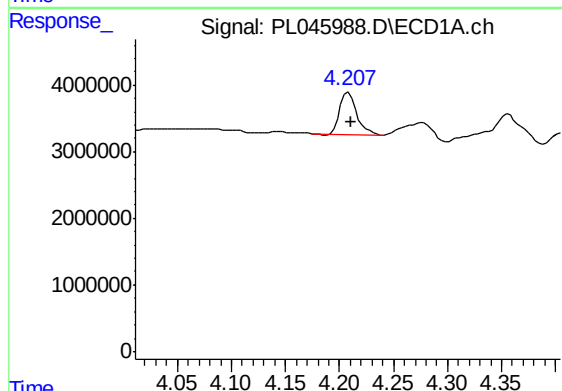


#23 Chlordane-1

R.T.: 4.208 min
Delta R.T.: -0.003 min
Response: 6863956
Conc: 20.37 ng/ml

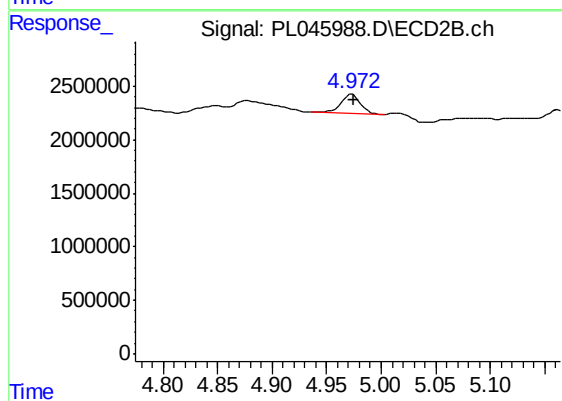

#23 Chlordane-1


R.T.: 4.973 min
Delta R.T.: -0.002 min
Response: 2141454
Conc: 18.99 ng/ml

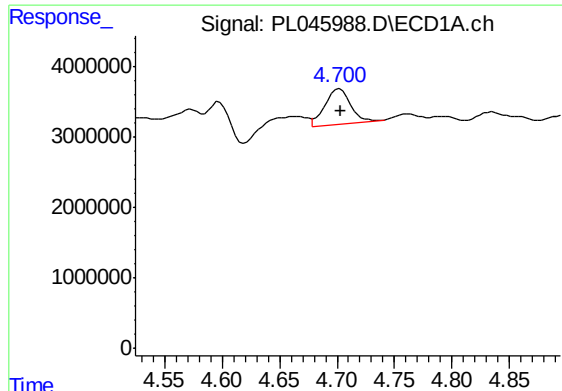

#24 Chlordane-2


R.T.: 4.702 min
Delta R.T.: -0.002 min
Response: 7693752
Conc: 19.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
AU-05-031419-A

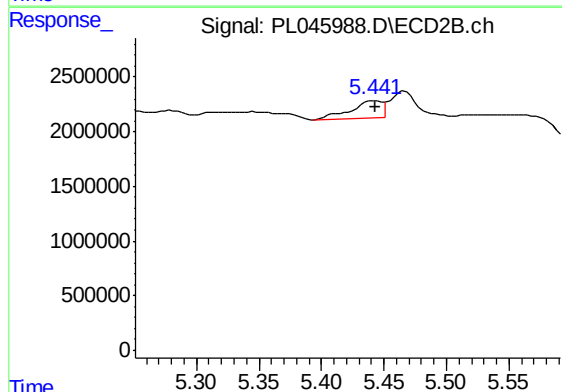


#24 Chlordane-2

R.T.: 5.442 min
Delta R.T.: 0.000 min
Response: 2835620
Conc: 23.47 ng/ml

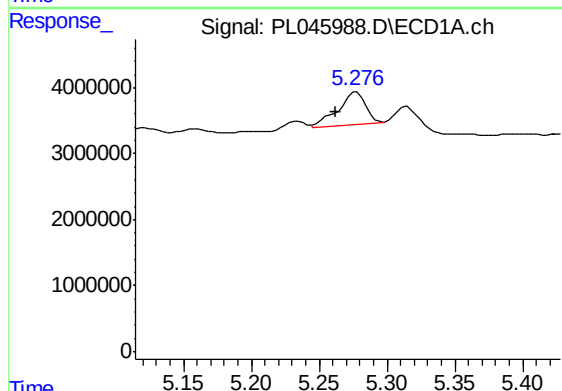


#25 Chlordane-3

R.T.: 5.278 min
Delta R.T.: 0.016 min
Response: 6820623
Conc: 5.95 ng/ml

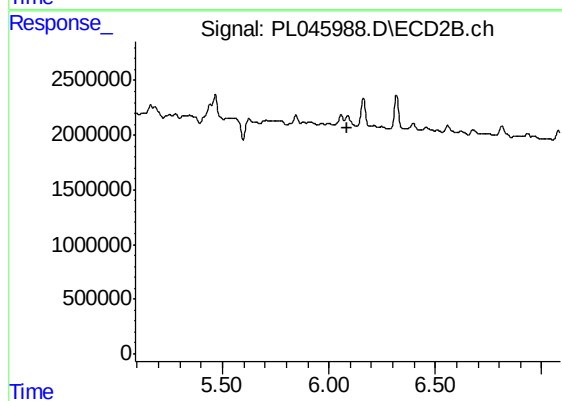

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.089 min
Response: 0
Conc: N.D.

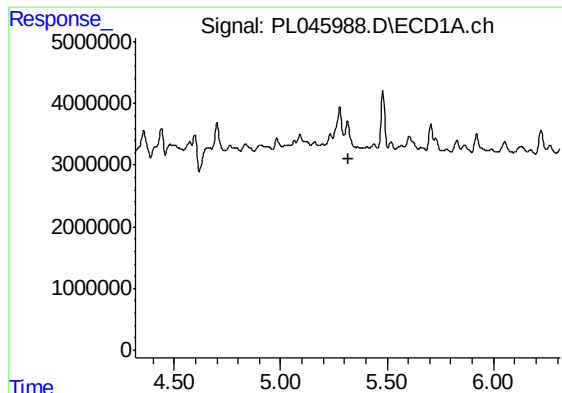

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.317 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
AU-05-031419-A

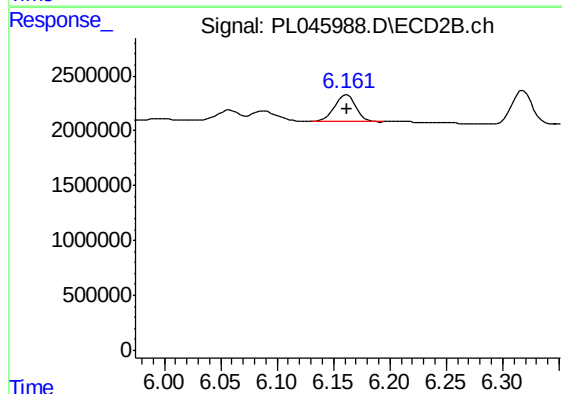


#26 Chlordane-4

R.T.: 6.162 min
Delta R.T.: 0.000 min
Response: 3322263
Conc: 7.10 ng/ml

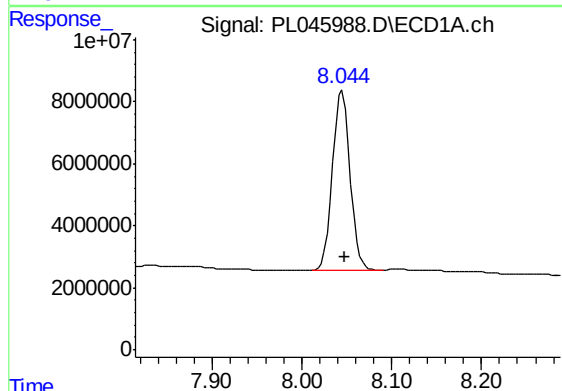

#28 Decachlorobiphenyl

R.T.: 8.045 min
Delta R.T.: -0.002 min
Response: 78950577
Conc: 9.44 ng/ml

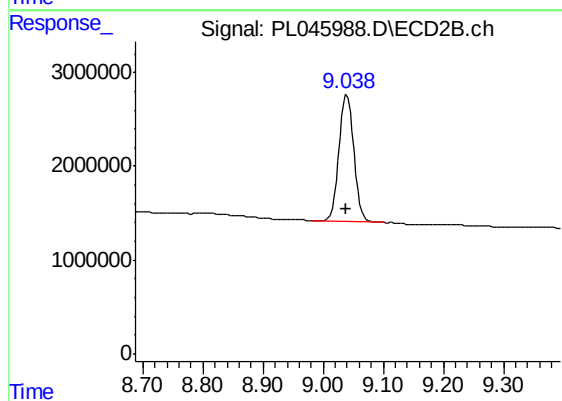

#28 Decachlorobiphenyl

R.T.: 9.040 min
Delta R.T.: 0.000 min
Response: 23425949
Conc: 10.25 ng/ml