

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031519\
 Data File : PL046014.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2019 22:23
 Operator : AJ\SJ
 Sample : K1698-01 10X
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TR-04-031419

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 23:11:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.361	3.981	7564172	2379728	1.100	1.111
28)	SA Decachlor...	8.044	9.040	9819330	3036546	1.174	1.329
Target Compounds							
6)	B beta-BHC	0.000	4.841	0	2447900	N.D.	1.928 #
24)	Chlordane-2	4.706	0.000	6551014	0	16.936	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031519\
Data File : PL046014.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2019 22:23
Operator : AJ\SJ
Sample : K1698-01 10X
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TR-04-031419

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 23:11:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

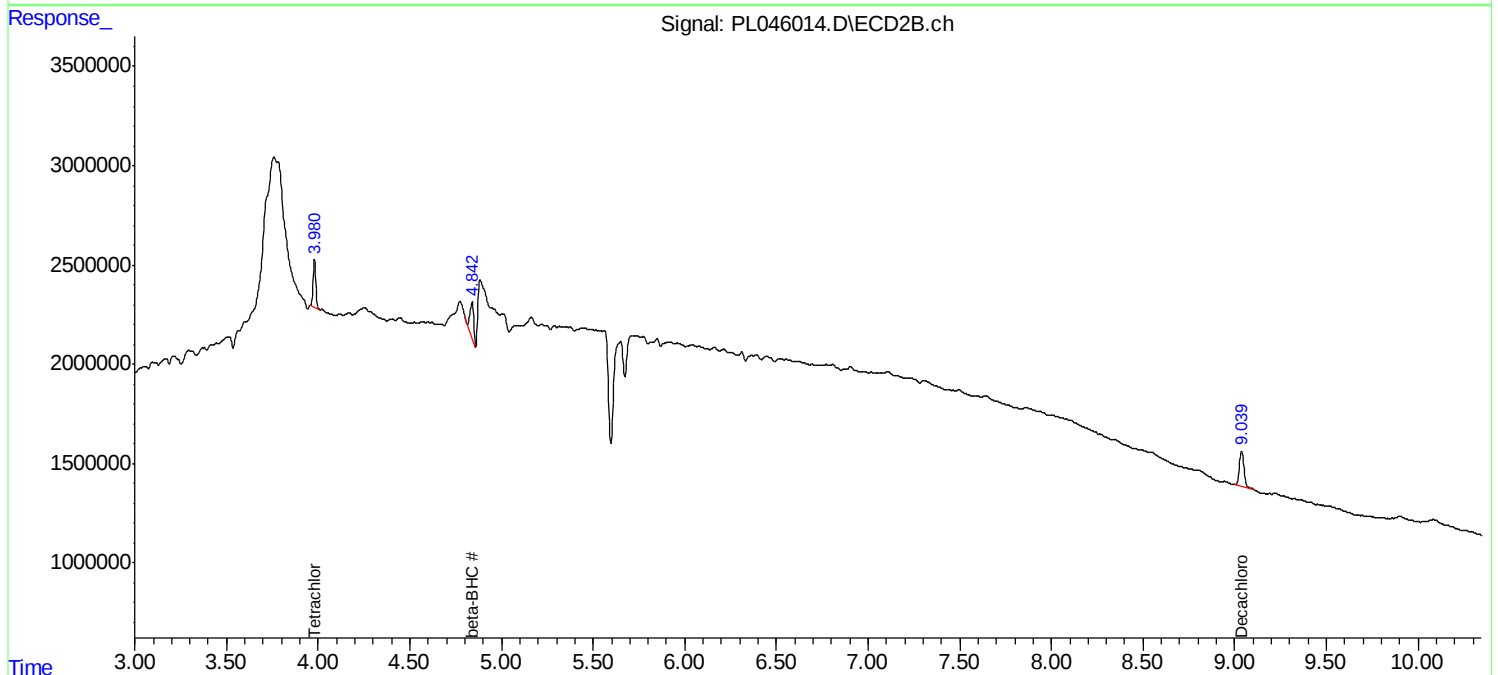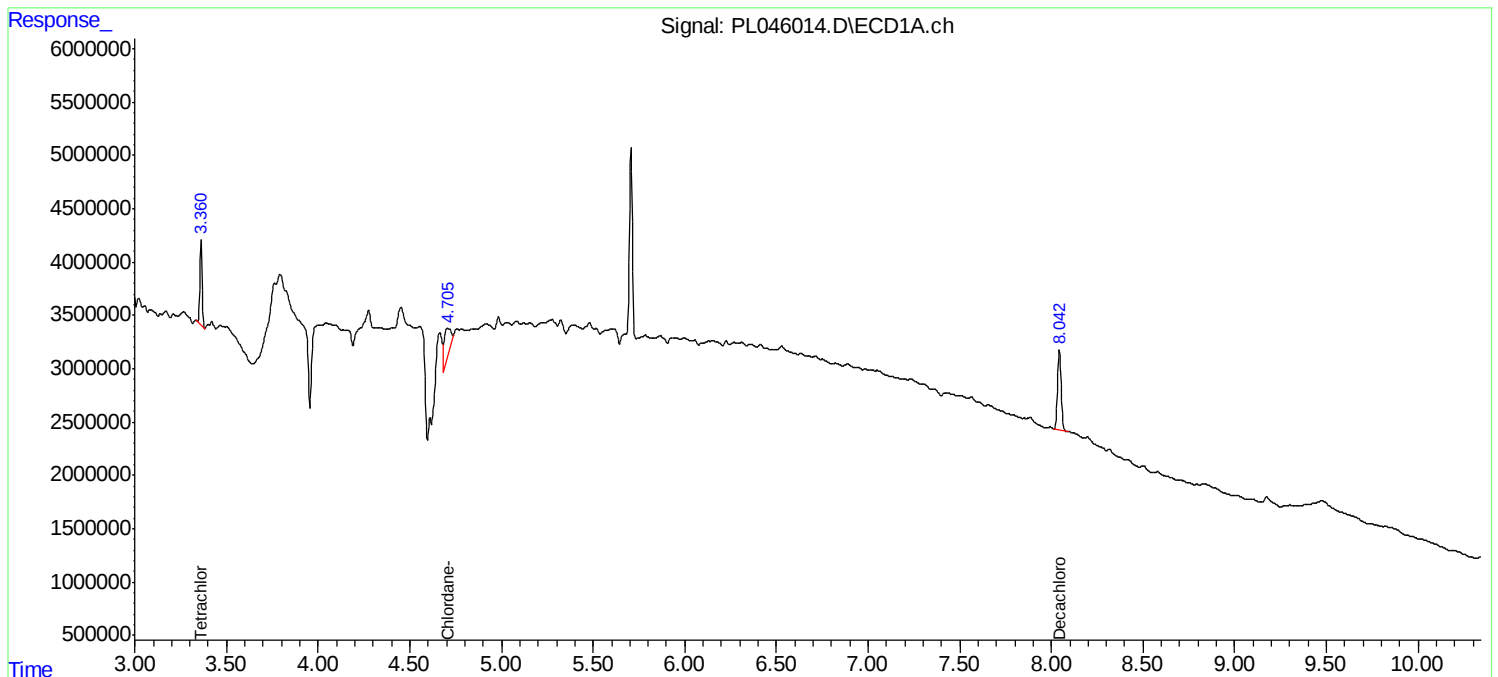


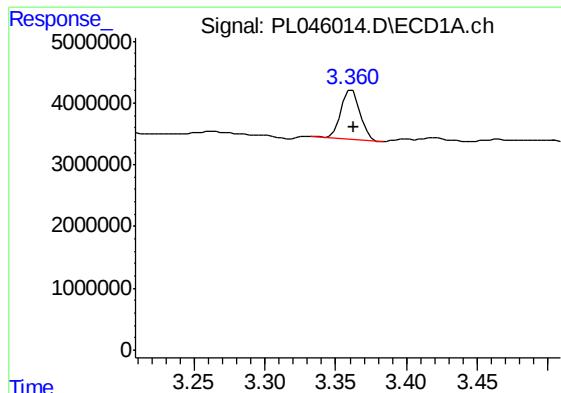

#1 Tetrachloro-m-xylene


R.T.: 3.361 min
Delta R.T.: -0.002 min
Response: 7564172
Conc: 1.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-04-031419

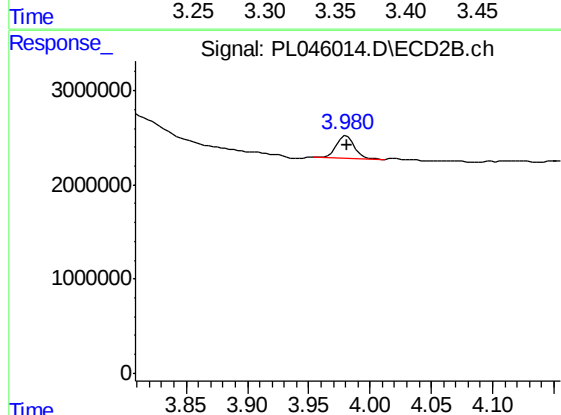


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 2379728
Conc: 1.11 ng/ml

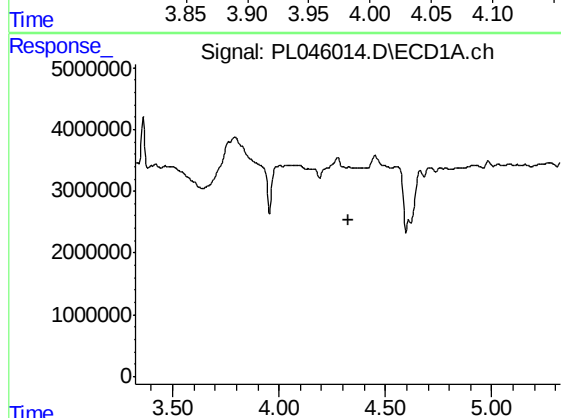


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.324 min
Response: 0
Conc: N.D.

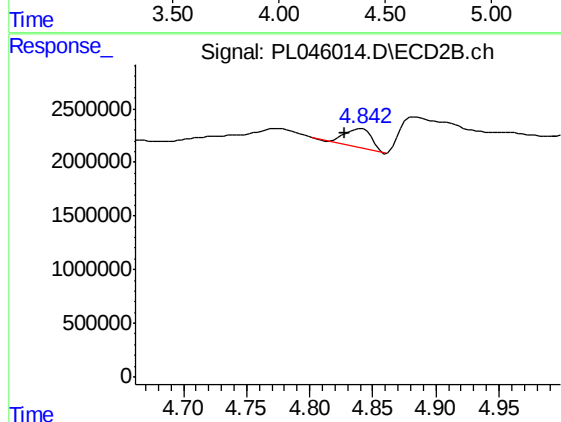

#6 beta-BHC


R.T.: 4.841 min
Delta R.T.: 0.013 min
Response: 2447900
Conc: 1.93 ng/ml

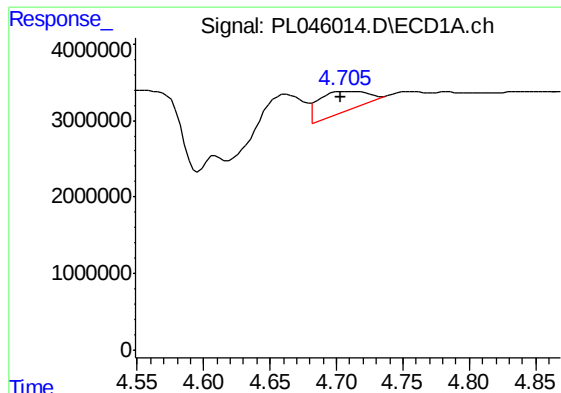

#24 Chlordane-2


R.T.: 4.706 min
Delta R.T.: 0.003 min
Response: 6551014
Conc: 16.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-04-031419

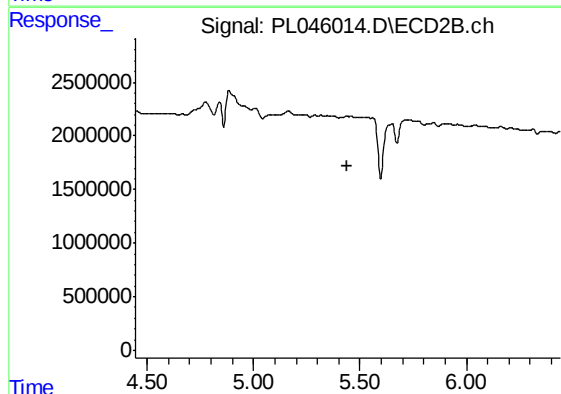


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.443 min
Response: 0
Conc: N.D.

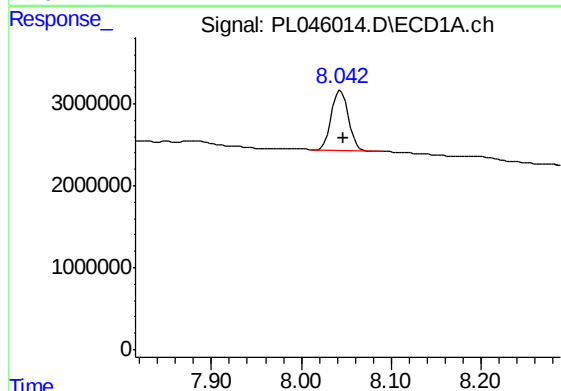

#28 Decachlorobiphenyl

R.T.: 8.044 min
Delta R.T.: -0.003 min
Response: 9819330
Conc: 1.17 ng/ml

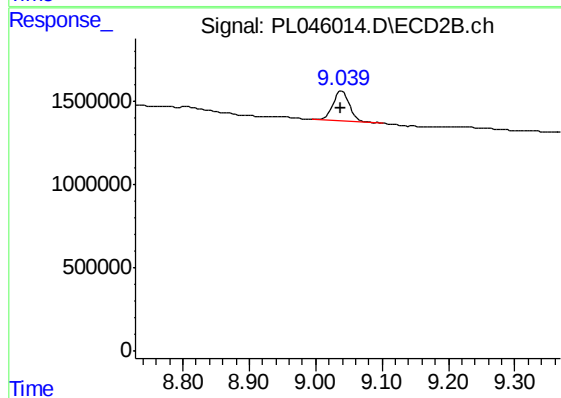

#28 Decachlorobiphenyl

R.T.: 9.040 min
Delta R.T.: 0.000 min
Response: 3036546
Conc: 1.33 ng/ml