

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031519\
 Data File : PL046030.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2019 02:54
 Operator : AJ\SJ
 Sample : K1911-06
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RBR200051

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 05:42:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.362	3.981	109.1E6	35413475	15.857	16.536
28)	SA Decachlor...	8.044	9.040	161.2E6	45289352	19.263	19.821
Target Compounds							
2)	A alpha-BHC	3.822f	0.000	3470193	0	0.312	N.D. #
3)	MA gamma-BHC...	4.078	0.000	6709656	0	0.664	N.D. #
4)	MA Heptachlor	0.000	5.167	0	2168059	N.D.	0.729 #
9)	A Endosulfan I	5.397f	0.000	23202411	0	2.596	N.D. #
10)	B gamma-Chl...	0.000	6.075	0	1544062	N.D.	0.576 #
13)	MA Dieldrin	5.596	0.000	2705162	0	0.283	N.D. #
14)	MA Endrin	5.870	0.000	16480380	0	1.830	N.D. #
23)	Chlordane-1	4.236f	0.000	10010988	0	29.712	N.D. #
25)	Chlordane-3	0.000	6.075	0	1544062	N.D.	3.963 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031519\
Data File : PL046030.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2019 02:54
Operator : AJ\SJ
Sample : K1911-06
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RBR200051

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 05:42:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

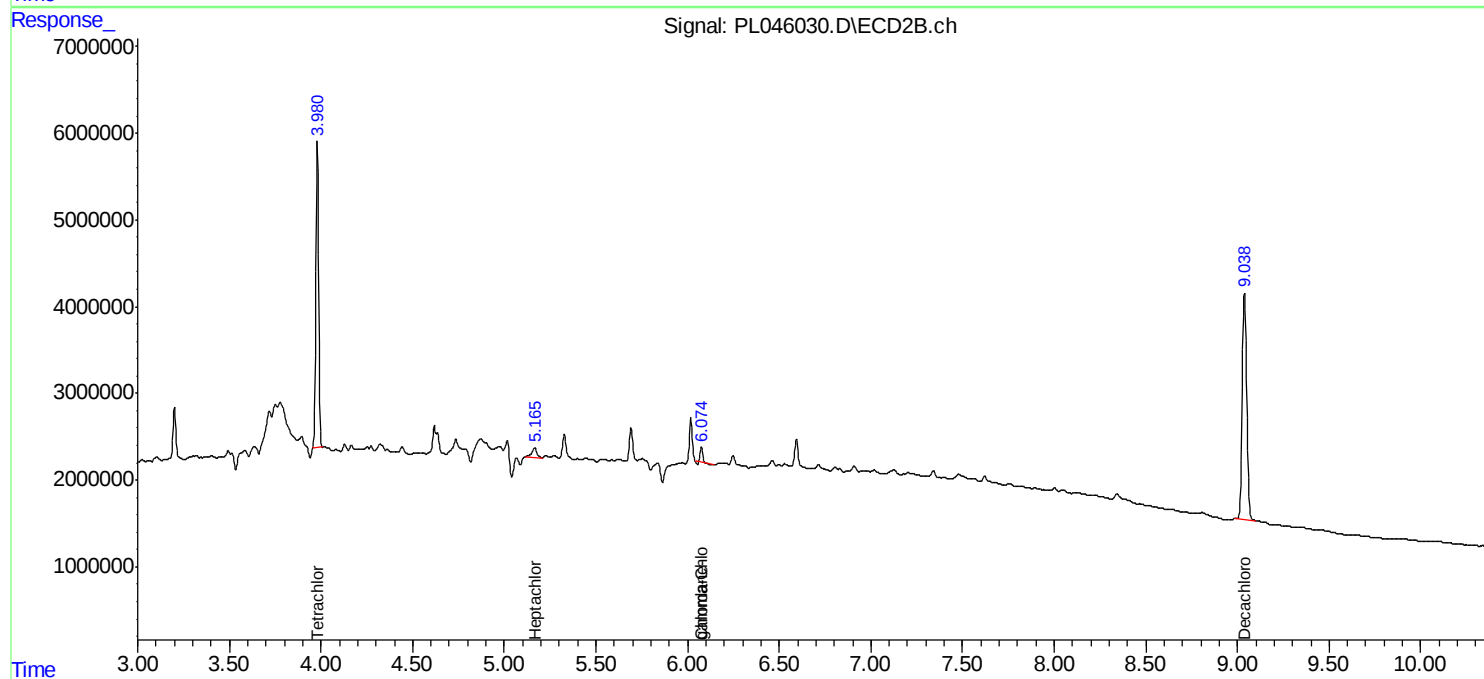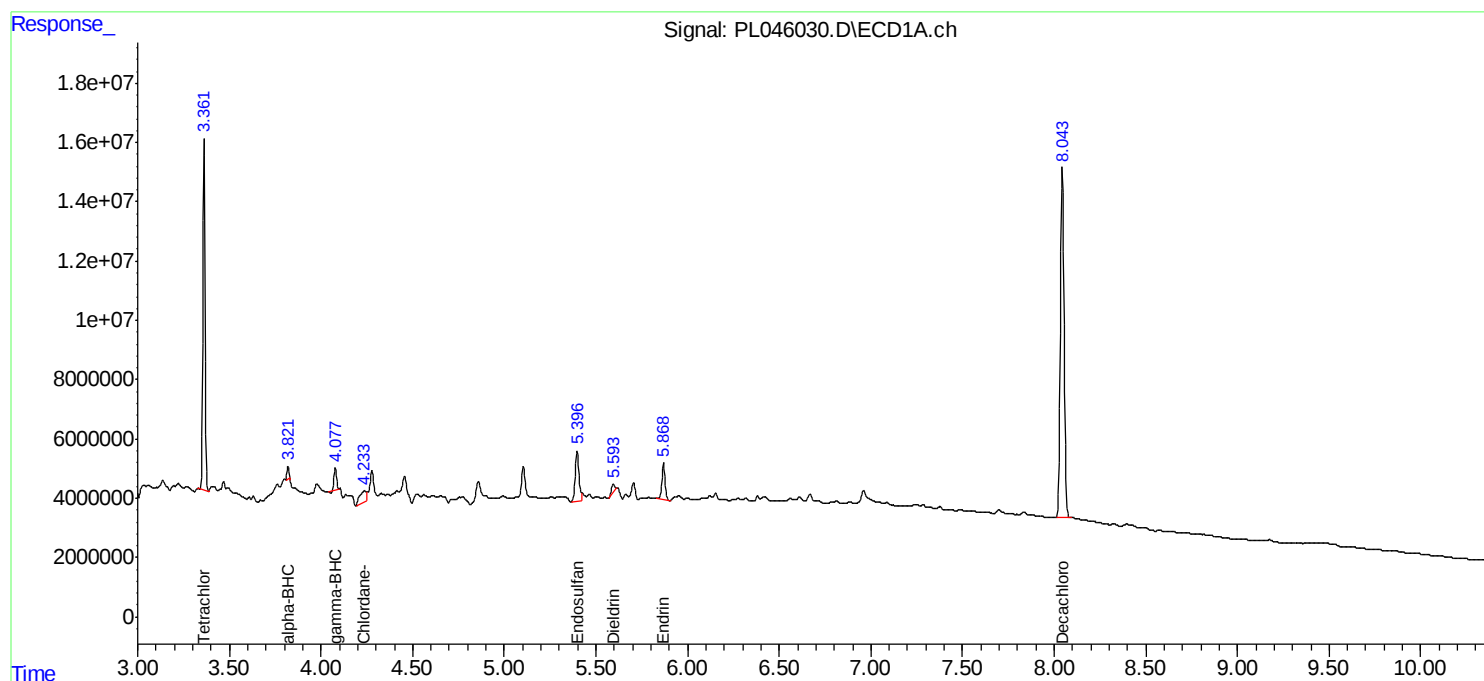


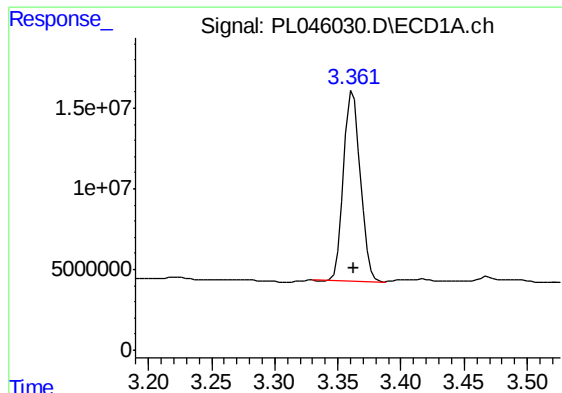

#1 Tetrachloro-m-xylene


R.T.: 3.362 min
Delta R.T.: 0.000 min
Response: 109083927
Conc: 15.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
RBR200051

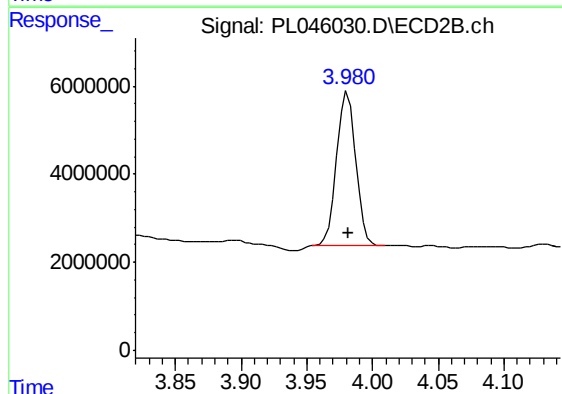


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 35413475
Conc: 16.54 ng/ml

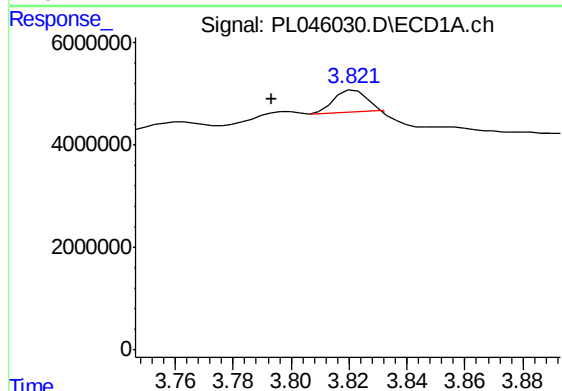


#2 alpha-BHC

R.T.: 3.822 min
Delta R.T.: 0.028 min
Response: 3470193
Conc: 0.31 ng/ml

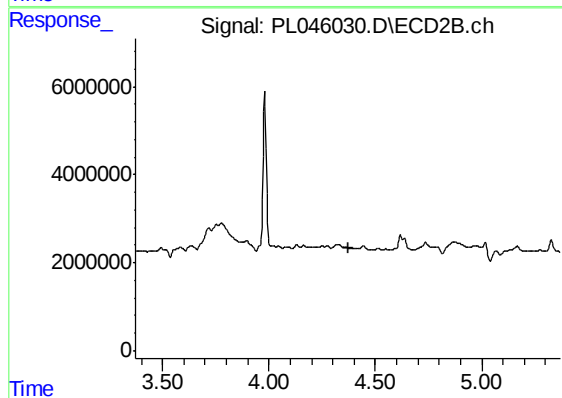

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.371 min
Response: 0
Conc: N.D.

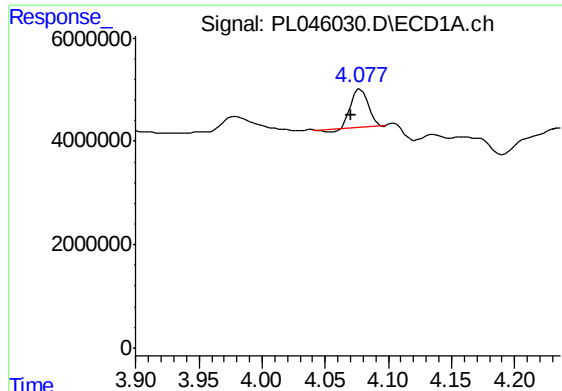

#3 gamma-BHC (Lindane)


R.T.: 4.078 min
Delta R.T.: 0.007 min
Response: 6709656
Conc: 0.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
RBR200051

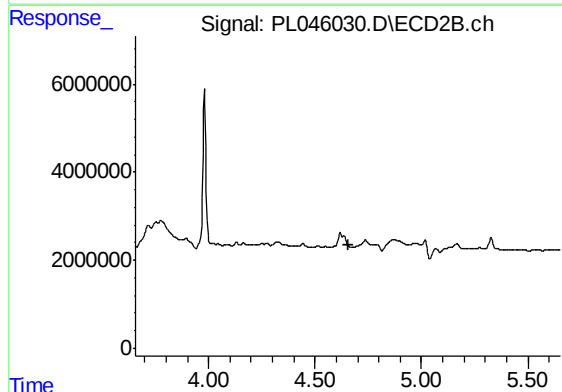


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.656 min
Response: 0
Conc: N.D.

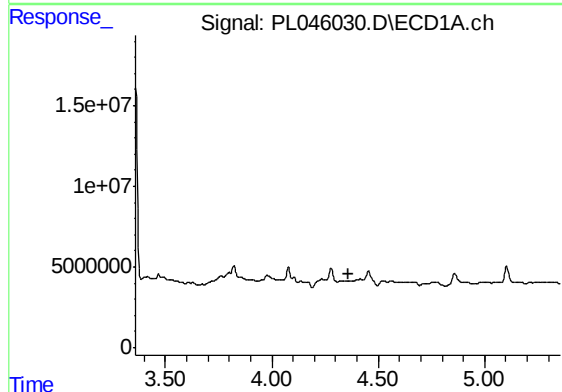


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.358 min
Response: 0
Conc: N.D.

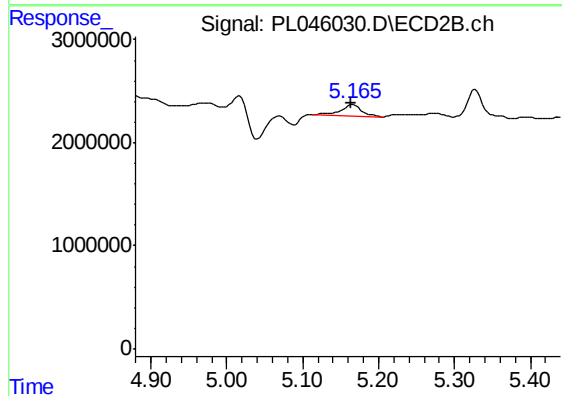

#4 Heptachlor


R.T.: 5.167 min
Delta R.T.: 0.003 min
Response: 2168059
Conc: 0.73 ng/ml

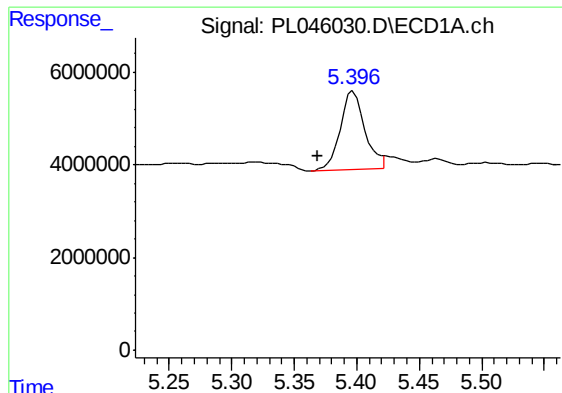

#9 Endosulfan I


R.T.: 5.397 min
Delta R.T.: 0.028 min
Response: 23202411
Conc: 2.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
RBR200051

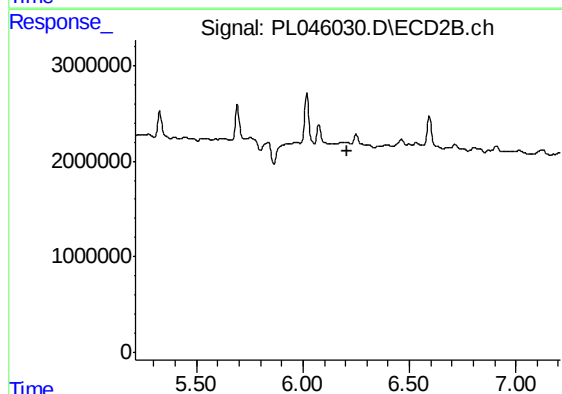


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.210 min
Response: 0
Conc: N.D.

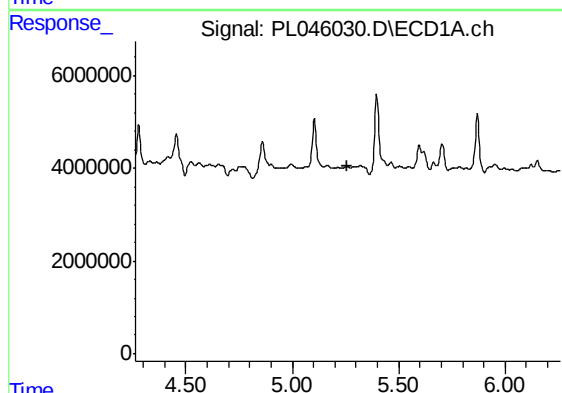


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.261 min
Response: 0
Conc: N.D.

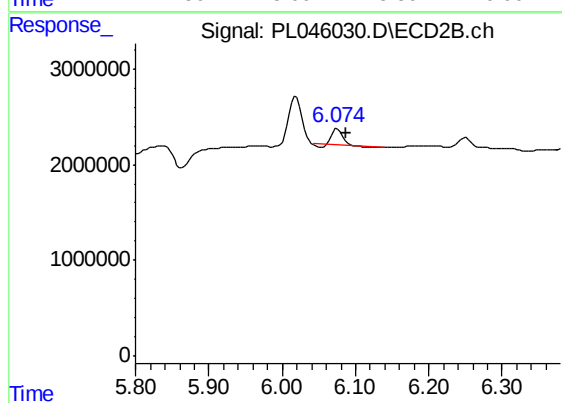

#10 gamma-Chlordane


R.T.: 6.075 min
Delta R.T.: -0.013 min
Response: 1544062
Conc: 0.58 ng/ml

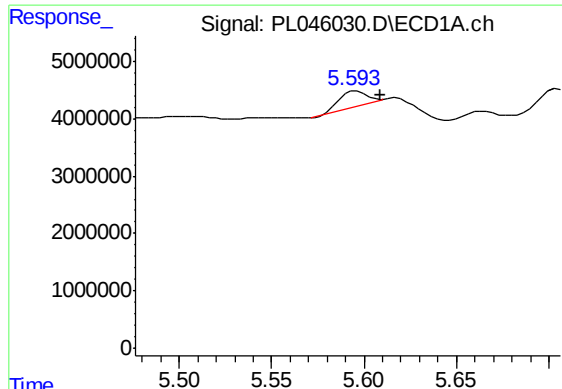

#13 Dieldrin


R.T.: 5.596 min
Delta R.T.: -0.013 min
Response: 2705162
Conc: 0.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
RBR200051

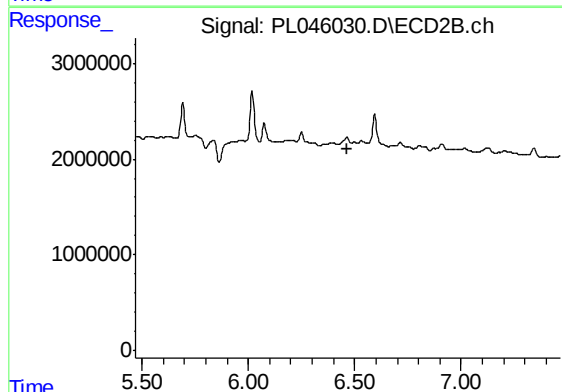


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.467 min
Response: 0
Conc: N.D.

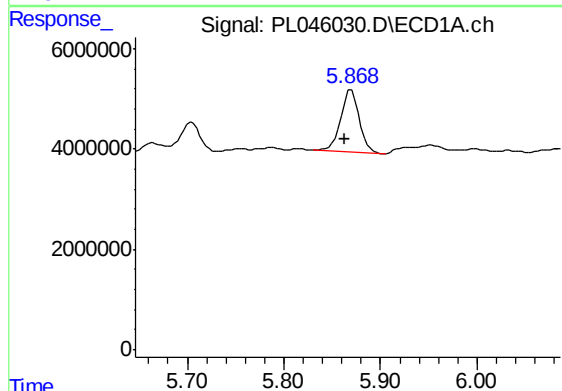


#14 Endrin

R.T.: 5.870 min
Delta R.T.: 0.007 min
Response: 16480380
Conc: 1.83 ng/ml

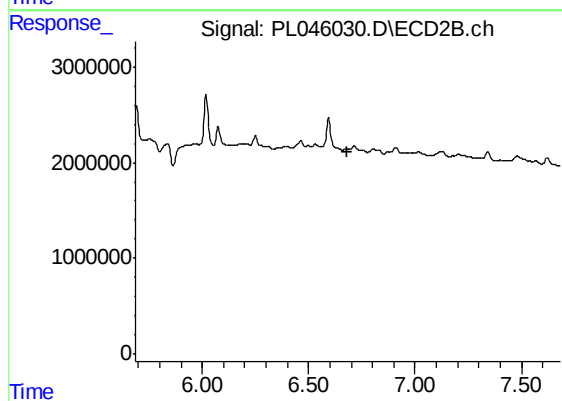

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.684 min
Response: 0
Conc: N.D.

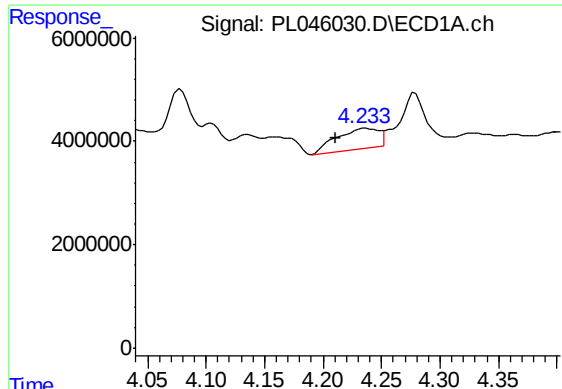

#23 Chlordane-1


R.T.: 4.236 min
Delta R.T.: 0.025 min
Response: 10010988
Conc: 29.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
RBR200051

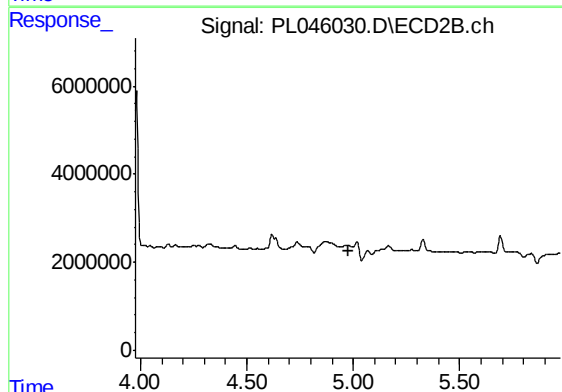


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.975 min
Response: 0
Conc: N.D.

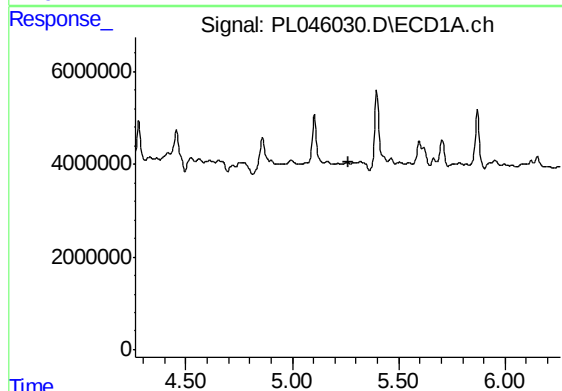


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.262 min
Response: 0
Conc: N.D.

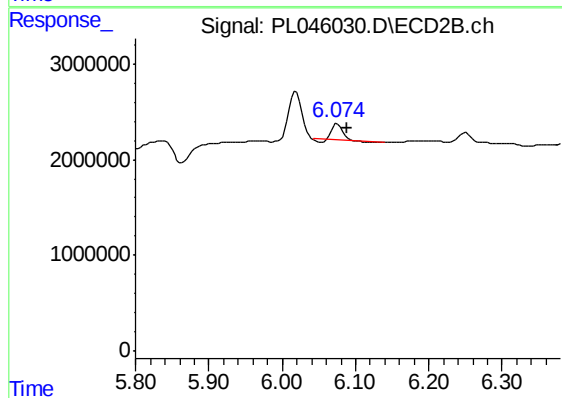

#25 Chlordane-3


R.T.: 6.075 min
Delta R.T.: -0.013 min
Response: 1544062
Conc: 3.96 ng/ml

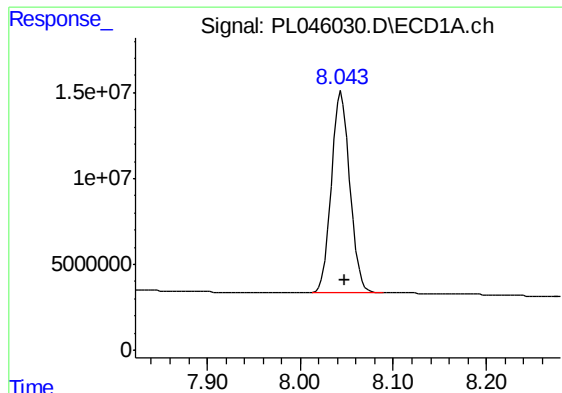

#28 Decachlorobiphenyl

R.T.: 8.044 min
Delta R.T.: -0.003 min
Response: 161179163
Conc: 19.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
RBR200051

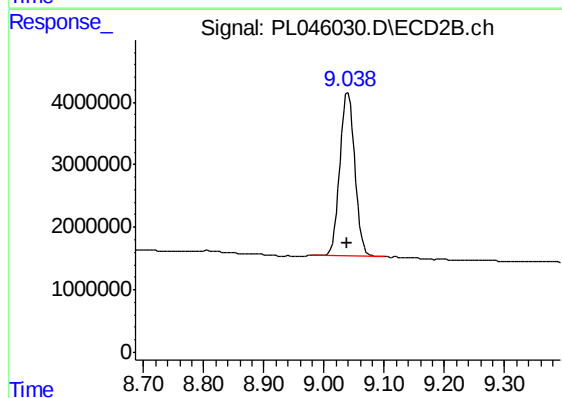

#28 Decachlorobiphenyl

R.T.: 9.040 min
Delta R.T.: 0.000 min
Response: 45289352
Conc: 19.82 ng/ml