

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031519\
 Data File : PL046026.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2019 01:14
 Operator : AJ\SJ
 Sample : K1897-04
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 01:44:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.362	3.982	131.3E6	41628105	19.082	19.438
28)	SA Decachlor...	8.044	9.040	162.1E6	48240999	19.369	21.113
Target Compounds							
13)	MA Dieldrin	5.607	6.467	11795111	3848103	1.234	1.497



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031519\
Data File : PL046026.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2019 01:14
Operator : AJ\SJ
Sample : K1897-04
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 01:44:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

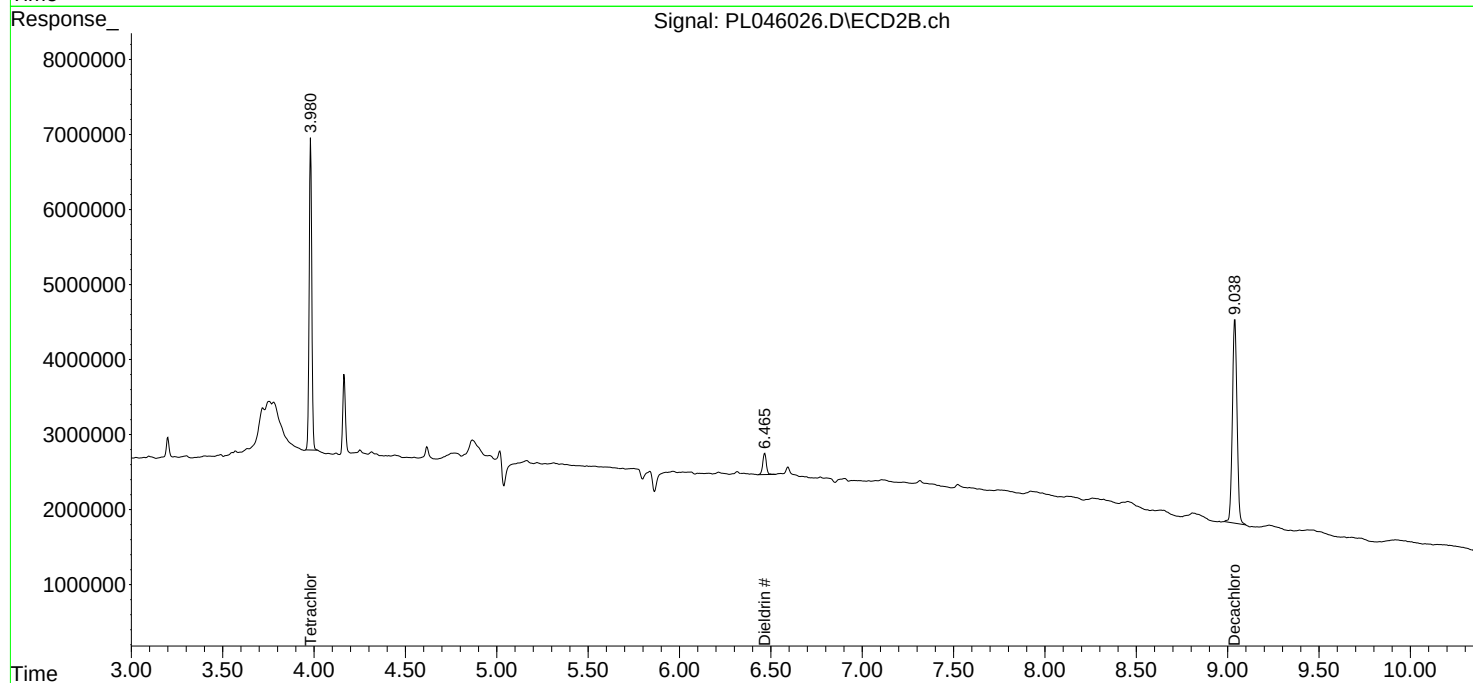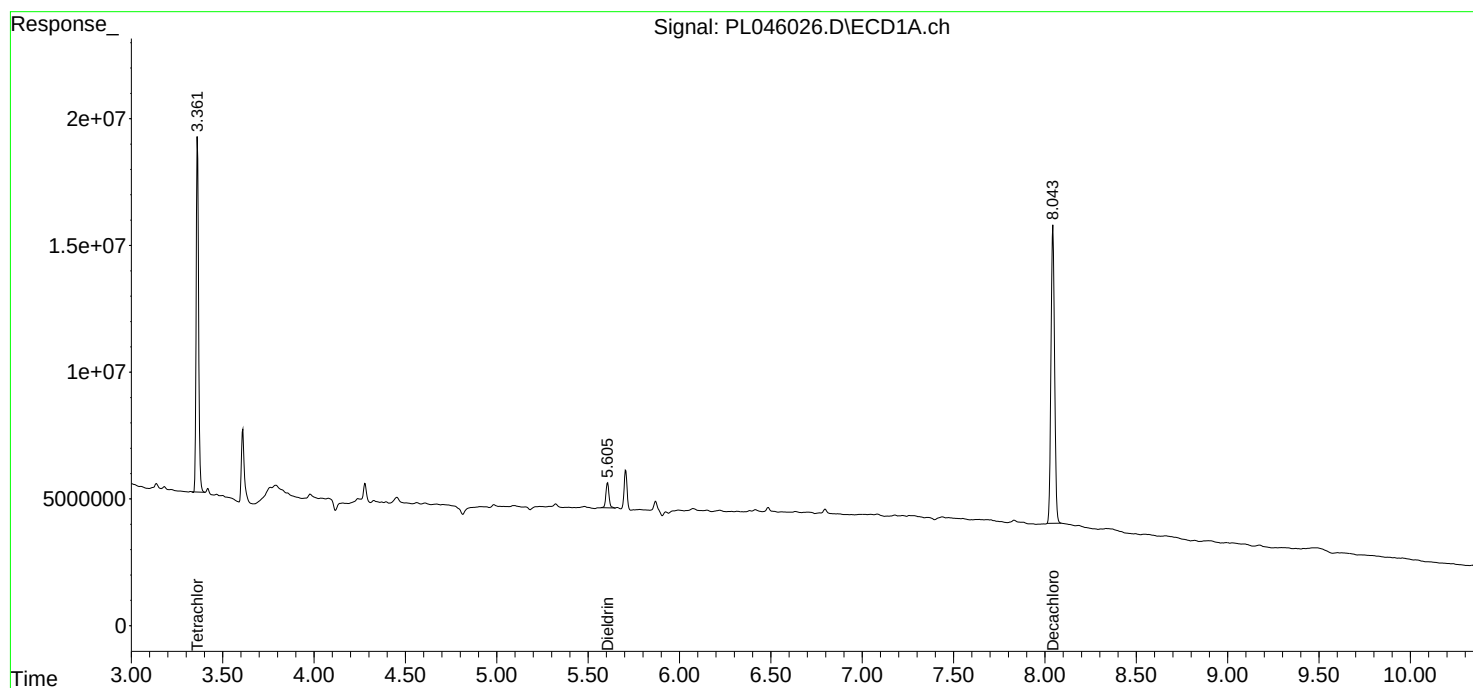


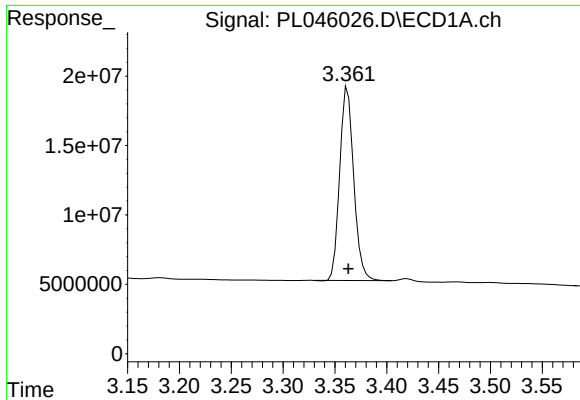

#1 Tetrachloro-m-xylene


R.T.: 3.362 min
Delta R.T.: 0.000 min
Response: 131270615
Conc: 19.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

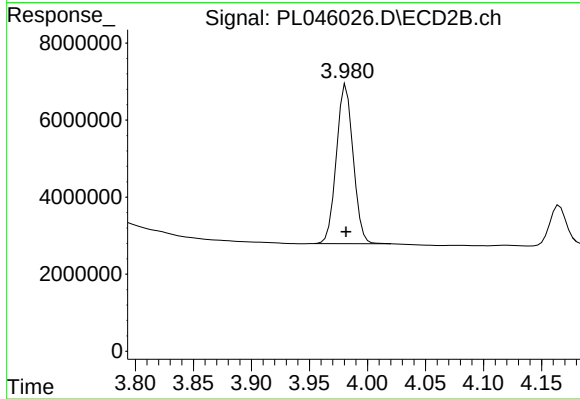


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 41628105
Conc: 19.44 ng/ml

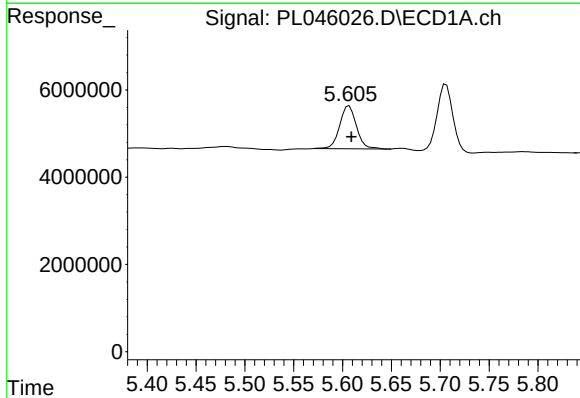


#13 Dieldrin

R.T.: 5.607 min
Delta R.T.: -0.002 min
Response: 11795111
Conc: 1.23 ng/ml

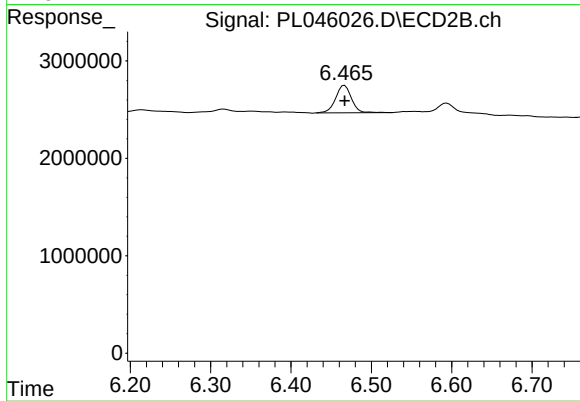

#13 Dieldrin

R.T.: 6.467 min
Delta R.T.: 0.000 min
Response: 3848103
Conc: 1.50 ng/ml

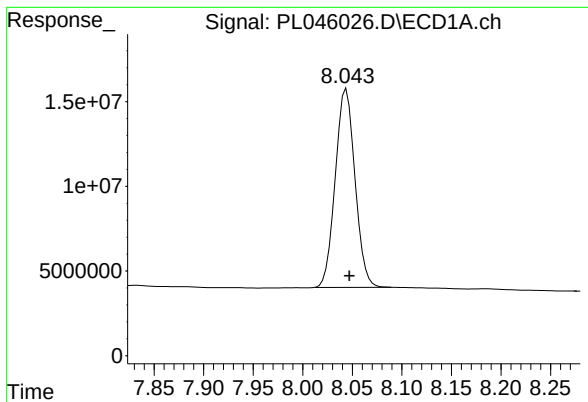

#28 Decachlorobiphenyl


R.T.: 8.044 min

Delta R.T.: -0.003 min

Response: 162071912

Conc: 19.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-1

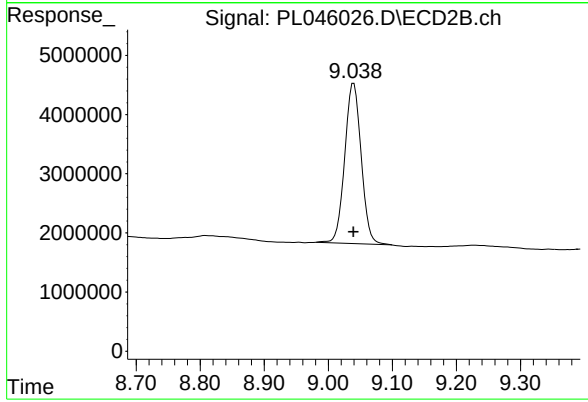

#28 Decachlorobiphenyl

R.T.: 9.040 min

Delta R.T.: 0.000 min

Response: 48240999

Conc: 21.11 ng/ml