

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031519\
 Data File : PL046054.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2019 09:03
 Operator : AJ\SJ
 Sample : K1930-14
 Misc :
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-6

Manual Integrations
 APPROVED

Sohil
 3/18/2019 11:40:53 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 01:22:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.362	3.981	114.5E6	35823372	16.642	16.728
28) SA Decachlor...	8.043	9.039	88816316	25928753	10.614	11.348
Target Compounds						
12) B 4,4'-DDE	5.481	6.317	14327468	4181221	1.632	1.790
17) MA 4,4'-DDT	6.226	7.104	4832519	1423824	0.644m	0.721m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031519\
Data File : PL046054.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2019 09:03
Operator : AJ\SJ
Sample : K1930-14
Misc :
ALS Vial : 75 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-6


Manual Integrations
APPROVED

Sohil
3/18/2019 11:40:53 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 01:22:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

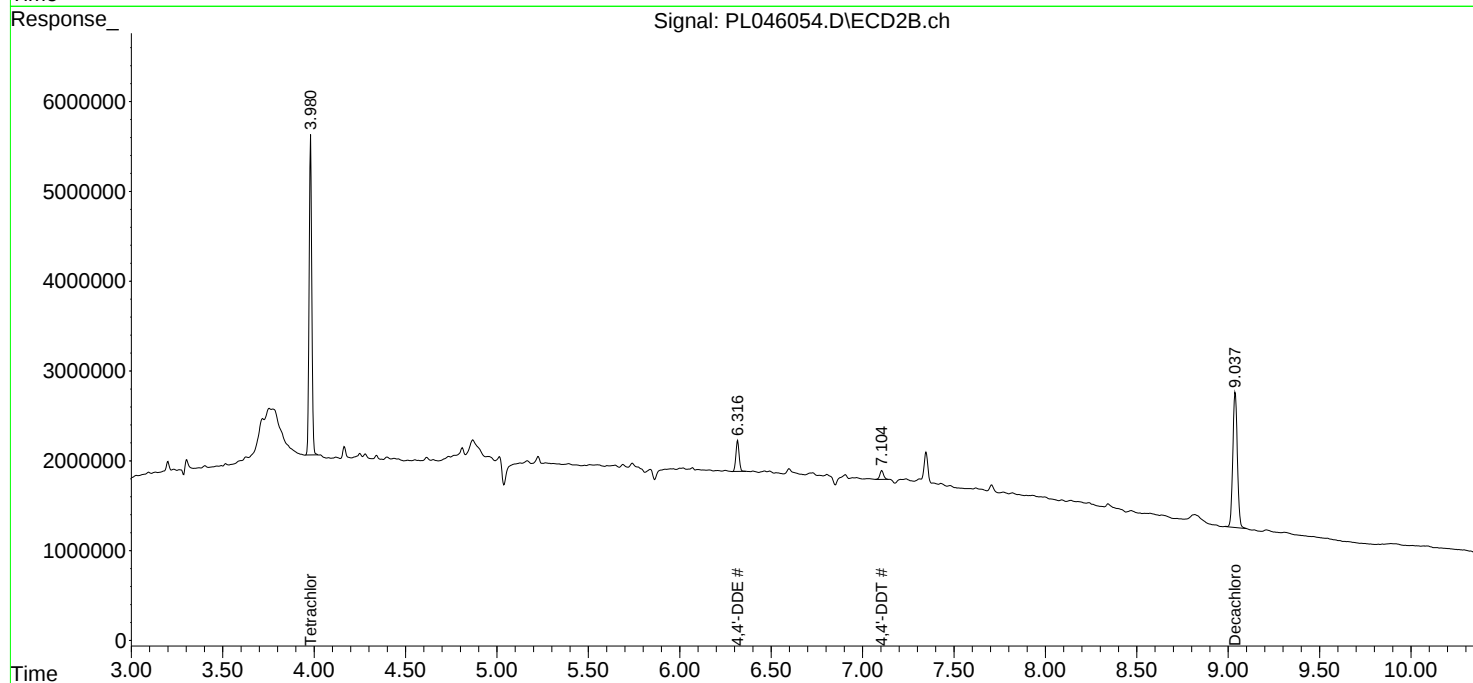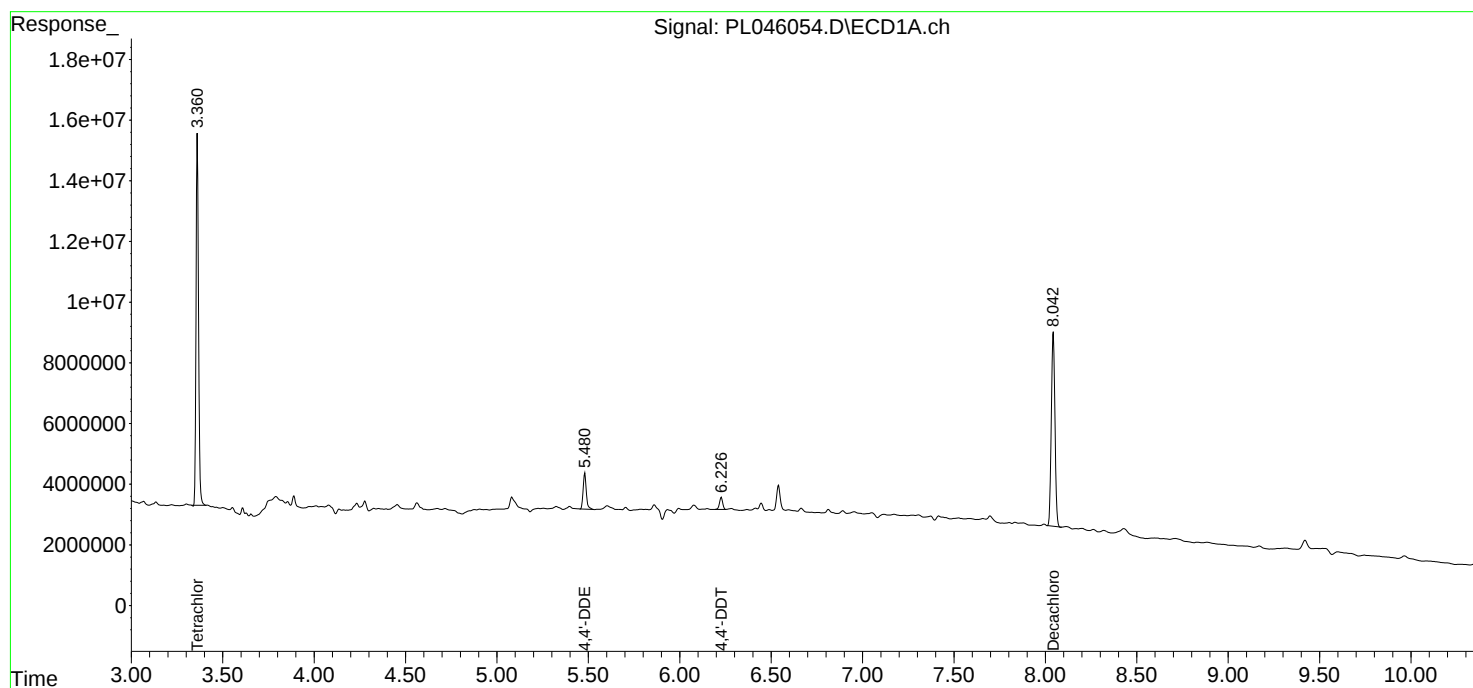

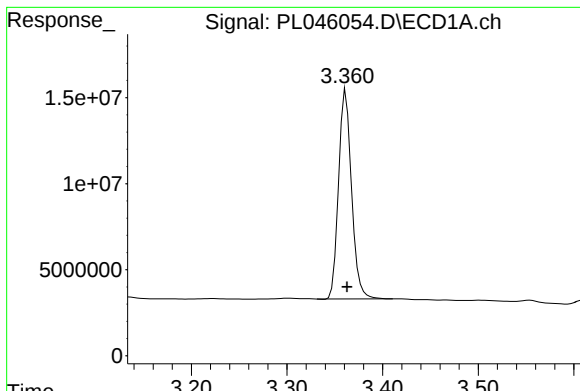


#1 Tetrachloro-m-xylene

R.T.: 3.362 min
Delta R.T.: -0.001 min
Response: 114488362
Conc: 16.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6


Manual Integrations
APPROVED

Sohil
3/18/2019 11:40:53 AM

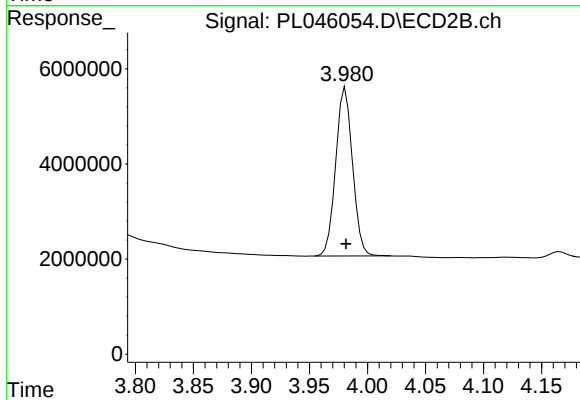


#1 Tetrachloro-m-xylene

R.T.: 3.981 min
Delta R.T.: 0.000 min
Response: 35823372
Conc: 16.73 ng/ml

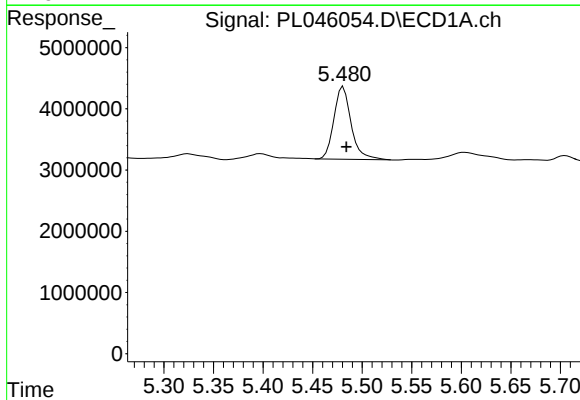


#12 4,4'-DDE

R.T.: 5.481 min
Delta R.T.: -0.003 min
Response: 14327468
Conc: 1.63 ng/ml

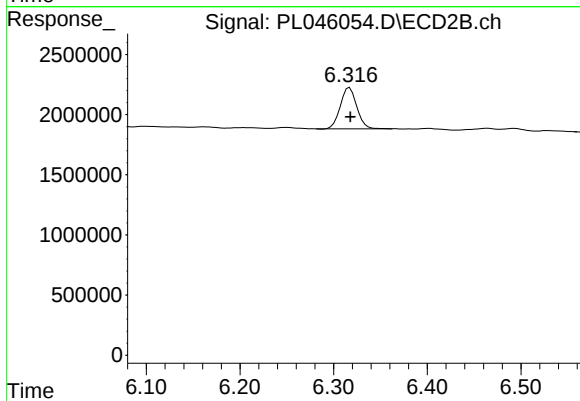

#12 4,4'-DDE

R.T.: 6.317 min
Delta R.T.: -0.001 min
Response: 4181221
Conc: 1.79 ng/ml

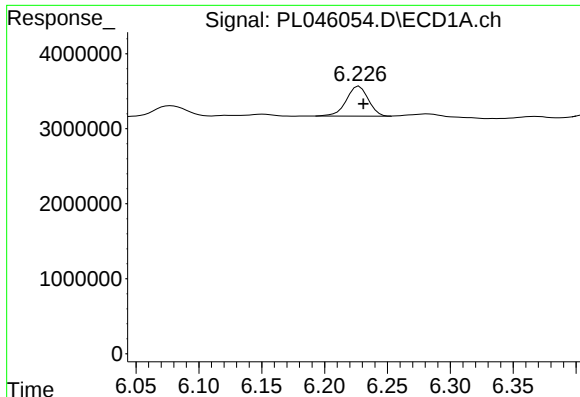


#17 4,4'-DDT

R.T.: 6.226 min
Delta R.T.: -0.005 min
Response: 4832519
Conc: 0.64 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-6


Manual Integrations
APPROVED

Sohil
3/18/2019 11:40:53 AM

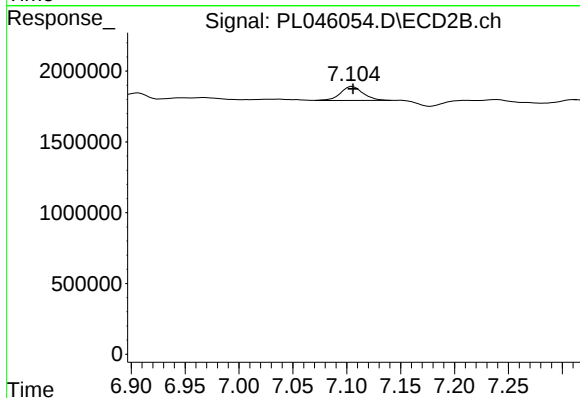


#17 4,4'-DDT

R.T.: 7.104 min
Delta R.T.: -0.002 min
Response: 1423824
Conc: 0.72 ng/ml m

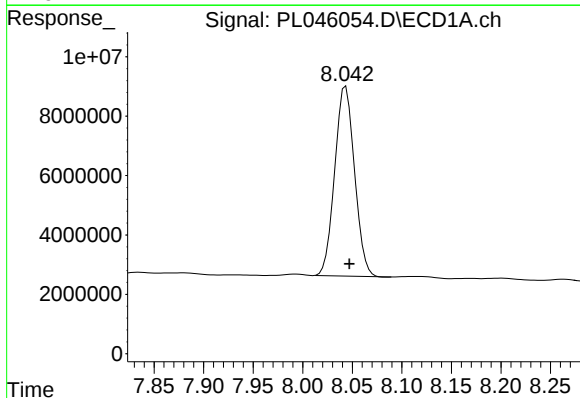

#28 Decachlorobiphenyl

R.T.: 8.043 min
Delta R.T.: -0.004 min
Response: 88816316
Conc: 10.61 ng/ml

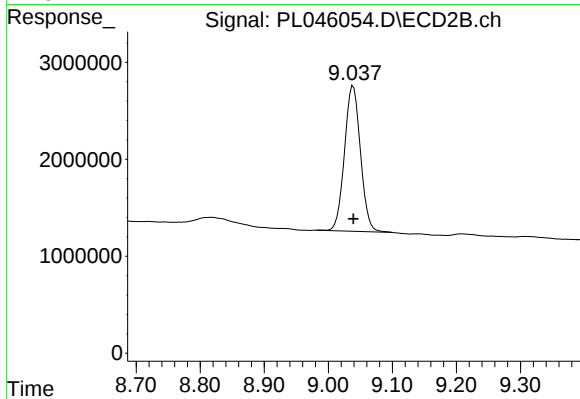

#28 Decachlorobiphenyl

R.T.: 9.039 min
Delta R.T.: 0.000 min
Response: 25928753
Conc: 11.35 ng/ml