

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031521\
 Data File : PL065297.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2021 09:25
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 02:04:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031321.M
 Quant Title : GC Extractables
 QLast Update : Sat Mar 13 01:11:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.294	3.885	49240431	59474389	20.900	21.592
28)	SA Decachlor...	7.939	8.895	45934792	39700836	21.316	21.610
Target Compounds							
6)	B beta-BHC	0.000	4.745	0	9360750	N.D.	5.363 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031521\
Data File : PL065297.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2021 09:25
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 02:04:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031321.M
Quant Title : GC Extractables
QLast Update : Sat Mar 13 01:11:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

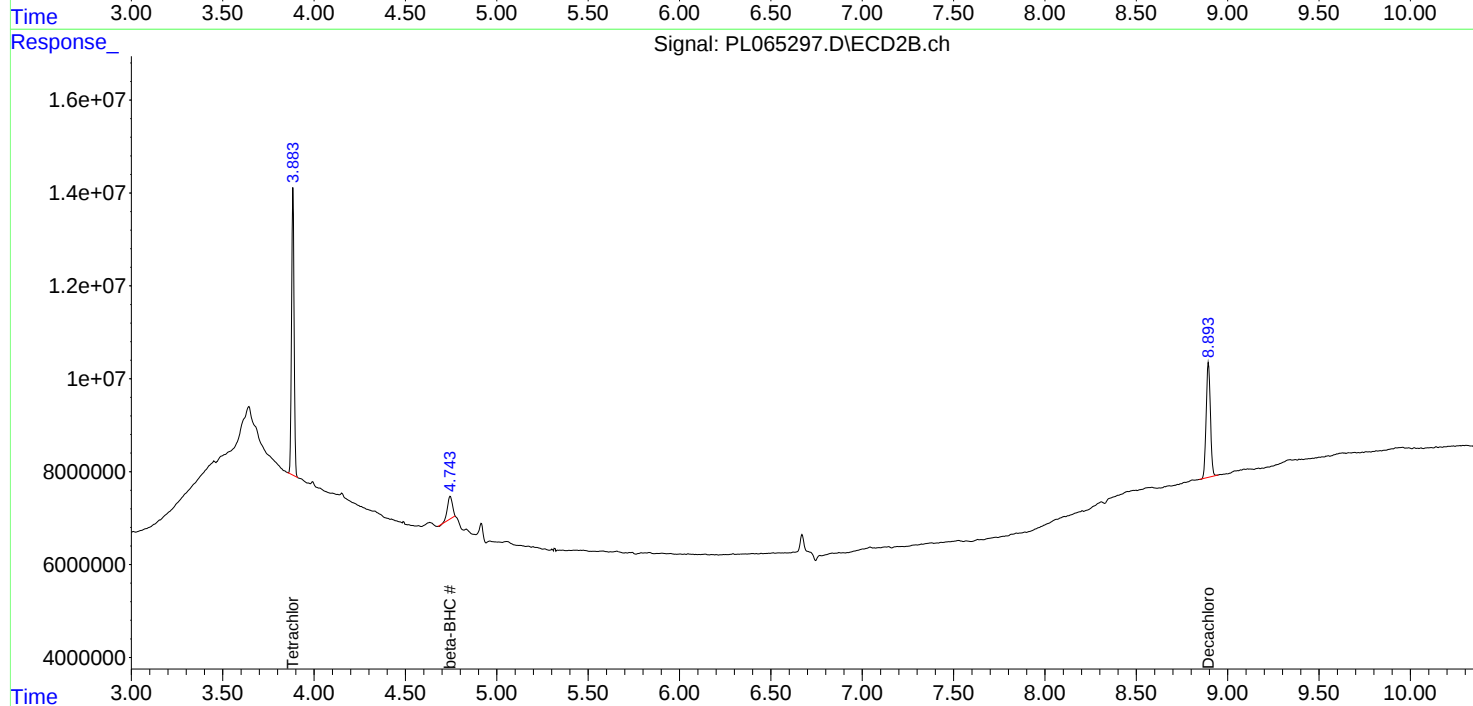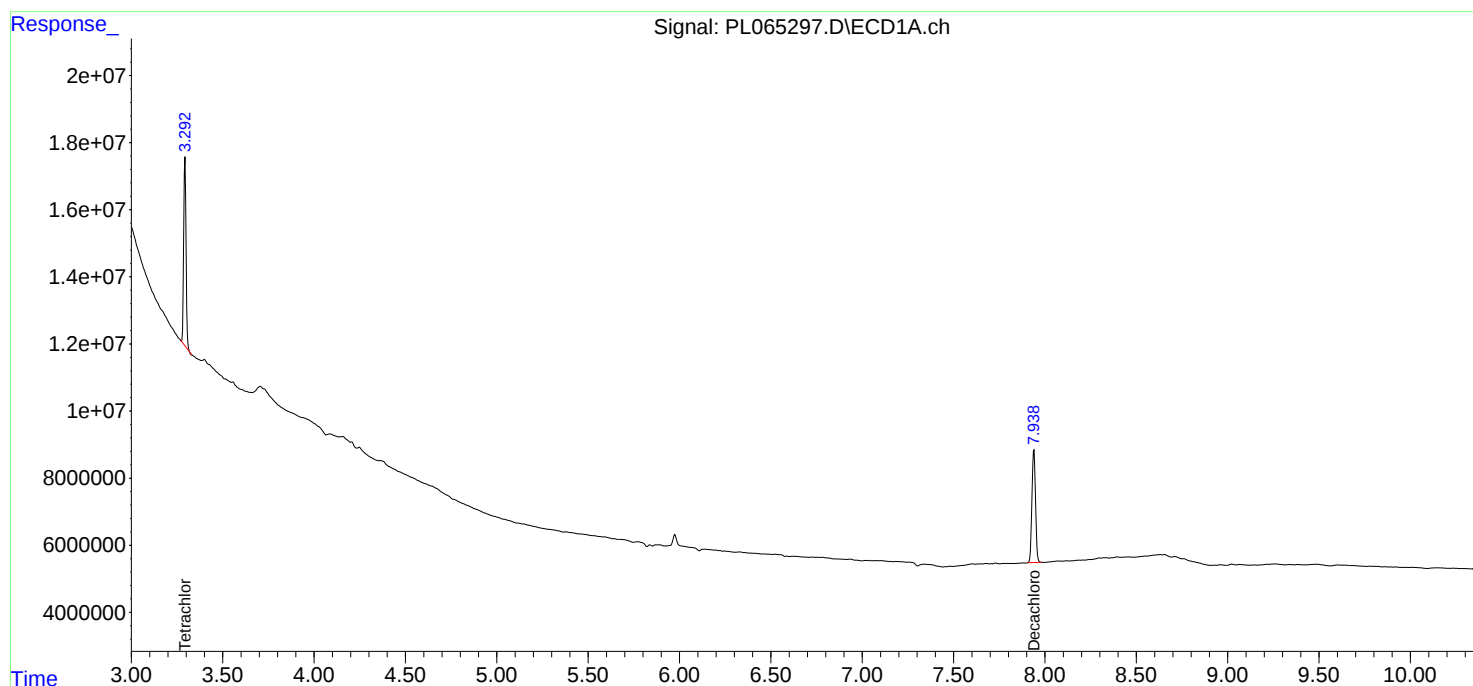


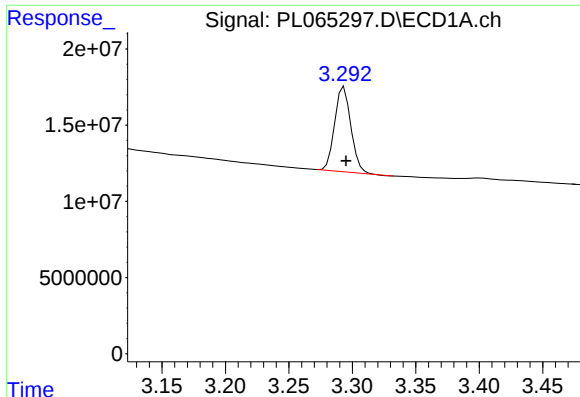

#1 Tetrachloro-m-xylene


R.T.: 3.294 min
Delta R.T.: -0.001 min
Response: 49240431
Conc: 20.90 ng/ml

Instrument :
ECD_L
ClientSampleId :

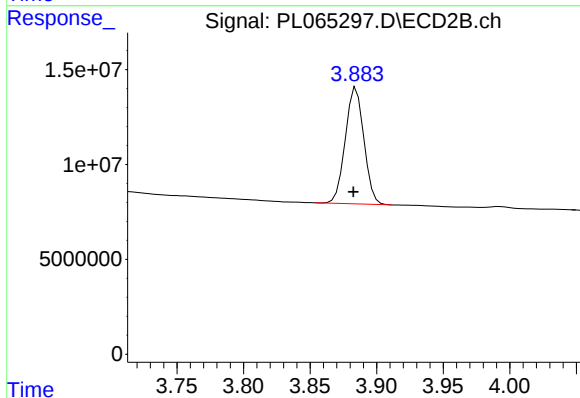


#1 Tetrachloro-m-xylene

R.T.: 3.885 min
Delta R.T.: 0.002 min
Response: 59474389
Conc: 21.59 ng/ml

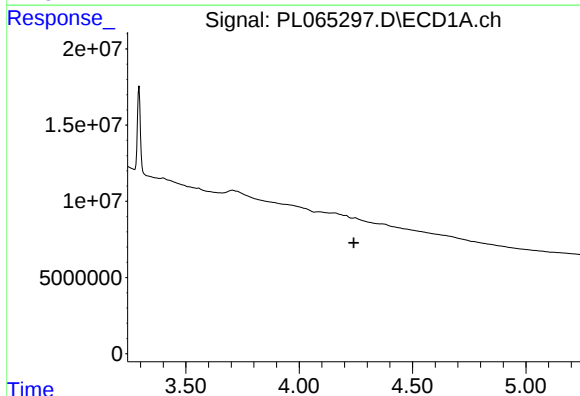


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.241 min
Response: 0
Conc: N.D.

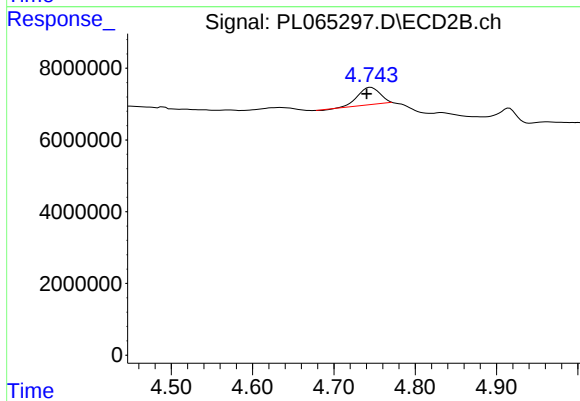

#6 beta-BHC


R.T.: 4.745 min
Delta R.T.: 0.005 min
Response: 9360750
Conc: 5.36 ng/ml

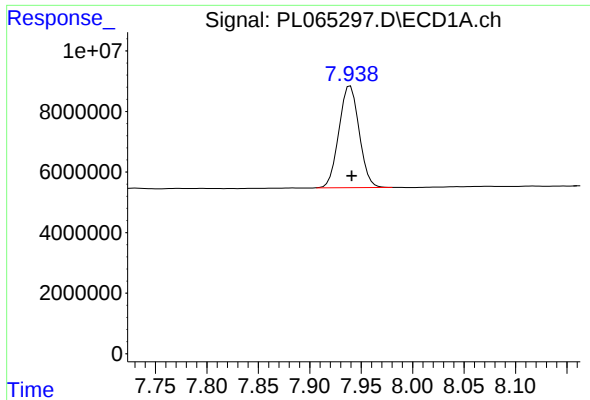

#28 Decachlorobiphenyl

R.T.: 7.939 min
Delta R.T.: -0.001 min
Response: 45934792
Conc: 21.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

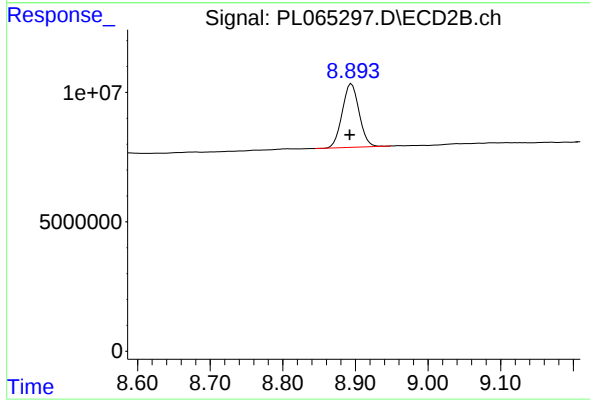

#28 Decachlorobiphenyl

R.T.: 8.895 min
Delta R.T.: 0.002 min
Response: 39700836
Conc: 21.61 ng/ml