

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031521\
 Data File : PL065303.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2021 14:46
 Operator : AR\AJ
 Sample : M1648-09
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP2-30802:05

Manual Integrations
 APPROVED

Ankita
 3/17/2021 4:35:34 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 12:28:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031321.M
 Quant Title : GC Extractables
 QLast Update : Sat Mar 13 01:11:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.294	3.884	37401715	56256972	15.875	20.424m#
28)	SA Decachlor...	7.939	8.893	24619469	20549045	11.425	11.185
Target Compounds							
15)	B Endosulfa...	6.035	6.797	4477402	2269601	1.827m	1.016m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031521\
Data File : PL065303.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2021 14:46
Operator : AR\AJ
Sample : M1648-09
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
COMP2-30802:05


Manual Integrations
APPROVED

Ankita
3/17/2021 4:35:34 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 12:28:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031321.M
Quant Title : GC Extractables
QLast Update : Sat Mar 13 01:11:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

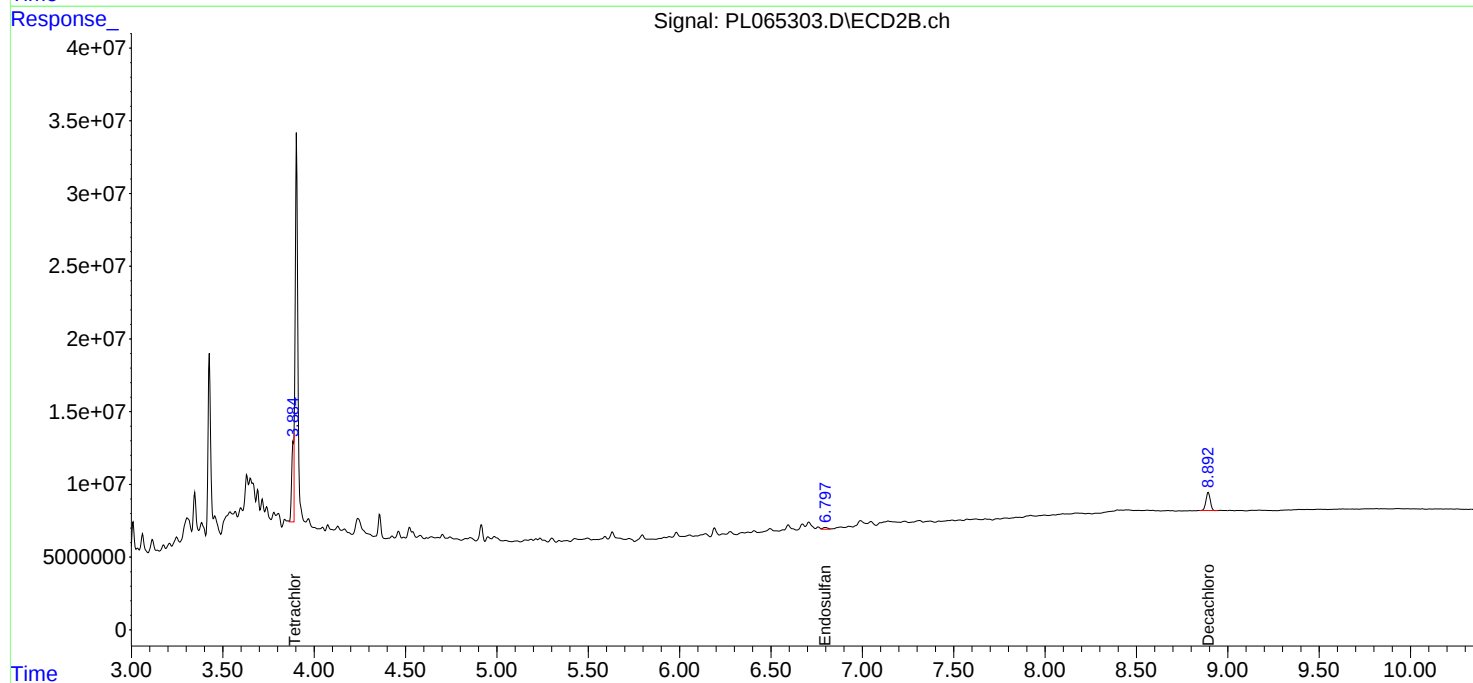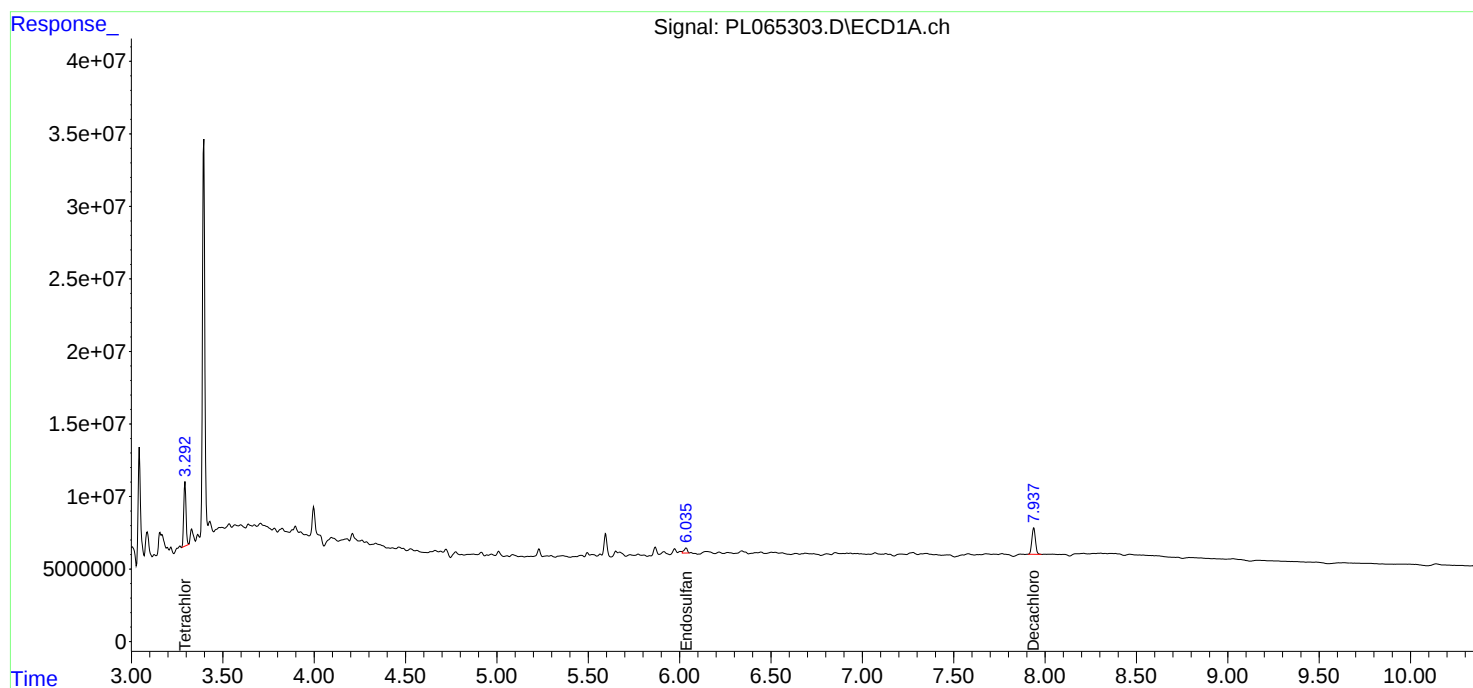

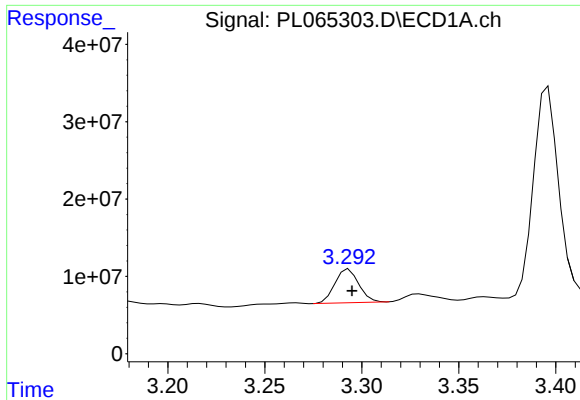


#1 Tetrachloro-m-xylene

R.T.: 3.294 min
Delta R.T.: -0.001 min
Response: 37401715
Conc: 15.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP2-30802:05


Manual Integrations
APPROVED

Ankita
3/17/2021 4:35:34 PM

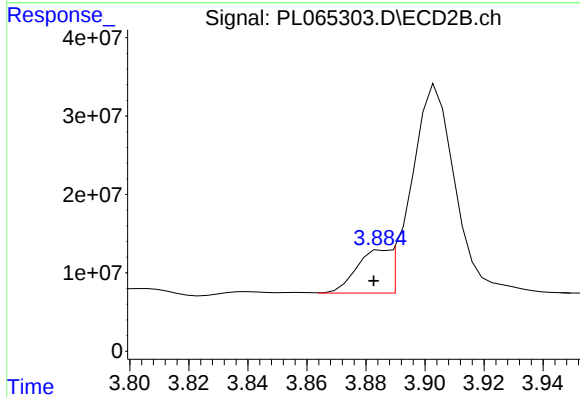


#1 Tetrachloro-m-xylene

R.T.: 3.884 min
Delta R.T.: 0.001 min
Response: 56256972
Conc: 20.42 ng/ml m

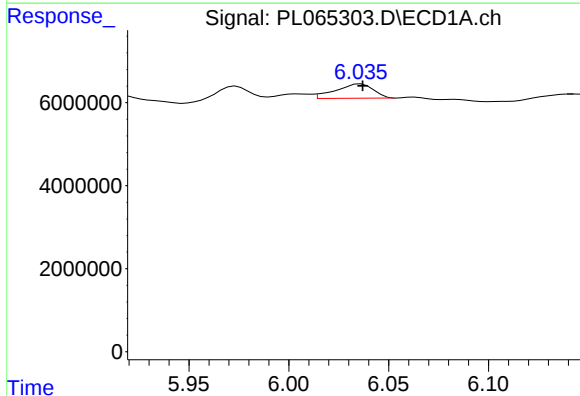


#15 Endosulfan II

R.T.: 6.035 min
Delta R.T.: -0.002 min
Response: 4477402
Conc: 1.83 ng/ml m

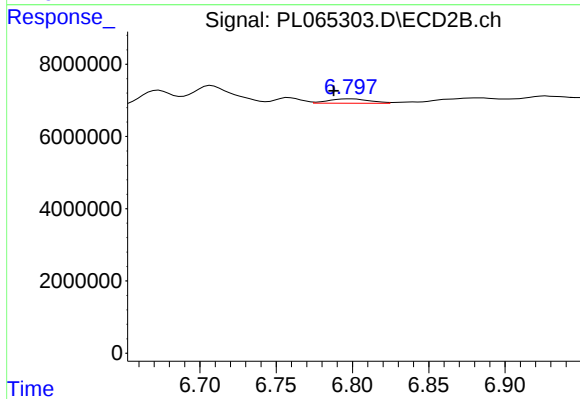

#15 Endosulfan II

R.T.: 6.797 min
Delta R.T.: 0.009 min
Response: 2269601
Conc: 1.02 ng/ml m

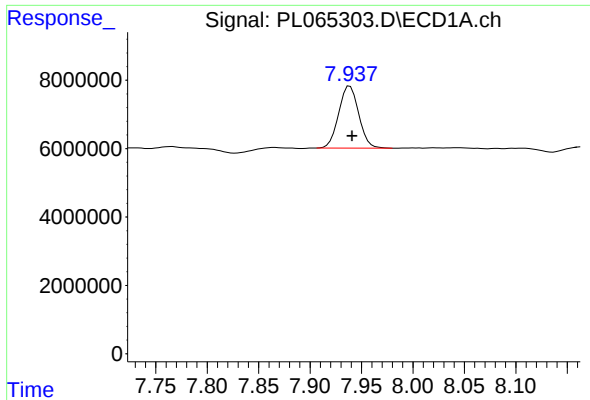


#28 Decachlorobiphenyl

R.T.: 7.939 min
Delta R.T.: -0.002 min
Response: 24619469
Conc: 11.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP2-30802:05

Manual Integrations
APPROVED

Ankita
3/17/2021 4:35:34 PM

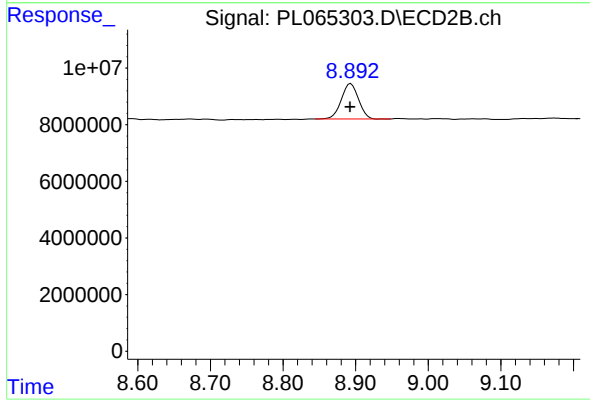

#28 Decachlorobiphenyl

R.T.: 8.893 min
Delta R.T.: 0.000 min
Response: 20549045
Conc: 11.19 ng/ml