

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031521\
 Data File : PL065307.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2021 15:42
 Operator : AR\AJ
 Sample : M1668-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CL-02-031221

Manual Integrations
 APPROVED

Ankita
 3/16/2021 11:13:29 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 02:07:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031321.M
 Quant Title : GC Extractables
 QLast Update : Sat Mar 13 01:11:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.293	3.884	26681066	32844268	11.325	11.924
28)	SA Decachlor...	7.938	8.893	29220445	25645650	13.560	13.959
Target Compounds							
11)	B alpha-Chl...	5.224	6.045	2012066	4778042	0.664m	1.641m#
12)	B 4,4'-DDE	5.391	6.205	1598574	3073375	0.540m	1.108m#
17)	MA 4,4'-DDT	6.128	6.994	1339975	1120732	0.691m	0.552m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031521\
Data File : PL065307.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2021 15:42
Operator : AR\AJ
Sample : M1668-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
CL-02-031221


Manual Integrations
APPROVED

Ankita
3/16/2021 11:13:29 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 02:07:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031321.M
Quant Title : GC Extractables
QLast Update : Sat Mar 13 01:11:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

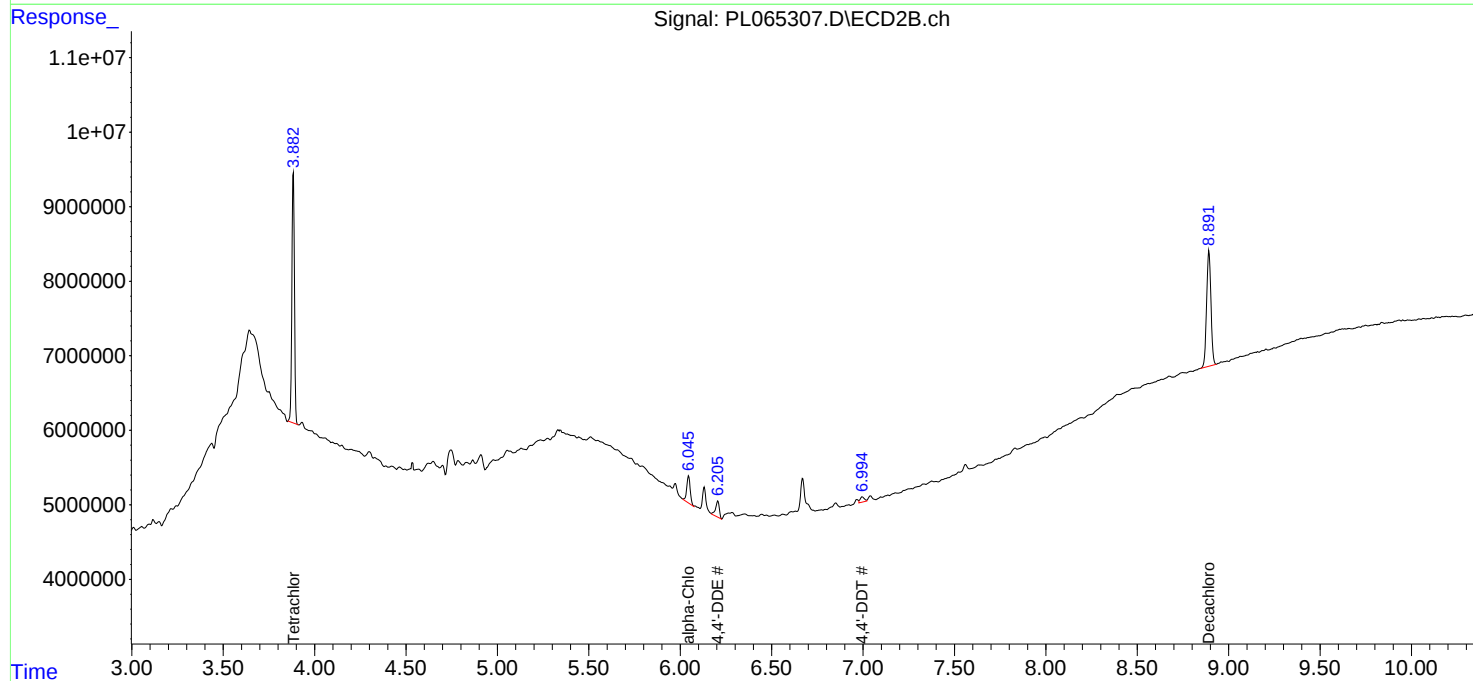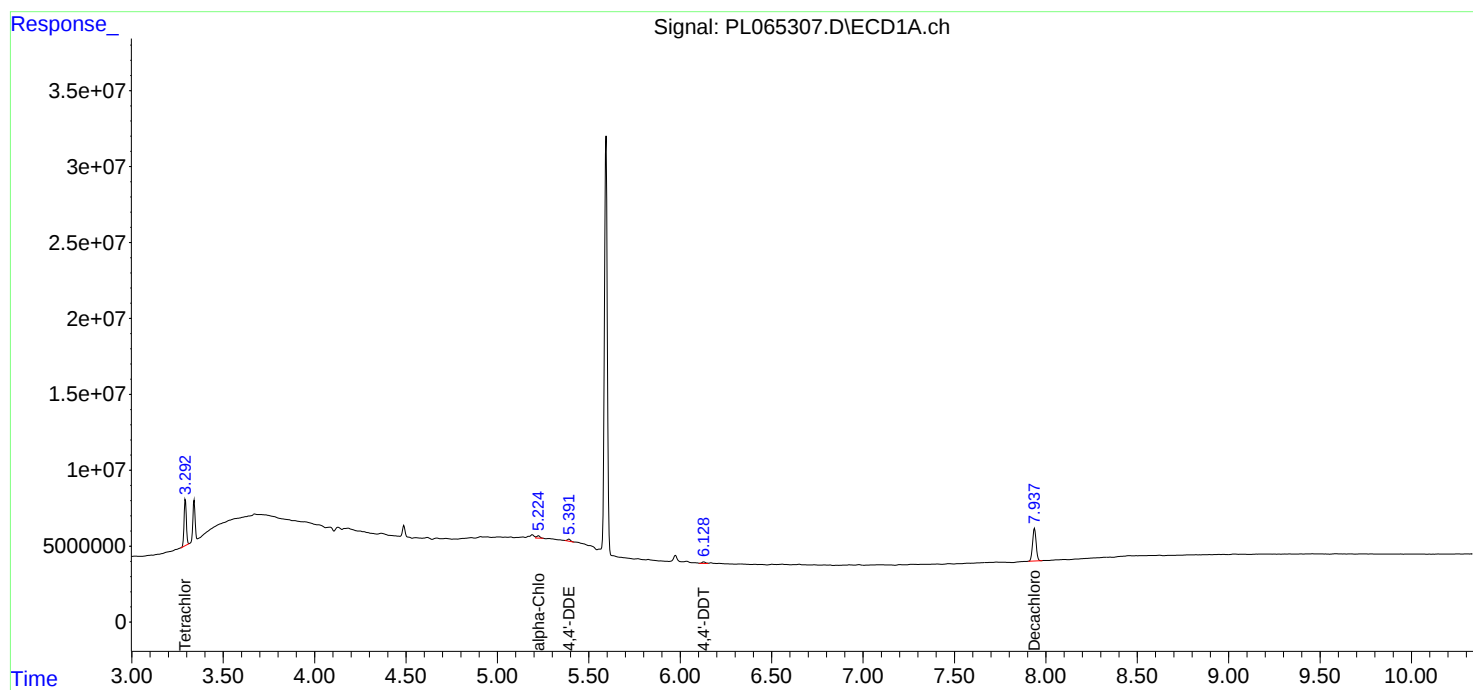

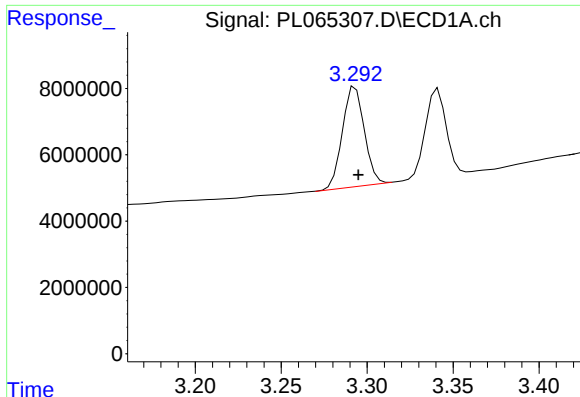


#1 Tetrachloro-m-xylene

R.T.: 3.293 min
Delta R.T.: -0.002 min
Response: 26681066
Conc: 11.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-031221


Manual Integrations
APPROVED

Ankita
3/16/2021 11:13:29 AM

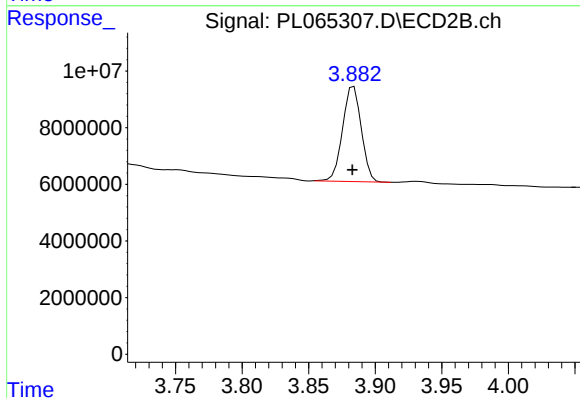


#1 Tetrachloro-m-xylene

R.T.: 3.884 min
Delta R.T.: 0.001 min
Response: 32844268
Conc: 11.92 ng/ml

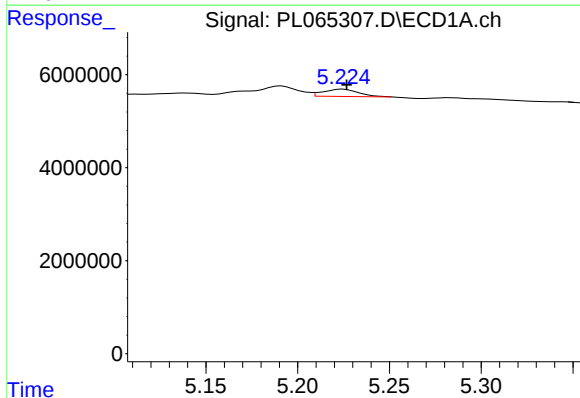


#11 alpha-Chlordane

R.T.: 5.224 min
Delta R.T.: -0.003 min
Response: 2012066
Conc: 0.66 ng/ml m

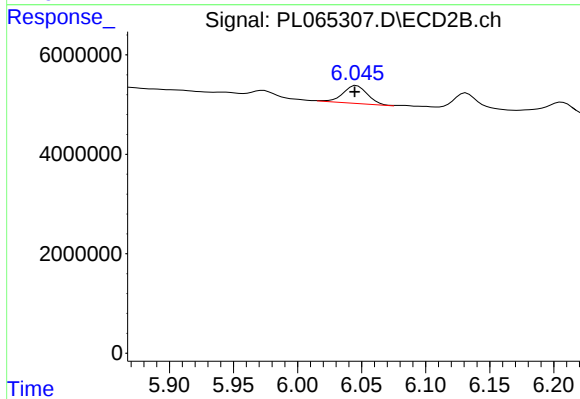

#11 alpha-Chlordane

R.T.: 6.045 min
Delta R.T.: 0.000 min
Response: 4778042
Conc: 1.64 ng/ml m

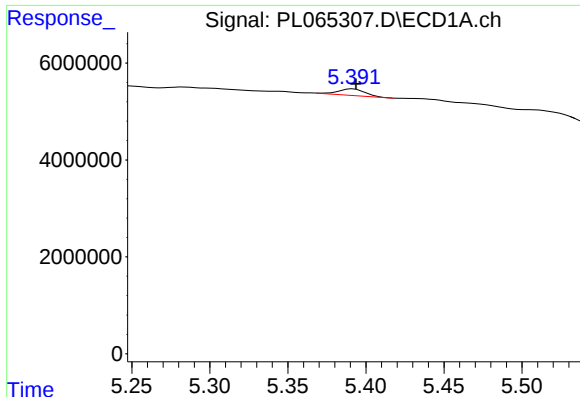


#12 4,4'-DDE

R.T.: 5.391 min
Delta R.T.: -0.003 min
Response: 1598574
Conc: 0.54 ng/ml m

Instrument :
ECD_L
ClientSampleId :
CL-02-031221


Manual Integrations
APPROVED

Ankita
3/16/2021 11:13:29 AM

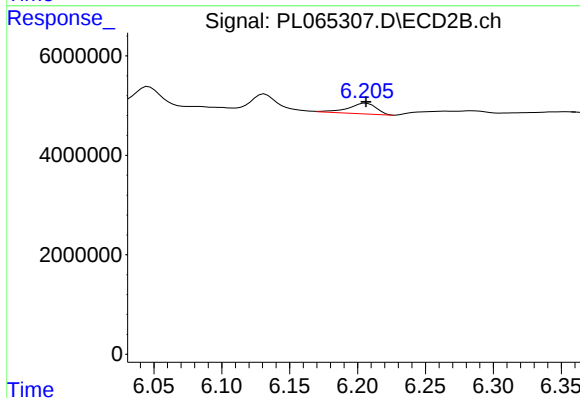


#12 4,4'-DDE

R.T.: 6.205 min
Delta R.T.: -0.001 min
Response: 3073375
Conc: 1.11 ng/ml m

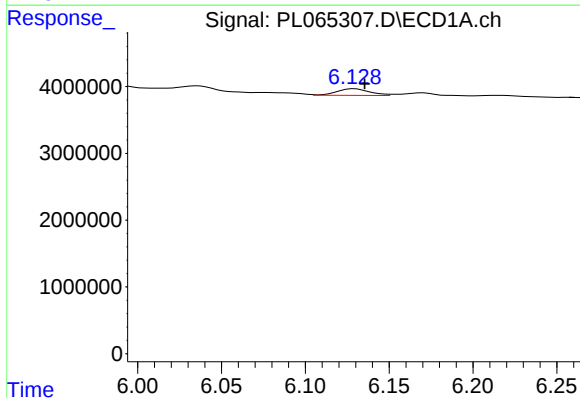


#17 4,4'-DDT

R.T.: 6.128 min
Delta R.T.: -0.007 min
Response: 1339975
Conc: 0.69 ng/ml m

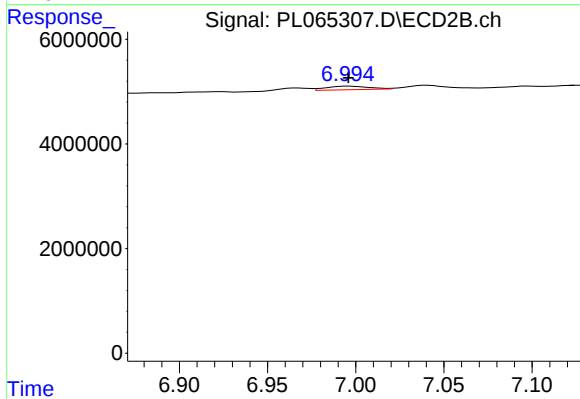

#17 4,4'-DDT

R.T.: 6.994 min
Delta R.T.: -0.002 min
Response: 1120732
Conc: 0.55 ng/ml m

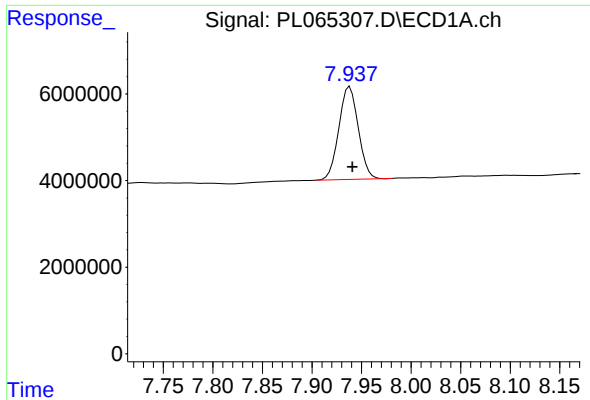


#28 Decachlorobiphenyl

R.T.: 7.938 min
Delta R.T.: -0.003 min
Response: 29220445
Conc: 13.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
CL-02-031221

Manual Integrations
APPROVED

Ankita
3/16/2021 11:13:29 AM

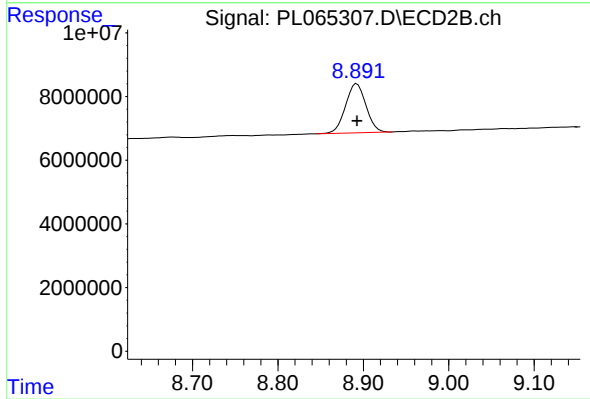

#28 Decachlorobiphenyl

R.T.: 8.893 min
Delta R.T.: 0.000 min
Response: 25645650
Conc: 13.96 ng/ml