

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031521\
 Data File : PL065315.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2021 17:37
 Operator : AR\AJ
 Sample : M1670-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HA-9A

Manual Integrations
 APPROVED

Ankita
 3/16/2021 11:13:35 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 18:43:17 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031321.M
 Quant Title : GC Extractables
 QLast Update : Sat Mar 13 01:11:50 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.294	3.883	28355046	34494762	12.035	12.523
28)	SA Decachlor...	7.938	8.893	15839687	13404950	7.351	7.296
Target Compounds							
17)	MA 4,4'-DDT	6.132	6.992	1828451	3209114	0.943m	1.581m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031521\
Data File : PL065315.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2021 17:37
Operator : AR\AJ
Sample : M1670-06
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
HA-9A


Manual Integrations
APPROVED

Ankita
3/16/2021 11:13:35 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 18:43:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031321.M
Quant Title : GC Extractables
QLast Update : Sat Mar 13 01:11:50 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

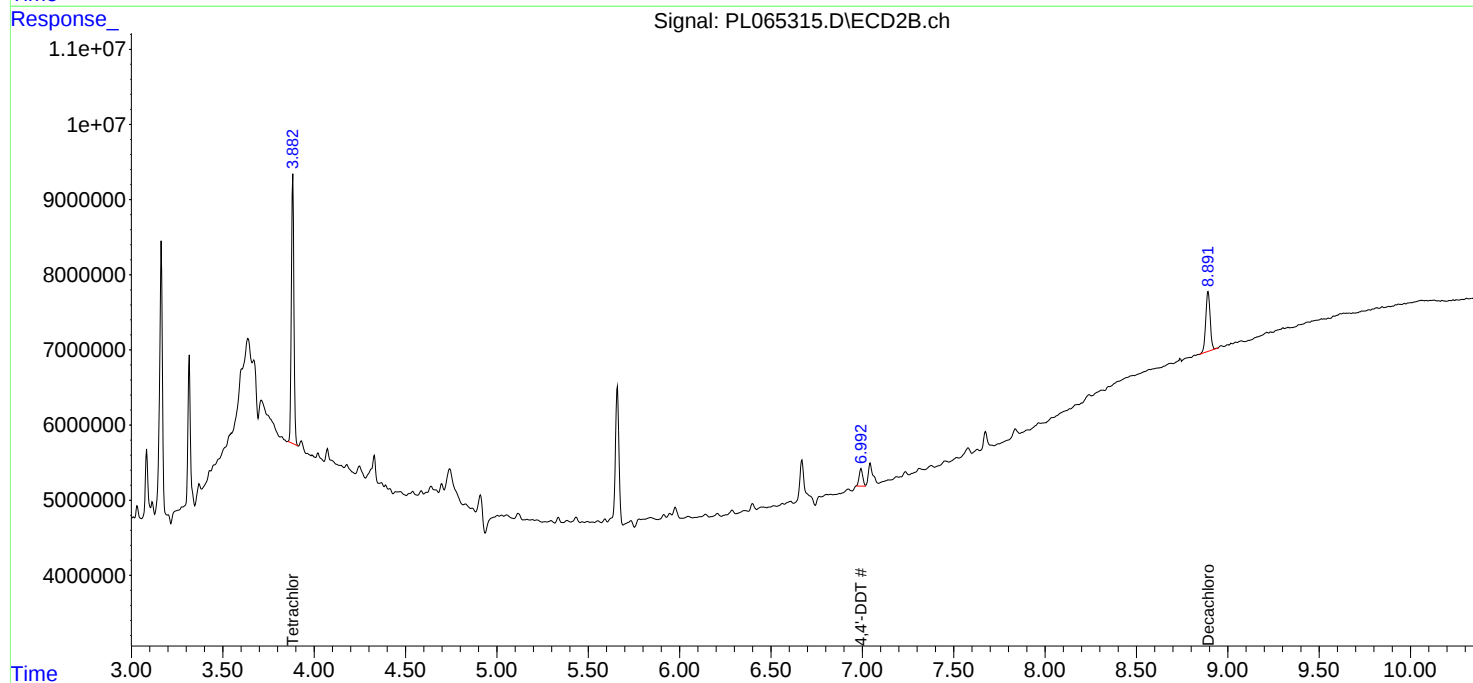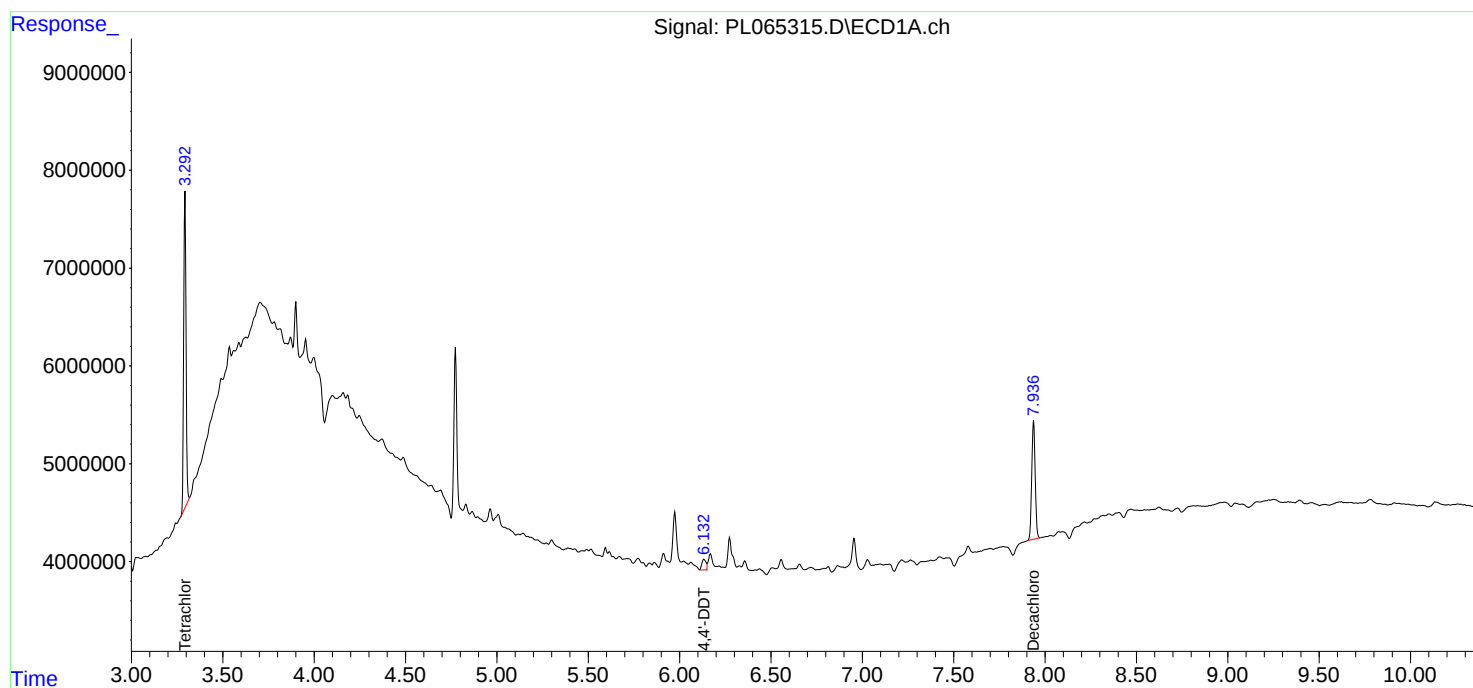

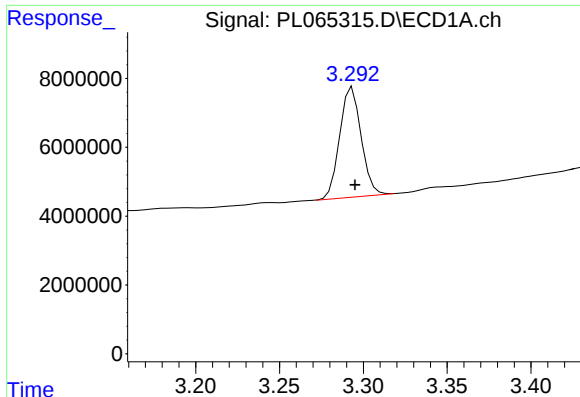


#1 Tetrachloro-m-xylene

R.T.: 3.294 min
Delta R.T.: -0.001 min
Response: 28355046
Conc: 12.04 ng/ml

Instrument :
ECD_L
ClientSampleId :
HA-9A


Manual Integrations
APPROVED

Ankita
3/16/2021 11:13:35 AM

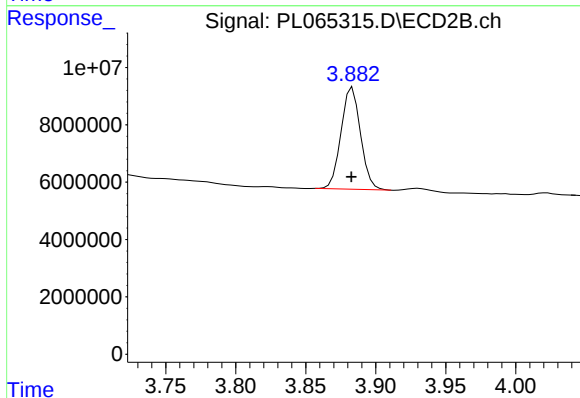


#1 Tetrachloro-m-xylene

R.T.: 3.883 min
Delta R.T.: 0.000 min
Response: 34494762
Conc: 12.52 ng/ml

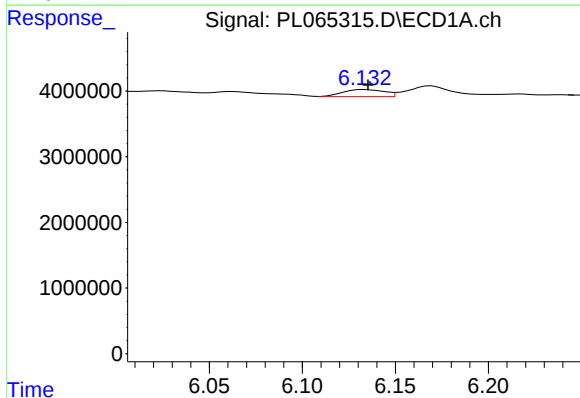


#17 4,4'-DDT

R.T.: 6.132 min
Delta R.T.: -0.003 min
Response: 1828451
Conc: 0.94 ng/ml m

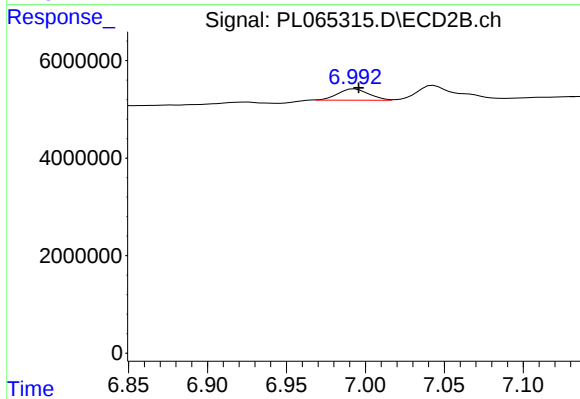

#17 4,4'-DDT

R.T.: 6.992 min
Delta R.T.: -0.004 min
Response: 3209114
Conc: 1.58 ng/ml m

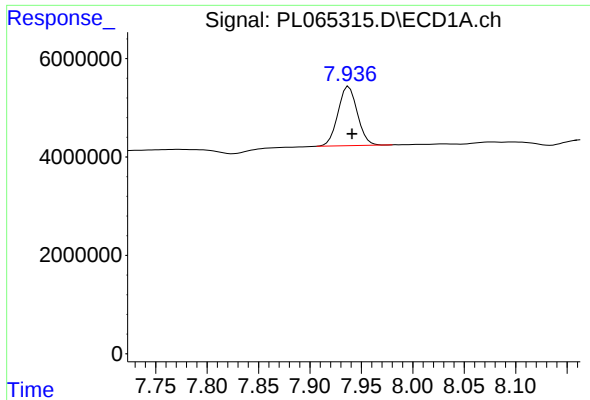


#28 Decachlorobiphenyl

R.T.: 7.938 min
Delta R.T.: -0.003 min
Response: 15839687
Conc: 7.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
HA-9A

Manual Integrations
APPROVED

Ankita
3/16/2021 11:13:35 AM

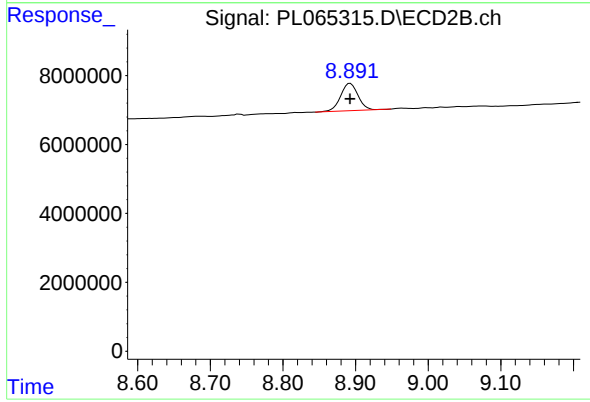

#28 Decachlorobiphenyl

R.T.: 8.893 min
Delta R.T.: 0.000 min
Response: 13404950
Conc: 7.30 ng/ml