

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031522\
 Data File : PL073403.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2022 16:51
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 03:34:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.646	5.491	6823966	35971898	21.306	21.917
28)	SA Decachlor...	10.419	11.332	10347114	37537875	20.348	20.992
Target Compounds							
6)	B beta-BHC	6.131f	6.664f	45882	464408	0.223	0.446 #
7)	B delta-BHC	0.000	6.958	0	1405070	N.D.	0.652 #
8)	B Heptachlo...	0.000	7.927	0	95444	N.D.	0.048 #
10)	B gamma-Chl...	7.343f	8.195	42986	1094701	0.098	0.536 #
14)	MA Endrin	8.093f	0.000	146212	0	0.377	N.D. #
15)	B Endosulfa...	8.352f	9.053f	165628	359110	0.424	0.234 #
16)	A 4,4'-DDD	0.000	9.001	0	234651	N.D.	0.161 #
17)	MA 4,4'-DDT	0.000	9.306	0	364157	N.D.	0.223 #
19)	B Endosulfa...	0.000	9.447	0	180549	N.D.	0.115 #
25)	Chlordane-3	7.343f	8.195	42986	1094701	1.053	4.038 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031522\
Data File : PL073403.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2022 16:51
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 03:34:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

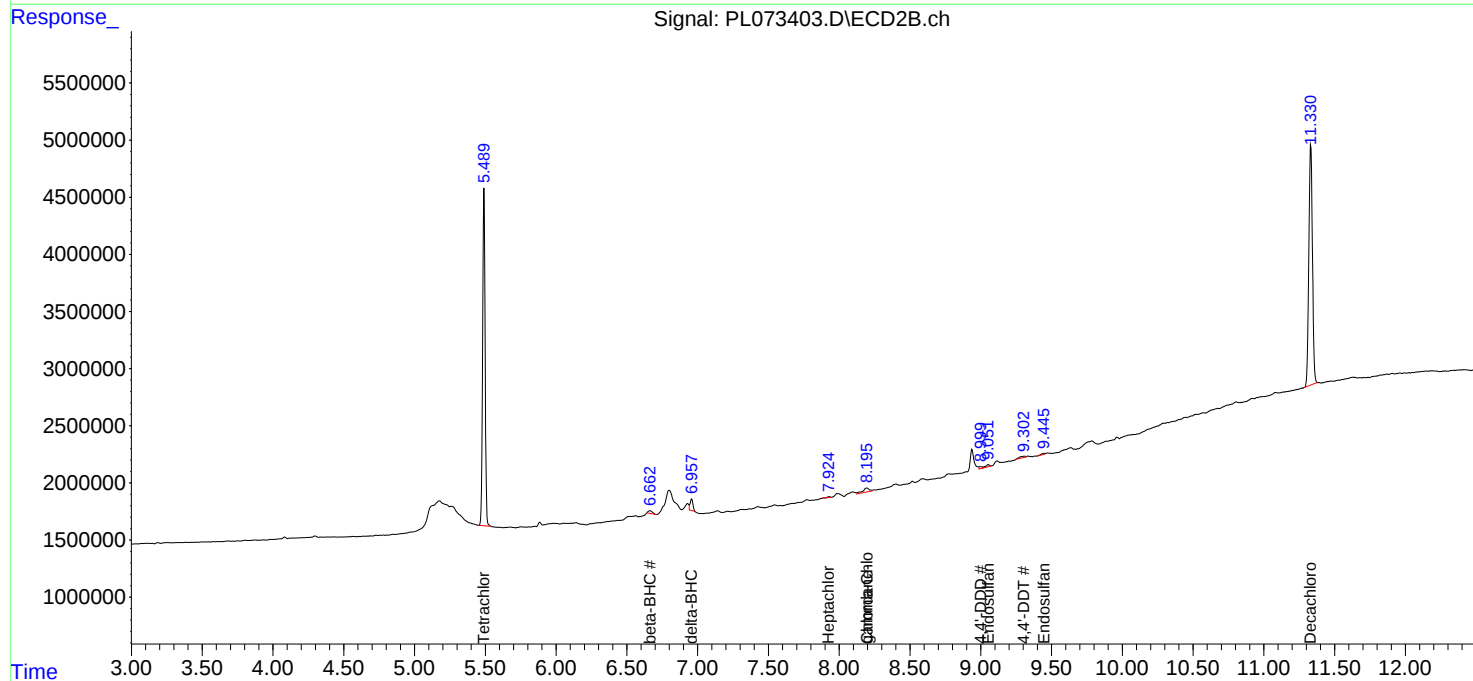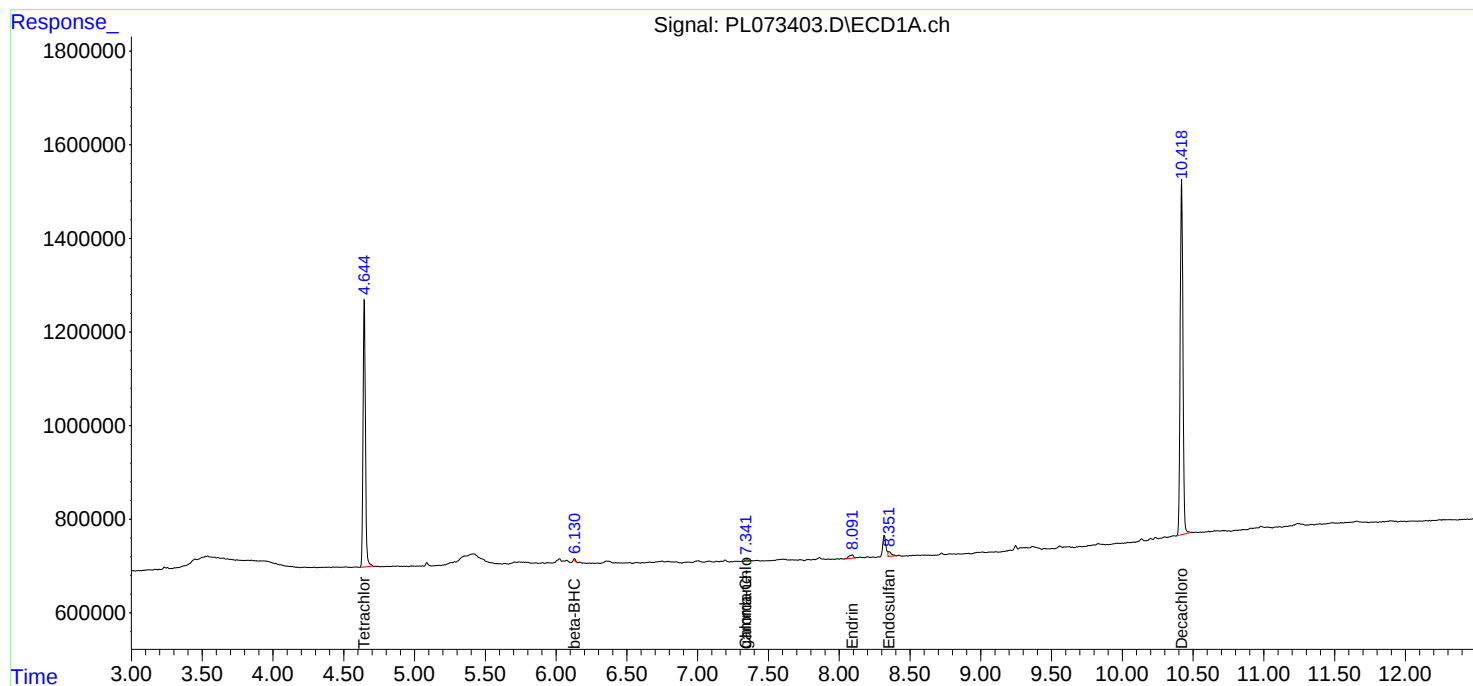


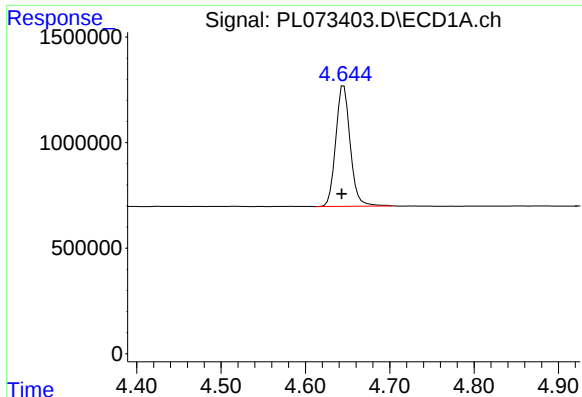

#1 Tetrachloro-m-xylene


R.T.: 4.646 min
Delta R.T.: 0.003 min
Response: 6823966
Conc: 21.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

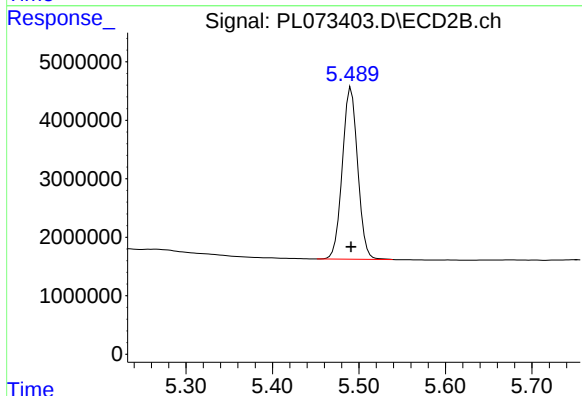


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: 0.000 min
Response: 35971898
Conc: 21.92 ng/ml

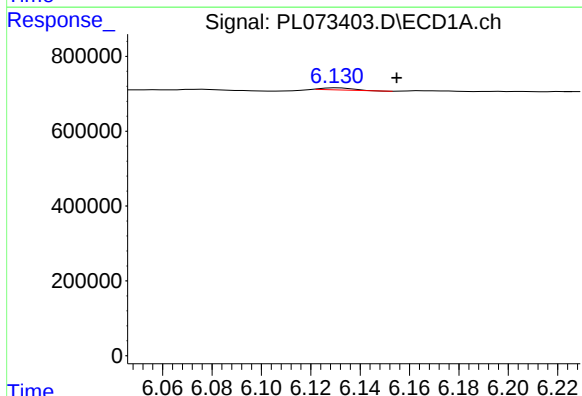


#6 beta-BHC

R.T.: 6.131 min
Delta R.T.: -0.024 min
Response: 45882
Conc: 0.22 ng/ml

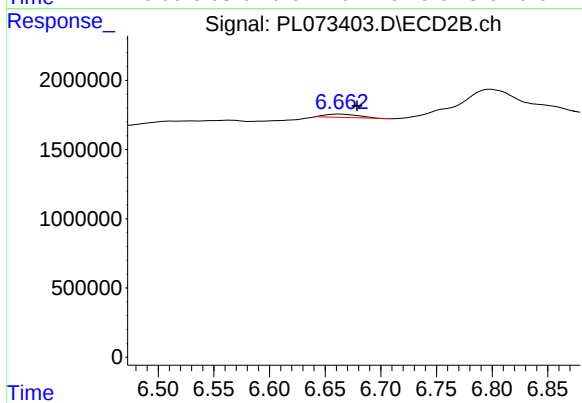

#6 beta-BHC


R.T.: 6.664 min
Delta R.T.: -0.015 min
Response: 464408
Conc: 0.45 ng/ml

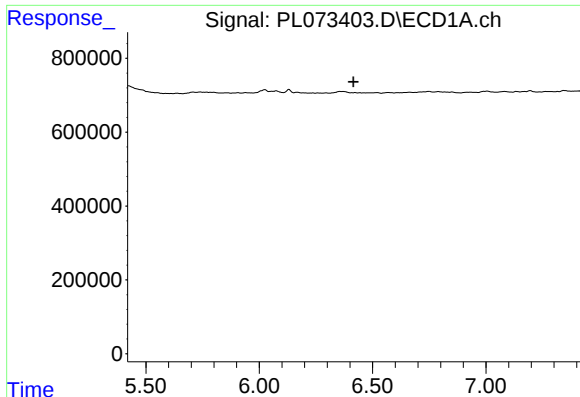

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.416 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

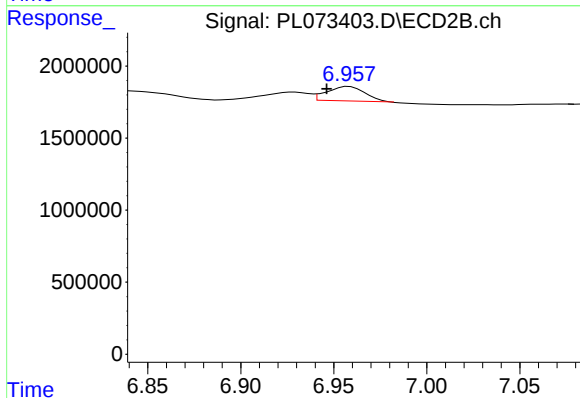


#7 delta-BHC

R.T.: 6.958 min
Delta R.T.: 0.012 min
Response: 1405070
Conc: 0.65 ng/ml

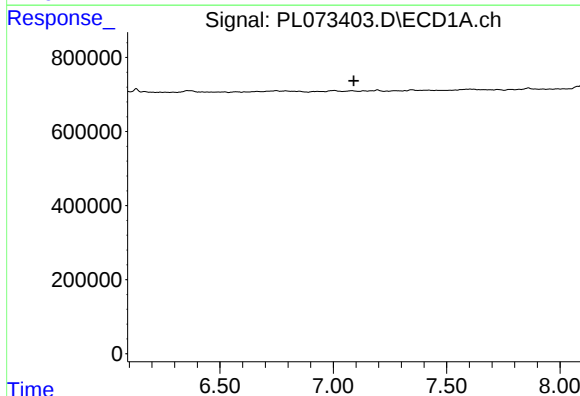


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.090 min
Response: 0
Conc: N.D.

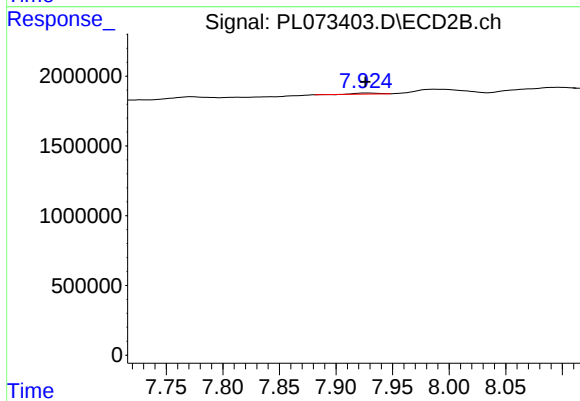

#8 Heptachlor epoxide


R.T.: 7.927 min
Delta R.T.: 0.000 min
Response: 95444
Conc: 0.05 ng/ml

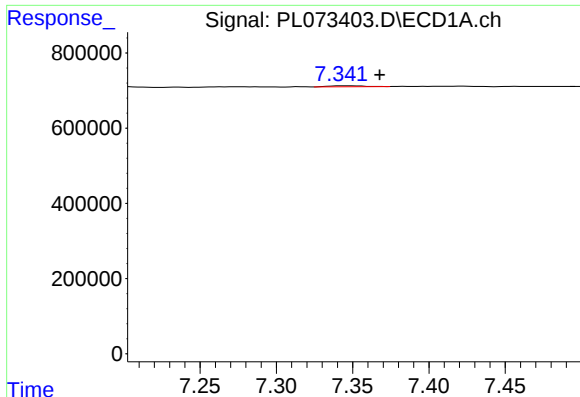

#10 gamma-Chlordane


R.T.: 7.343 min
Delta R.T.: -0.025 min
Response: 42986
Conc: 0.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

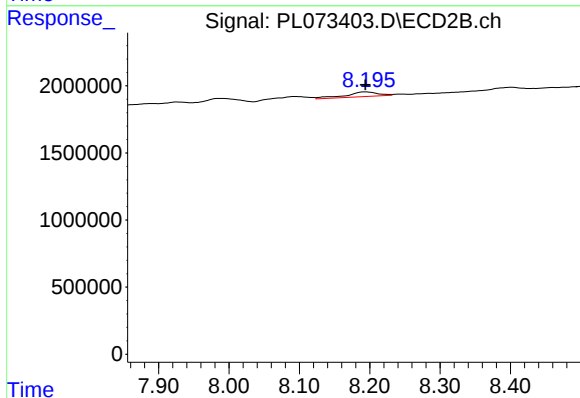


#10 gamma-Chlordane

R.T.: 8.195 min
Delta R.T.: 0.001 min
Response: 1094701
Conc: 0.54 ng/ml

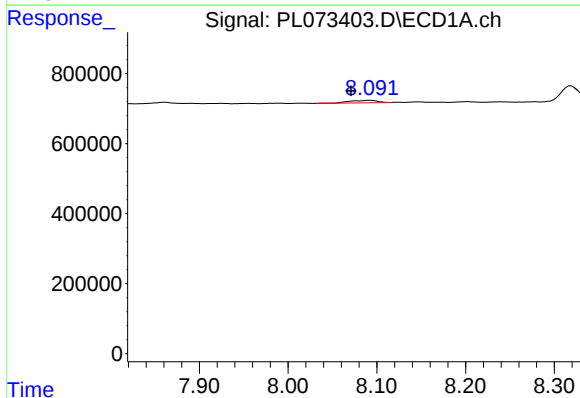


#14 Endrin

R.T.: 8.093 min
Delta R.T.: 0.022 min
Response: 146212
Conc: 0.38 ng/ml

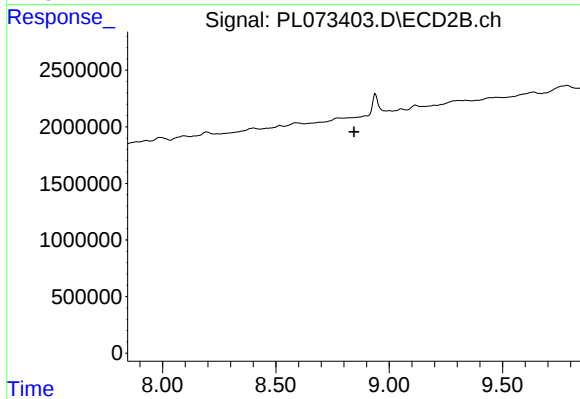

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 8.845 min
Response: 0
Conc: N.D.

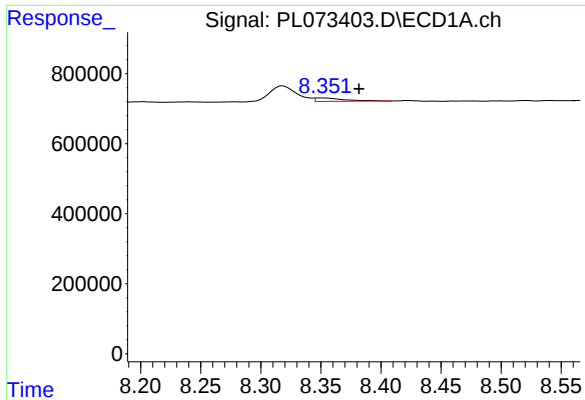

#15 Endosulfan II


R.T.: 8.352 min
Delta R.T.: -0.029 min
Response: 165628
Conc: 0.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

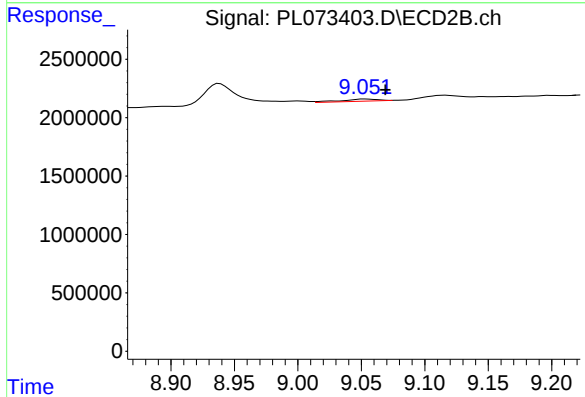


#15 Endosulfan II

R.T.: 9.053 min
Delta R.T.: -0.016 min
Response: 359110
Conc: 0.23 ng/ml

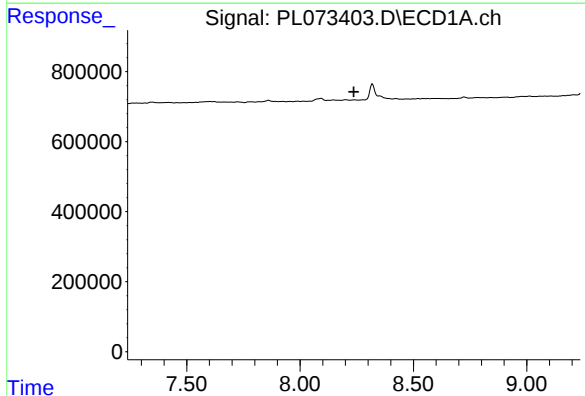


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.237 min
Response: 0
Conc: N.D.

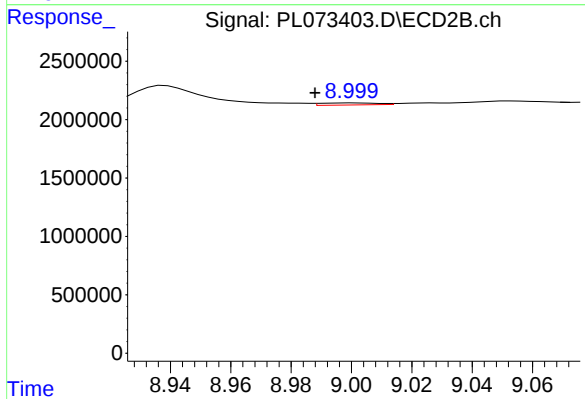

#16 4,4'-DDD


R.T.: 9.001 min
Delta R.T.: 0.013 min
Response: 234651
Conc: 0.16 ng/ml

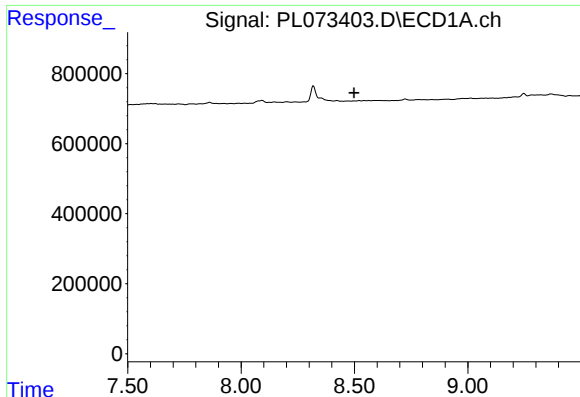

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.499 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

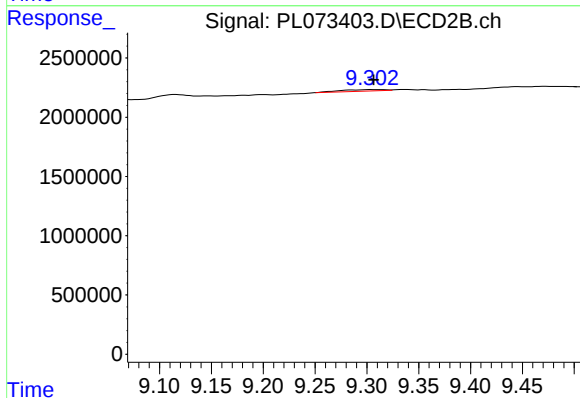


#17 4,4'-DDT

R.T.: 9.306 min
Delta R.T.: 0.000 min
Response: 364157
Conc: 0.22 ng/ml

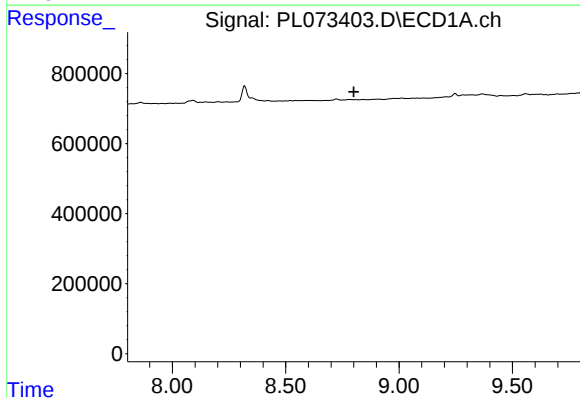


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 8.801 min
Response: 0
Conc: N.D.

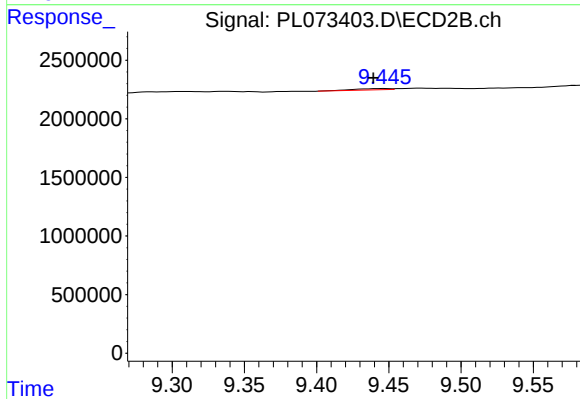

#19 Endosulfan Sulfate


R.T.: 9.447 min
Delta R.T.: 0.007 min
Response: 180549
Conc: 0.11 ng/ml

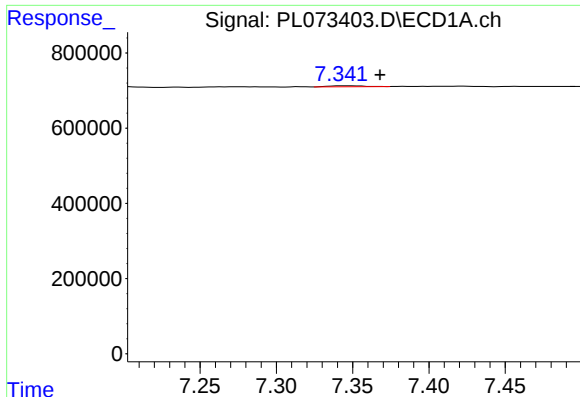

#25 Chlordane-3


R.T.: 7.343 min
Delta R.T.: -0.025 min
Response: 42986
Conc: 1.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

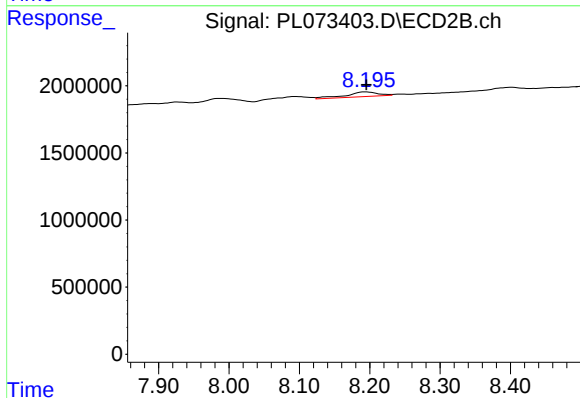


#25 Chlordane-3

R.T.: 8.195 min
Delta R.T.: 0.000 min
Response: 1094701
Conc: 4.04 ng/ml

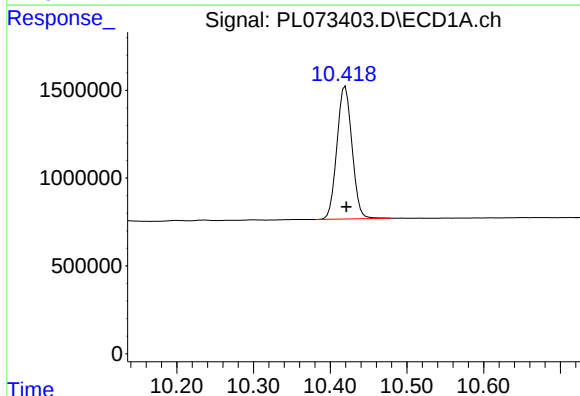

#28 Decachlorobiphenyl

R.T.: 10.419 min
Delta R.T.: -0.001 min
Response: 10347114
Conc: 20.35 ng/ml

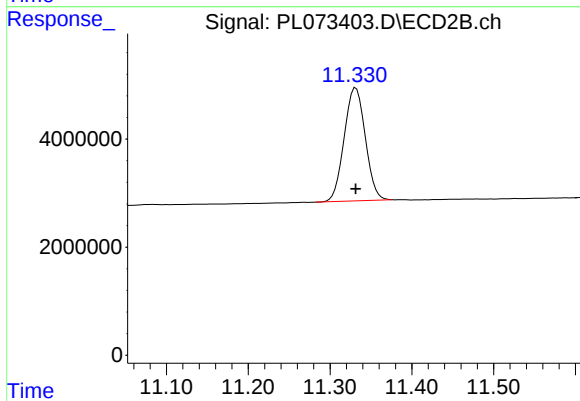

#28 Decachlorobiphenyl

R.T.: 11.332 min
Delta R.T.: 0.000 min
Response: 37537875
Conc: 20.99 ng/ml