

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031524\
 Data File : PL088600.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Mar 2024 14:54
 Operator : AR\AJ
 Sample : P1746-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-01-4.0-6.0-DUP

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 03/15/2024
 Supervised By :Ankita Jodhani 03/15/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 14 20:14:40 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 13 15:45:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.632	2.852	55049352	27935813	20.774m	20.961
2) SA Decachlor...	9.300	8.081	36644103	20771833	14.824m	15.319

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031524\
Data File : PL088600.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Mar 2024 14:54
Operator : AR\AJ
Sample : P1746-03
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SB-01-4.0-6.0-DUP


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/15/2024
Supervised By : Ankita Jodhani 03/15/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 14 20:14:40 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
Quant Title : GC Extractables
QLast Update : Wed Mar 13 15:45:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

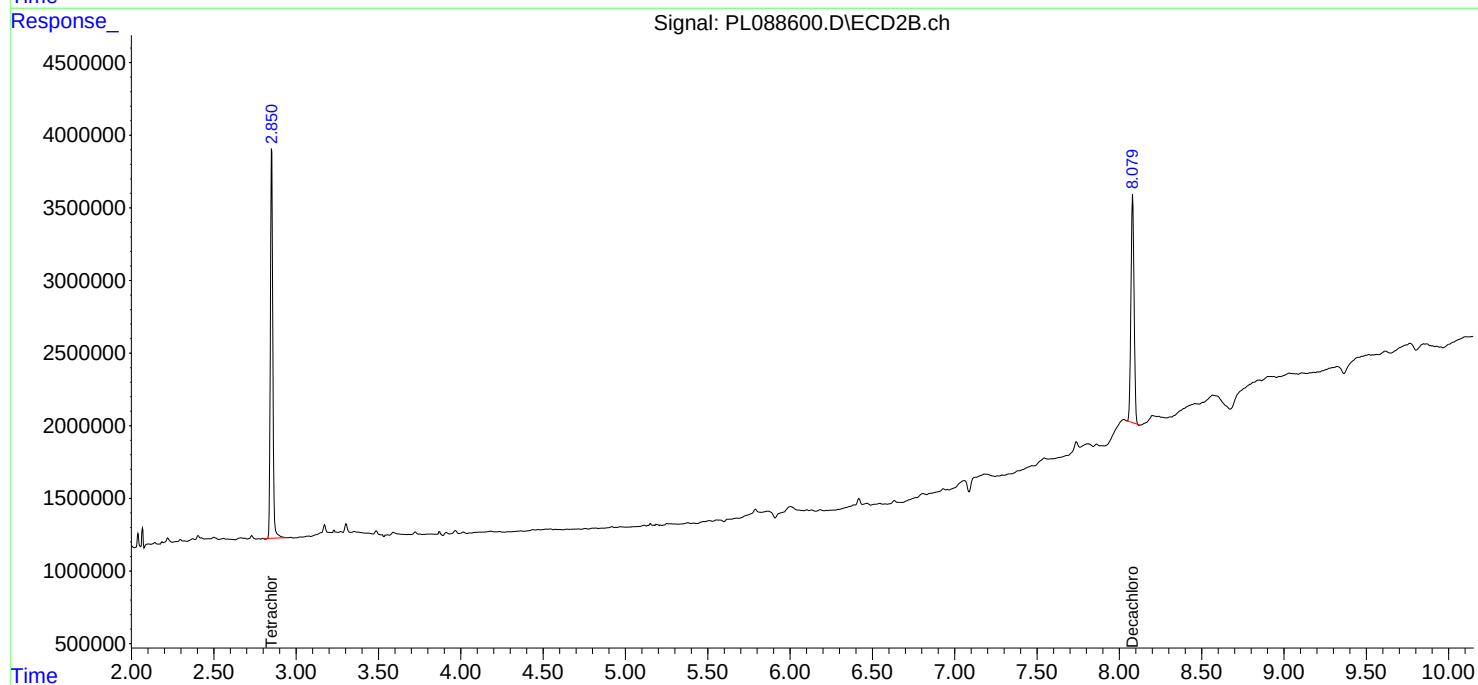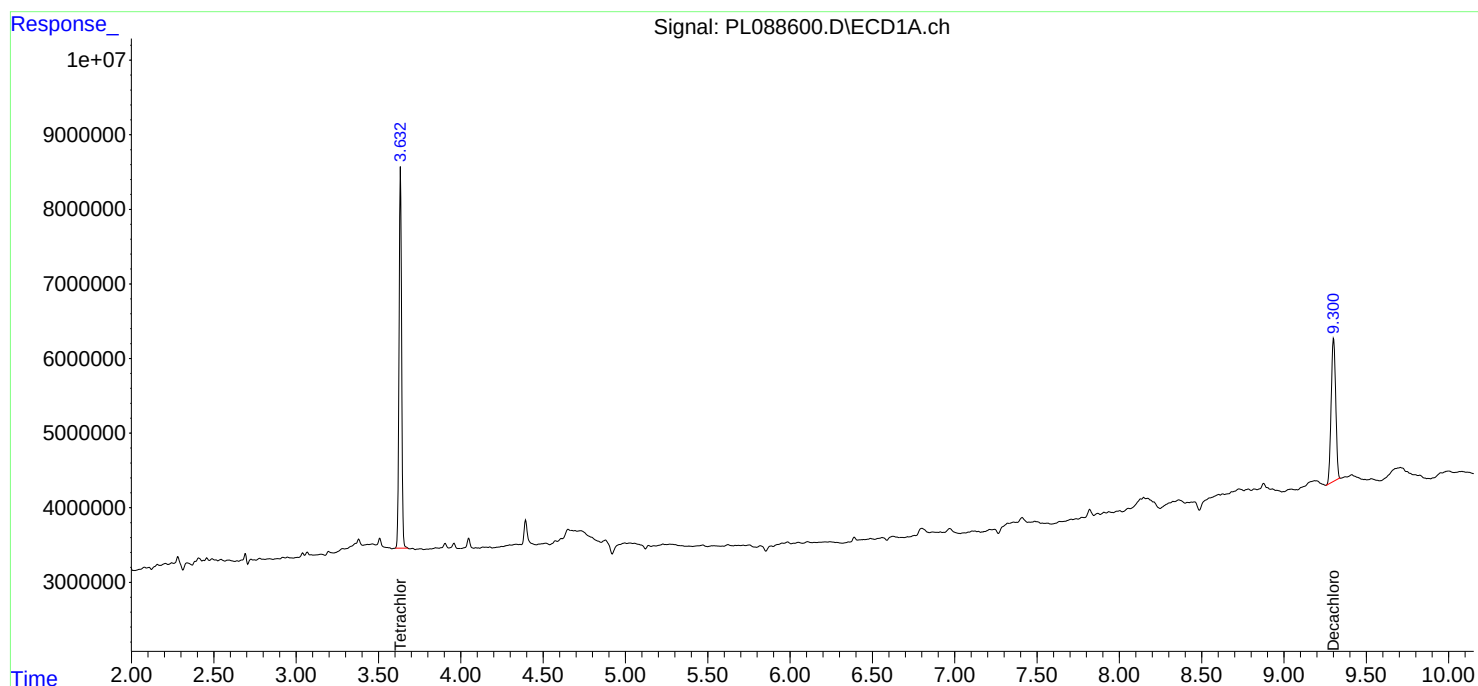

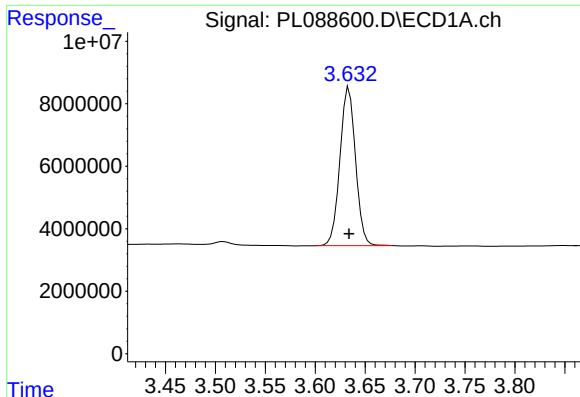


#1 Tetrachloro-m-xylene

R.T.: 3.632 min
Delta R.T.: -0.002 min
Response: 55049352
Conc: 20.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-01-4.0-6.0-DUP


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/15/2024
Supervised By :Ankita Jodhani 03/15/2024

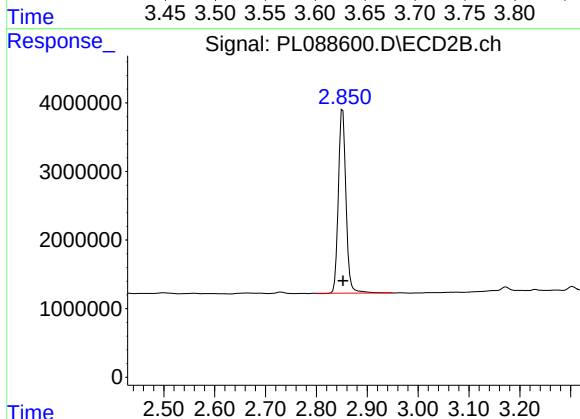


#1 Tetrachloro-m-xylene

R.T.: 2.852 min
Delta R.T.: 0.000 min
Response: 27935813
Conc: 20.96 ng/ml

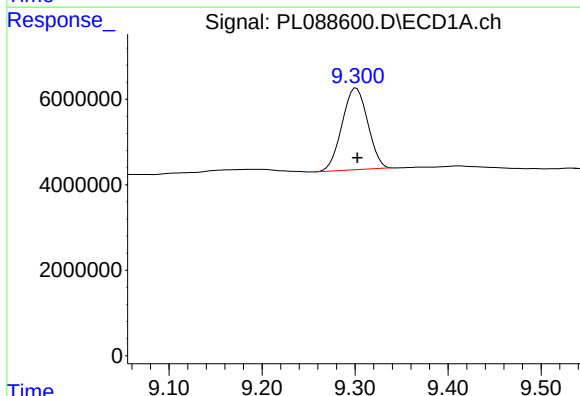

#28 Decachlorobiphenyl

R.T.: 9.300 min
Delta R.T.: -0.003 min
Response: 36644103
Conc: 14.82 ng/ml m

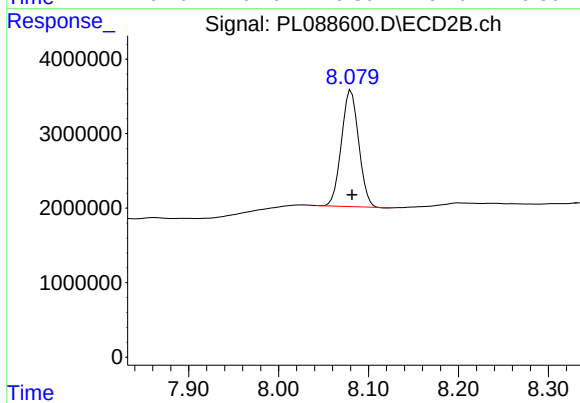

#28 Decachlorobiphenyl

R.T.: 8.081 min
Delta R.T.: -0.001 min
Response: 20771833
Conc: 15.32 ng/ml