

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031621\
 Data File : PL065321.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2021 08:56
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 05:38:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031621.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 17 04:35:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds



Target Compounds						
16) A	4,4'-DDD	0.000	6.670f	0	4806772	N.D. 1.904 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031621\
Data File : PL065321.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2021 08:56
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 05:38:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031621.M
Quant Title : GC Extractables
QLast Update : Wed Mar 17 04:35:29 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

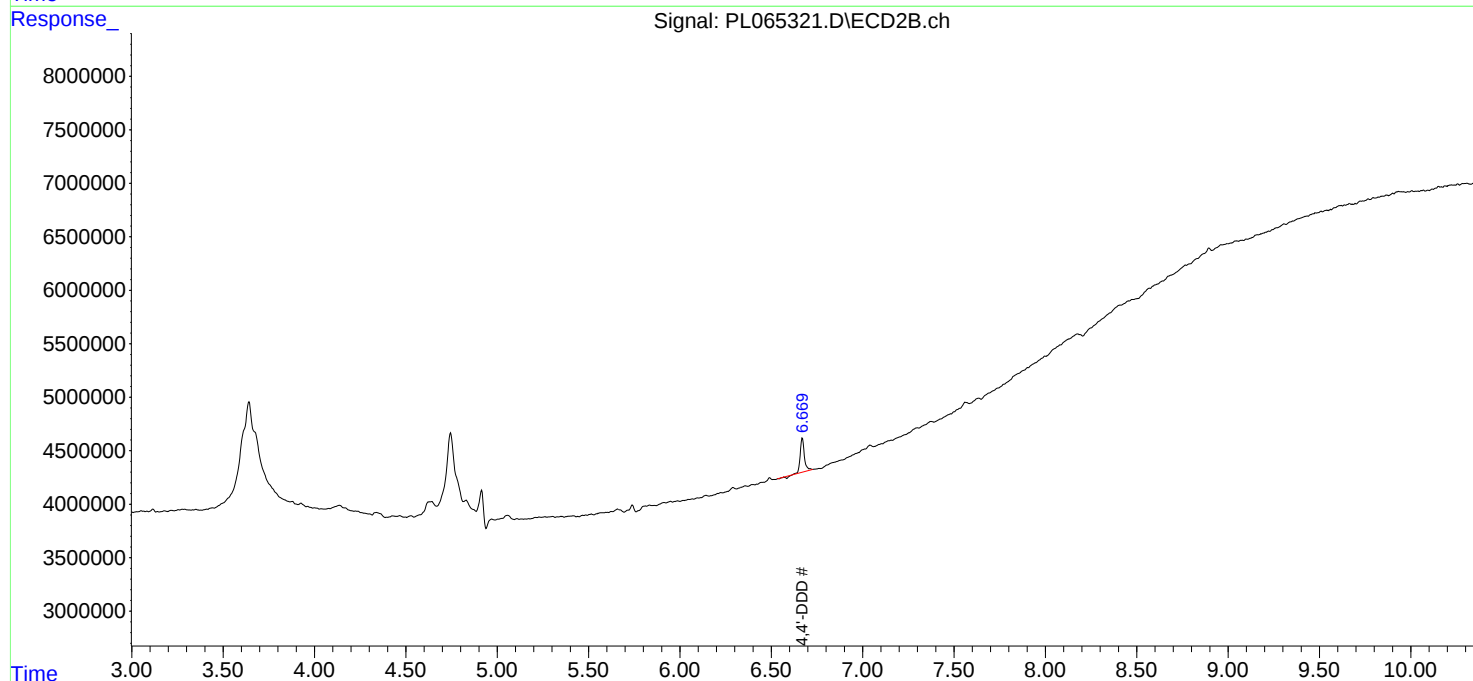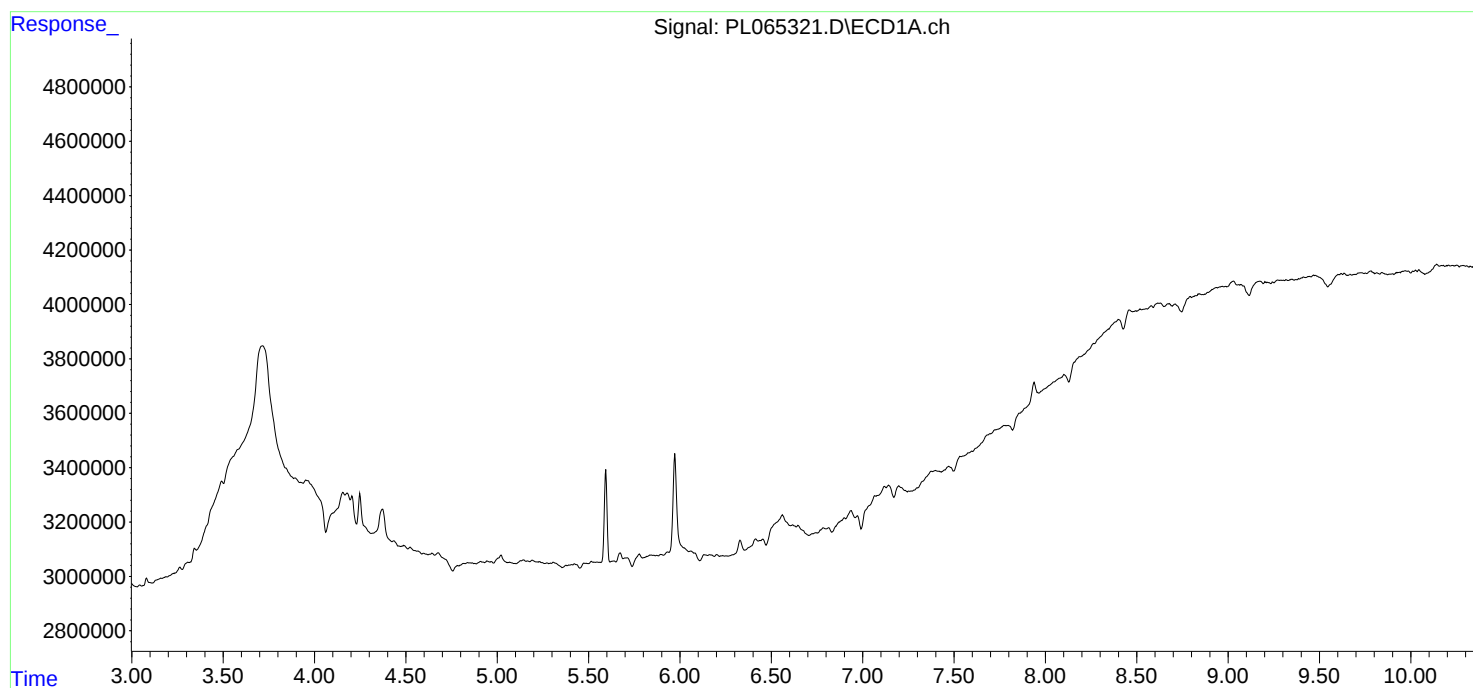

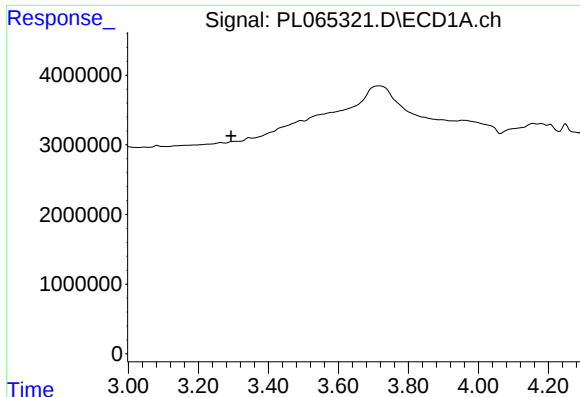


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.293 min
Response: 0
Conc: N.D.

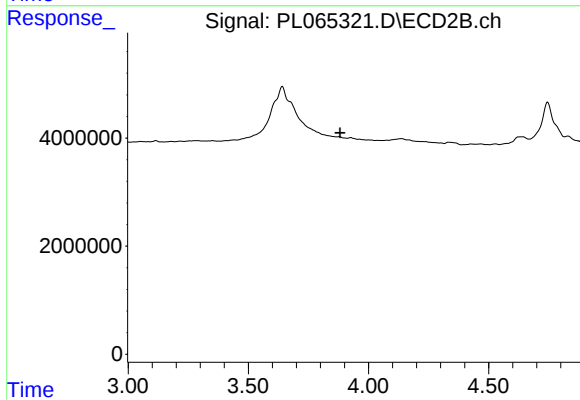


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.882 min
Response: 0
Conc: N.D.

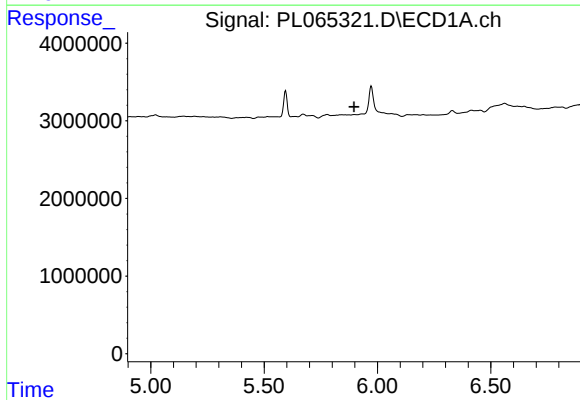


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.897 min
Response: 0
Conc: N.D.

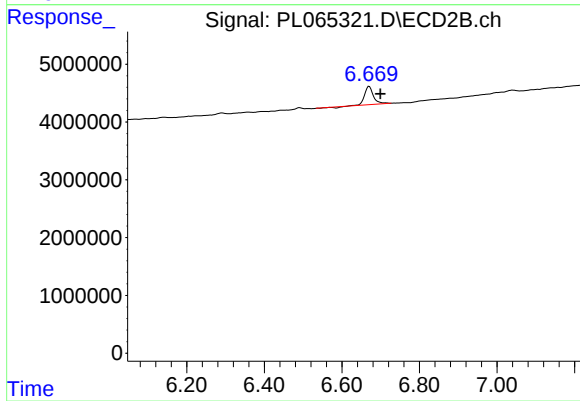


#16 4,4'-DDD

R.T.: 6.670 min
Delta R.T.: -0.029 min
Response: 4806772
Conc: 1.90 ng/ml

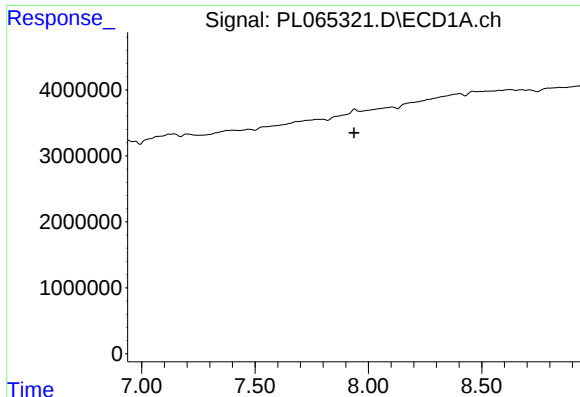

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.936 min
Response: 0
Conc: N.D.

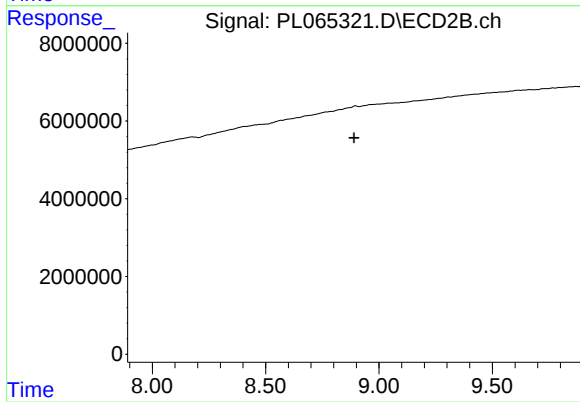

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.890 min
Response: 0
Conc: N.D.