

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031621\
 Data File : PL065335.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2021 17:48
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 04:26:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031621.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 17 04:25:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.292	3.882	196.8E6	206.3E6	76.435	74.913
28)	SA Decachlor...	7.937	8.890	171.4E6	143.1E6	73.132	73.240
Target Compounds							
23)	Chlordane-1	4.129	4.863	68688185	84657056	727.817	703.062
24)	Chlordane-2	4.617	5.329	79301436	86369840	731.159	733.585
25)	Chlordane-3	5.169	5.973	237.7E6	319.3E6	760.182	737.305
26)	Chlordane-4	5.224	6.044	207.4E6	366.2E6	747.987	733.888
27)	Chlordane-5	6.038	6.849	75939549	69188451	758.175	738.150


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031621\
Data File : PL065335.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2021 17:48
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 04:26:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031621.M
Quant Title : GC Extractables
QLast Update : Wed Mar 17 04:25:32 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

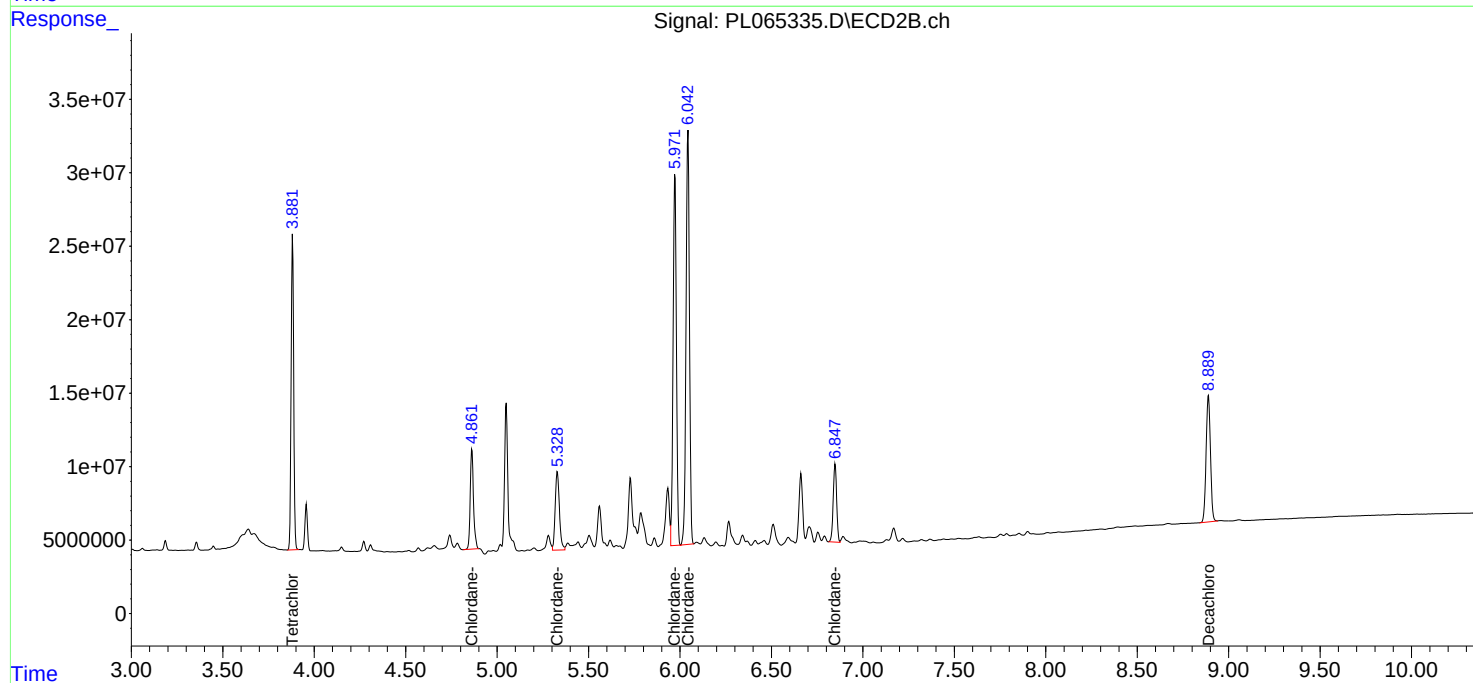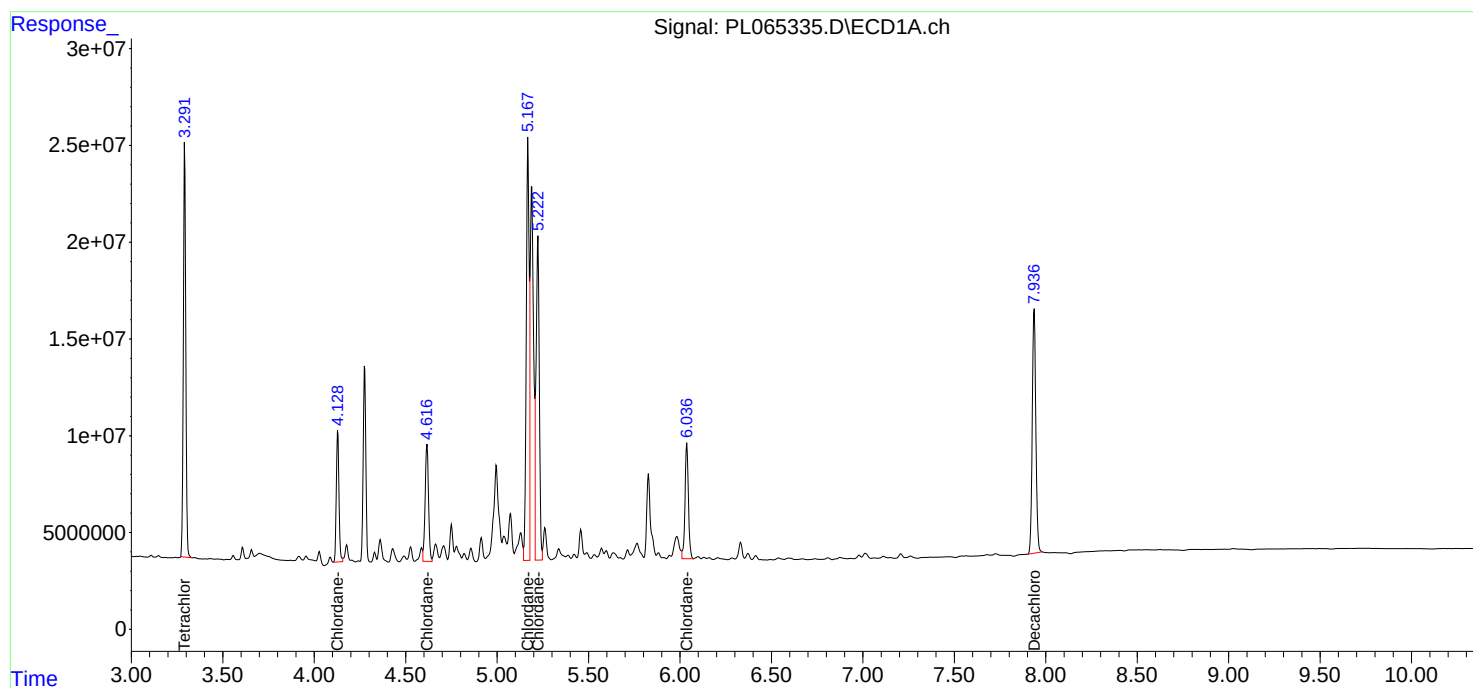

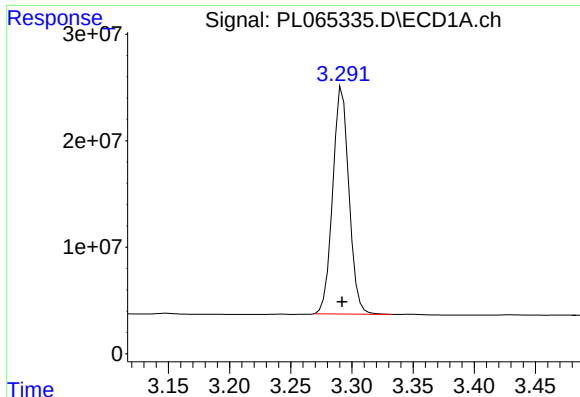


#1 Tetrachloro-m-xylene

R.T.: 3.292 min
Delta R.T.: 0.000 min
Response: 196792082
Conc: 76.43 ng/ml

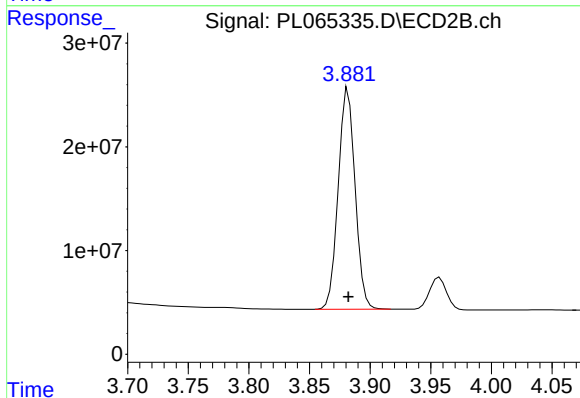


#1 Tetrachloro-m-xylene

R.T.: 3.882 min
Delta R.T.: 0.000 min
Response: 206334482
Conc: 74.91 ng/ml

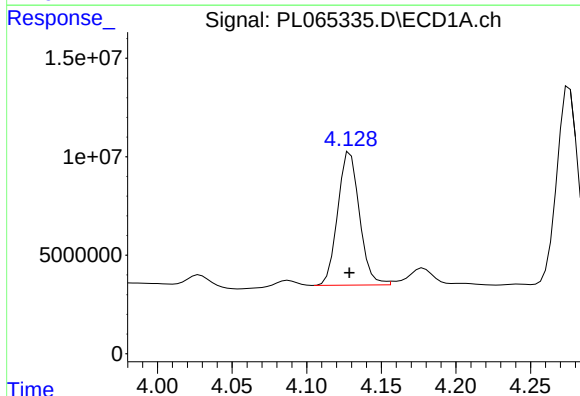


#23 Chlordane-1

R.T.: 4.129 min
Delta R.T.: 0.000 min
Response: 68688185
Conc: 727.82 ng/ml

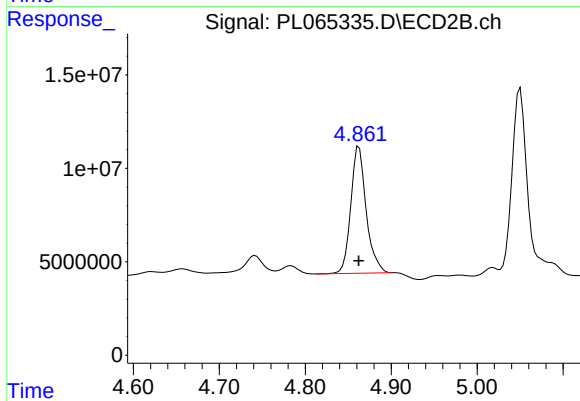


#23 Chlordane-1

R.T.: 4.863 min
Delta R.T.: 0.000 min
Response: 84657056
Conc: 703.06 ng/ml

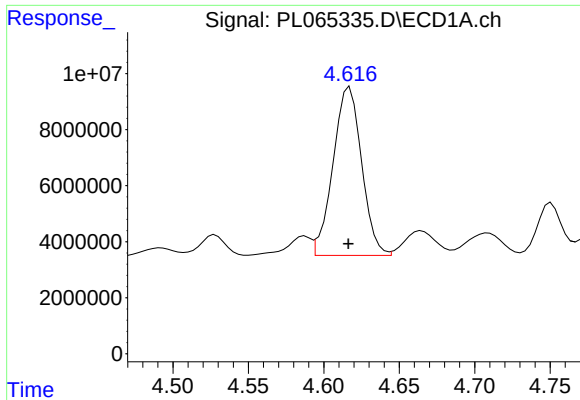


#24 Chlordane-2

R.T.: 4.617 min
Delta R.T.: 0.000 min
Response: 79301436
Conc: 731.16 ng/ml

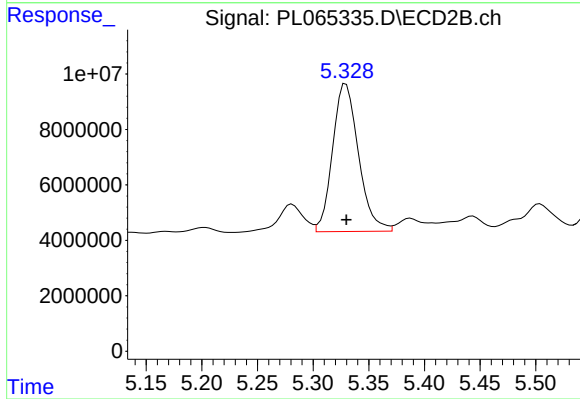


#24 Chlordane-2

R.T.: 5.329 min
Delta R.T.: 0.000 min
Response: 86369840
Conc: 733.58 ng/ml

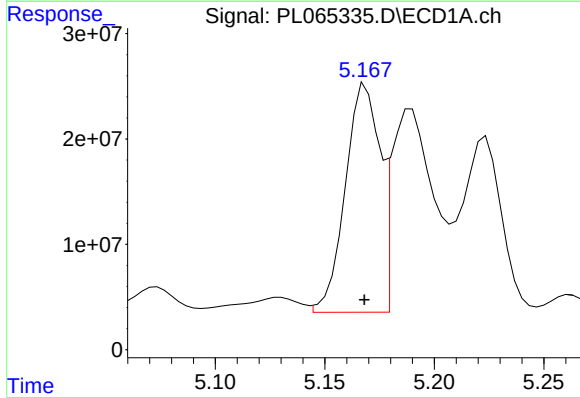


#25 Chlordane-3

R.T.: 5.169 min
Delta R.T.: 0.000 min
Response: 237744014
Conc: 760.18 ng/ml

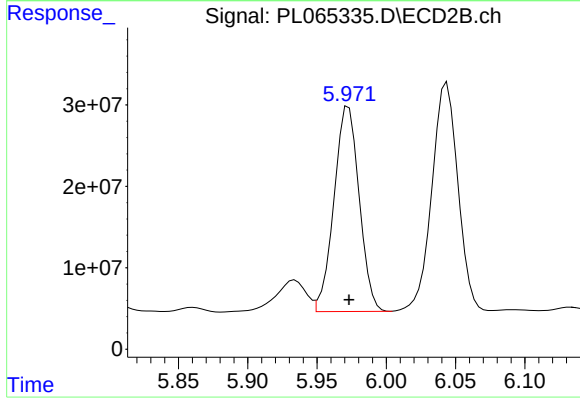


#25 Chlordane-3

R.T.: 5.973 min
Delta R.T.: 0.000 min
Response: 319255580
Conc: 737.30 ng/ml

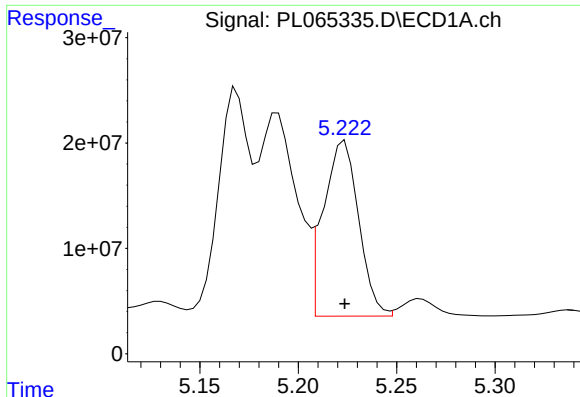


#26 Chlordane-4

R.T.: 5.224 min
Delta R.T.: 0.000 min
Response: 207370517
Conc: 747.99 ng/ml

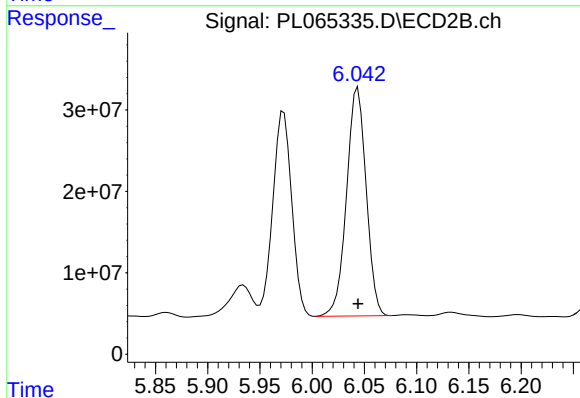


#26 Chlordane-4

R.T.: 6.044 min
Delta R.T.: 0.000 min
Response: 366220591
Conc: 733.89 ng/ml

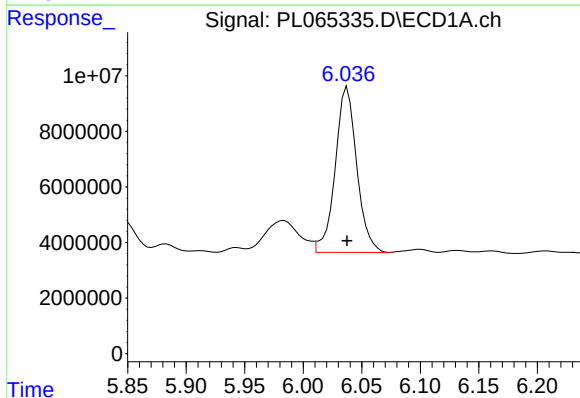


#27 Chlordane-5

R.T.: 6.038 min
Delta R.T.: 0.000 min
Response: 75939549
Conc: 758.18 ng/ml

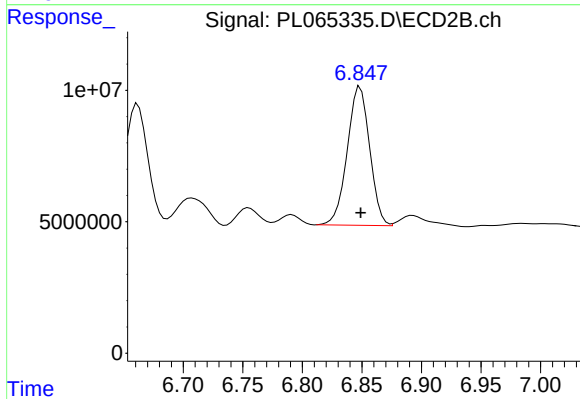

#27 Chlordane-5

R.T.: 6.849 min
Delta R.T.: 0.000 min
Response: 69188451
Conc: 738.15 ng/ml

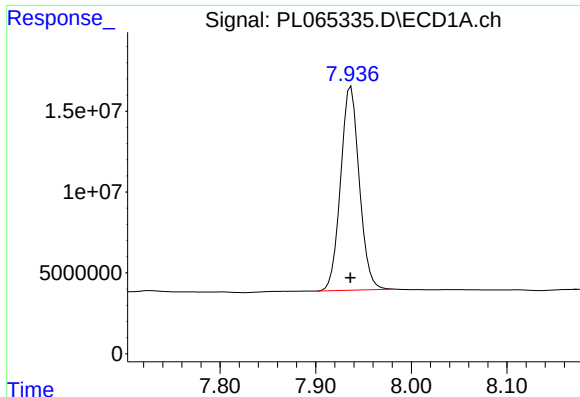


#28 Decachlorobiphenyl

R.T.: 7.937 min

Delta R.T.: 0.000 min

Response: 171386891

Conc: 73.13 ng/ml

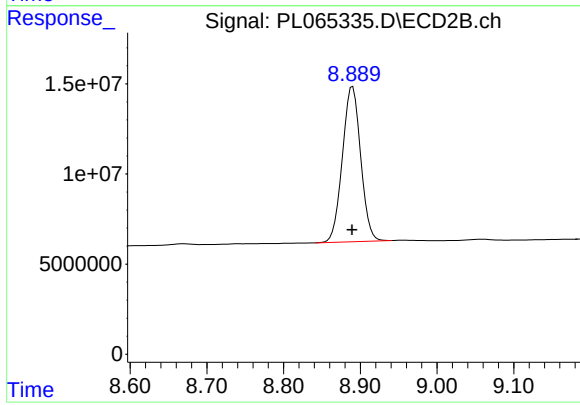

#28 Decachlorobiphenyl

R.T.: 8.890 min

Delta R.T.: 0.000 min

Response: 143118316

Conc: 73.24 ng/ml