

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031621\
 Data File : PL065328.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2021 16:07
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 05:39:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031621.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 17 04:35:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.293	3.882	51709765	61674269	21.266	21.364
28)	SA Decachlor...	7.937	8.890	51188472	42477876	20.847	20.881
Target Compounds							
9)	A Endosulfan I	5.275	6.094	27961466	30919360	9.782	10.356
10)	B gamma-Chl...	5.168	5.973	31503470	31562232	10.176	9.903
12)	B 4,4'-DDE	5.392	6.206	52794169	61934894	19.726	20.776
13)	MA Dieldrin	5.513	6.352	57950901	65712505	19.898	20.990
19)	B Endosulfa...	6.413	7.133	50194757	48967862	18.932	19.495
20)	A Methoxychlor	6.679	7.458	111.6E6	106.4E6	99.956	94.694
21)	B Endrin ke...	6.891	7.603	53950317	52591869	18.972	19.315



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031621\
Data File : PL065328.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2021 16:07
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 05:39:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031621.M
Quant Title : GC Extractables
QLast Update : Wed Mar 17 04:35:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

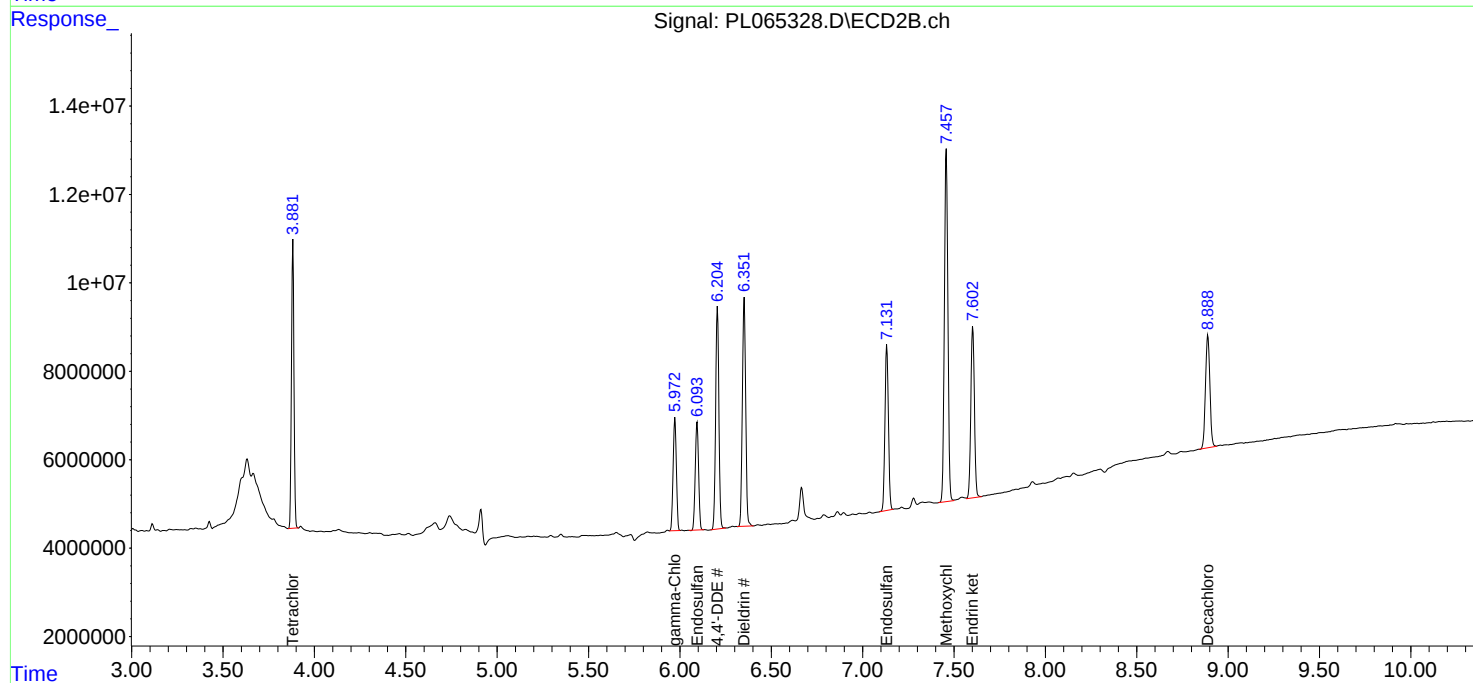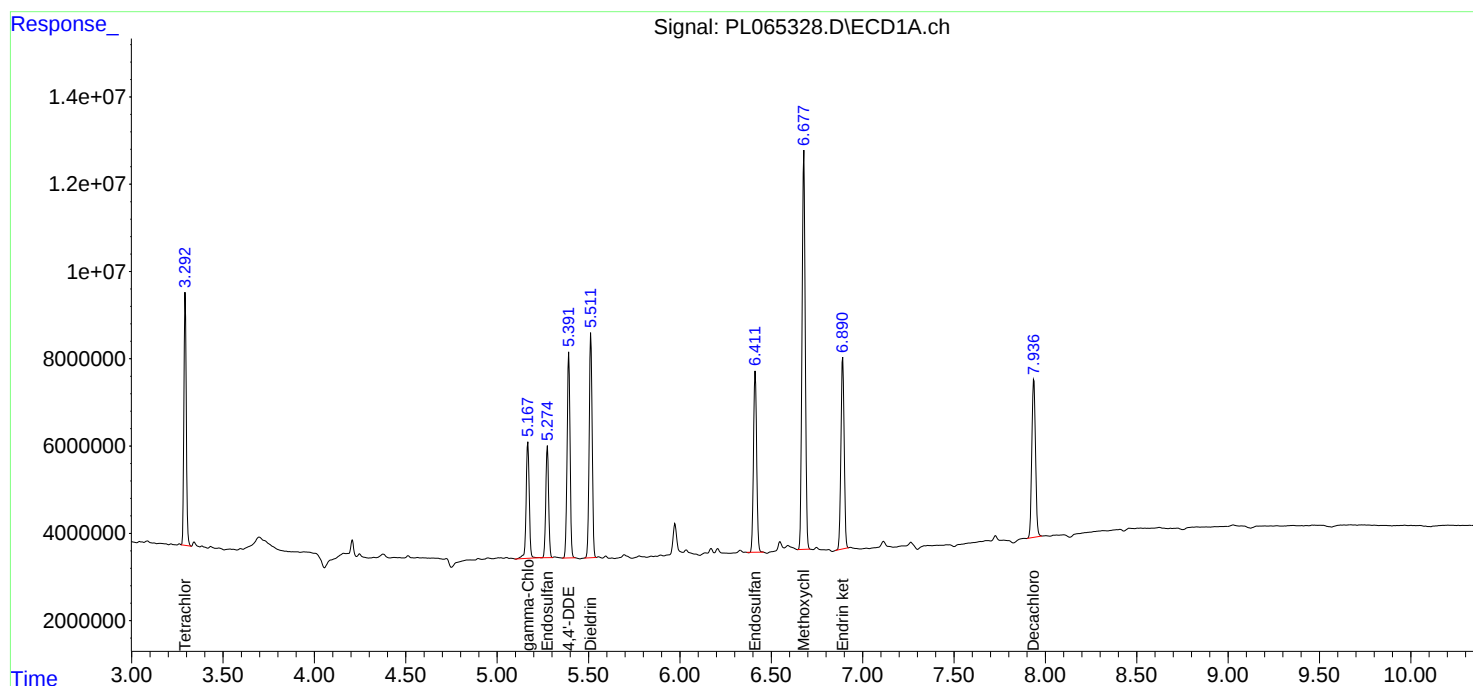


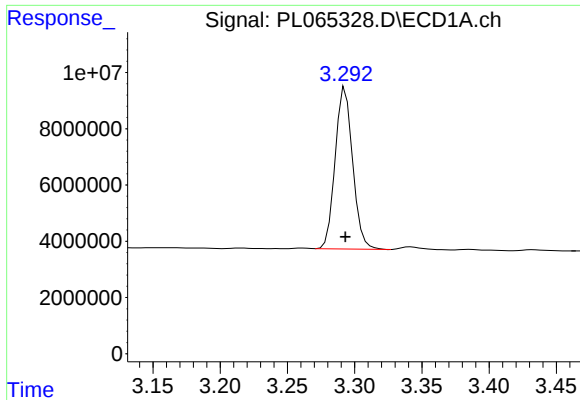

#1 Tetrachloro-m-xylene


R.T.: 3.293 min
Delta R.T.: 0.000 min
Response: 51709765
Conc: 21.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

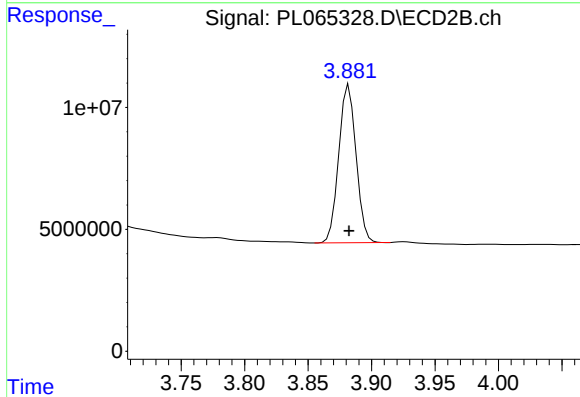


#1 Tetrachloro-m-xylene

R.T.: 3.882 min
Delta R.T.: 0.000 min
Response: 61674269
Conc: 21.36 ng/ml

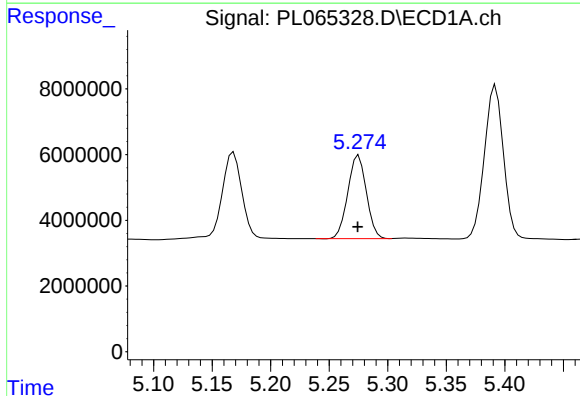


#9 Endosulfan I

R.T.: 5.275 min
Delta R.T.: 0.000 min
Response: 27961466
Conc: 9.78 ng/ml

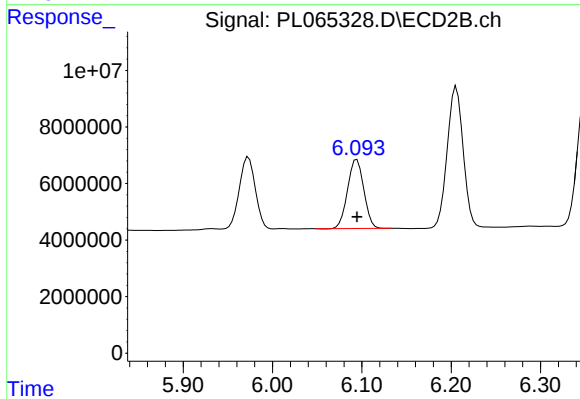

#9 Endosulfan I


R.T.: 6.094 min
Delta R.T.: 0.000 min
Response: 30919360
Conc: 10.36 ng/ml

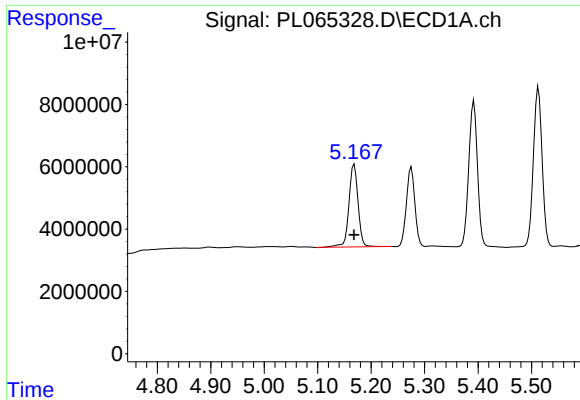

#10 gamma-Chlordane


R.T.: 5.168 min
Delta R.T.: 0.000 min
Response: 31503470
Conc: 10.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

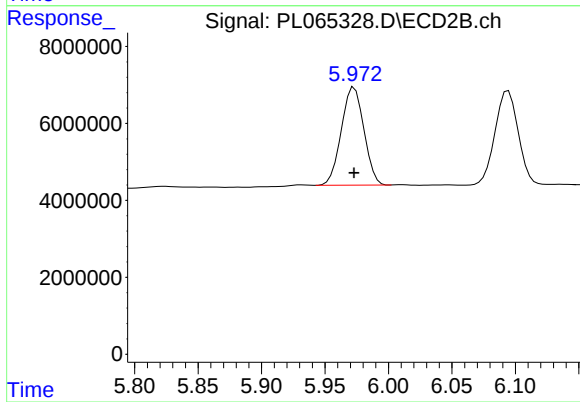


#10 gamma-Chlordane

R.T.: 5.973 min
Delta R.T.: 0.000 min
Response: 31562232
Conc: 9.90 ng/ml

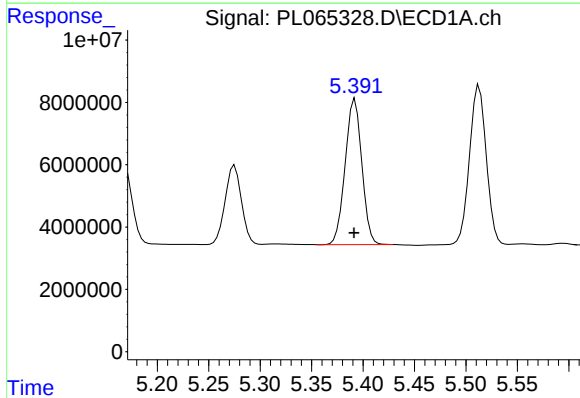


#12 4,4'-DDE

R.T.: 5.392 min
Delta R.T.: 0.000 min
Response: 52794169
Conc: 19.73 ng/ml

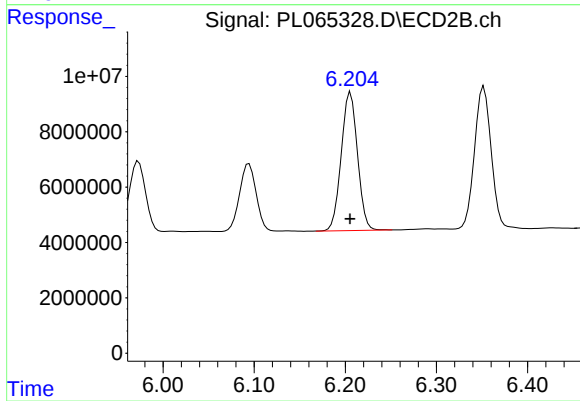

#12 4,4'-DDE


R.T.: 6.206 min
Delta R.T.: 0.000 min
Response: 61934894
Conc: 20.78 ng/ml

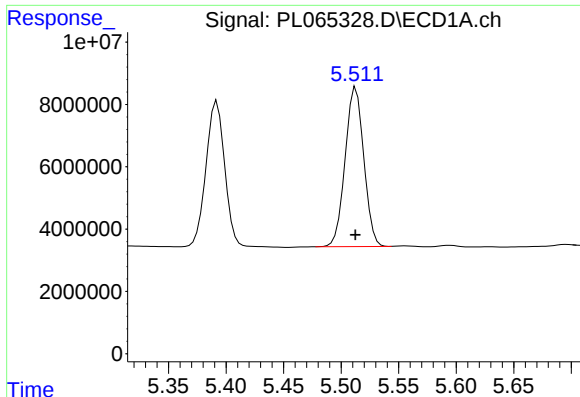

#13 Dieldrin


R.T.: 5.513 min
Delta R.T.: 0.000 min
Response: 57950901
Conc: 19.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

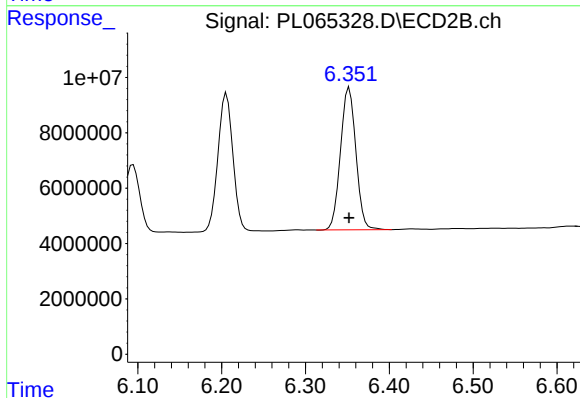


#13 Dieldrin

R.T.: 6.352 min
Delta R.T.: 0.000 min
Response: 65712505
Conc: 20.99 ng/ml

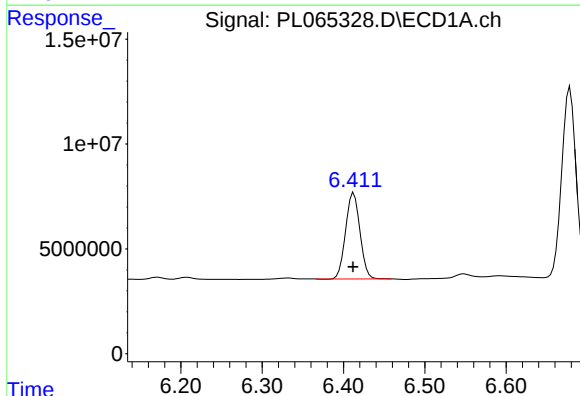


#19 Endosulfan Sulfate

R.T.: 6.413 min
Delta R.T.: 0.001 min
Response: 50194757
Conc: 18.93 ng/ml

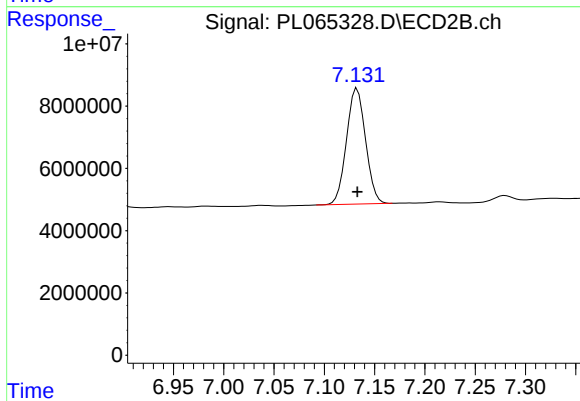

#19 Endosulfan Sulfate


R.T.: 7.133 min
Delta R.T.: 0.000 min
Response: 48967862
Conc: 19.49 ng/ml

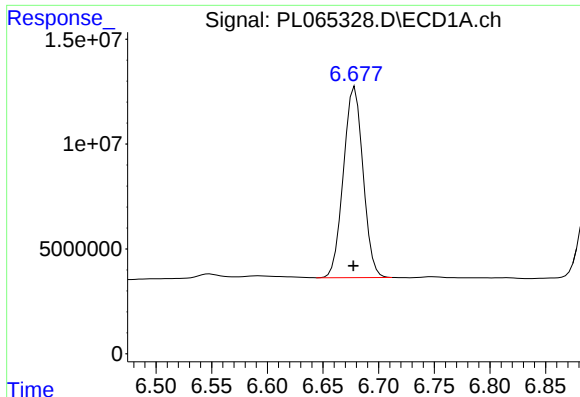

#20 Methoxychlor


R.T.: 6.679 min
Delta R.T.: 0.001 min
Response: 111593895
Conc: 99.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

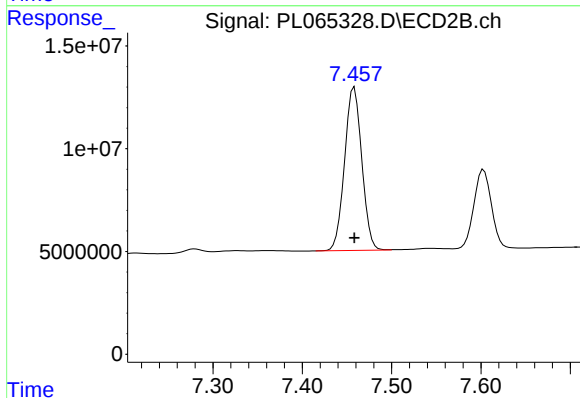


#20 Methoxychlor

R.T.: 7.458 min
Delta R.T.: 0.000 min
Response: 106383135
Conc: 94.69 ng/ml

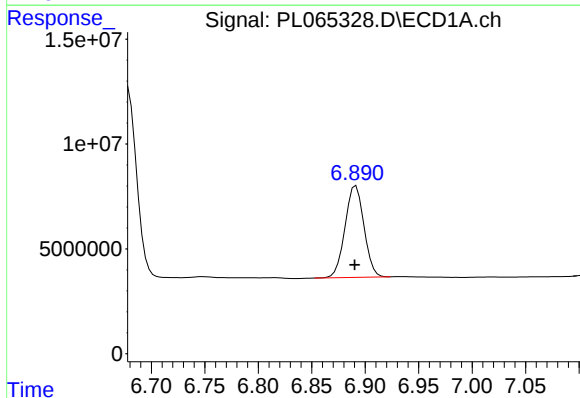


#21 Endrin ketone

R.T.: 6.891 min
Delta R.T.: 0.001 min
Response: 53950317
Conc: 18.97 ng/ml

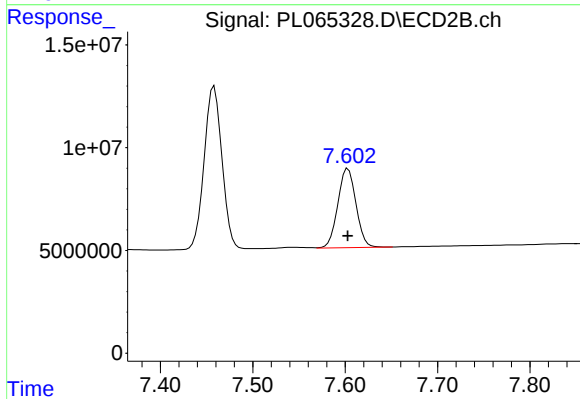

#21 Endrin ketone


R.T.: 7.603 min
Delta R.T.: 0.000 min
Response: 52591869
Conc: 19.32 ng/ml

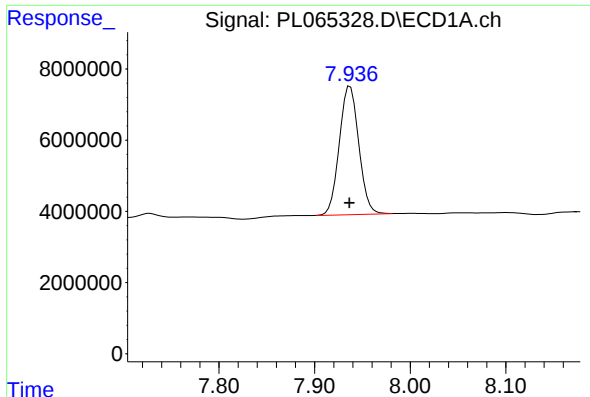

#28 Decachlorobiphenyl

R.T.: 7.937 min
Delta R.T.: 0.000 min
Response: 51188472
Conc: 20.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

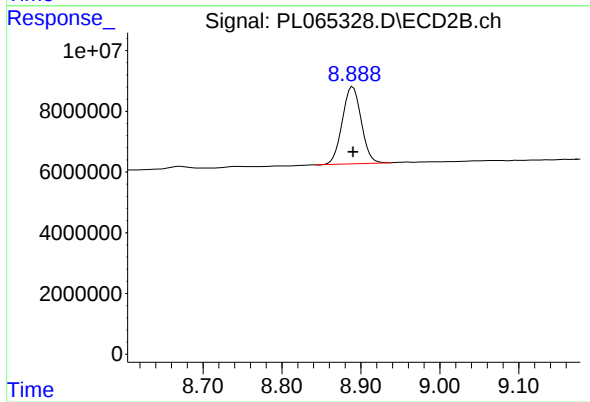

#28 Decachlorobiphenyl

R.T.: 8.890 min
Delta R.T.: 0.000 min
Response: 42477876
Conc: 20.88 ng/ml