

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031621\
 Data File : PL065334.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2021 17:33
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 04:26:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031621.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 17 04:25:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.292	3.882	263.0E6	271.1E6	102.163	98.421
28)	SA Decachlor...	7.936	8.890	225.5E6	187.3E6	96.237	95.831
Target Compounds							
23)	Chlordane-1	4.129	4.863	91724181	112.8E6	971.905	936.875
24)	Chlordane-2	4.617	5.330	104.9E6	114.1E6	967.121	968.712
25)	Chlordane-3	5.169	5.973	311.7E6	425.5E6	996.570	982.607
26)	Chlordane-4	5.223	6.044	282.1E6	487.8E6	1017.708	977.462
27)	Chlordane-5	6.037	6.849	102.4E6	92219615	1022.023	983.862



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031621\
Data File : PL065334.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2021 17:33
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 04:26:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031621.M
Quant Title : GC Extractables
QLast Update : Wed Mar 17 04:25:32 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

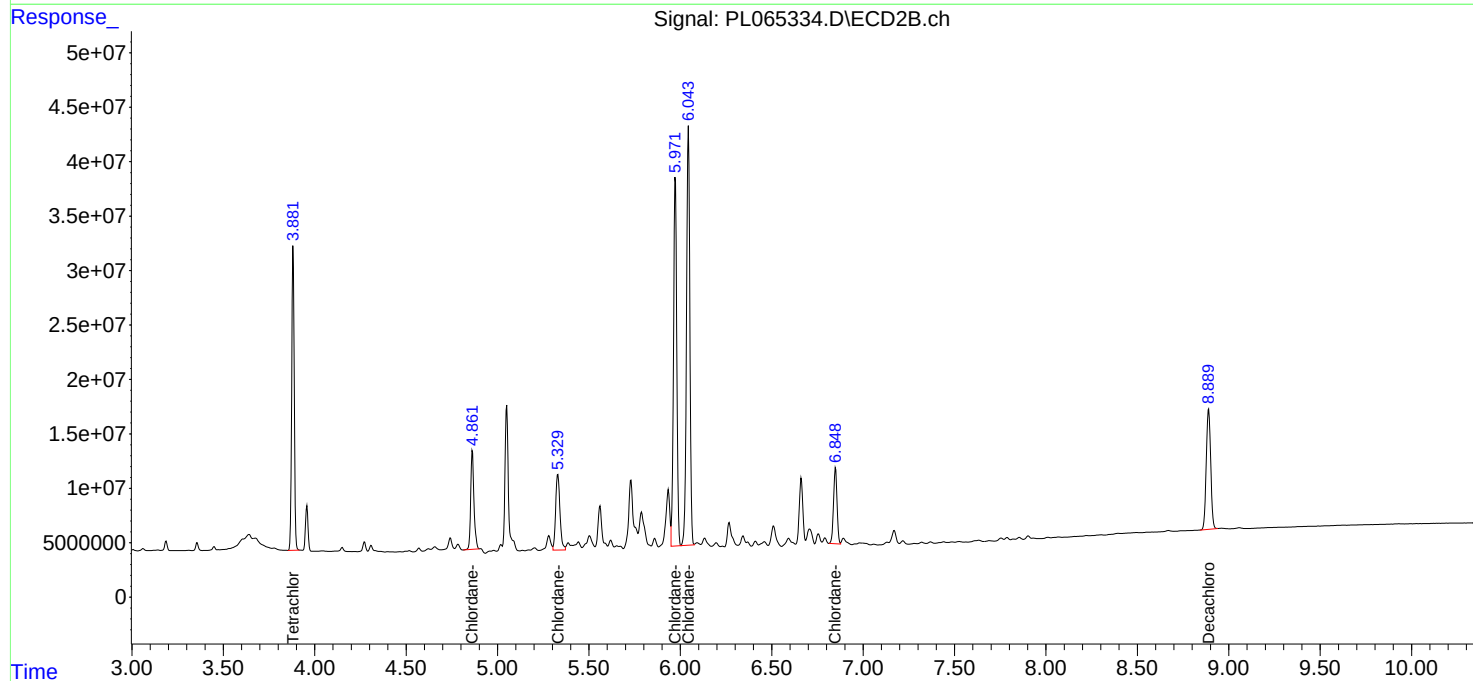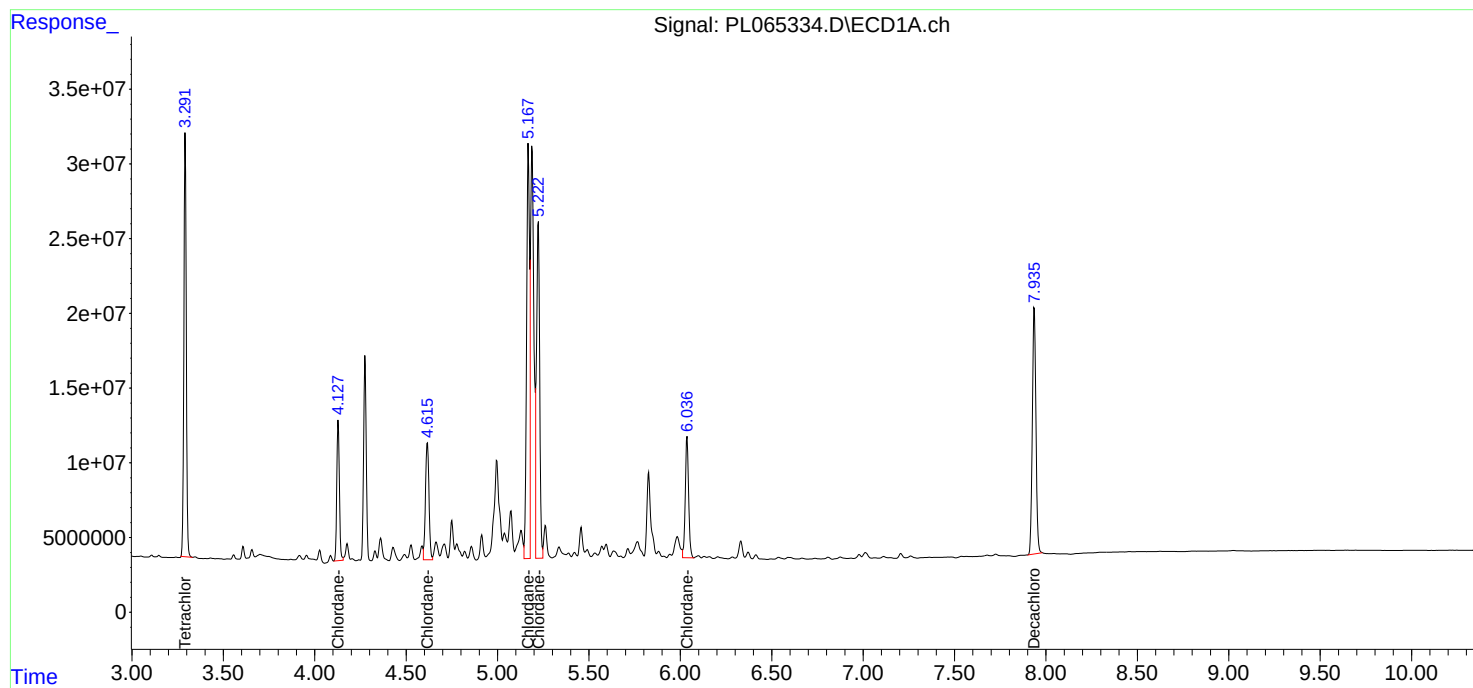


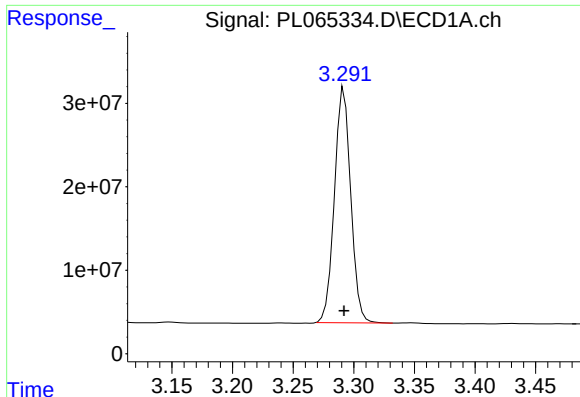

#1 Tetrachloro-m-xylene


R.T.: 3.292 min
Delta R.T.: 0.000 min
Response: 263032042
Conc: 102.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

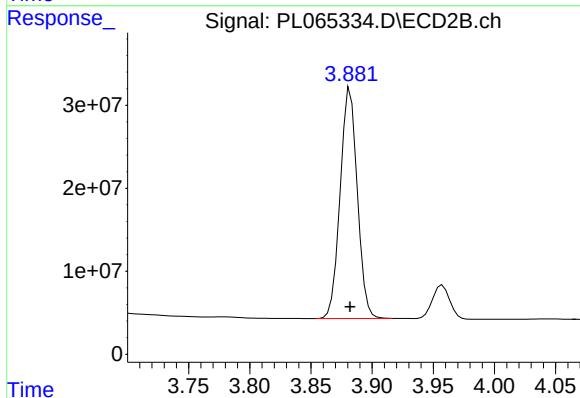


#1 Tetrachloro-m-xylene

R.T.: 3.882 min
Delta R.T.: 0.000 min
Response: 271081401
Conc: 98.42 ng/ml

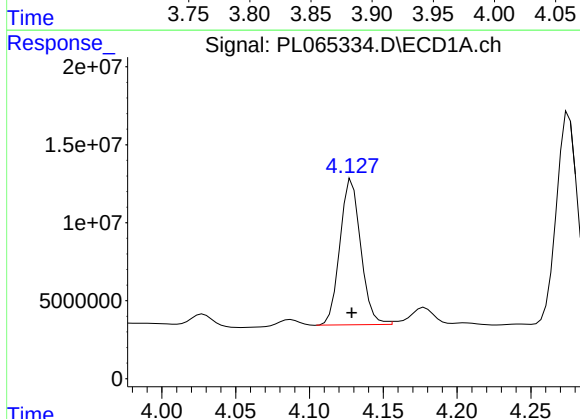


#23 Chlordane-1

R.T.: 4.129 min
Delta R.T.: 0.000 min
Response: 91724181
Conc: 971.90 ng/ml

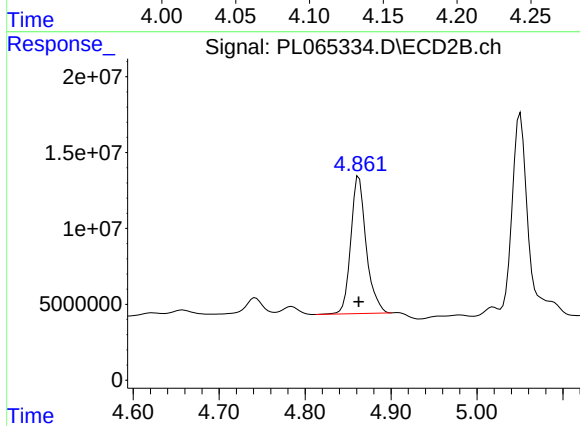

#23 Chlordane-1


R.T.: 4.863 min
Delta R.T.: 0.000 min
Response: 112810872
Conc: 936.87 ng/ml

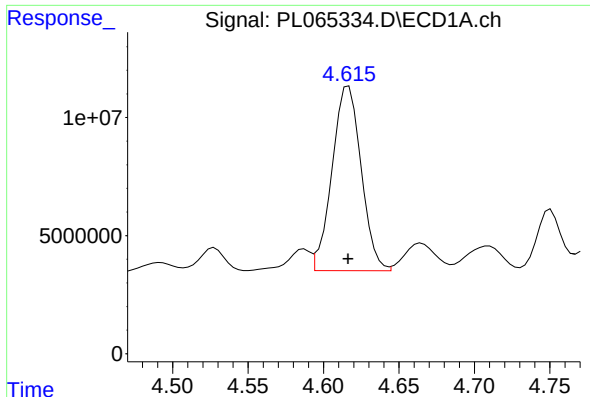

#24 Chlordane-2


R.T.: 4.617 min
Delta R.T.: 0.000 min
Response: 104893876
Conc: 967.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

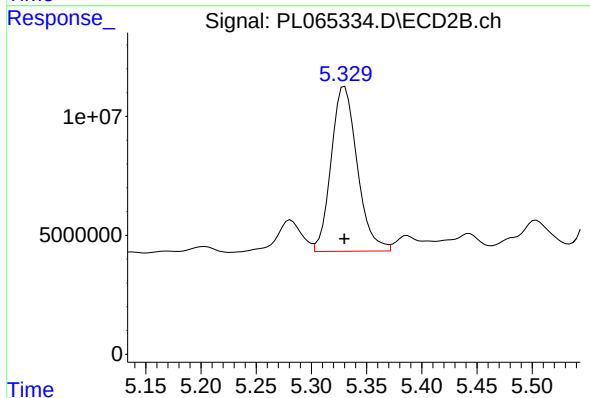


#24 Chlordane-2

R.T.: 5.330 min
Delta R.T.: 0.000 min
Response: 114052948
Conc: 968.71 ng/ml

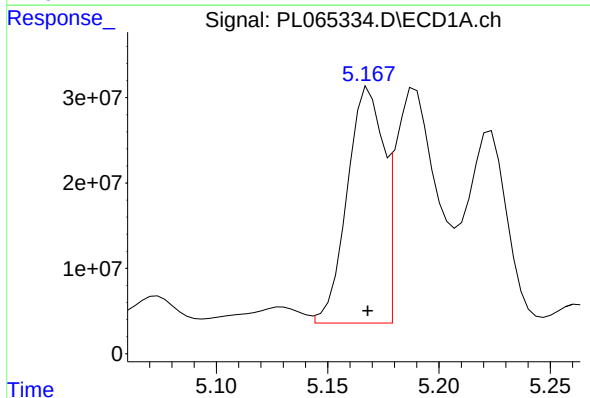


#25 Chlordane-3

R.T.: 5.169 min
Delta R.T.: 0.000 min
Response: 311673279
Conc: 996.57 ng/ml

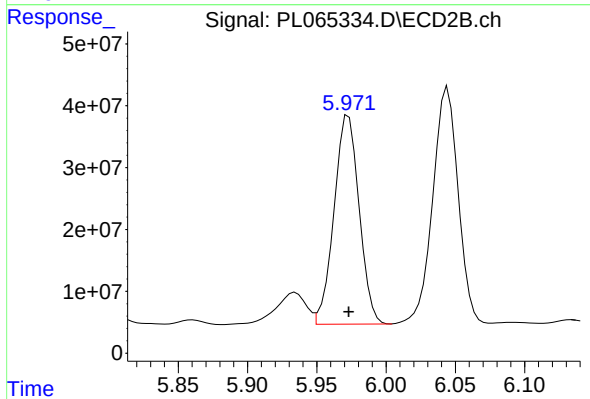

#25 Chlordane-3


R.T.: 5.973 min
Delta R.T.: 0.000 min
Response: 425472321
Conc: 982.61 ng/ml

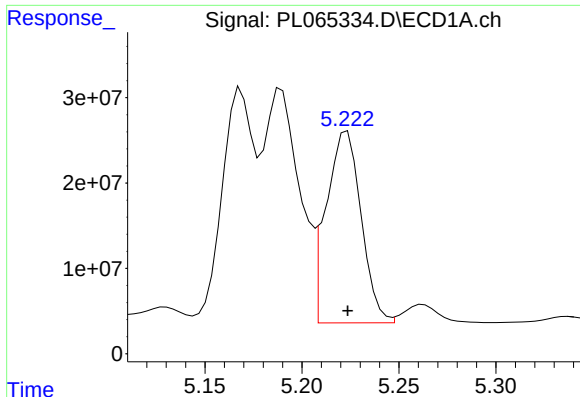

#26 Chlordane-4


R.T.: 5.223 min
Delta R.T.: 0.000 min
Response: 282147455
Conc: 1017.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

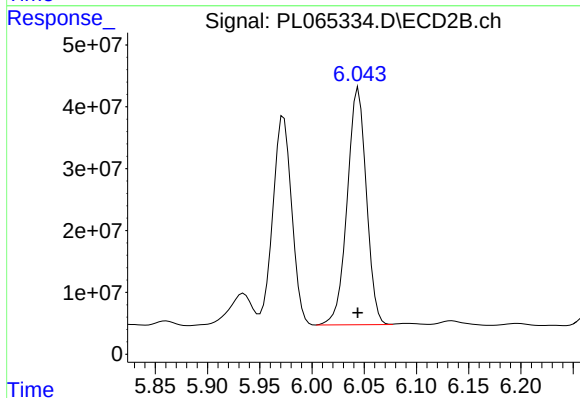


#26 Chlordane-4

R.T.: 6.044 min
Delta R.T.: 0.000 min
Response: 487767807
Conc: 977.46 ng/ml

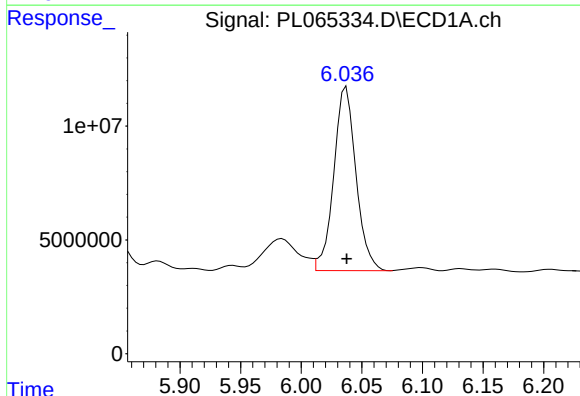


#27 Chlordane-5

R.T.: 6.037 min
Delta R.T.: 0.000 min
Response: 102366765
Conc: 1022.02 ng/ml

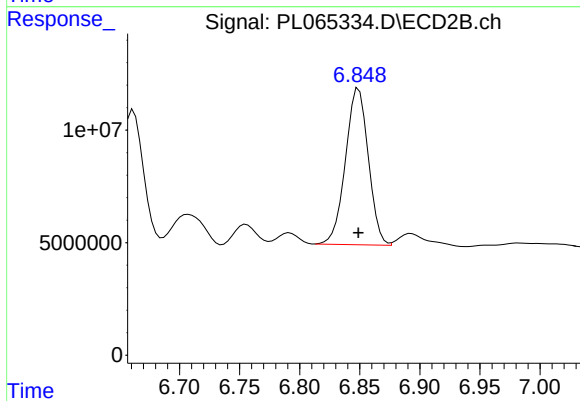

#27 Chlordane-5


R.T.: 6.849 min
Delta R.T.: 0.000 min
Response: 92219615
Conc: 983.86 ng/ml

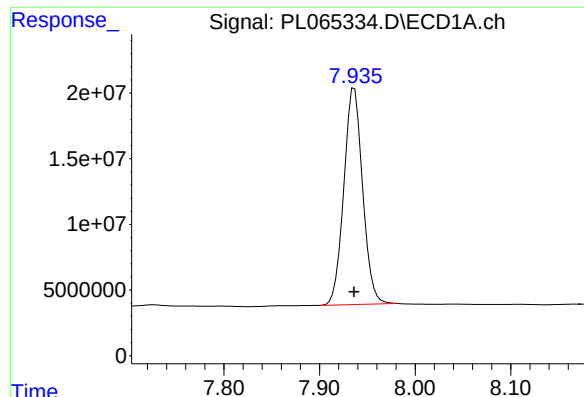

#28 Decachlorobiphenyl

R.T.: 7.936 min
Delta R.T.: 0.000 min
Response: 225532467
Conc: 96.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

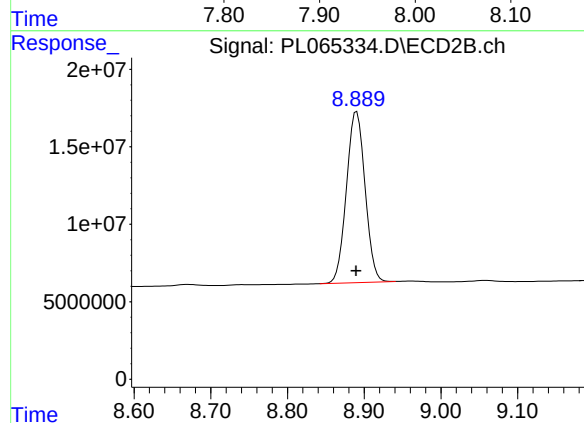

#28 Decachlorobiphenyl

R.T.: 8.890 min
Delta R.T.: 0.000 min
Response: 187261747
Conc: 95.83 ng/ml