

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031621\
 Data File : PL065336.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2021 18:02
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 04:26:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031621.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 17 04:25:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.292	3.882	128.7E6	137.7E6	50.000	50.000
28)	SA Decachlor...	7.936	8.889	117.2E6	97704405	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.129	4.862	47187840	60205959	500.000	500.000
24)	Chlordane-2	4.616	5.330	54229953	58868364	500.000	500.000
25)	Chlordane-3	5.168	5.973	156.4E6	216.5E6	500.000	500.000
26)	Chlordane-4	5.224	6.044	138.6E6	249.5E6	500.000	500.000
27)	Chlordane-5	6.037	6.849	50080458	46866110	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031621\
Data File : PL065336.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2021 18:02
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 04:26:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031621.M
Quant Title : GC Extractables
QLast Update : Wed Mar 17 04:25:32 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

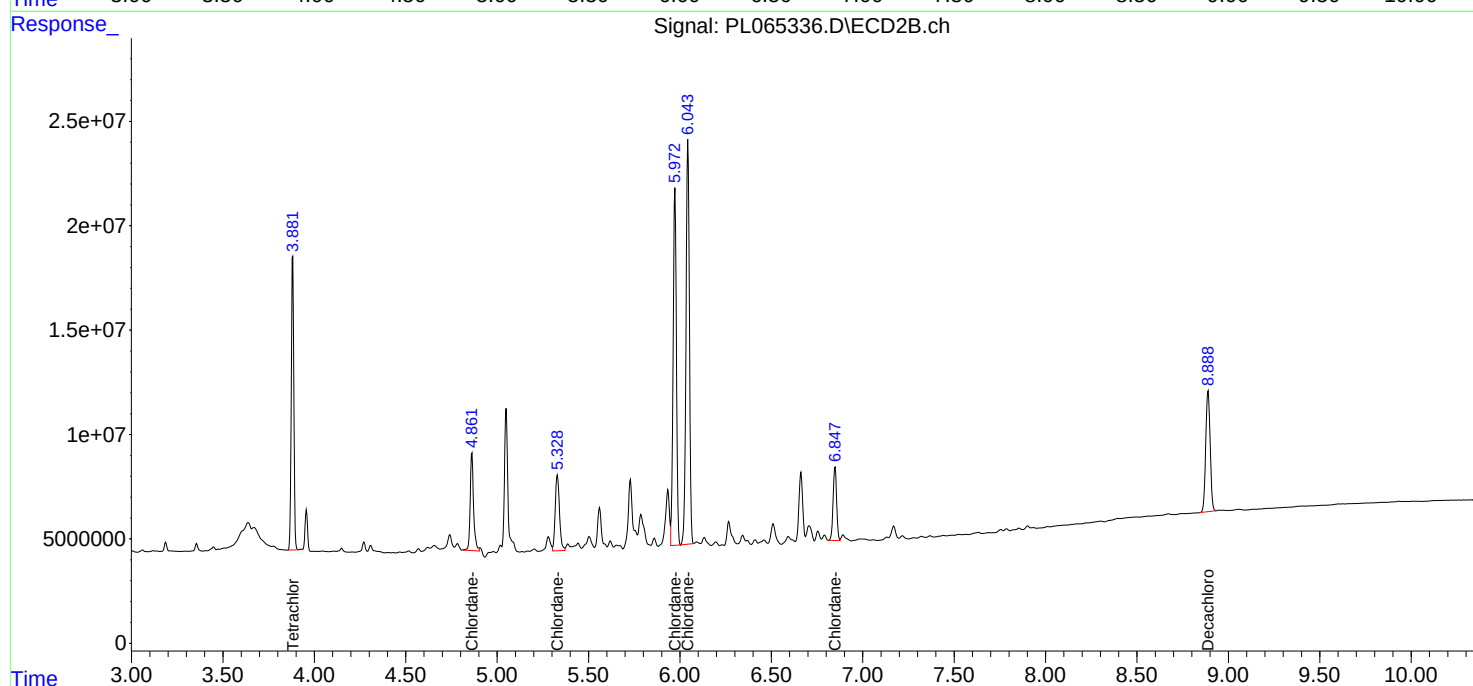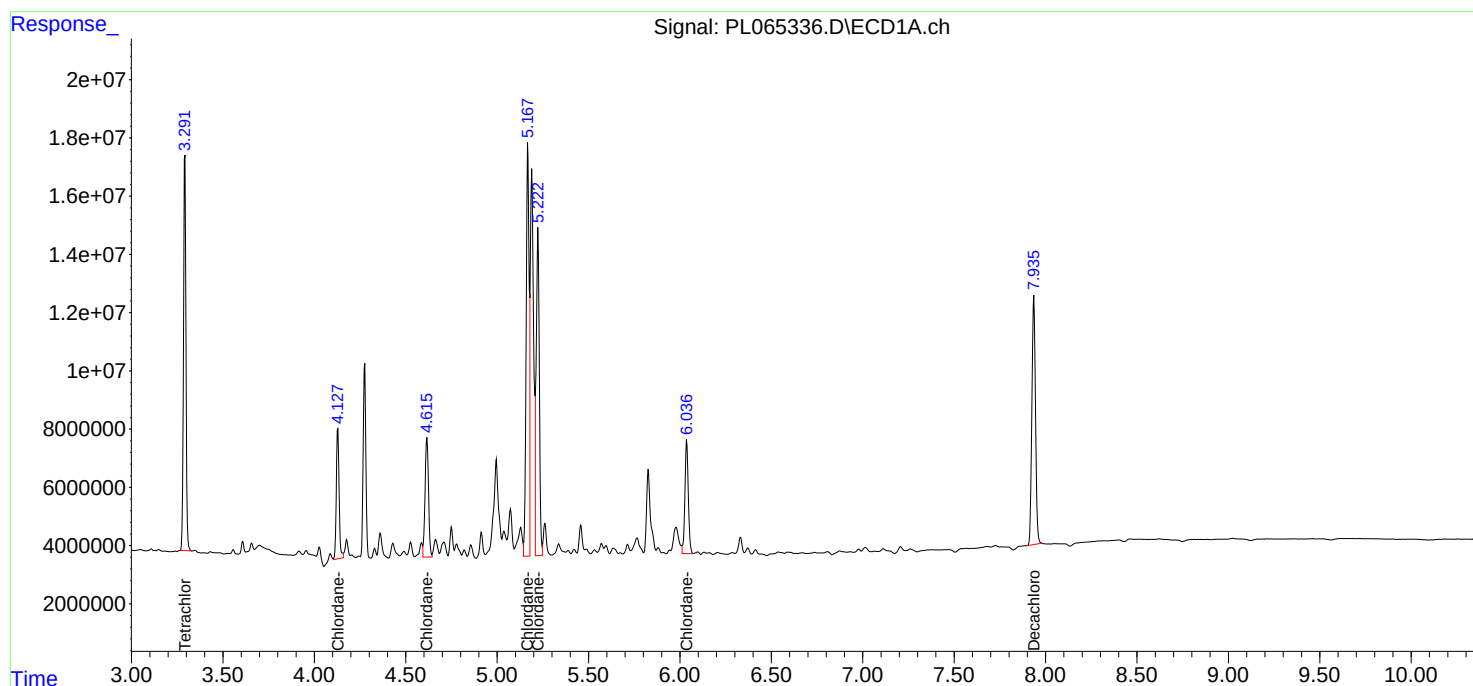


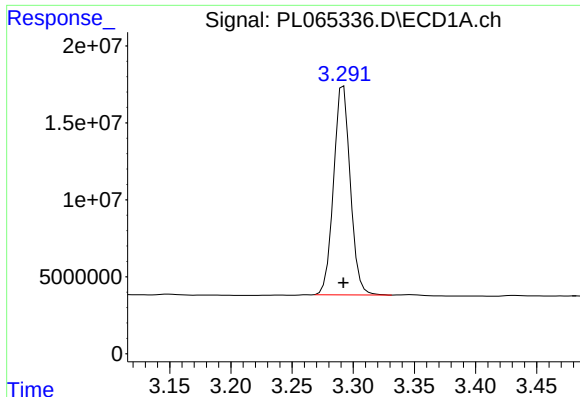

#1 Tetrachloro-m-xylene


R.T.: 3.292 min
Delta R.T.: 0.000 min
Response: 128732177
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

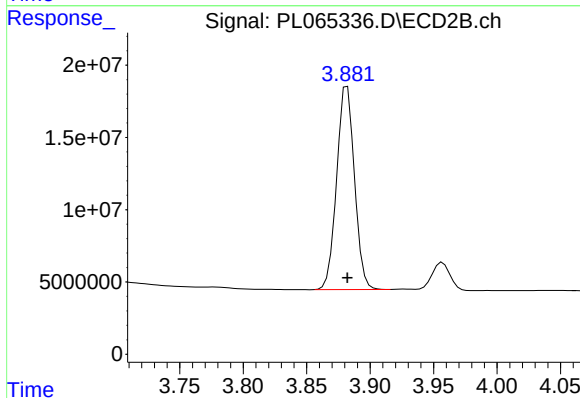


#1 Tetrachloro-m-xylene

R.T.: 3.882 min
Delta R.T.: 0.000 min
Response: 137715602
Conc: 50.00 ng/ml

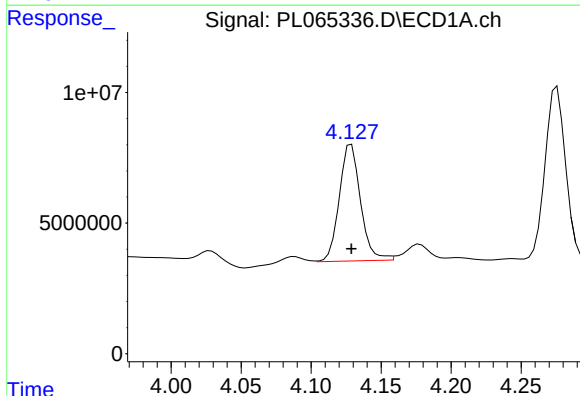


#23 Chlordane-1

R.T.: 4.129 min
Delta R.T.: 0.000 min
Response: 47187840
Conc: 500.00 ng/ml

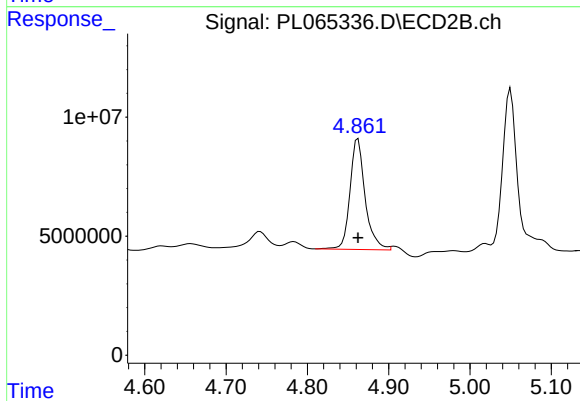

#23 Chlordane-1


R.T.: 4.862 min
Delta R.T.: 0.000 min
Response: 60205959
Conc: 500.00 ng/ml

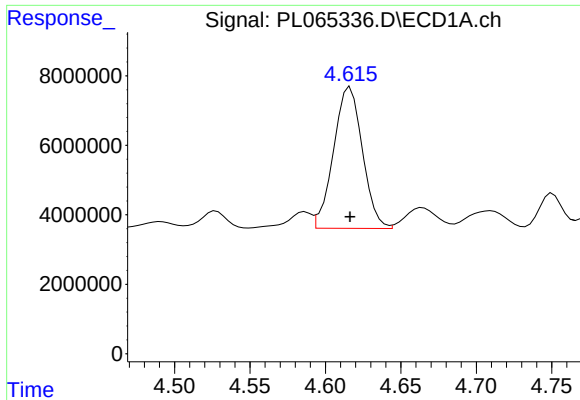

#24 Chlordane-2


R.T.: 4.616 min
Delta R.T.: 0.000 min
Response: 54229953
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

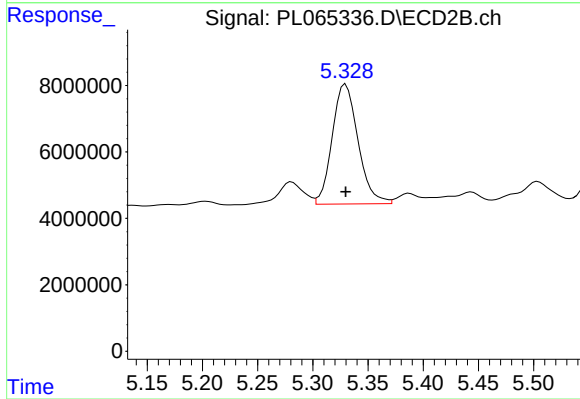


#24 Chlordane-2

R.T.: 5.330 min
Delta R.T.: 0.000 min
Response: 58868364
Conc: 500.00 ng/ml

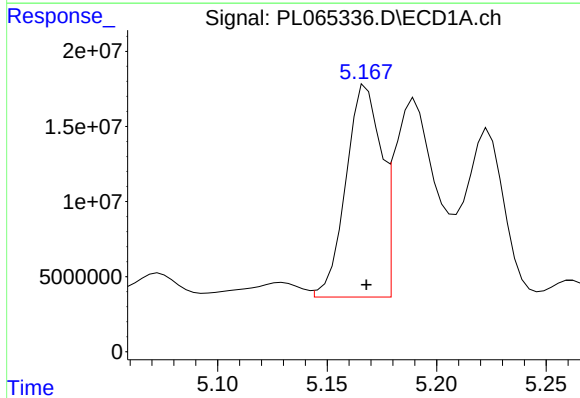


#25 Chlordane-3

R.T.: 5.168 min
Delta R.T.: 0.000 min
Response: 156372987
Conc: 500.00 ng/ml

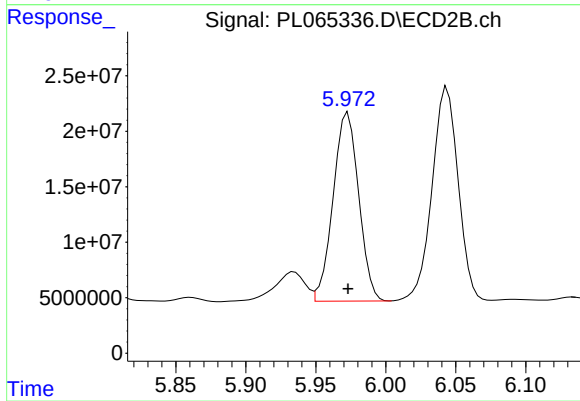

#25 Chlordane-3


R.T.: 5.973 min
Delta R.T.: 0.000 min
Response: 216501713
Conc: 500.00 ng/ml

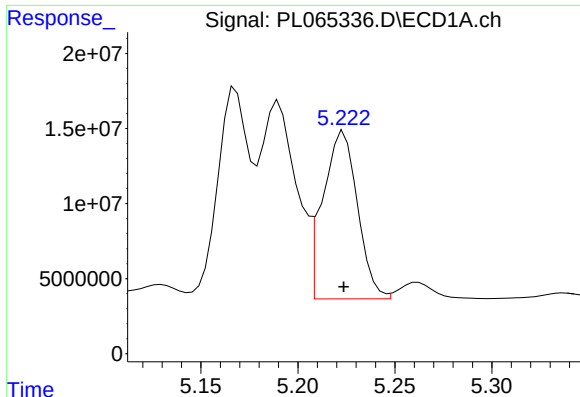

#26 Chlordane-4


R.T.: 5.224 min
Delta R.T.: 0.000 min
Response: 138619075
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

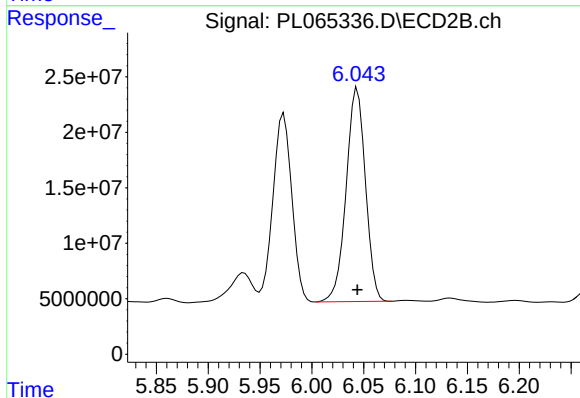


#26 Chlordane-4

R.T.: 6.044 min
Delta R.T.: 0.000 min
Response: 249507257
Conc: 500.00 ng/ml

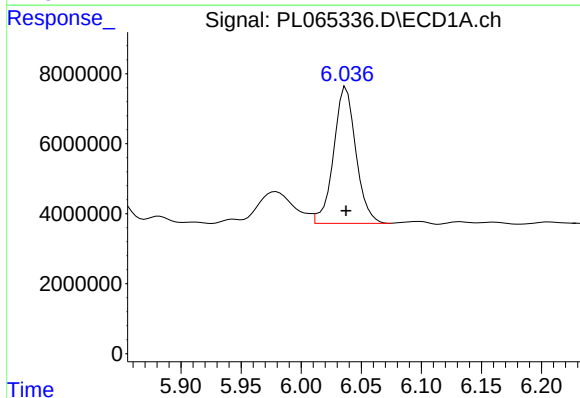


#27 Chlordane-5

R.T.: 6.037 min
Delta R.T.: 0.000 min
Response: 50080458
Conc: 500.00 ng/ml

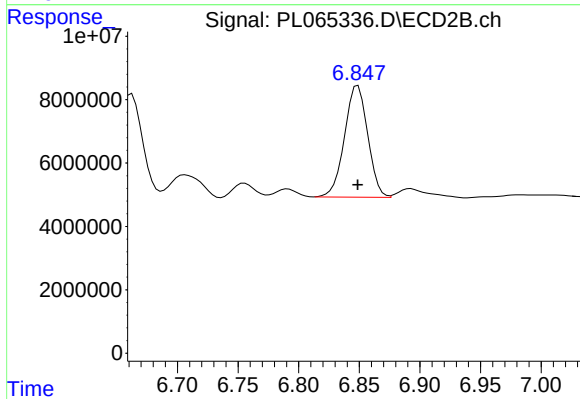

#27 Chlordane-5

R.T.: 6.849 min
Delta R.T.: 0.000 min
Response: 46866110
Conc: 500.00 ng/ml

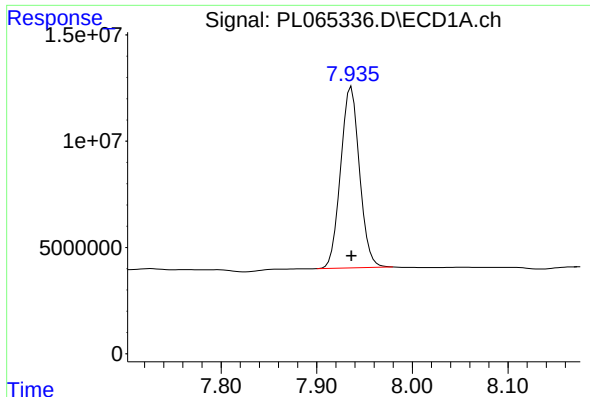

#28 Decachlorobiphenyl


R.T.: 7.936 min

Delta R.T.: 0.000 min

Response: 117175859

Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

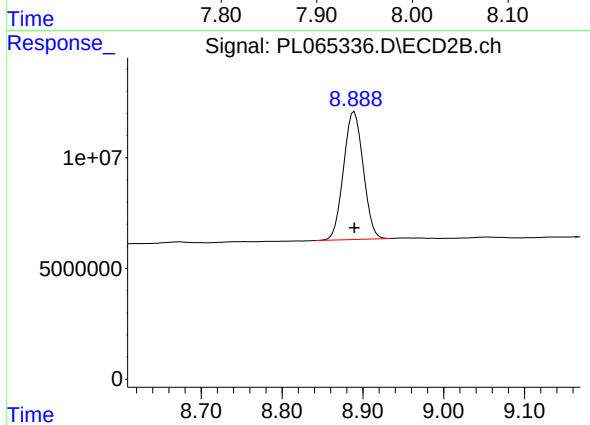

#28 Decachlorobiphenyl

R.T.: 8.889 min

Delta R.T.: 0.000 min

Response: 97704405

Conc: 50.00 ng/ml