

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031621\
 Data File : PL065337.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2021 18:16
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 04:26:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031621.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 17 04:25:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.292	3.882	61256556	69293650	23.792	25.158
28)	SA Decachlor...	7.937	8.890	60914437	50230239	25.993	25.705
Target Compounds							
23)	Chlordane-1	4.129	4.862	24663668	31237239	261.335	259.420
24)	Chlordane-2	4.616	5.330	27934293	29364675	257.554	249.410
25)	Chlordane-3	5.168	5.973	76058004	108.8E6	243.194	251.280
26)	Chlordane-4	5.223	6.044	69711964	126.2E6	251.452	252.925
27)	Chlordane-5	6.037	6.849	24558163	22888966	245.187	244.195



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031621\
Data File : PL065337.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2021 18:16
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 04:26:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031621.M
Quant Title : GC Extractables
QLast Update : Wed Mar 17 04:25:32 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

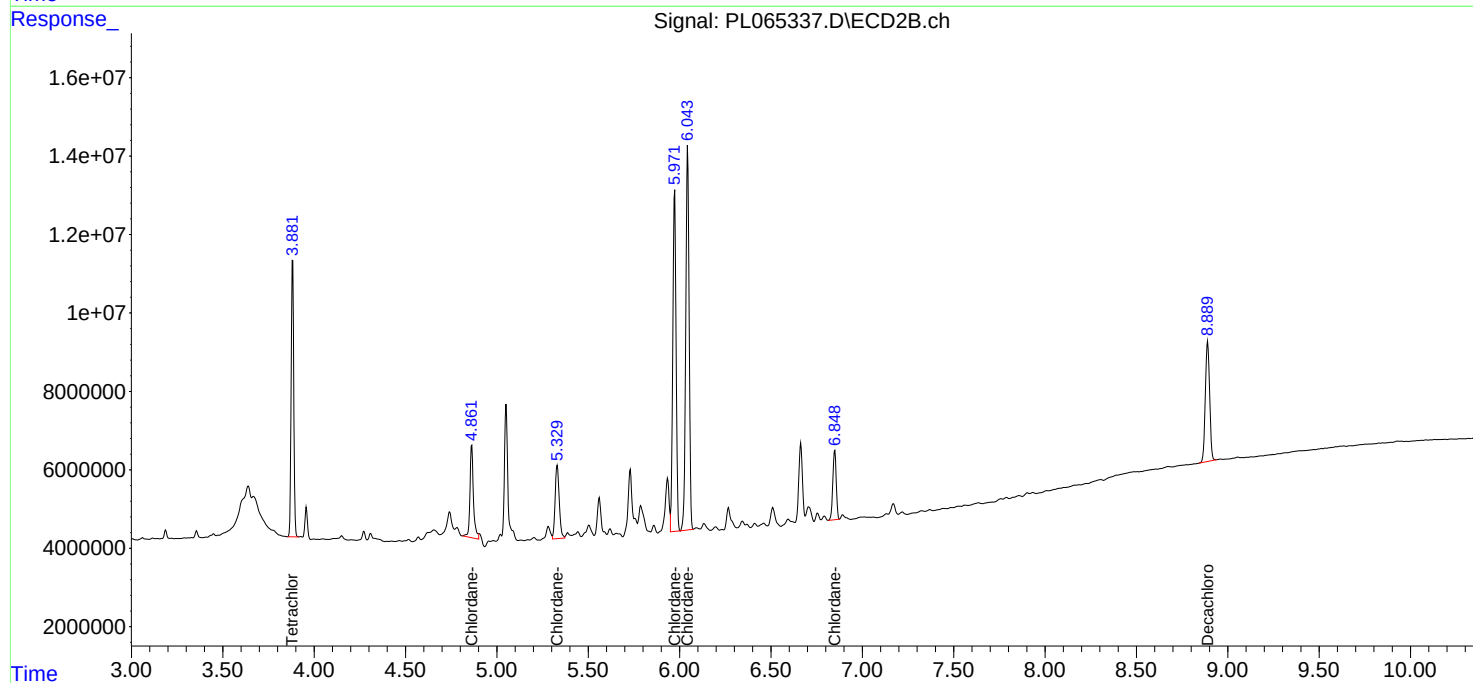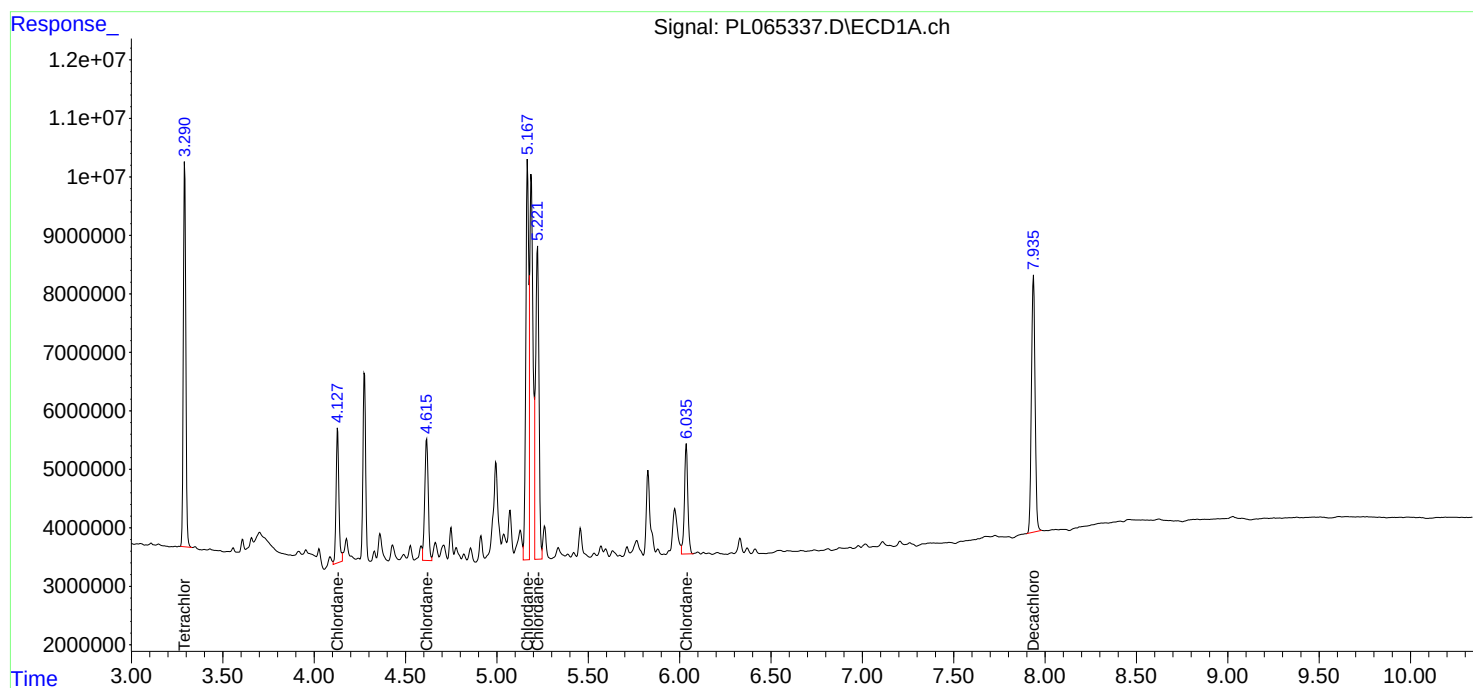


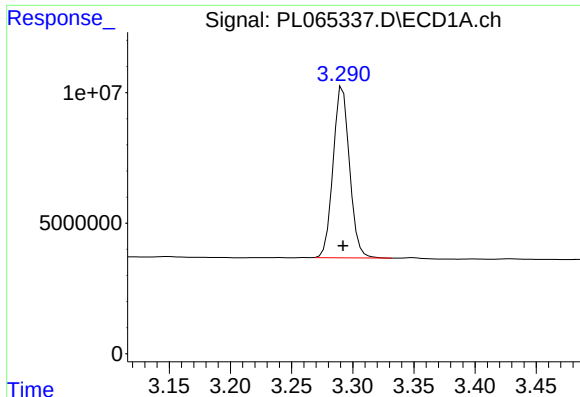

#1 Tetrachloro-m-xylene


R.T.: 3.292 min
Delta R.T.: 0.000 min
Response: 61256556
Conc: 23.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

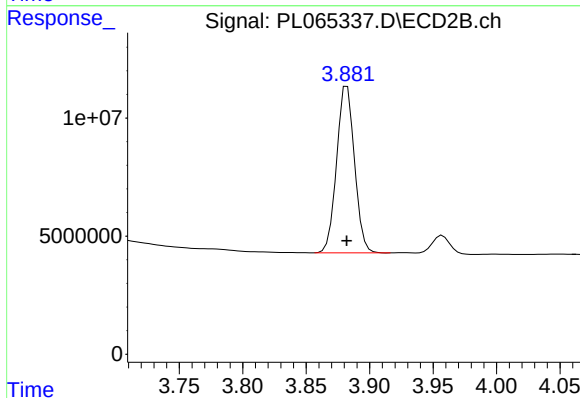


#1 Tetrachloro-m-xylene

R.T.: 3.882 min
Delta R.T.: 0.000 min
Response: 69293650
Conc: 25.16 ng/ml

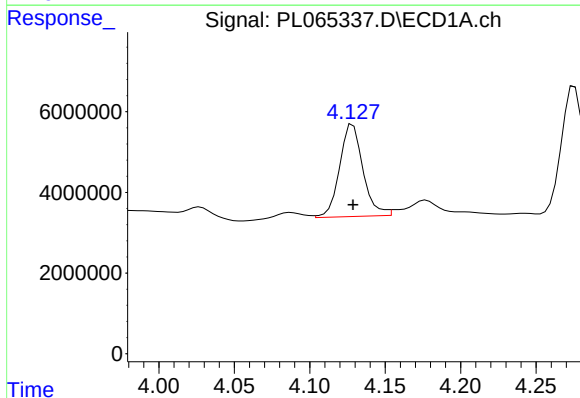


#23 Chlordane-1

R.T.: 4.129 min
Delta R.T.: 0.000 min
Response: 24663668
Conc: 261.33 ng/ml

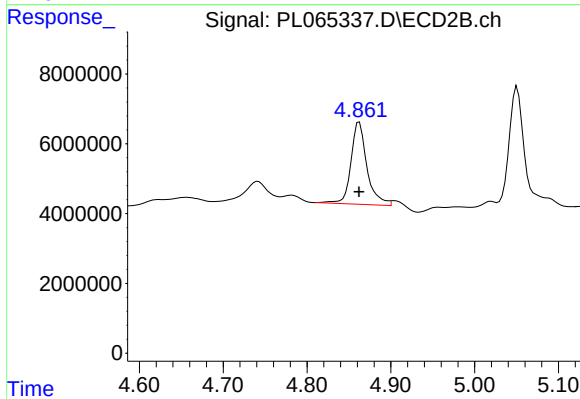

#23 Chlordane-1


R.T.: 4.862 min
Delta R.T.: 0.000 min
Response: 31237239
Conc: 259.42 ng/ml

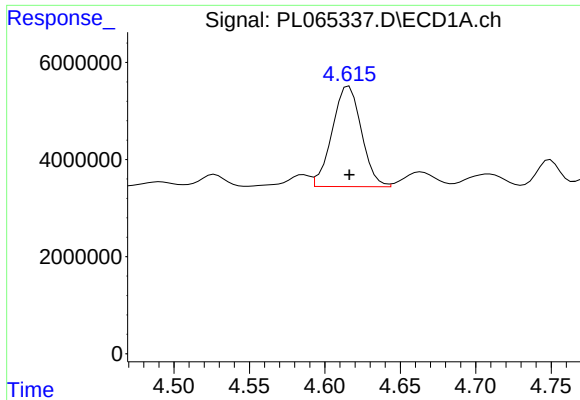

#24 Chlordane-2


R.T.: 4.616 min
Delta R.T.: 0.000 min
Response: 27934293
Conc: 257.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

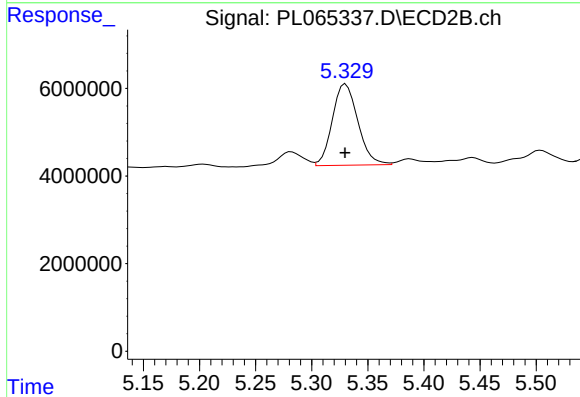


#24 Chlordane-2

R.T.: 5.330 min
Delta R.T.: 0.000 min
Response: 29364675
Conc: 249.41 ng/ml

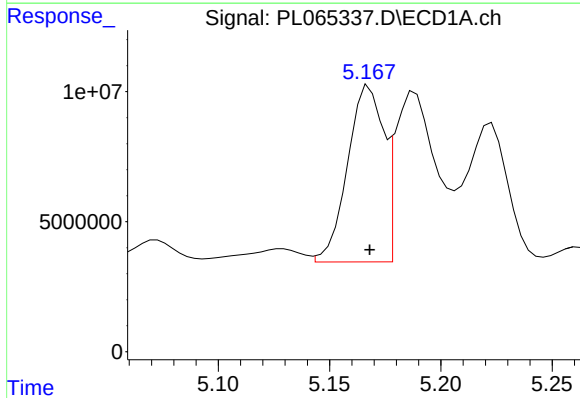


#25 Chlordane-3

R.T.: 5.168 min
Delta R.T.: 0.000 min
Response: 76058004
Conc: 243.19 ng/ml

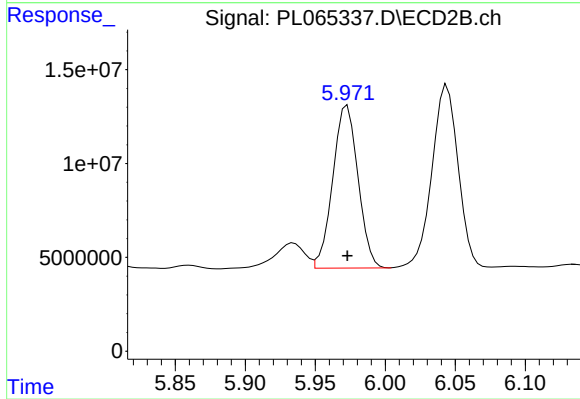

#25 Chlordane-3


R.T.: 5.973 min
Delta R.T.: 0.000 min
Response: 108805277
Conc: 251.28 ng/ml

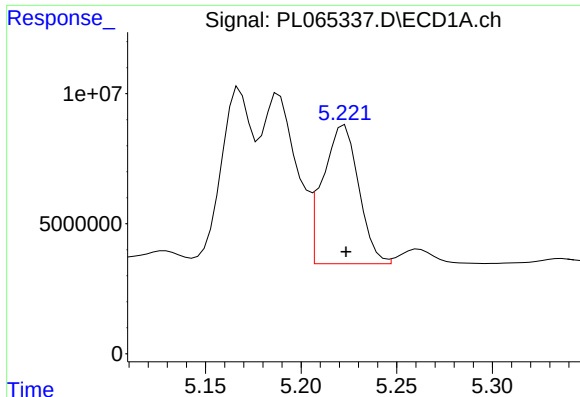

#26 Chlordane-4


R.T.: 5.223 min
Delta R.T.: 0.000 min
Response: 69711964
Conc: 251.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

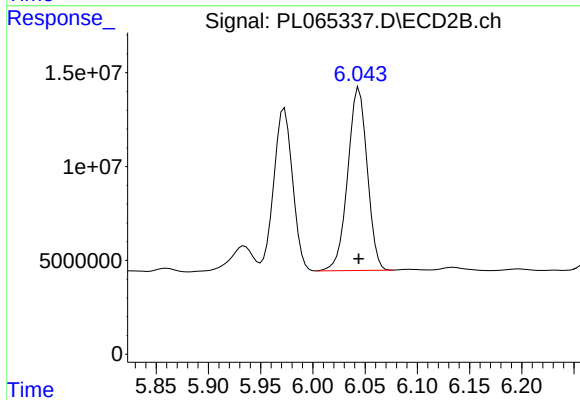


#26 Chlordane-4

R.T.: 6.044 min
Delta R.T.: 0.000 min
Response: 126213491
Conc: 252.93 ng/ml

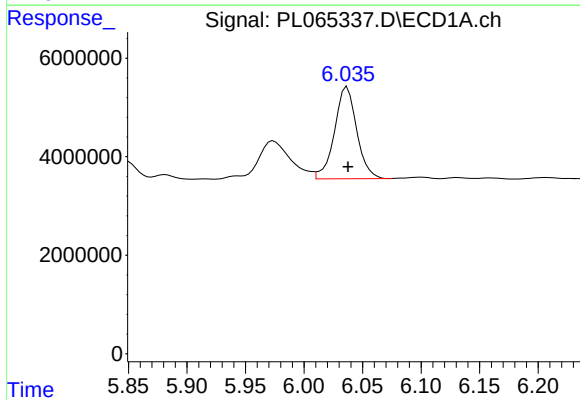


#27 Chlordane-5

R.T.: 6.037 min
Delta R.T.: 0.000 min
Response: 24558163
Conc: 245.19 ng/ml

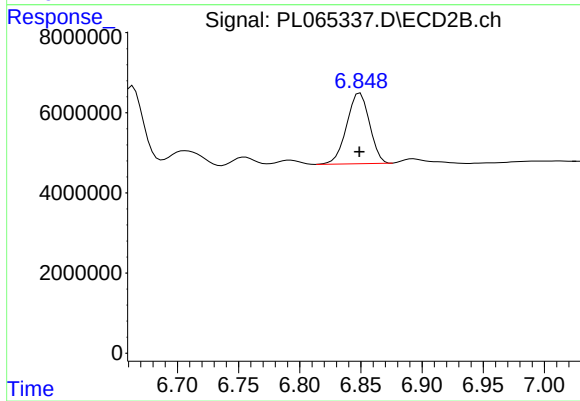

#27 Chlordane-5


R.T.: 6.849 min
Delta R.T.: 0.000 min
Response: 22888966
Conc: 244.20 ng/ml

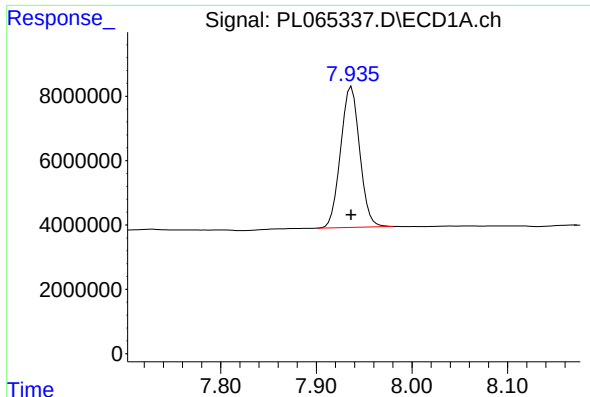

#28 Decachlorobiphenyl

R.T.: 7.937 min
Delta R.T.: 0.000 min
Response: 60914437
Conc: 25.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

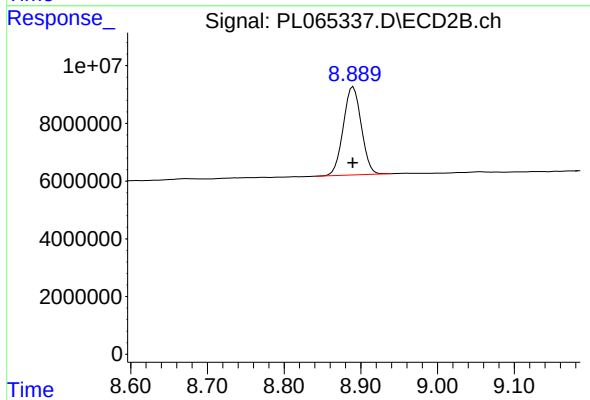

#28 Decachlorobiphenyl

R.T.: 8.890 min
Delta R.T.: 0.000 min
Response: 50230239
Conc: 25.71 ng/ml