

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031621\
 Data File : PL065345.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2021 20:11
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL031621

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 05:05:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031621.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 17 04:35:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.292	3.882	127.7E6	138.7E6	52.537	48.045
28)	SA Decachlor...	7.936	8.890	120.2E6	98527474	48.966	48.434
Target Compounds							
23)	Chlordane-1	4.129	4.863	47990001	61355973	490.503	538.012
24)	Chlordane-2	4.617	5.330	55759212	60177863	503.447	503.079
25)	Chlordane-3	5.168	5.974	157.5E6	217.8E6	506.617	495.600
26)	Chlordane-4	5.224	6.045	140.3E6	250.8E6	505.898	493.775
27)	Chlordane-5	6.038	6.850	51053478	46846222	503.995	508.801



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031621\
Data File : PL065345.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2021 20:11
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL031621

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 05:05:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031621.M
Quant Title : GC Extractables
QLast Update : Wed Mar 17 04:35:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

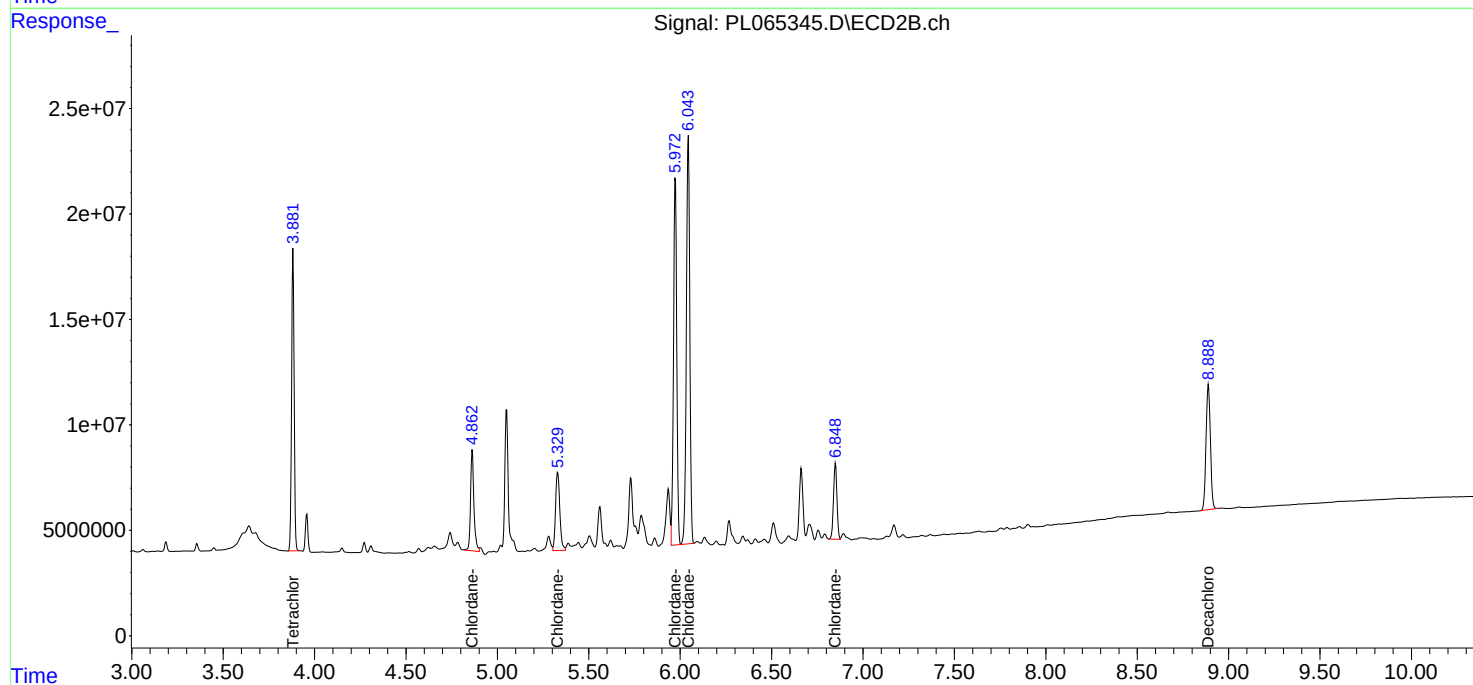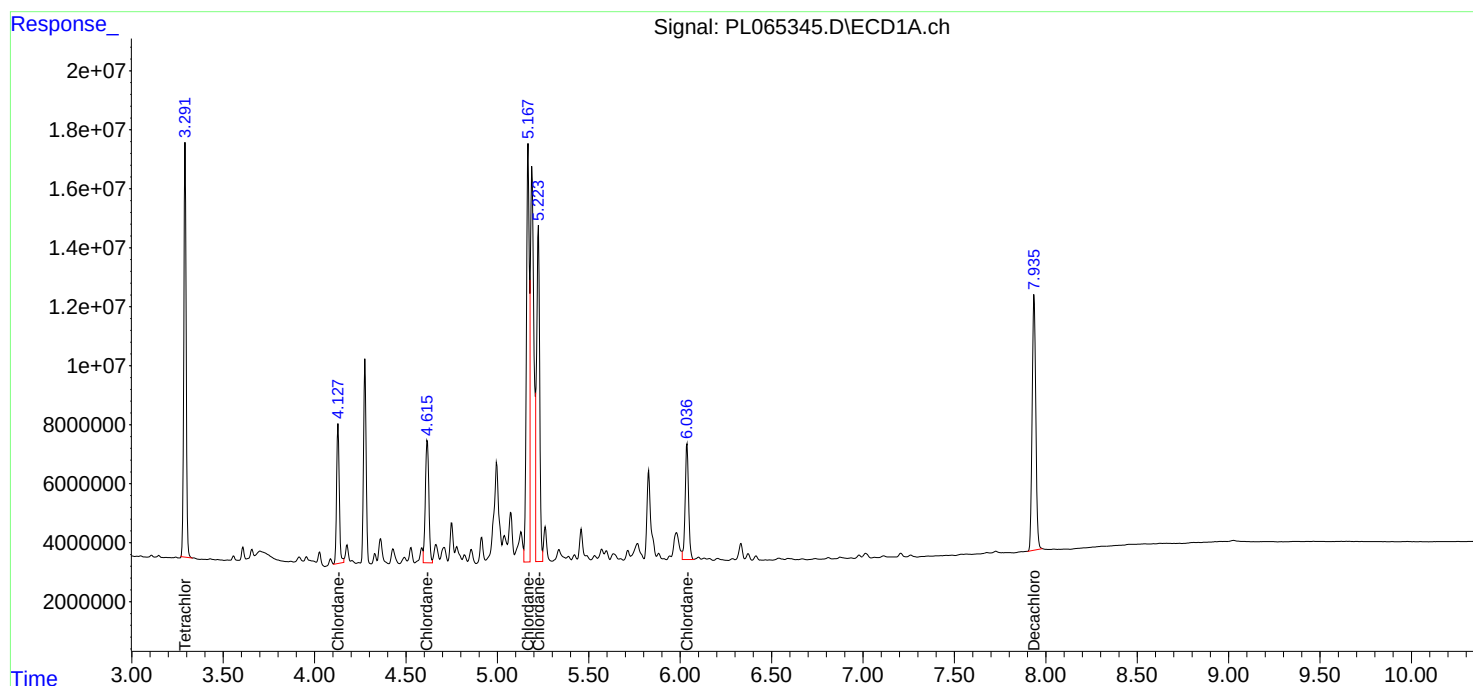


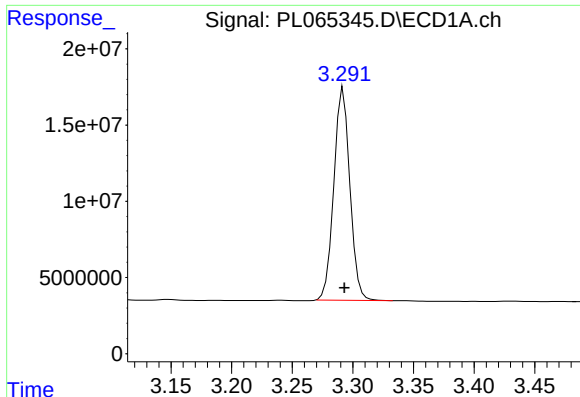

#1 Tetrachloro-m-xylene


R.T.: 3.292 min
Delta R.T.: 0.000 min
Response: 127749298
Conc: 52.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL031621

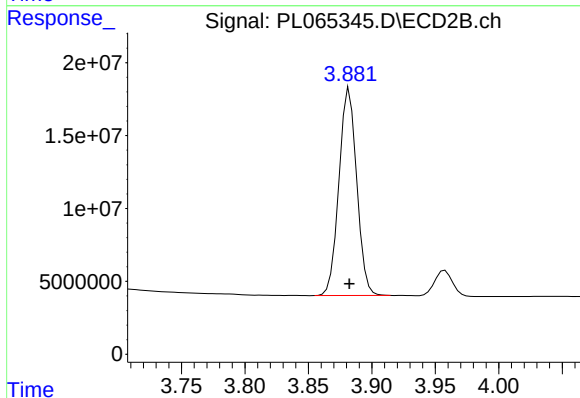


#1 Tetrachloro-m-xylene

R.T.: 3.882 min
Delta R.T.: 0.000 min
Response: 138700516
Conc: 48.05 ng/ml

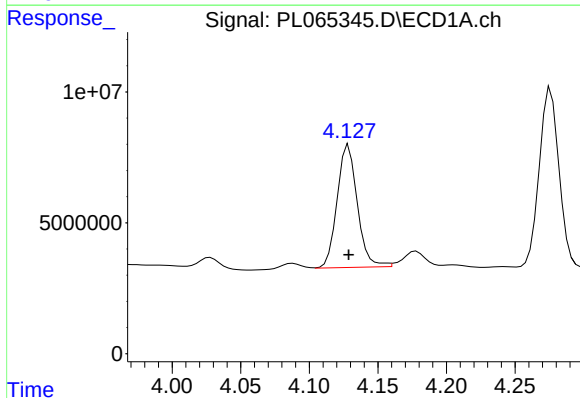


#23 Chlordane-1

R.T.: 4.129 min
Delta R.T.: 0.000 min
Response: 47990001
Conc: 490.50 ng/ml

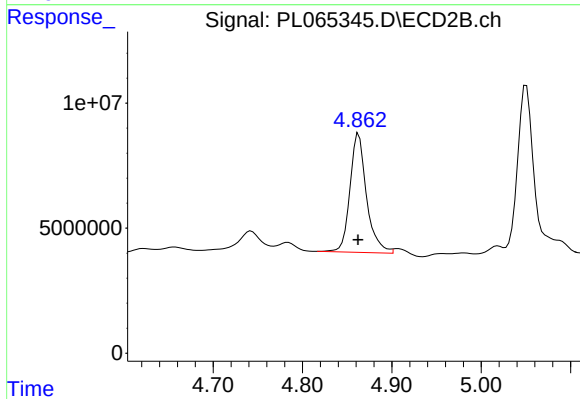

#23 Chlordane-1


R.T.: 4.863 min
Delta R.T.: 0.000 min
Response: 61355973
Conc: 538.01 ng/ml

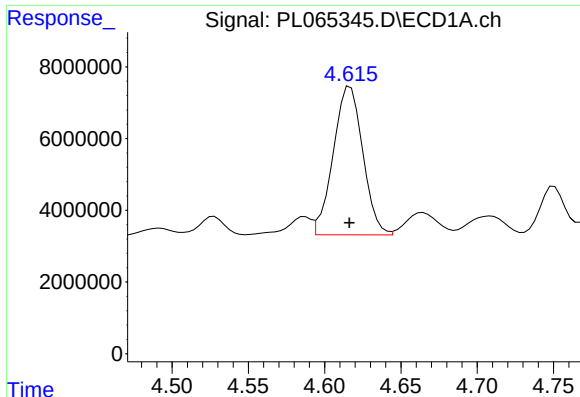

#24 Chlordane-2


R.T.: 4.617 min
Delta R.T.: 0.000 min
Response: 55759212
Conc: 503.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL031621

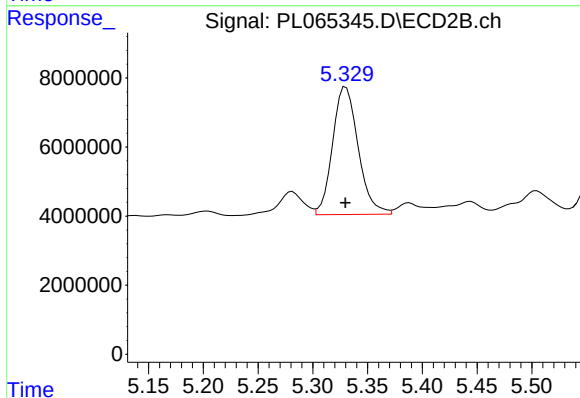


#24 Chlordane-2

R.T.: 5.330 min
Delta R.T.: 0.000 min
Response: 60177863
Conc: 503.08 ng/ml

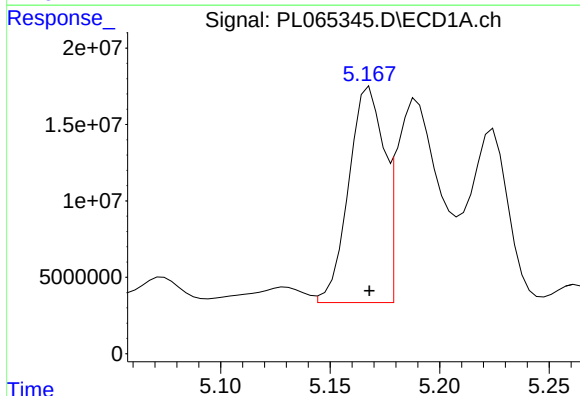


#25 Chlordane-3

R.T.: 5.168 min
Delta R.T.: 0.000 min
Response: 157483197
Conc: 506.62 ng/ml

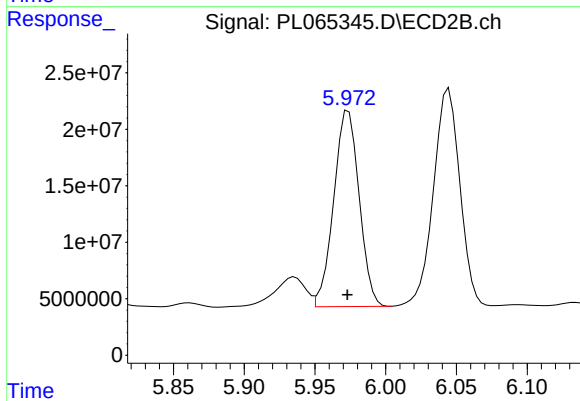

#25 Chlordane-3


R.T.: 5.974 min
Delta R.T.: 0.000 min
Response: 217817938
Conc: 495.60 ng/ml

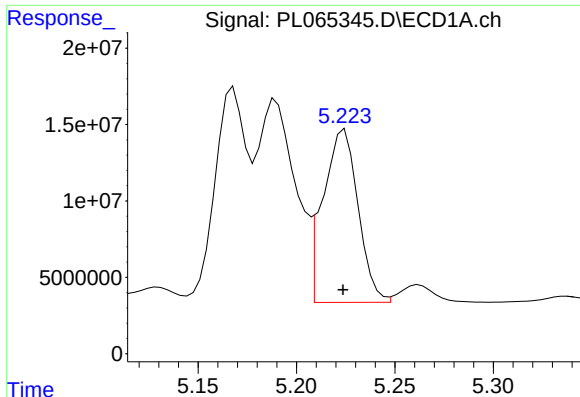

#26 Chlordane-4


R.T.: 5.224 min
Delta R.T.: 0.000 min
Response: 140339605
Conc: 505.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL031621

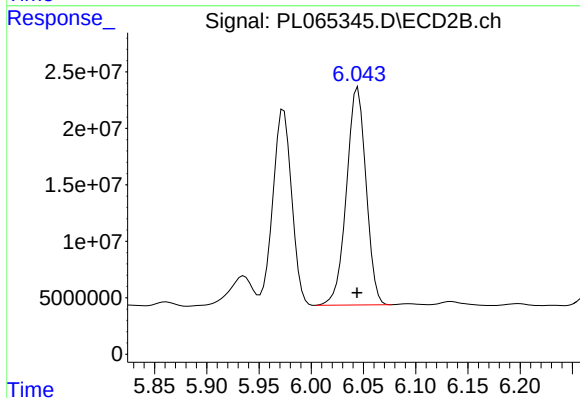


#26 Chlordane-4

R.T.: 6.045 min
Delta R.T.: 0.000 min
Response: 250761057
Conc: 493.77 ng/ml

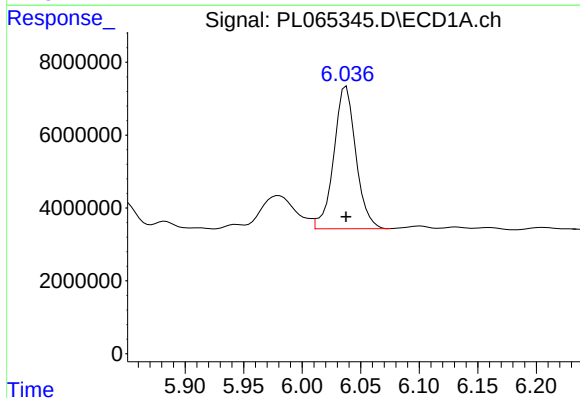


#27 Chlordane-5

R.T.: 6.038 min
Delta R.T.: 0.000 min
Response: 51053478
Conc: 504.00 ng/ml

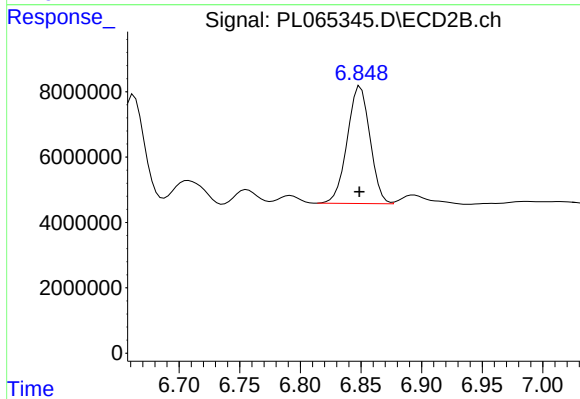

#27 Chlordane-5

R.T.: 6.850 min
Delta R.T.: 0.000 min
Response: 46846222
Conc: 508.80 ng/ml

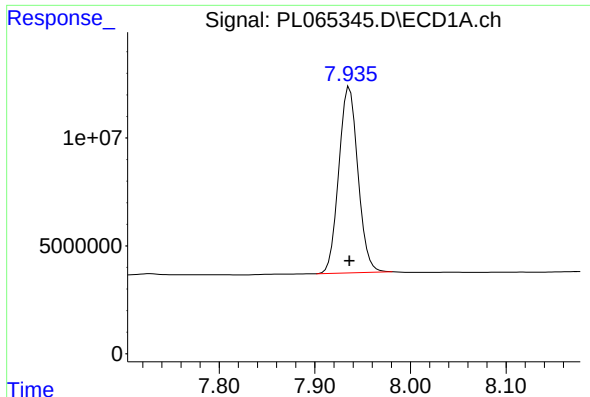

#28 Decachlorobiphenyl


R.T.: 7.936 min

Delta R.T.: 0.000 min

Response: 120231503

Conc: 48.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL031621

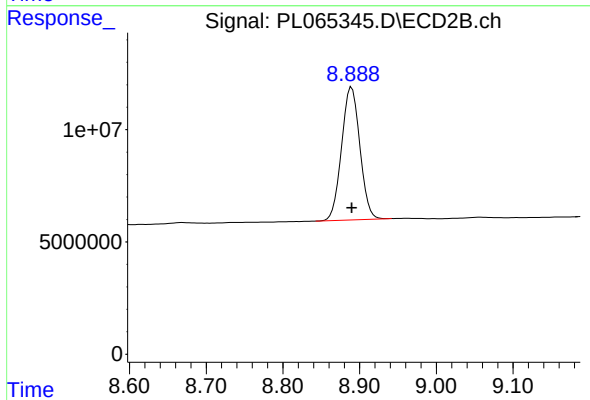

#28 Decachlorobiphenyl

R.T.: 8.890 min

Delta R.T.: 0.000 min

Response: 98527474

Conc: 48.43 ng/ml