

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031621\
 Data File : PL065360.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2021 23:45
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 05:05:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031621.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 17 04:35:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.292	3.882	123.8E6	132.8E6	50.914	46.008
28)	SA Decachlor...	7.936	8.889	113.9E6	94907833	46.384	46.655
Target Compounds							
23)	Chlordane-1	4.129	4.862	45063702	57085734	460.594	500.567
24)	Chlordane-2	4.617	5.330	52400296	55215482	473.119	461.594
25)	Chlordane-3	5.169	5.973	148.3E6	205.1E6	477.223	466.688
26)	Chlordane-4	5.224	6.044	131.9E6	236.7E6	475.332	466.088
27)	Chlordane-5	6.038	6.849	46966964	43570846	463.653	473.226



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031621\
Data File : PL065360.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2021 23:45
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 05:05:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031621.M
Quant Title : GC Extractables
QLast Update : Wed Mar 17 04:35:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

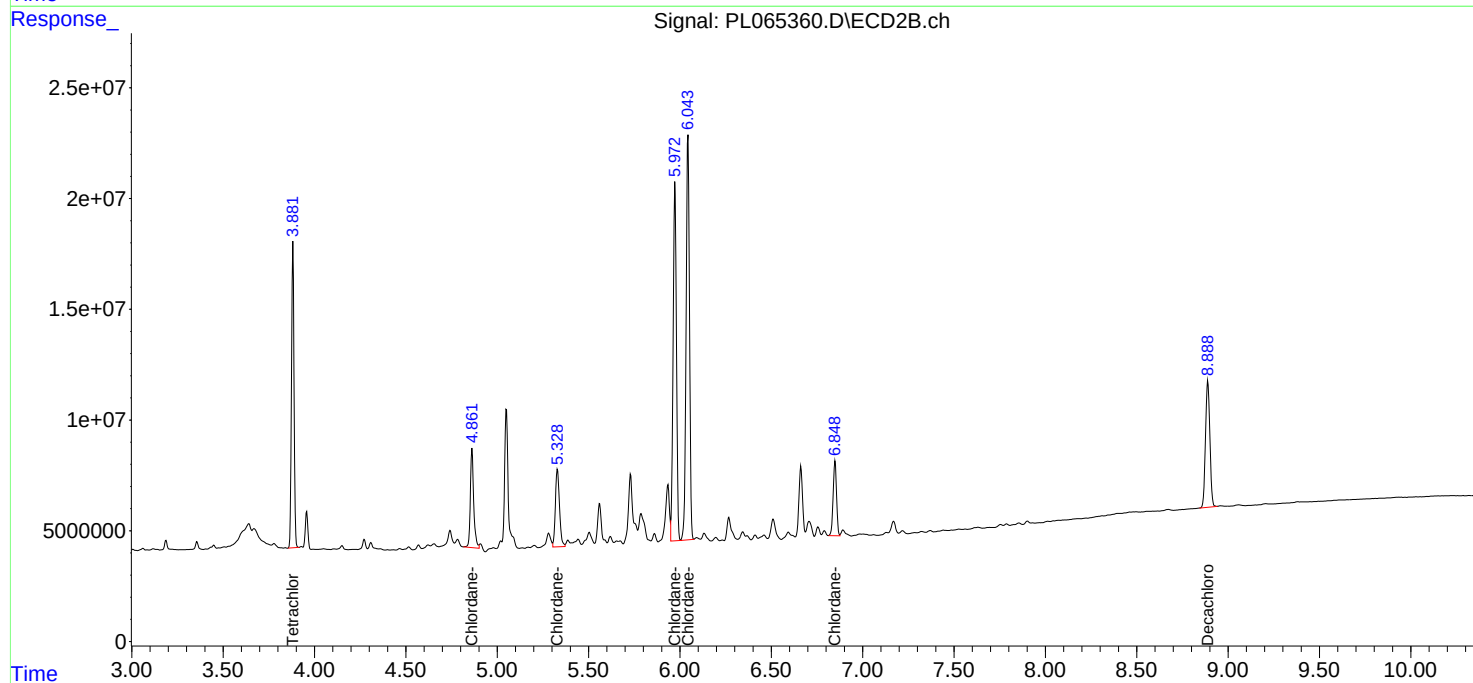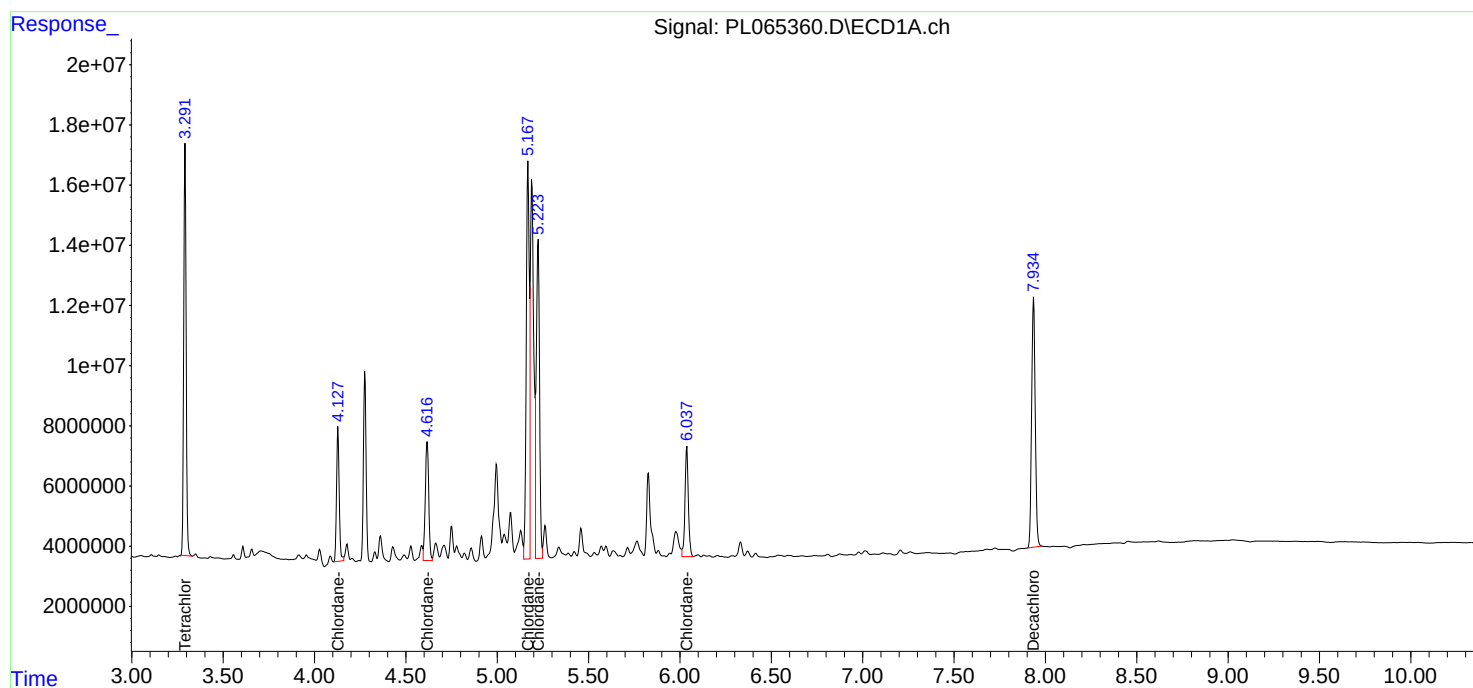


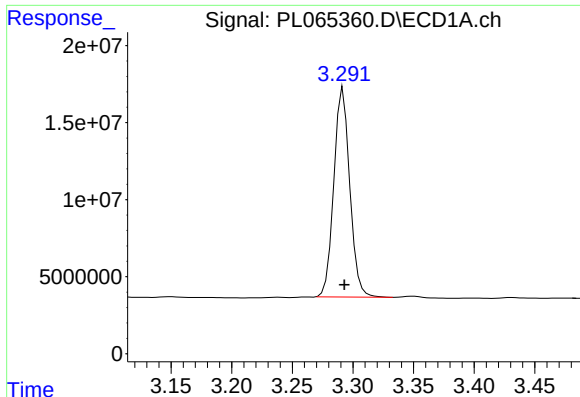

#1 Tetrachloro-m-xylene


R.T.: 3.292 min
Delta R.T.: 0.000 min
Response: 123802382
Conc: 50.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

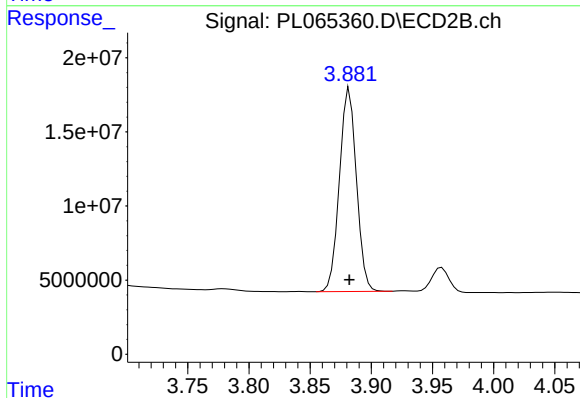


#1 Tetrachloro-m-xylene

R.T.: 3.882 min
Delta R.T.: 0.000 min
Response: 132819681
Conc: 46.01 ng/ml

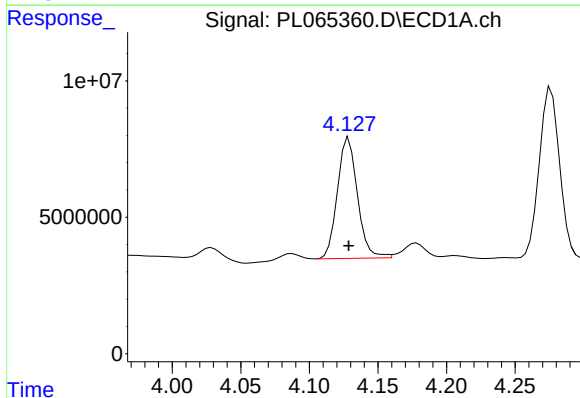


#23 Chlordane-1

R.T.: 4.129 min
Delta R.T.: 0.000 min
Response: 45063702
Conc: 460.59 ng/ml

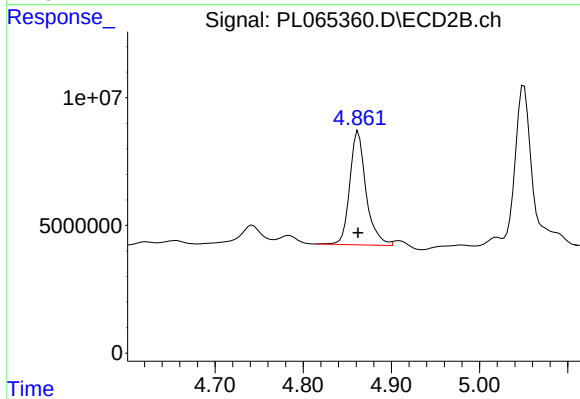

#23 Chlordane-1


R.T.: 4.862 min
Delta R.T.: 0.000 min
Response: 57085734
Conc: 500.57 ng/ml

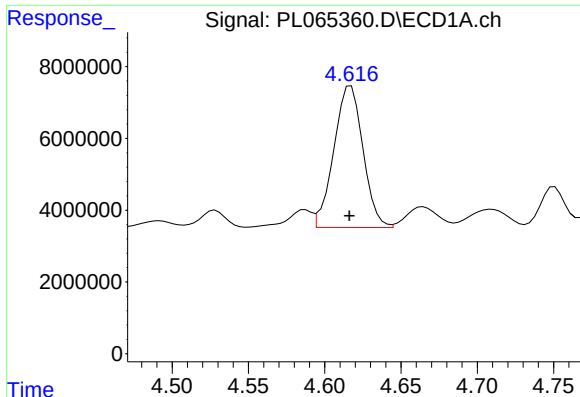

#24 Chlordane-2


R.T.: 4.617 min
Delta R.T.: 0.000 min
Response: 52400296
Conc: 473.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

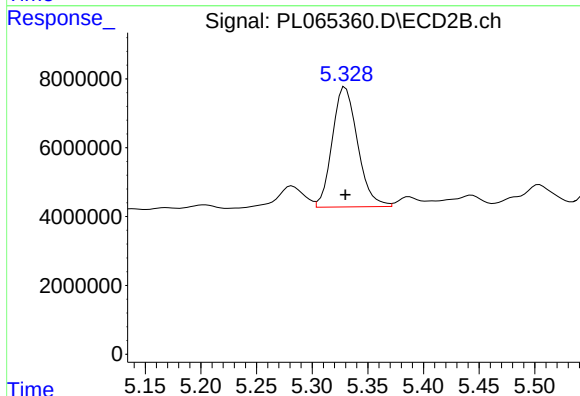


#24 Chlordane-2

R.T.: 5.330 min
Delta R.T.: 0.000 min
Response: 55215482
Conc: 461.59 ng/ml

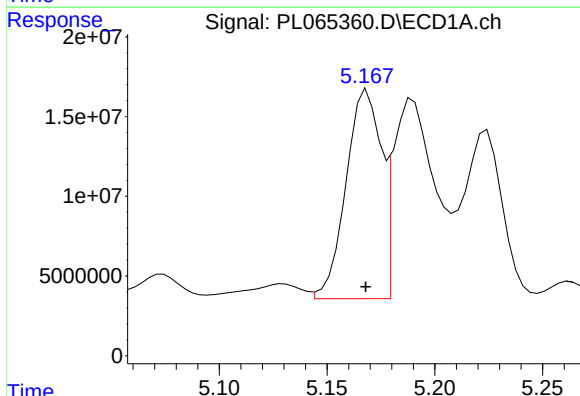


#25 Chlordane-3

R.T.: 5.169 min
Delta R.T.: 0.000 min
Response: 148345959
Conc: 477.22 ng/ml

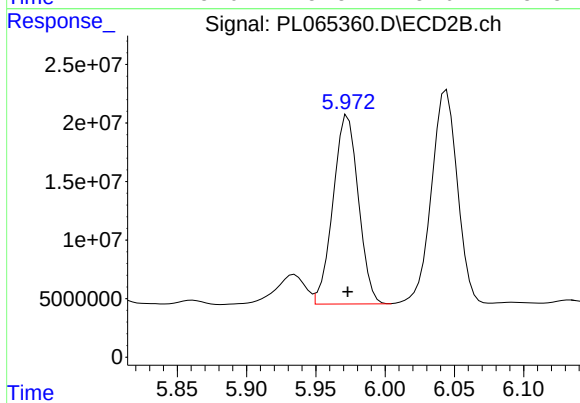

#25 Chlordane-3


R.T.: 5.973 min
Delta R.T.: 0.000 min
Response: 205111149
Conc: 466.69 ng/ml

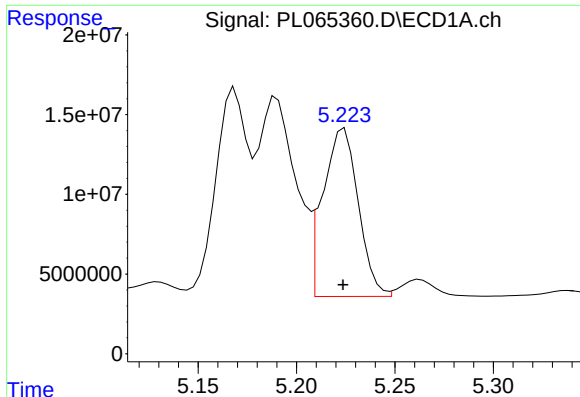

#26 Chlordane-4


R.T.: 5.224 min
Delta R.T.: 0.000 min
Response: 131860471
Conc: 475.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

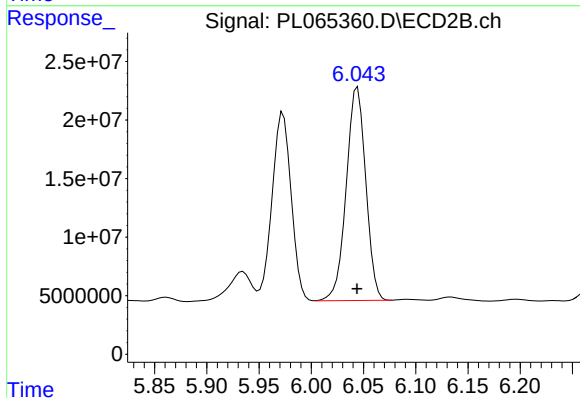


#26 Chlordane-4

R.T.: 6.044 min
Delta R.T.: 0.000 min
Response: 236700565
Conc: 466.09 ng/ml

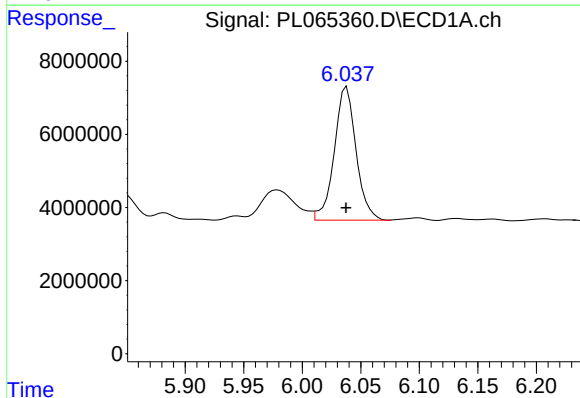


#27 Chlordane-5

R.T.: 6.038 min
Delta R.T.: 0.000 min
Response: 46966964
Conc: 463.65 ng/ml

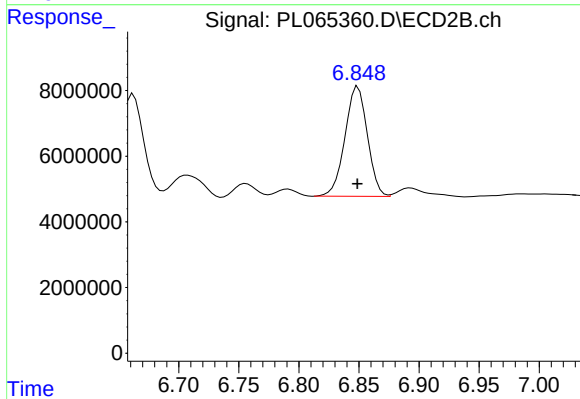

#27 Chlordane-5

R.T.: 6.849 min
Delta R.T.: 0.000 min
Response: 43570846
Conc: 473.23 ng/ml

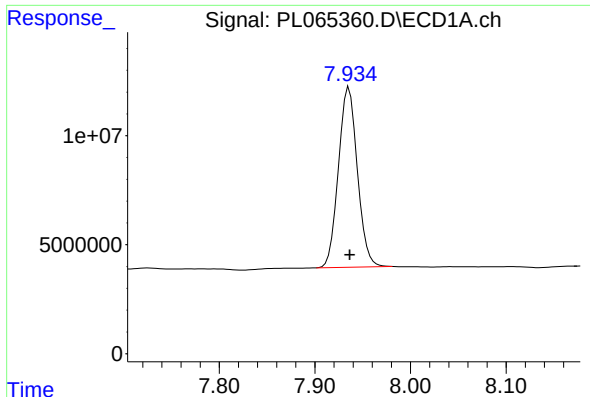

#28 Decachlorobiphenyl


R.T.: 7.936 min

Delta R.T.: 0.000 min

Response: 113890395

Conc: 46.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

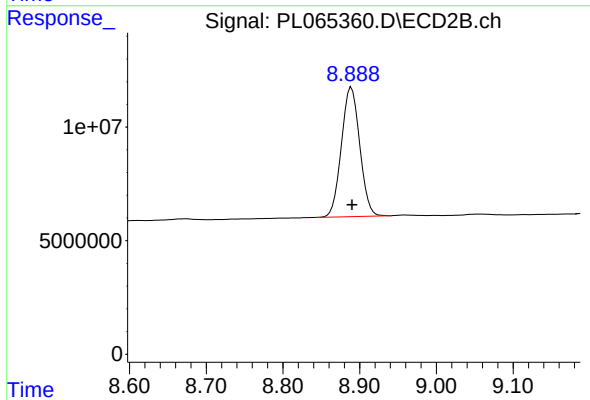

#28 Decachlorobiphenyl

R.T.: 8.889 min

Delta R.T.: 0.000 min

Response: 94907833

Conc: 46.66 ng/ml