

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031621\
 Data File : PL065372.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Mar 2021 03:40
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 05:07:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031621.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 17 04:35:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.292	3.883	125.9E6	135.3E6	51.767	46.866
28)	SA Decachlor...	7.937	8.891	116.3E6	95686892	47.358	47.038
Target Compounds							
23)	Chlordane-1	4.129	4.863	46500695	58624708	475.281	514.062
24)	Chlordane-2	4.617	5.331	54201005	57778371	489.378	483.019
25)	Chlordane-3	5.169	5.974	153.5E6	208.9E6	493.875	475.271
26)	Chlordane-4	5.224	6.045	136.1E6	240.2E6	490.589	472.920
27)	Chlordane-5	6.038	6.850	49110125	44292458	484.810	481.064



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031621\
Data File : PL065372.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Mar 2021 03:40
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 05:07:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031621.M
Quant Title : GC Extractables
QLast Update : Wed Mar 17 04:35:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

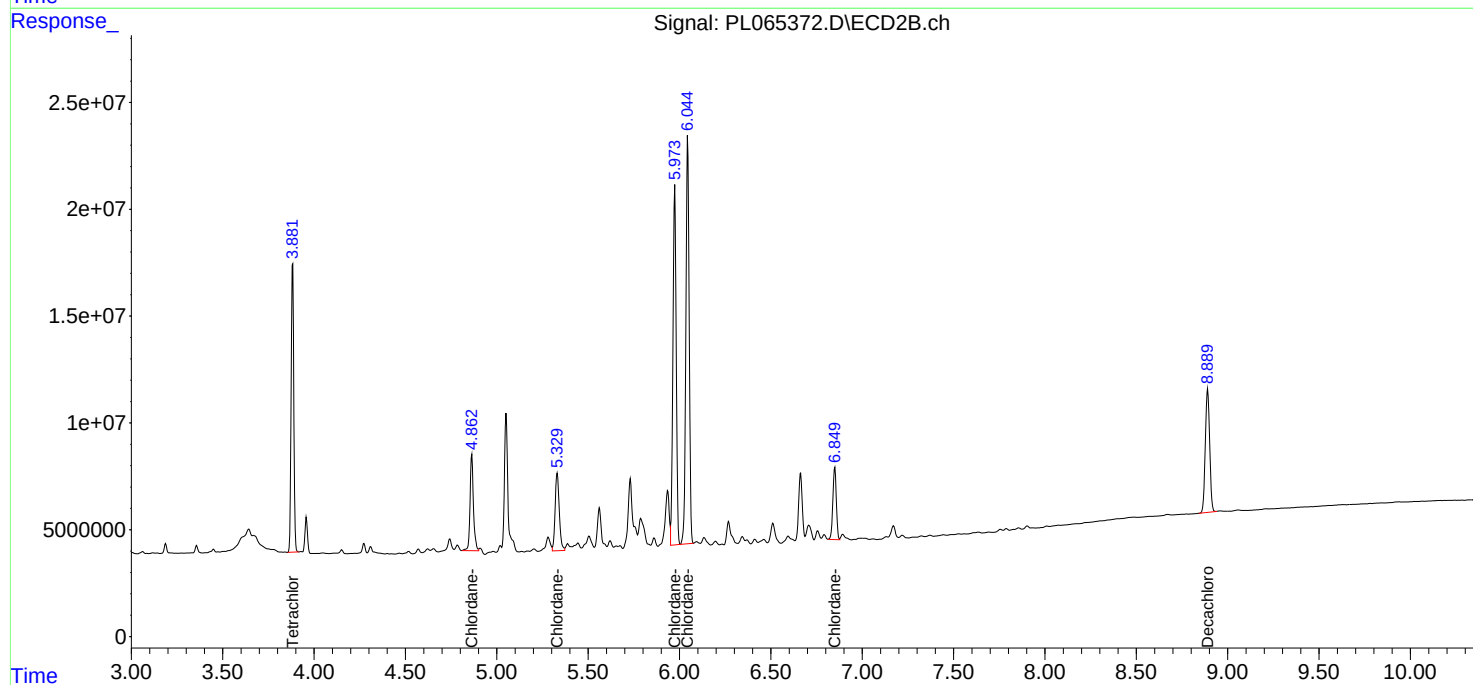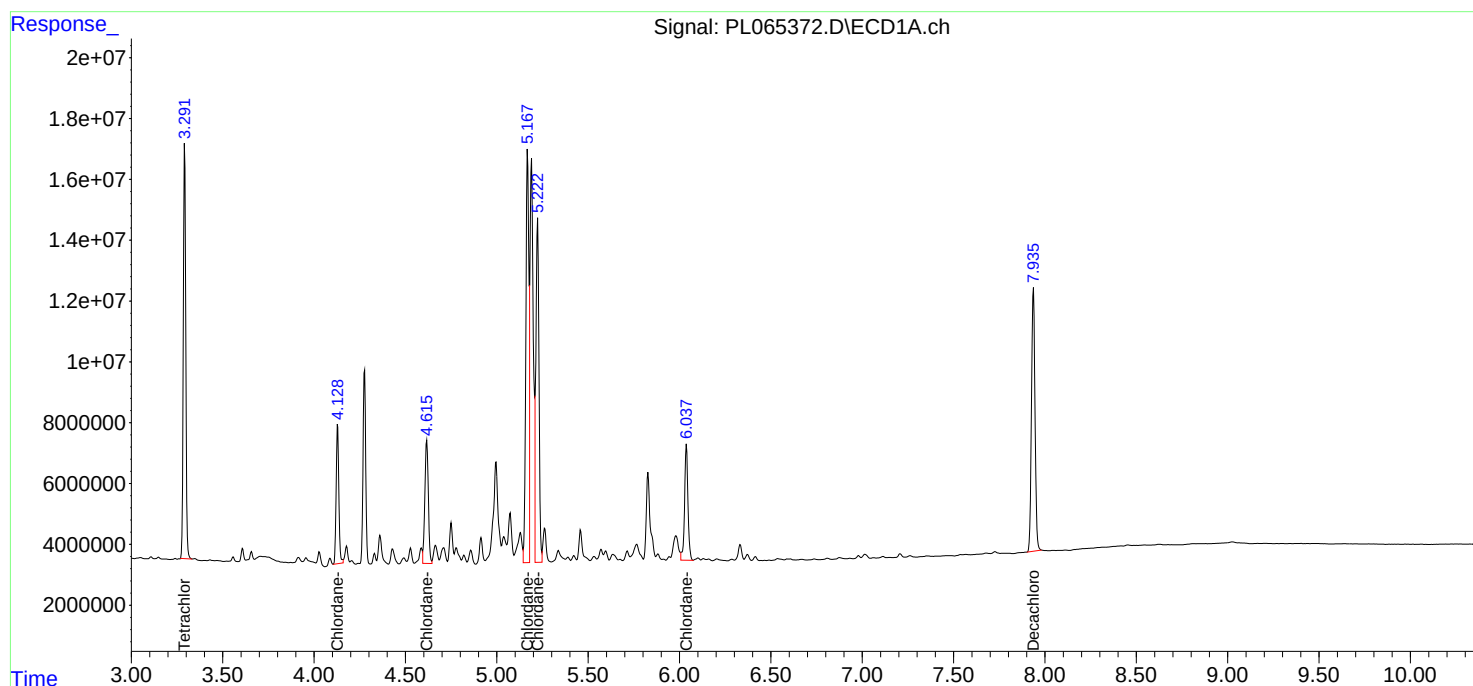


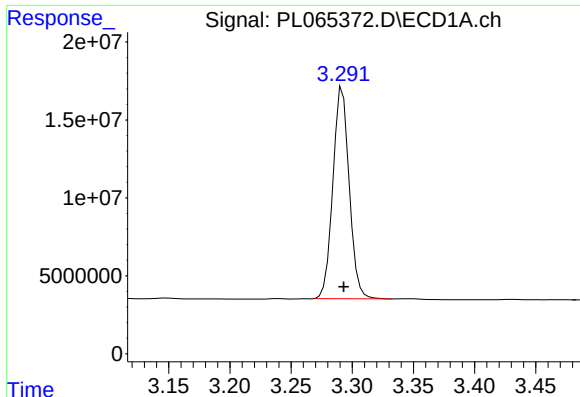

#1 Tetrachloro-m-xylene


R.T.: 3.292 min
Delta R.T.: 0.000 min
Response: 125875362
Conc: 51.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

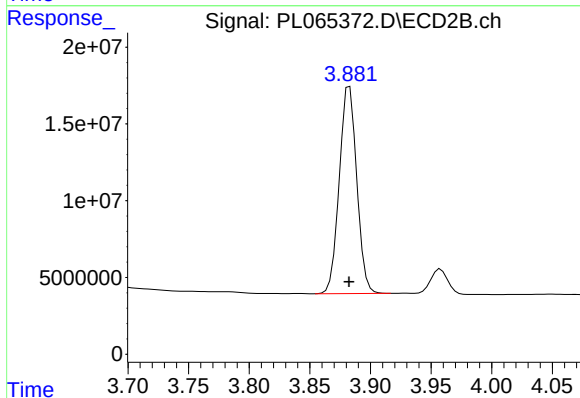


#1 Tetrachloro-m-xylene

R.T.: 3.883 min
Delta R.T.: 0.000 min
Response: 135296630
Conc: 46.87 ng/ml

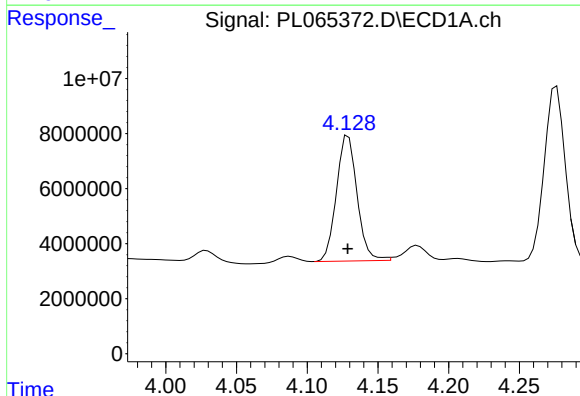


#23 Chlordane-1

R.T.: 4.129 min
Delta R.T.: 0.000 min
Response: 46500695
Conc: 475.28 ng/ml

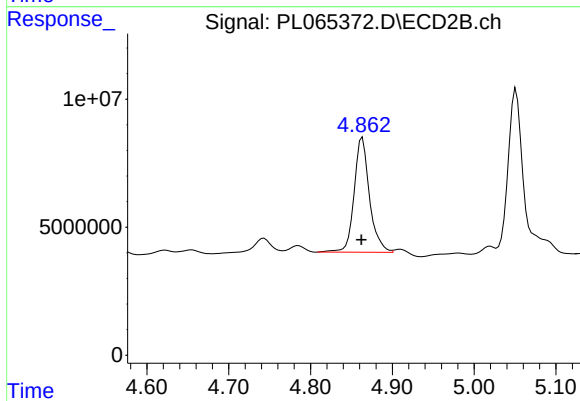

#23 Chlordane-1


R.T.: 4.863 min
Delta R.T.: 0.001 min
Response: 58624708
Conc: 514.06 ng/ml

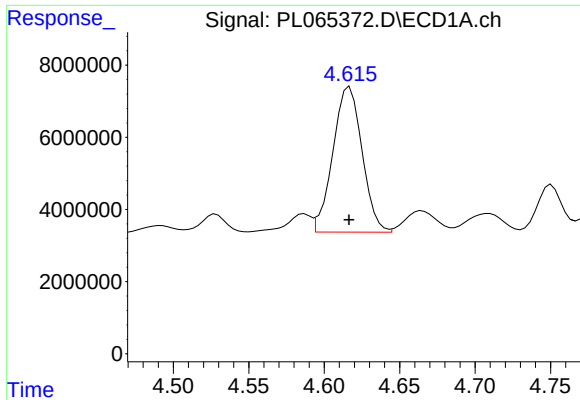

#24 Chlordane-2


R.T.: 4.617 min
Delta R.T.: 0.000 min
Response: 54201005
Conc: 489.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

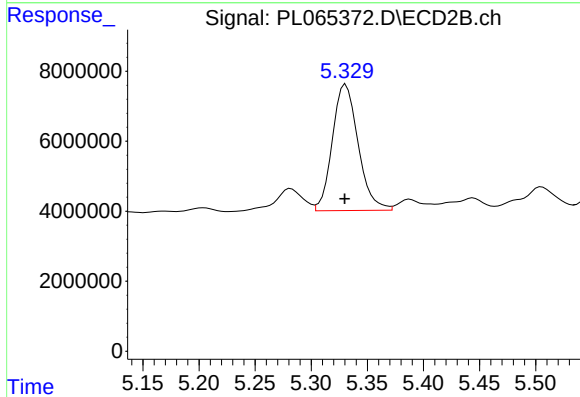


#24 Chlordane-2

R.T.: 5.331 min
Delta R.T.: 0.001 min
Response: 57778371
Conc: 483.02 ng/ml

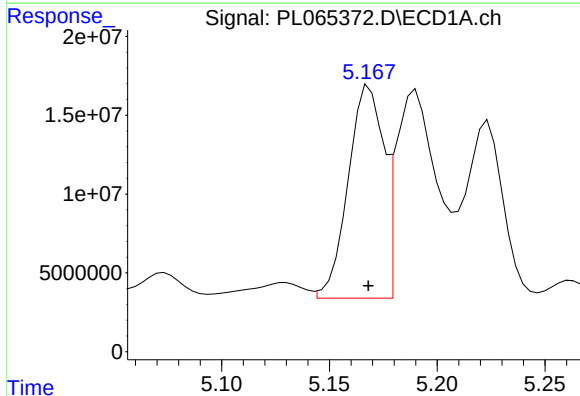


#25 Chlordane-3

R.T.: 5.169 min
Delta R.T.: 0.000 min
Response: 153522290
Conc: 493.88 ng/ml

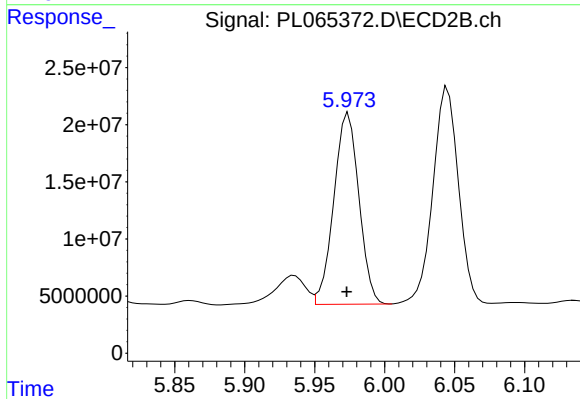

#25 Chlordane-3


R.T.: 5.974 min
Delta R.T.: 0.001 min
Response: 208883581
Conc: 475.27 ng/ml

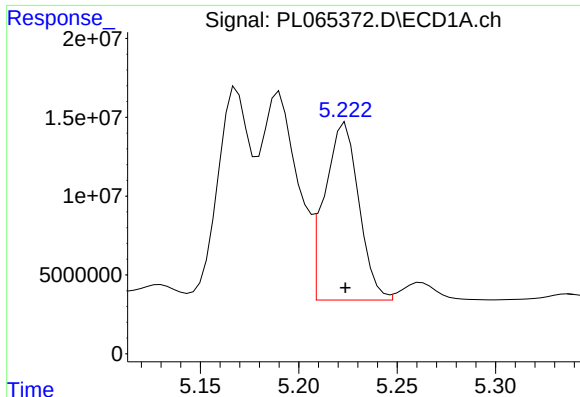

#26 Chlordane-4


R.T.: 5.224 min
Delta R.T.: 0.000 min
Response: 136092803
Conc: 490.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

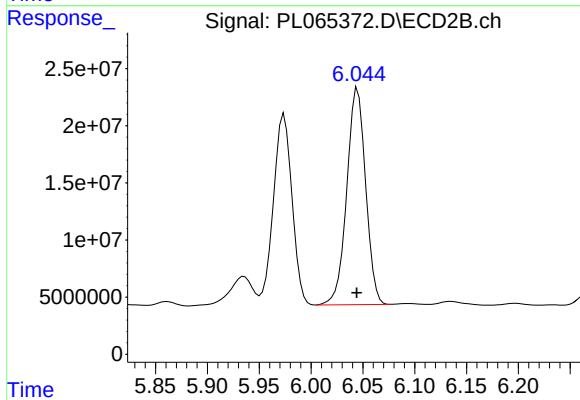


#26 Chlordane-4

R.T.: 6.045 min
Delta R.T.: 0.001 min
Response: 240170288
Conc: 472.92 ng/ml

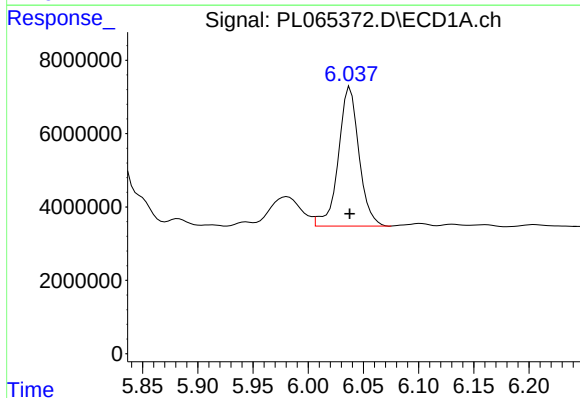


#27 Chlordane-5

R.T.: 6.038 min
Delta R.T.: 0.000 min
Response: 49110125
Conc: 484.81 ng/ml

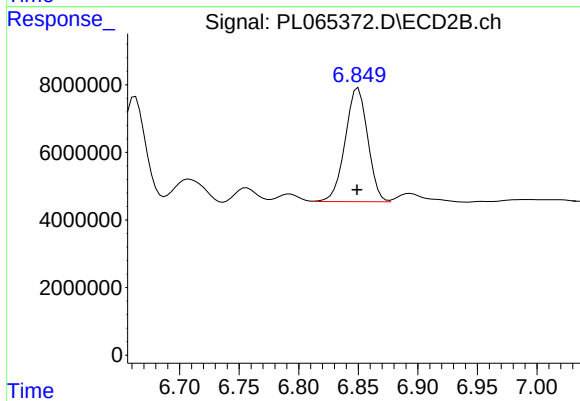

#27 Chlordane-5

R.T.: 6.850 min
Delta R.T.: 0.001 min
Response: 44292458
Conc: 481.06 ng/ml

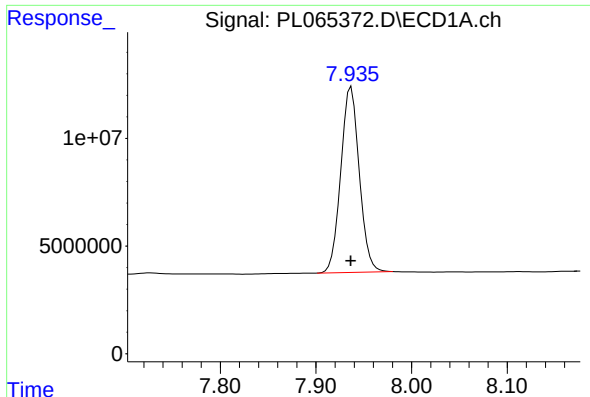

#28 Decachlorobiphenyl


R.T.: 7.937 min

Delta R.T.: 0.000 min

Response: 116282178

Conc: 47.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

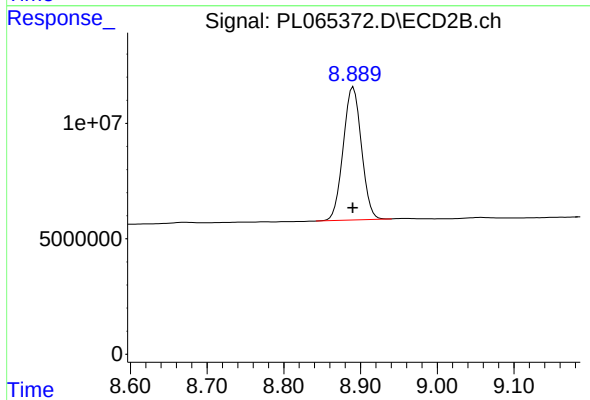

#28 Decachlorobiphenyl

R.T.: 8.891 min

Delta R.T.: 0.000 min

Response: 95686892

Conc: 47.04 ng/ml