

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031622\
 Data File : PL073406.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2022 09:14
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 01:52:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.643	5.491	6892160	36641664	21.519	22.325
28)	SA Decachlor...	10.418	11.330	10353056	35827104	20.360	20.036
Target Compounds							
6)	B beta-BHC	6.129f	6.681	49648	775936	0.241	0.744 #
7)	B delta-BHC	0.000	6.957	0	2663680	N.D.	1.237 #
9)	A Endosulfan I	0.000	8.323	0	245446	N.D.	0.134 #
10)	B gamma-Chl...	0.000	8.197	0	1004067	N.D.	0.492 #
14)	MA Endrin	8.091f	0.000	114590	0	0.295	N.D. #
15)	B Endosulfa...	8.355f	9.057	84727	177296	0.217	0.115 #
16)	A 4,4'-DDD	0.000	9.012f	0	232199	N.D.	0.159 #
17)	MA 4,4'-DDT	0.000	9.302	0	54929	N.D.	0.034 #
19)	B Endosulfa...	0.000	9.446	0	59637	N.D.	0.038 #
23)	Chlordane-1	0.000	6.850	0	980454	N.D.	14.352 #
25)	Chlordane-3	0.000	8.197	0	1004067	N.D.	3.703 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031622\
Data File : PL073406.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2022 09:14
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 01:52:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

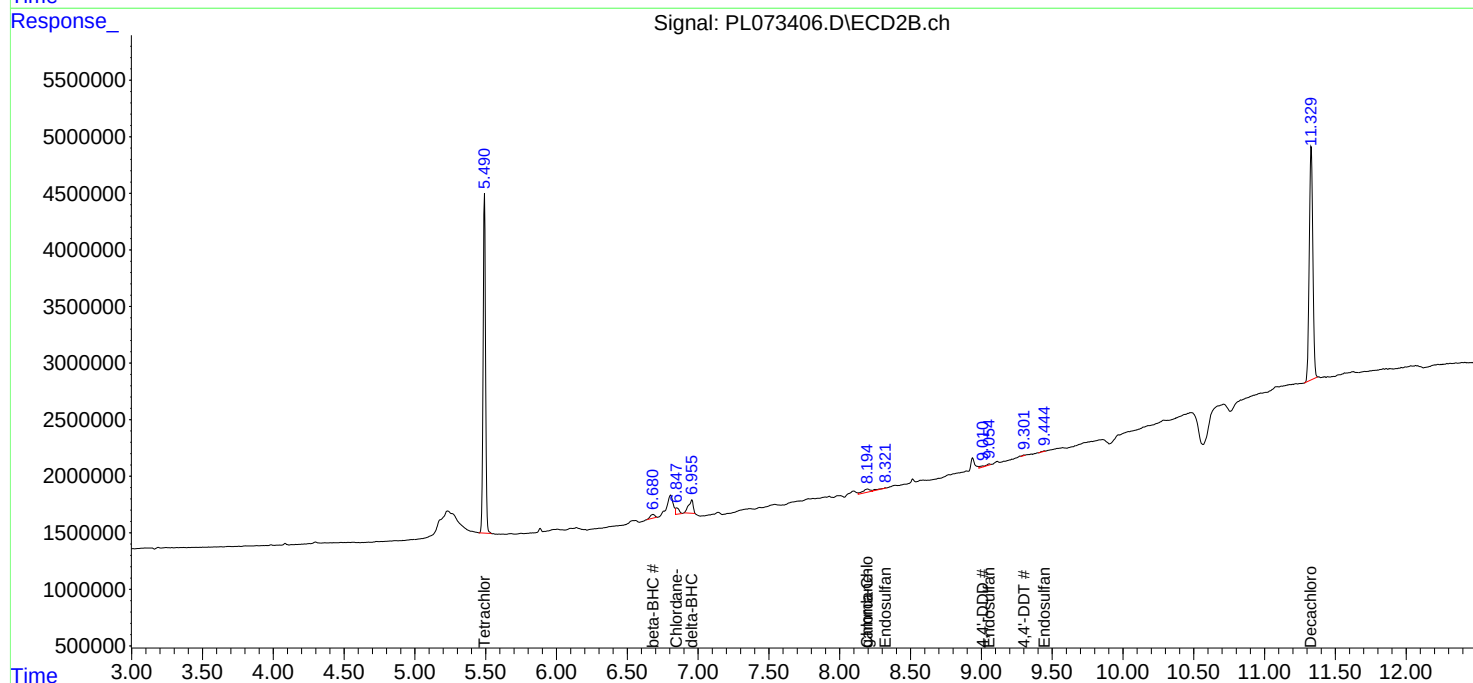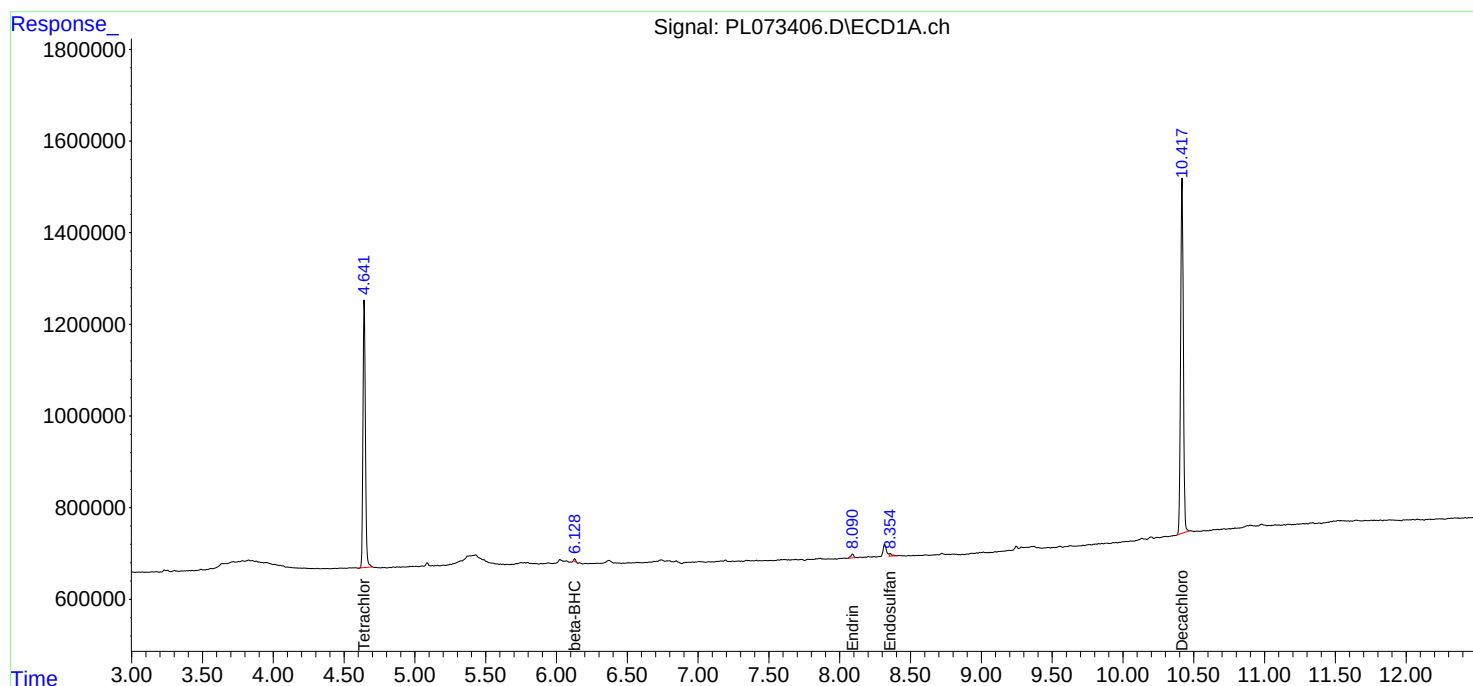


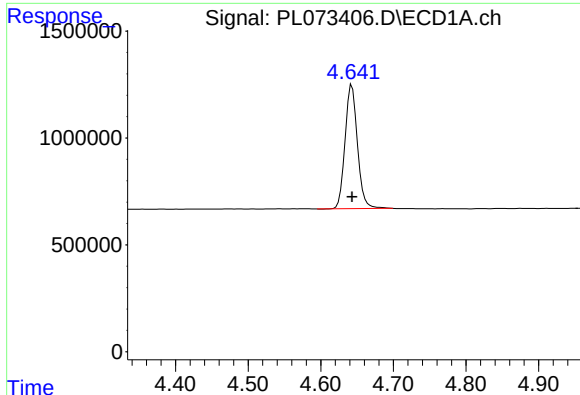

#1 Tetrachloro-m-xylene


R.T.: 4.643 min
Delta R.T.: 0.000 min
Response: 6892160
Conc: 21.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

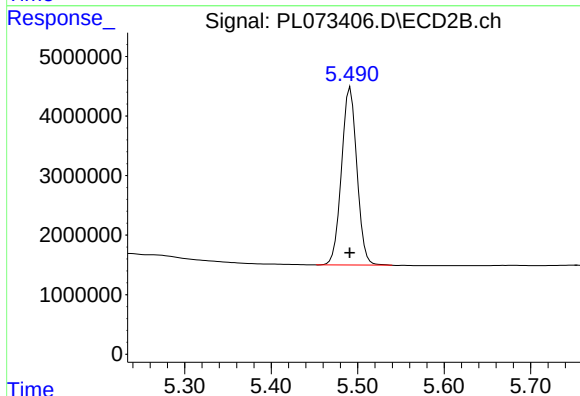


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: 0.000 min
Response: 36641664
Conc: 22.33 ng/ml

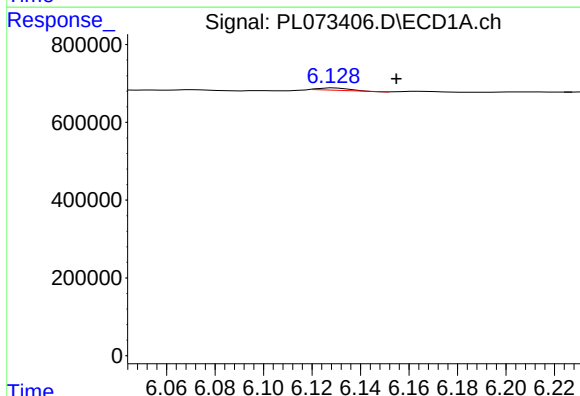


#6 beta-BHC

R.T.: 6.129 min
Delta R.T.: -0.026 min
Response: 49648
Conc: 0.24 ng/ml

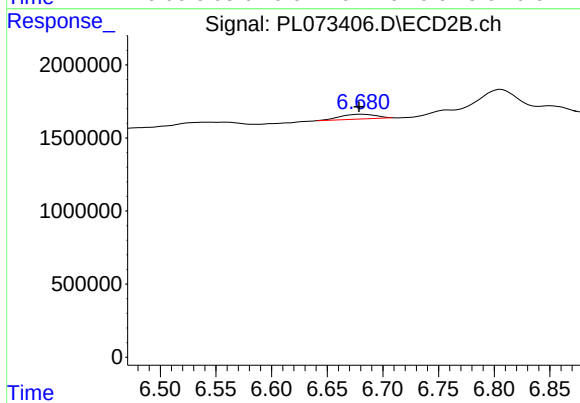

#6 beta-BHC


R.T.: 6.681 min
Delta R.T.: 0.003 min
Response: 775936
Conc: 0.74 ng/ml

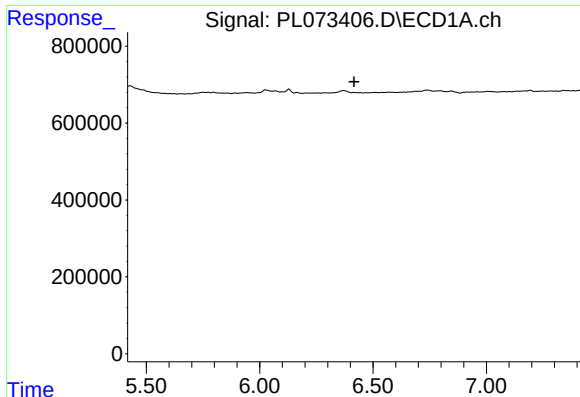

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.416 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

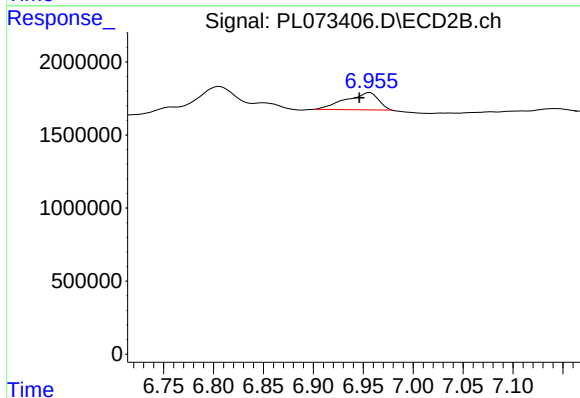


#7 delta-BHC

R.T.: 6.957 min
Delta R.T.: 0.010 min
Response: 2663680
Conc: 1.24 ng/ml

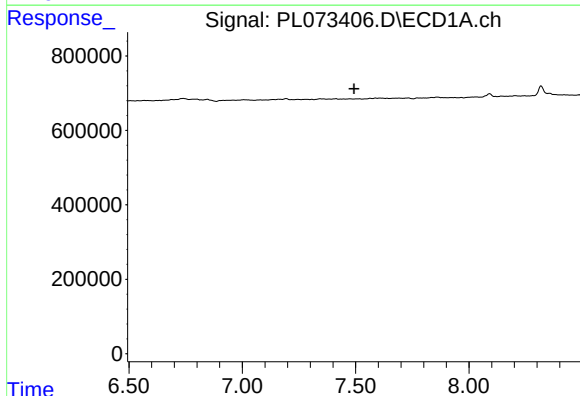


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 7.493 min
Response: 0
Conc: N.D.

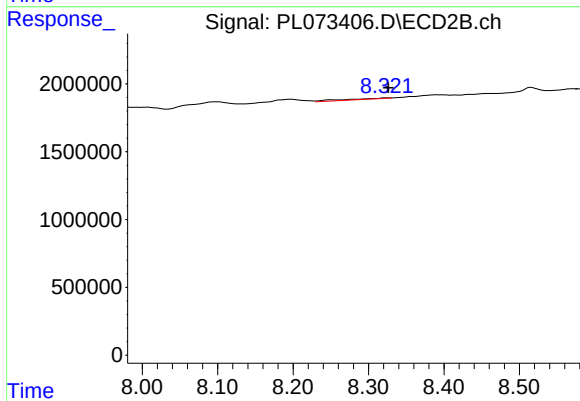

#9 Endosulfan I


R.T.: 8.323 min
Delta R.T.: -0.004 min
Response: 245446
Conc: 0.13 ng/ml

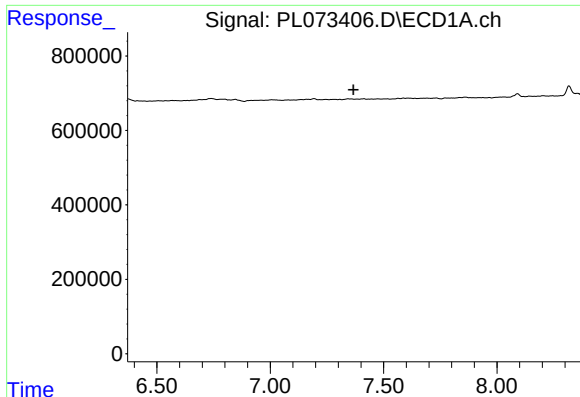

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

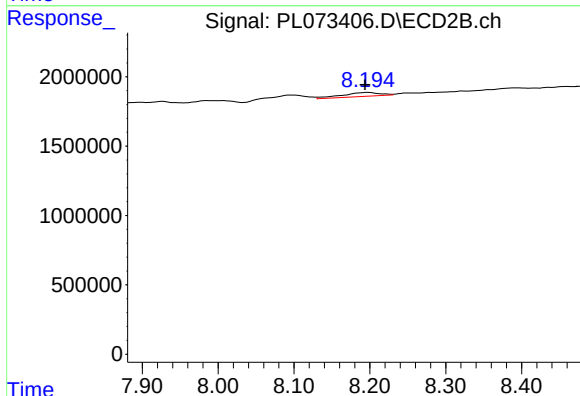


#10 gamma-Chlordane

R.T.: 8.197 min
Delta R.T.: 0.003 min
Response: 1004067
Conc: 0.49 ng/ml

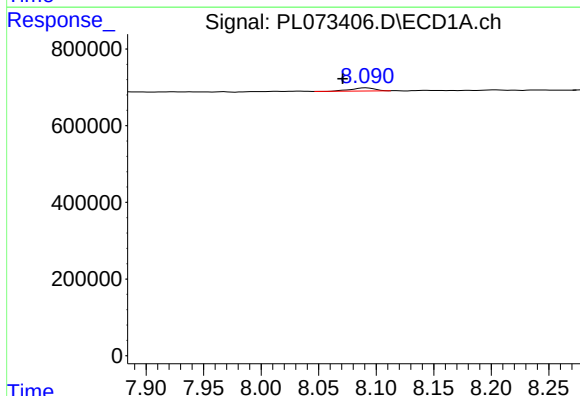


#14 Endrin

R.T.: 8.091 min
Delta R.T.: 0.020 min
Response: 114590
Conc: 0.30 ng/ml

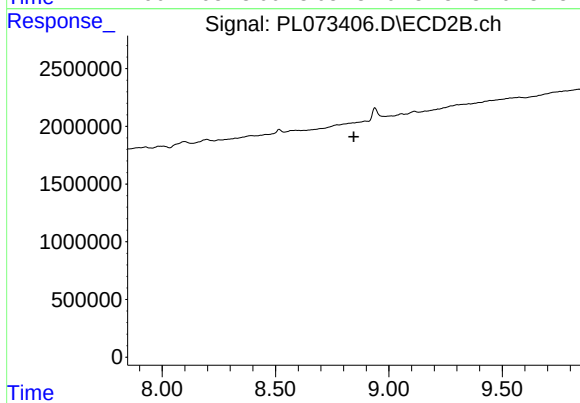

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 8.845 min
Response: 0
Conc: N.D.

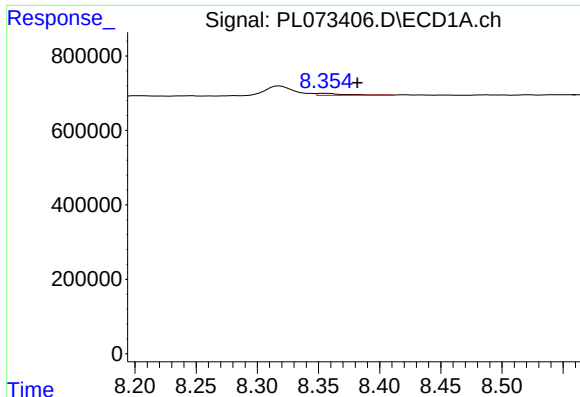

#15 Endosulfan II


R.T.: 8.355 min
Delta R.T.: -0.026 min
Response: 84727
Conc: 0.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

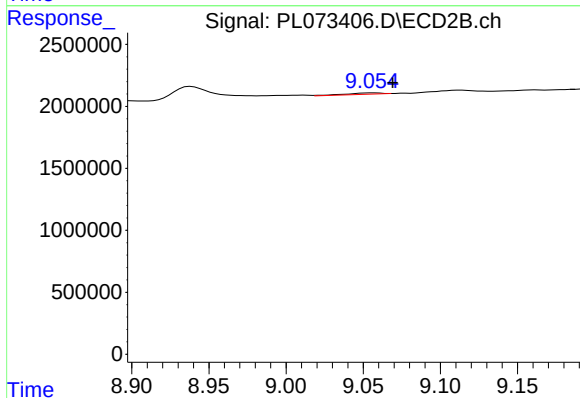


#15 Endosulfan II

R.T.: 9.057 min
Delta R.T.: -0.012 min
Response: 177296
Conc: 0.12 ng/ml

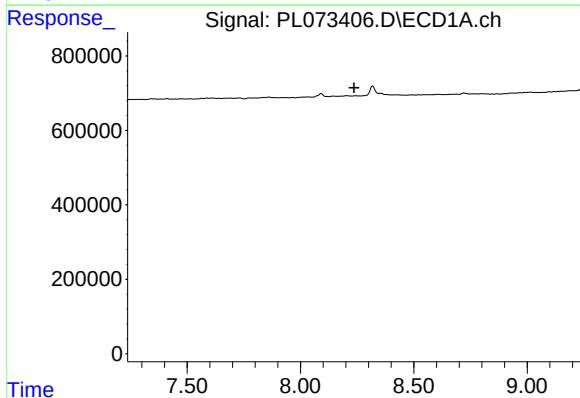


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.237 min
Response: 0
Conc: N.D.

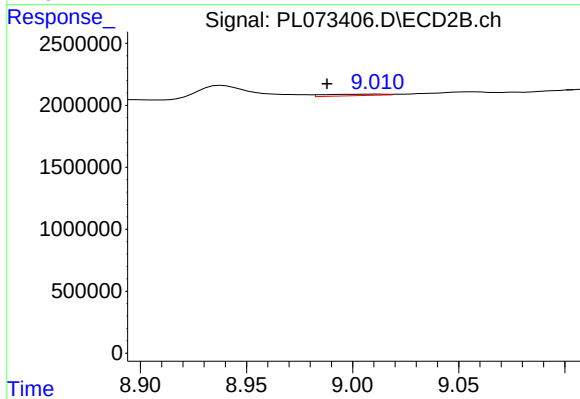

#16 4,4'-DDD


R.T.: 9.012 min
Delta R.T.: 0.024 min
Response: 232199
Conc: 0.16 ng/ml

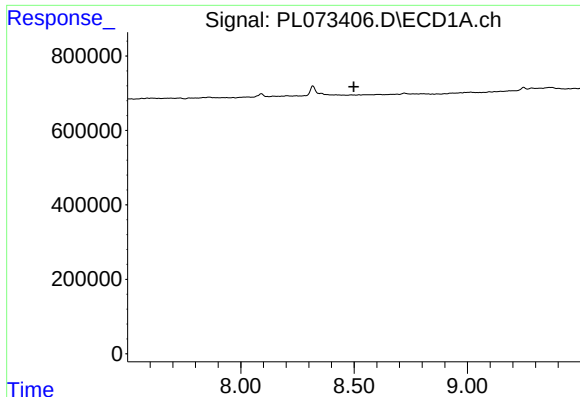

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.499 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

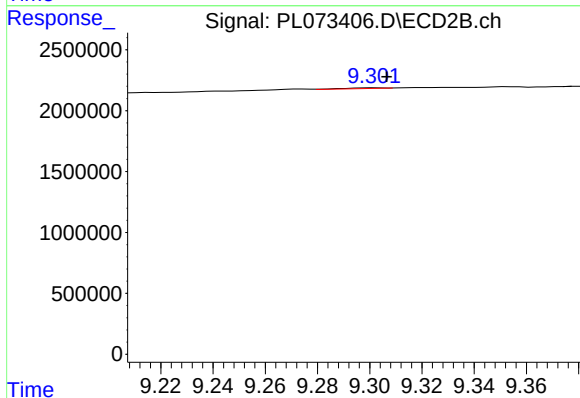


#17 4,4'-DDT

R.T.: 9.302 min
Delta R.T.: -0.005 min
Response: 54929
Conc: 0.03 ng/ml

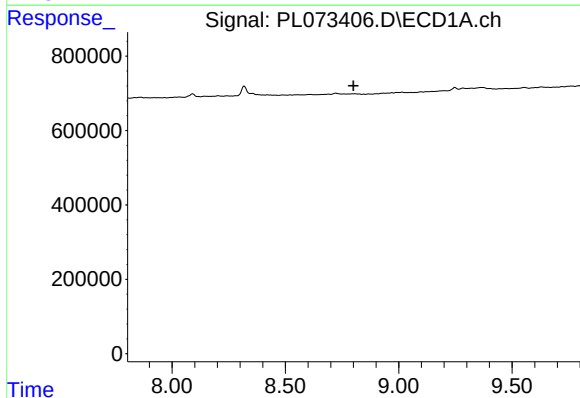


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T.: 8.801 min
Response: 0
Conc: N.D.

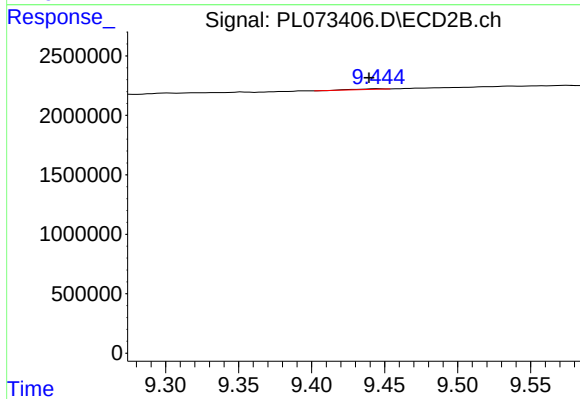

#19 Endosulfan Sulfate


R.T.: 9.446 min
Delta R.T.: 0.007 min
Response: 59637
Conc: 0.04 ng/ml

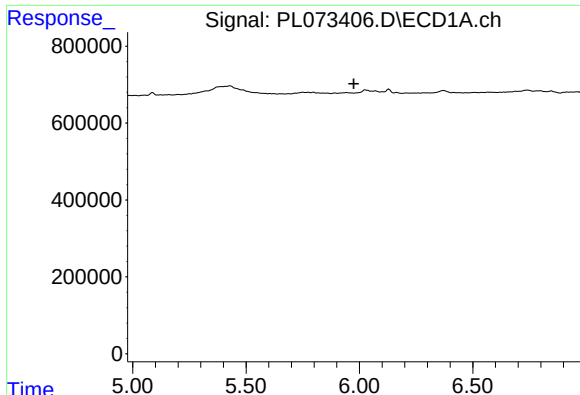

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.976 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

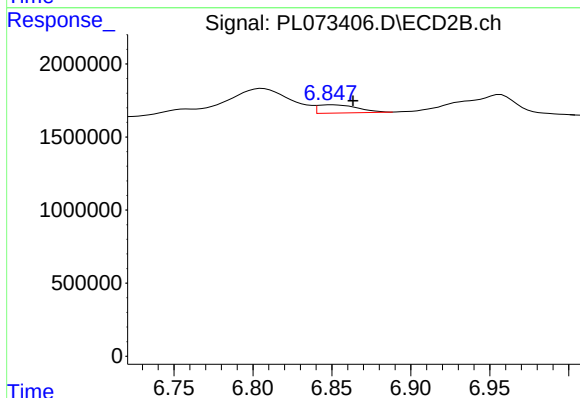


#23 Chlordane-1

R.T.: 6.850 min
Delta R.T.: -0.013 min
Response: 980454
Conc: 14.35 ng/ml

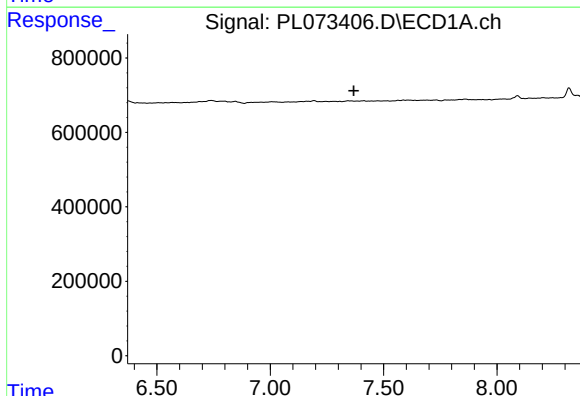


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

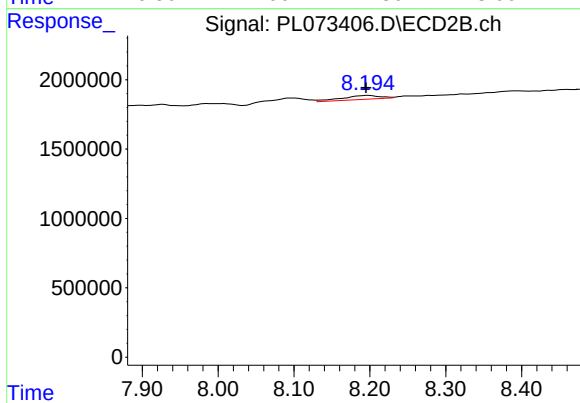

#25 Chlordane-3


R.T.: 8.197 min
Delta R.T.: 0.002 min
Response: 1004067
Conc: 3.70 ng/ml

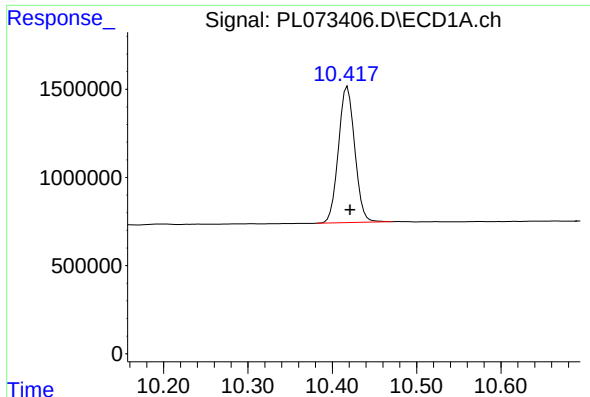

#28 Decachlorobiphenyl

R.T.: 10.418 min
Delta R.T.: -0.003 min
Response: 10353056
Conc: 20.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

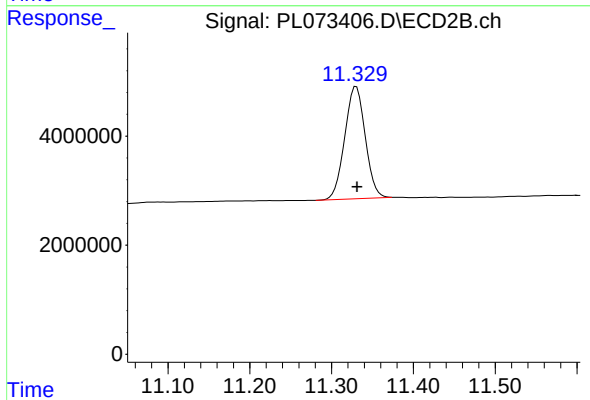

#28 Decachlorobiphenyl

R.T.: 11.330 min
Delta R.T.: -0.001 min
Response: 35827104
Conc: 20.04 ng/ml