

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031622\
 Data File : PL073431.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2022 19:13
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 01:56:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.642	5.491	6880498	37265792	21.482	22.706
28)	SA Decachlor...	10.416	11.330	10946649	39105652	21.527	21.869
Target Compounds							
6)	B beta-BHC	6.128f	6.675	36550	791798	0.178	0.760 #
7)	B delta-BHC	0.000	6.958	0	2416540	N.D.	1.122 #
8)	B Heptachlo...	0.000	7.926	0	481807	N.D.	0.241 #
10)	B gamma-Chl...	0.000	8.196	0	1258744	N.D.	0.616 #
12)	B 4,4'-DDE	0.000	8.456	0	47850	N.D.	0.027 #
14)	MA Endrin	8.090f	0.000	85872	0	0.221	N.D. #
15)	B Endosulfa...	8.353f	9.059	48824	834131	0.125	0.543 #
23)	Chlordane-1	0.000	6.853	0	977702	N.D.	14.312 #
25)	Chlordane-3	0.000	8.196	0	1258744	N.D.	4.643 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031622\
Data File : PL073431.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2022 19:13
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 01:56:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

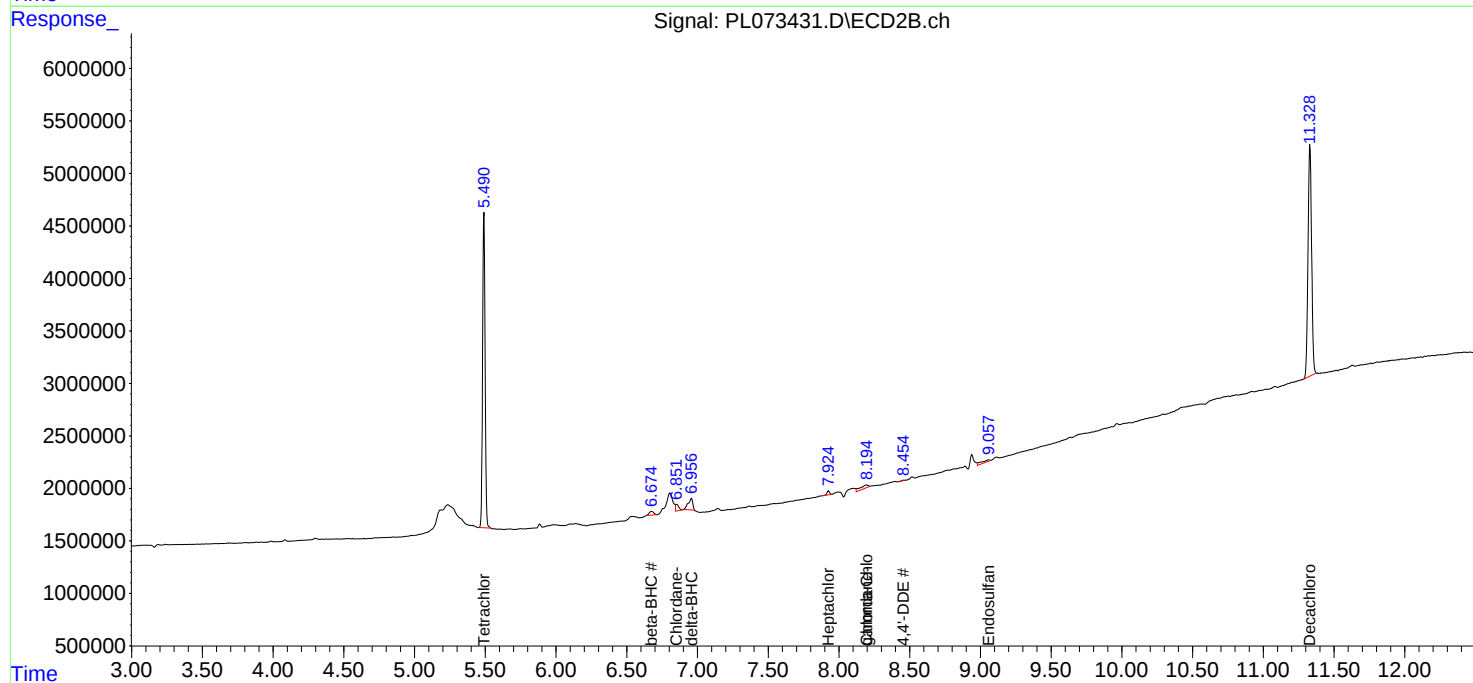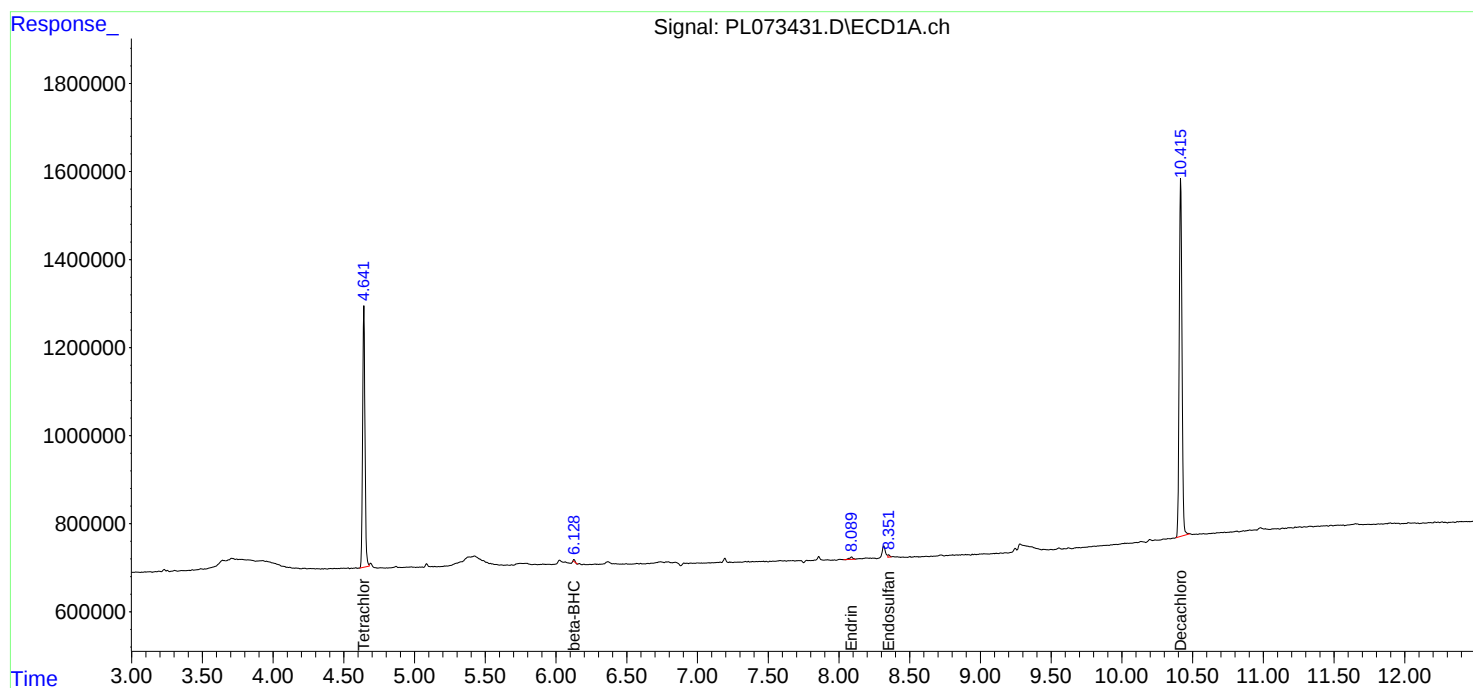


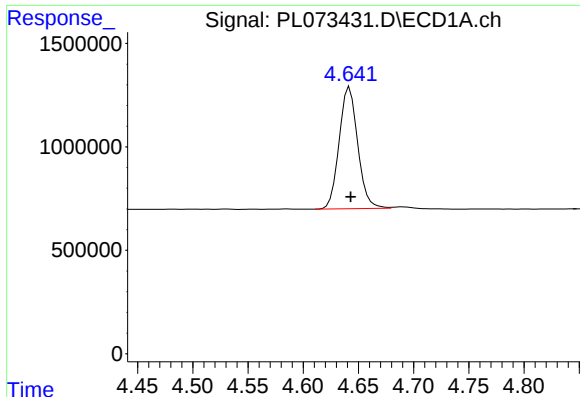

#1 Tetrachloro-m-xylene


R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 6880498
Conc: 21.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

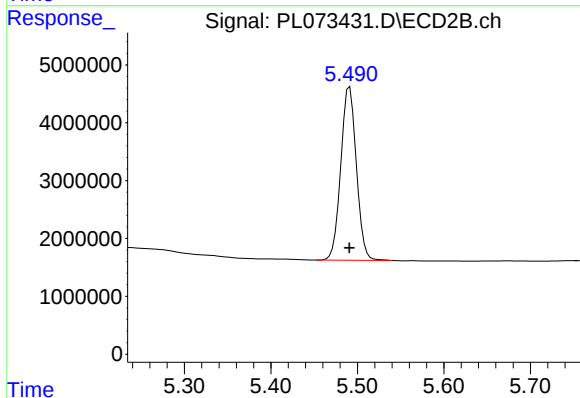


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: 0.000 min
Response: 37265792
Conc: 22.71 ng/ml

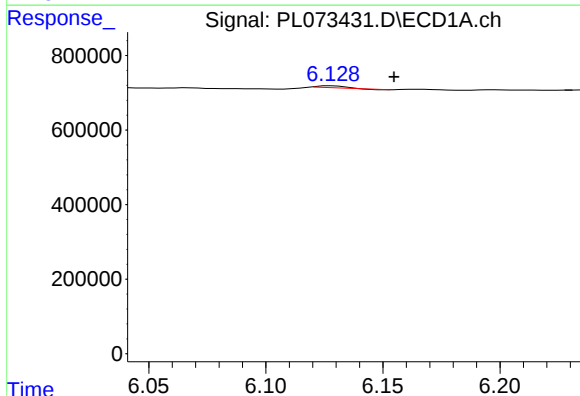


#6 beta-BHC

R.T.: 6.128 min
Delta R.T.: -0.027 min
Response: 36550
Conc: 0.18 ng/ml

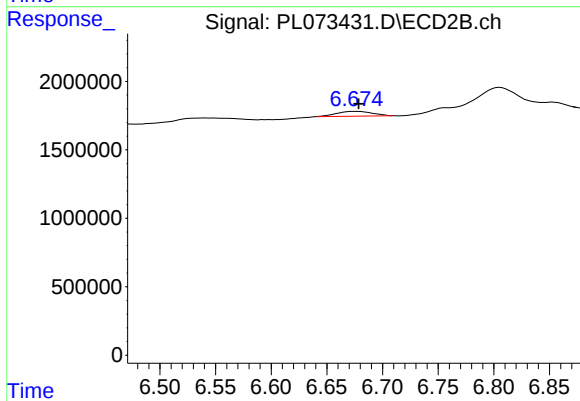

#6 beta-BHC


R.T.: 6.675 min
Delta R.T.: -0.003 min
Response: 791798
Conc: 0.76 ng/ml

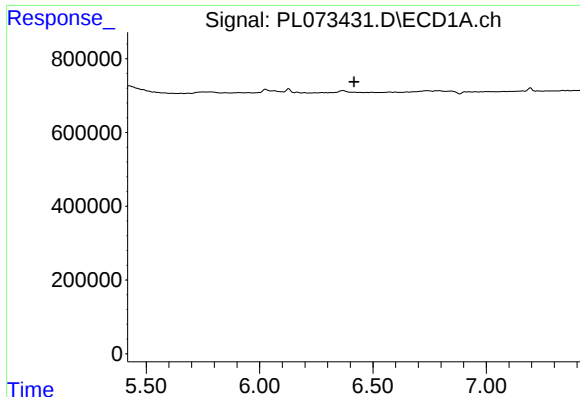

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.416 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

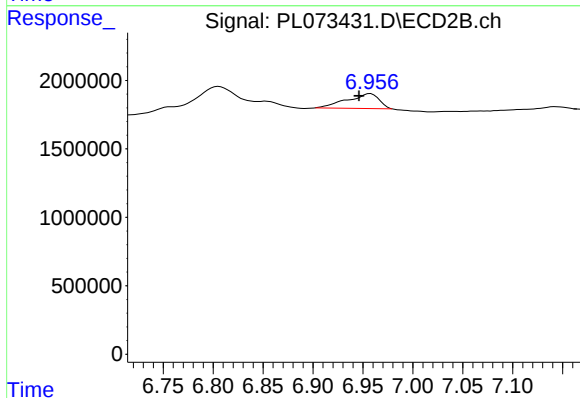


#7 delta-BHC

R.T.: 6.958 min
Delta R.T.: 0.011 min
Response: 2416540
Conc: 1.12 ng/ml

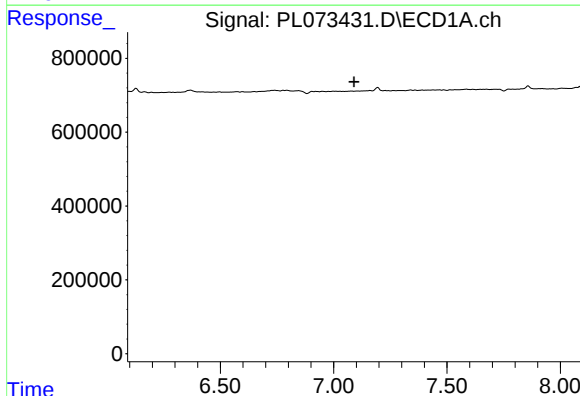


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 7.090 min
Response: 0
Conc: N.D.

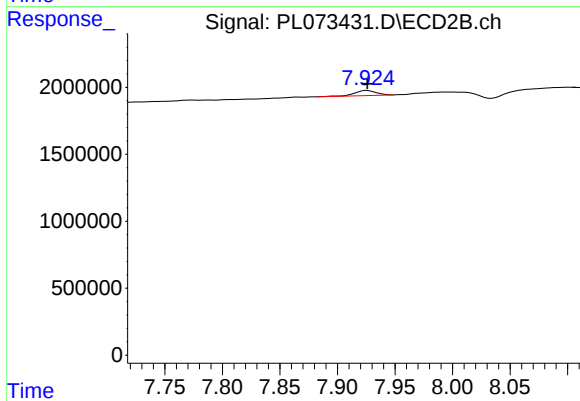

#8 Heptachlor epoxide


R.T.: 7.926 min
Delta R.T.: 0.000 min
Response: 481807
Conc: 0.24 ng/ml

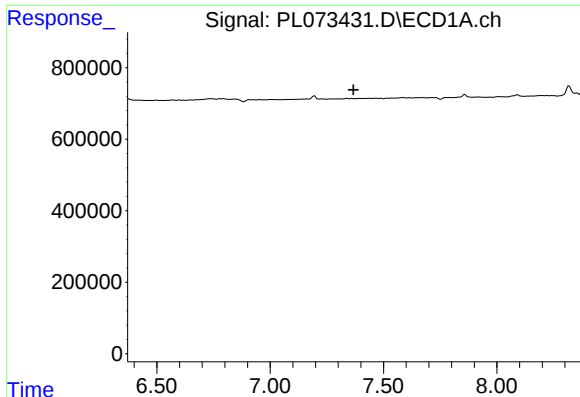

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

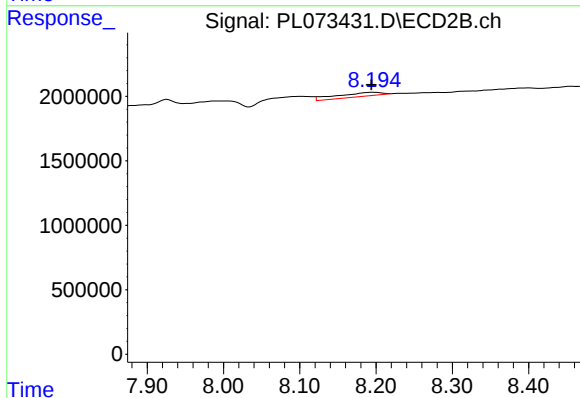


#10 gamma-Chlordane

R.T.: 8.196 min
Delta R.T.: 0.002 min
Response: 1258744
Conc: 0.62 ng/ml

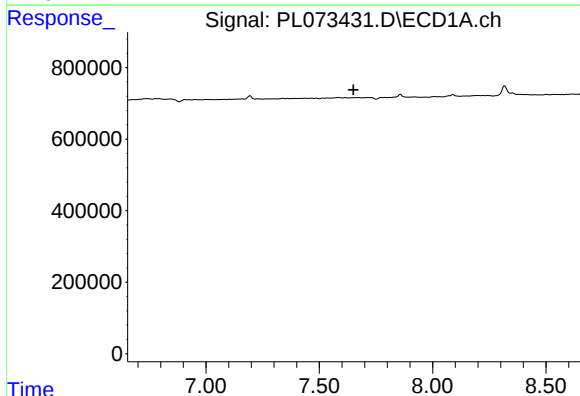


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 7.651 min
Response: 0
Conc: N.D.

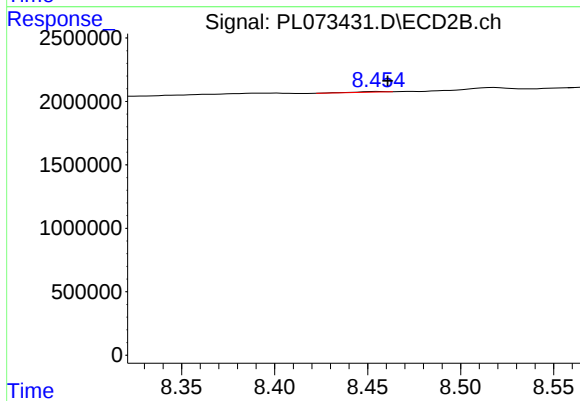

#12 4,4'-DDE


R.T.: 8.456 min
Delta R.T.: -0.005 min
Response: 47850
Conc: 0.03 ng/ml

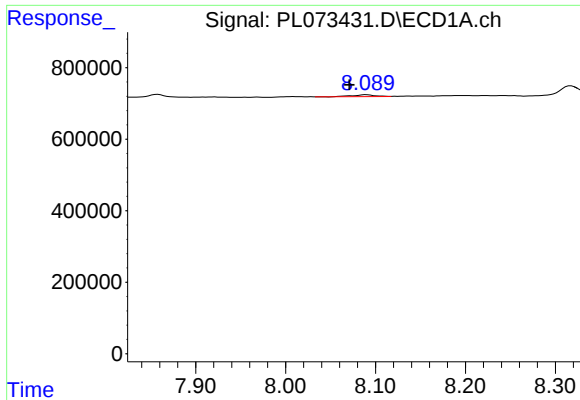

#14 Endrin


R.T.: 8.090 min
Delta R.T.: 0.019 min
Response: 85872
Conc: 0.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

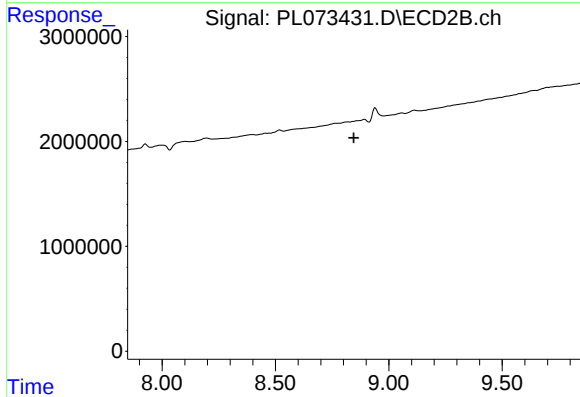


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.845 min
Response: 0
Conc: N.D.

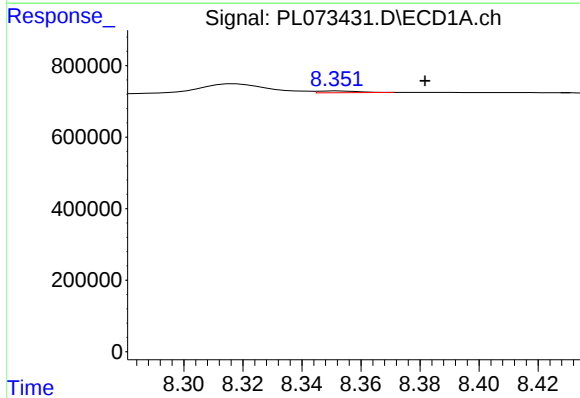


#15 Endosulfan II

R.T.: 8.353 min
Delta R.T.: -0.029 min
Response: 48824
Conc: 0.12 ng/ml

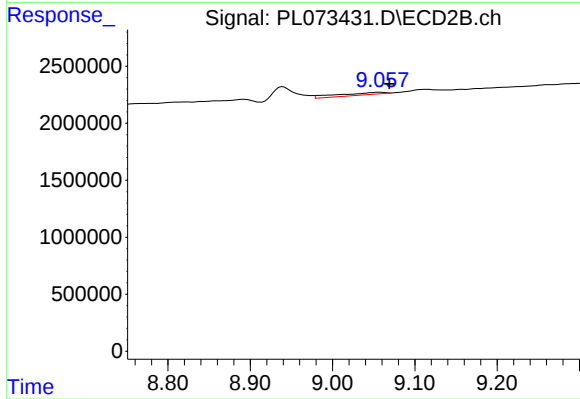

#15 Endosulfan II


R.T.: 9.059 min
Delta R.T.: -0.010 min
Response: 834131
Conc: 0.54 ng/ml

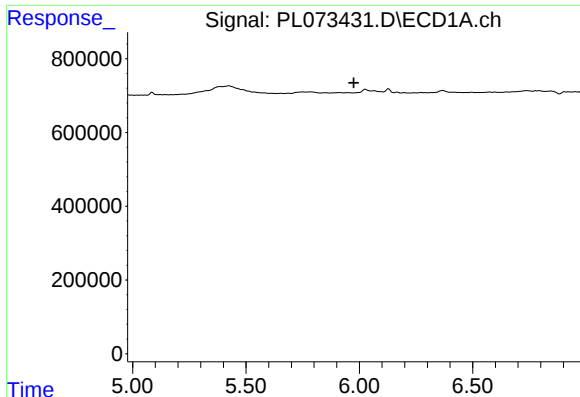

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.976 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

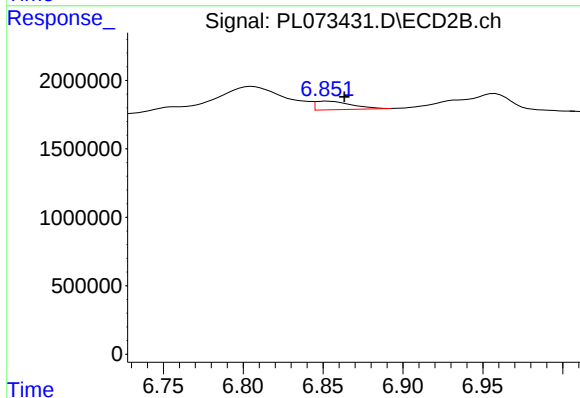


#23 Chlordane-1

R.T.: 6.853 min
Delta R.T.: -0.011 min
Response: 977702
Conc: 14.31 ng/ml

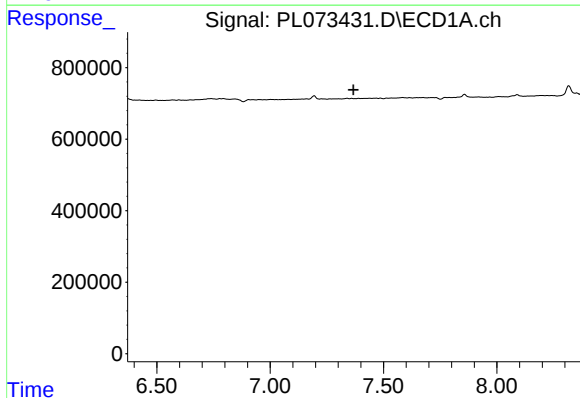


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

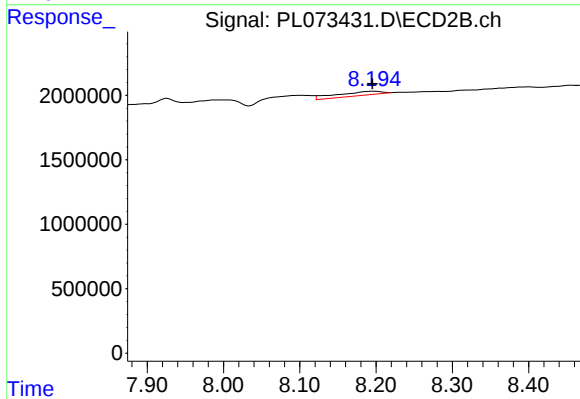

#25 Chlordane-3


R.T.: 8.196 min
Delta R.T.: 0.000 min
Response: 1258744
Conc: 4.64 ng/ml

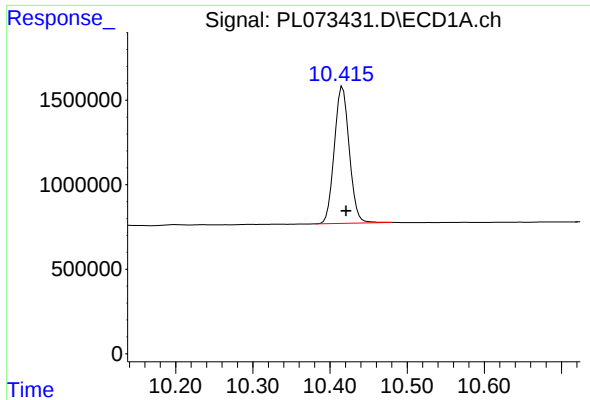

#28 Decachlorobiphenyl

R.T.: 10.416 min
Delta R.T.: -0.005 min
Response: 10946649
Conc: 21.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

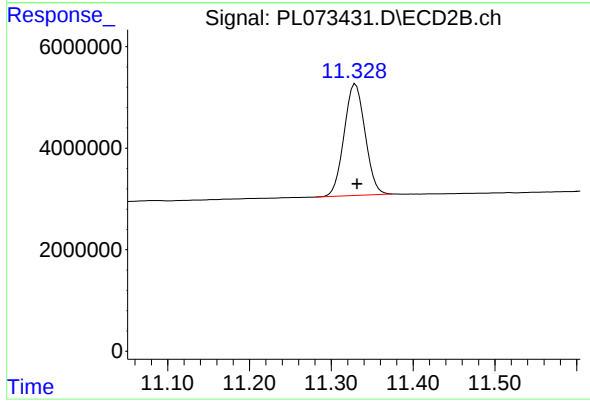

#28 Decachlorobiphenyl

R.T.: 11.330 min
Delta R.T.: -0.002 min
Response: 39105652
Conc: 21.87 ng/ml