

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031622\
 Data File : PL073409.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2022 10:11
 Operator : AR\AJ
 Sample : PCHLORCCC500 (Sig #1); PCHL,ORCCC500 (Sig #2)
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 01:53:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.649	5.489	18318024	81745613	57.193	49.807
28)	SA Decachlor...	10.421	11.331	23203666	81385192	45.632	45.513
Target Compounds							
23)	Chlordane-1	5.981	6.862	5504611	30748347	464.328	450.108
24)	Chlordane-2	6.670	7.445	7410684	34087884	454.284	474.275
25)	Chlordane-3	7.371	8.195	18330769	133.1E6	448.908	490.784
26)	Chlordane-4	7.440	8.281	19742671	161.9E6	445.449	488.811
27)	Chlordane-5	8.389	9.149	7502212	26264709	458.142	483.898



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031622\
Data File : PL073409.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2022 10:11
Operator : AR\AJ
Sample : PCHLORCCC500 (Sig #1); PCHL,ORCCC500 (Sig #2)
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 01:53:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

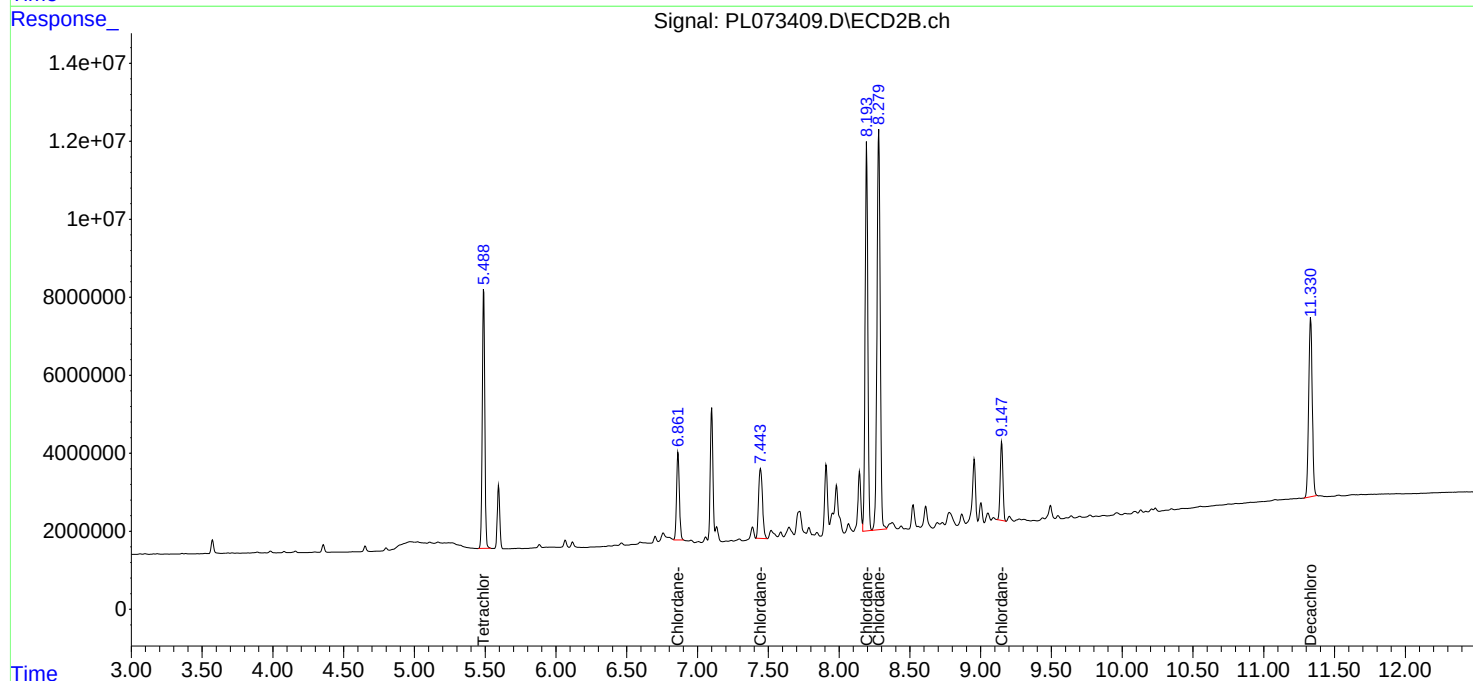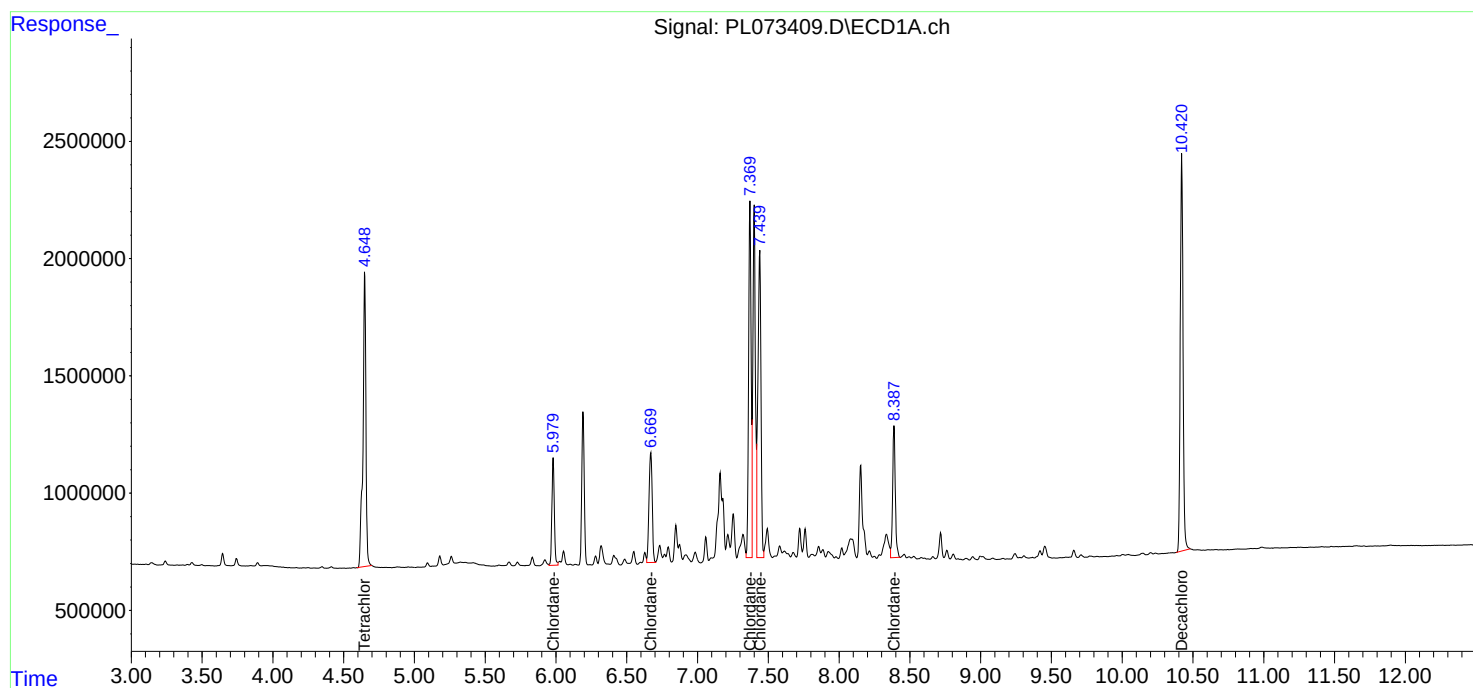


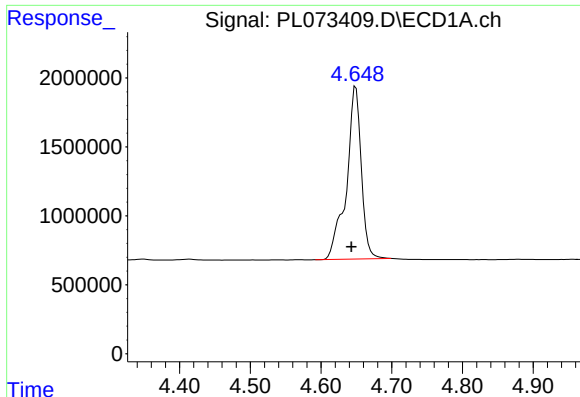

#1 Tetrachloro-m-xylene


R.T.: 4.649 min
Delta R.T.: 0.006 min
Response: 18318024
Conc: 57.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

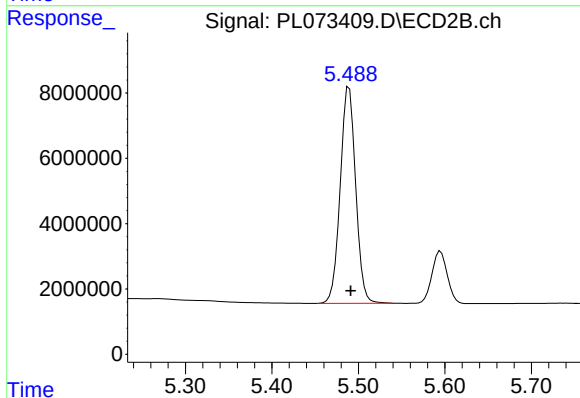


#1 Tetrachloro-m-xylene

R.T.: 5.489 min
Delta R.T.: -0.002 min
Response: 81745613
Conc: 49.81 ng/ml

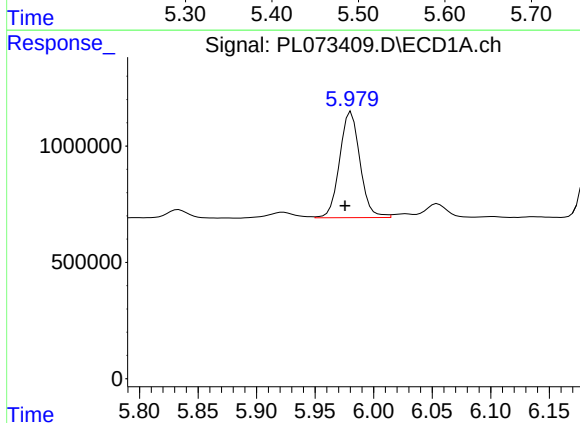


#23 Chlordane-1

R.T.: 5.981 min
Delta R.T.: 0.005 min
Response: 5504611
Conc: 464.33 ng/ml

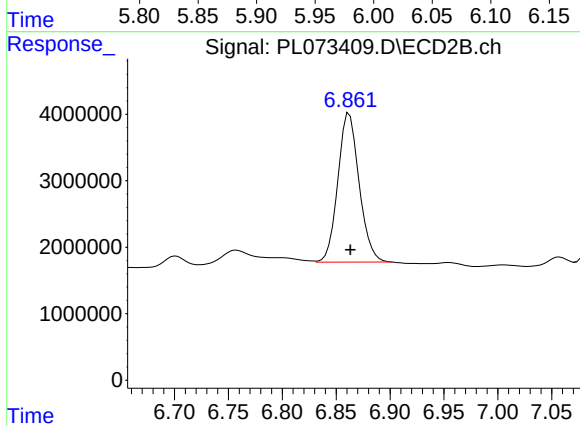

#23 Chlordane-1


R.T.: 6.862 min
Delta R.T.: -0.001 min
Response: 30748347
Conc: 450.11 ng/ml

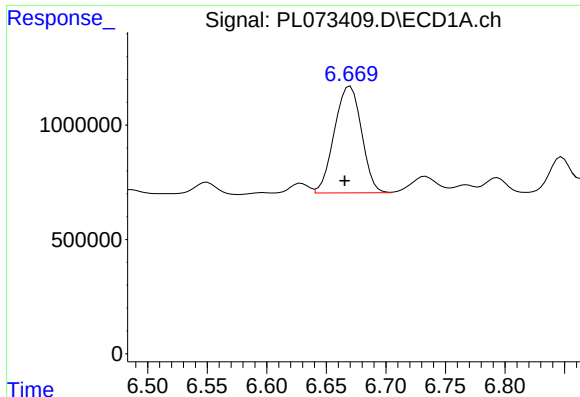

#24 Chlordane-2


R.T.: 6.670 min
Delta R.T.: 0.005 min
Response: 7410684
Conc: 454.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

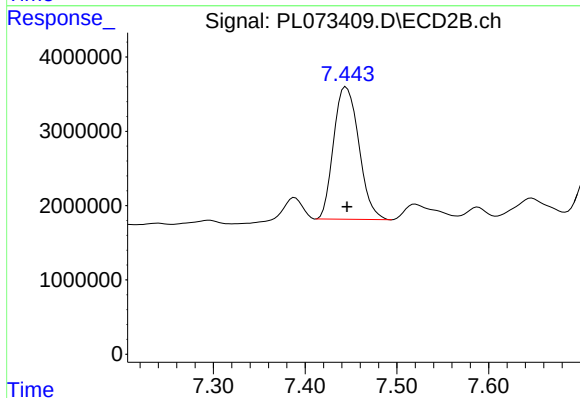


#24 Chlordane-2

R.T.: 7.445 min
Delta R.T.: 0.000 min
Response: 34087884
Conc: 474.27 ng/ml

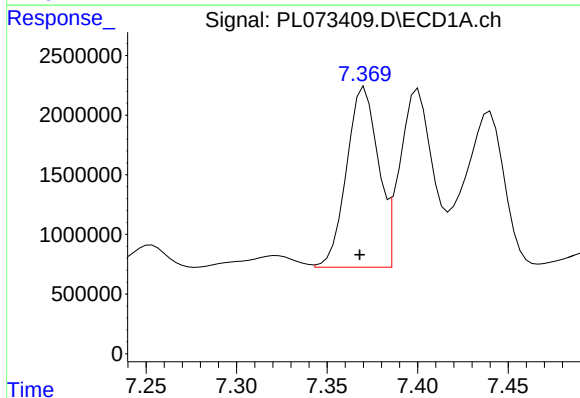


#25 Chlordane-3

R.T.: 7.371 min
Delta R.T.: 0.003 min
Response: 18330769
Conc: 448.91 ng/ml

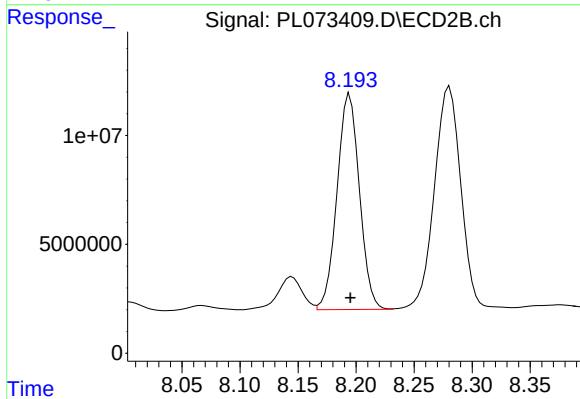

#25 Chlordane-3


R.T.: 8.195 min
Delta R.T.: 0.000 min
Response: 133067372
Conc: 490.78 ng/ml

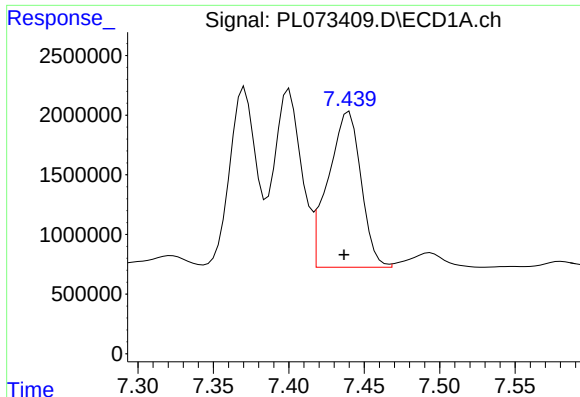

#26 Chlordane-4


R.T.: 7.440 min
Delta R.T.: 0.003 min
Response: 19742671
Conc: 445.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

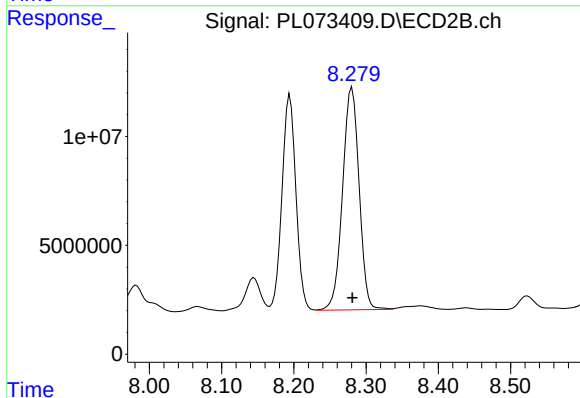


#26 Chlordane-4

R.T.: 8.281 min
Delta R.T.: 0.000 min
Response: 161920130
Conc: 488.81 ng/ml

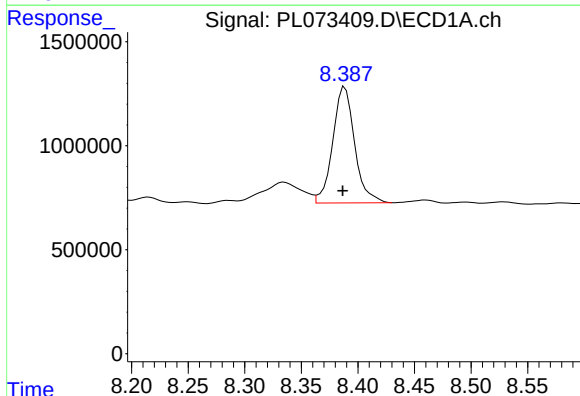


#27 Chlordane-5

R.T.: 8.389 min
Delta R.T.: 0.002 min
Response: 7502212
Conc: 458.14 ng/ml

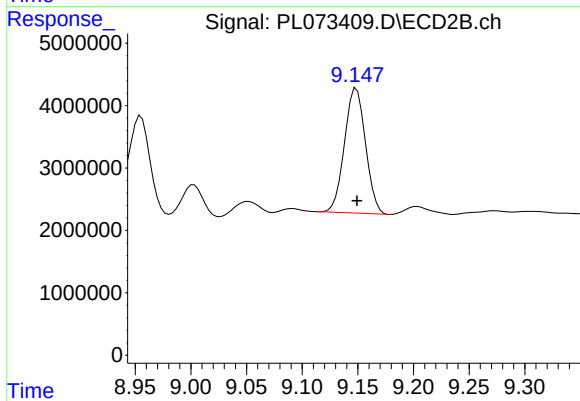

#27 Chlordane-5


R.T.: 9.149 min
Delta R.T.: 0.000 min
Response: 26264709
Conc: 483.90 ng/ml

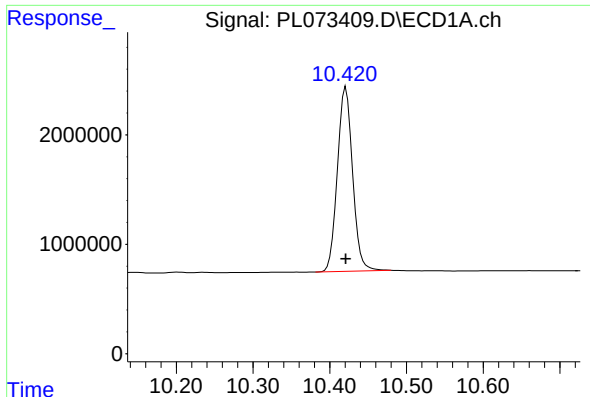

#28 Decachlorobiphenyl

R.T.: 10.421 min
Delta R.T.: 0.000 min
Response: 23203666
Conc: 45.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

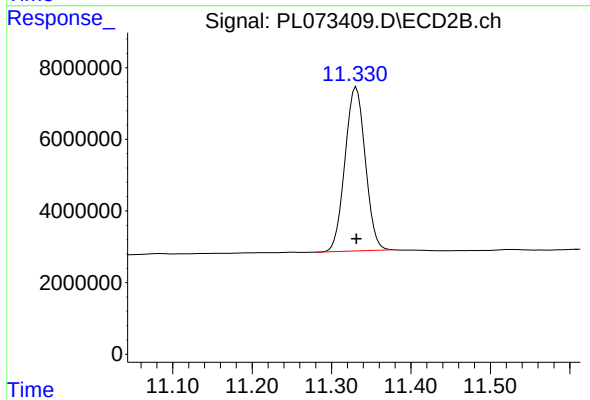

#28 Decachlorobiphenyl

R.T.: 11.331 min
Delta R.T.: 0.000 min
Response: 81385192
Conc: 45.51 ng/ml