

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031622\
 Data File : PL073422.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2022 16:45
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 01:55:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.643	5.491	19781124	88200687	61.761	53.740
28)	SA Decachlor...	10.419	11.330	24024455	87708827	47.246	49.049
Target Compounds							
23)	Chlordane-1	5.975	6.863	5734360	34784596	483.708	509.192
24)	Chlordane-2	6.665	7.445	7844317	37443569	480.866	520.963
25)	Chlordane-3	7.366	8.194	19622463	147.1E6	480.541	542.409
26)	Chlordane-4	7.435	8.281	21139106	178.8E6	476.957	539.739
27)	Chlordane-5	8.384	9.148	7811725	28702920	477.044	528.819



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031622\
Data File : PL073422.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2022 16:45
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 01:55:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

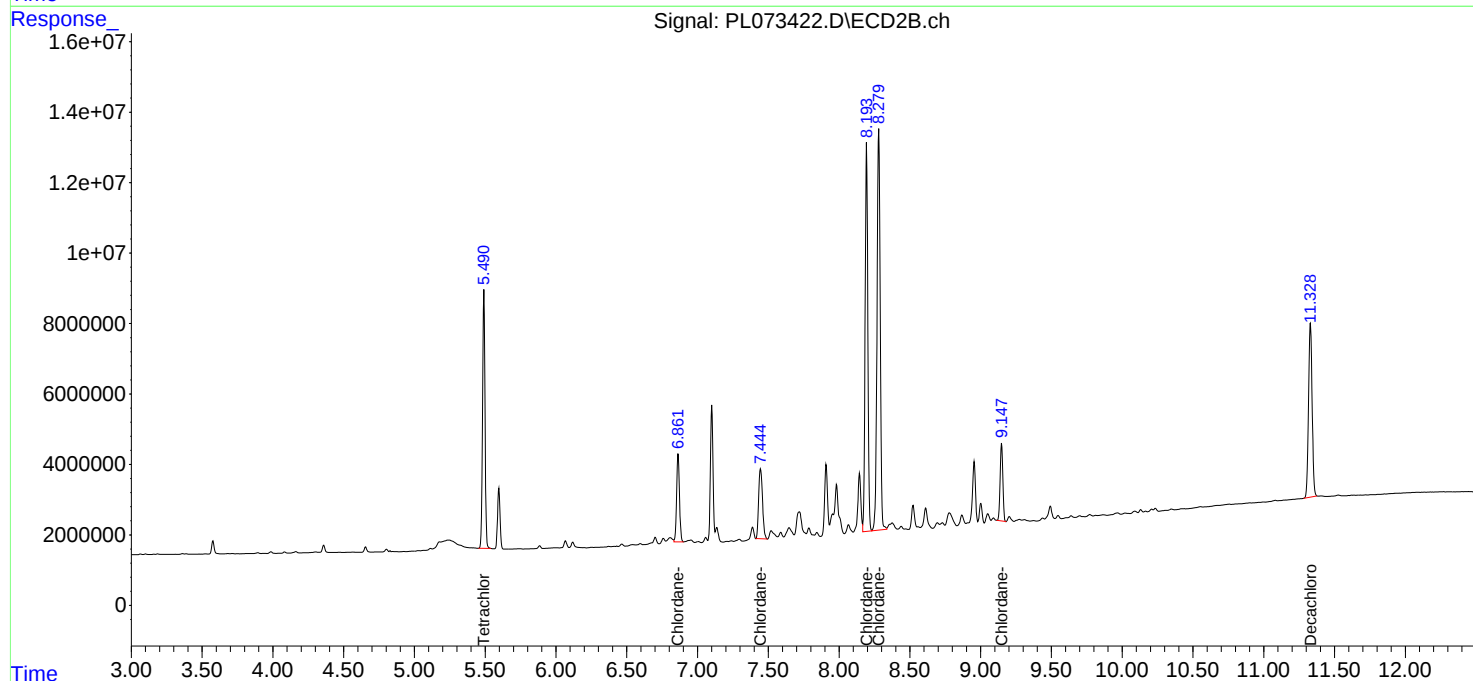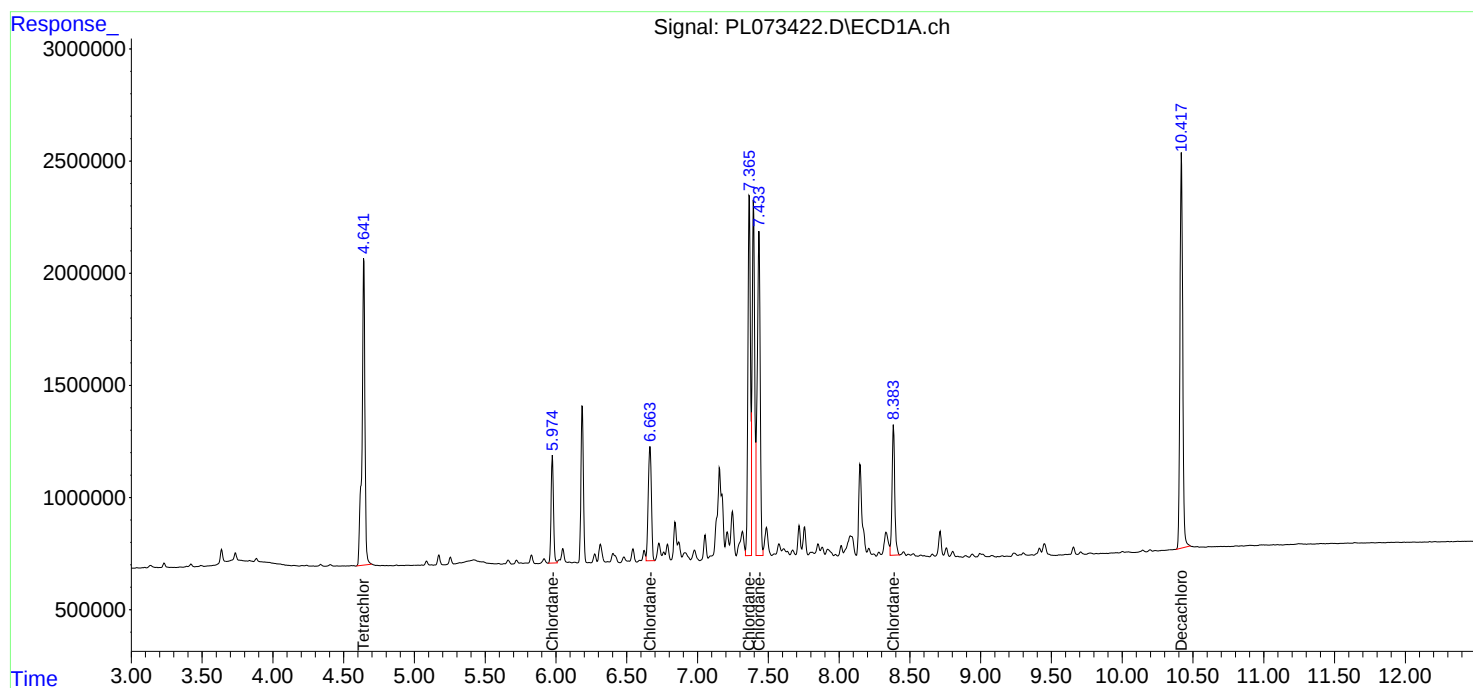


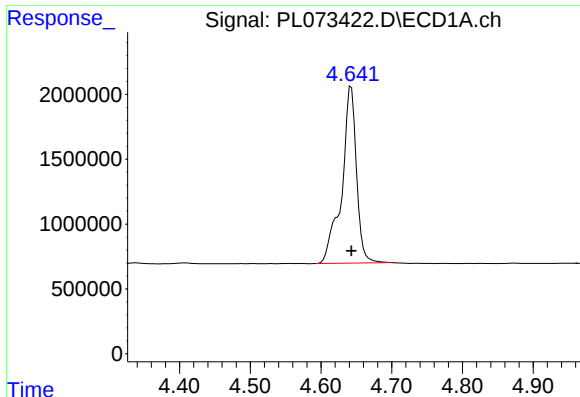

#1 Tetrachloro-m-xylene


R.T.: 4.643 min
Delta R.T.: 0.000 min
Response: 19781124
Conc: 61.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

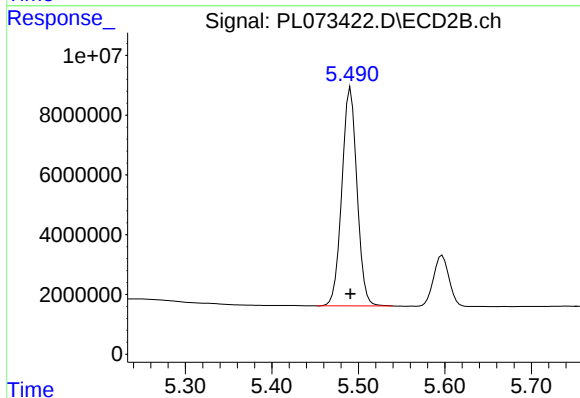


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: 0.000 min
Response: 88200687
Conc: 53.74 ng/ml

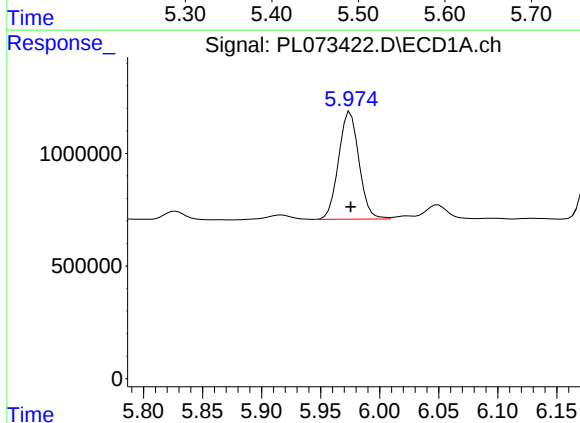


#23 Chlordane-1

R.T.: 5.975 min
Delta R.T.: 0.000 min
Response: 5734360
Conc: 483.71 ng/ml

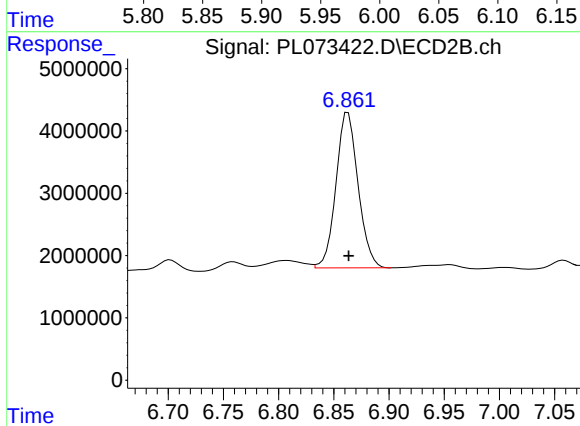

#23 Chlordane-1


R.T.: 6.863 min
Delta R.T.: 0.000 min
Response: 34784596
Conc: 509.19 ng/ml

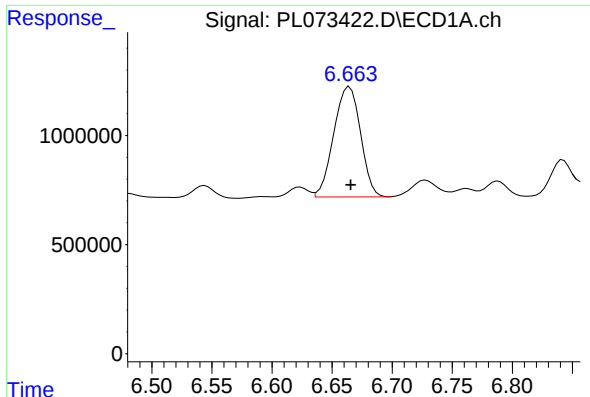

#24 Chlordane-2


R.T.: 6.665 min
Delta R.T.: 0.000 min
Response: 7844317
Conc: 480.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

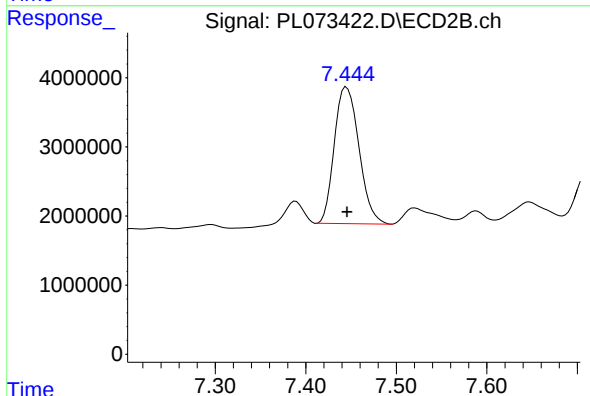


#24 Chlordane-2

R.T.: 7.445 min
Delta R.T.: 0.000 min
Response: 37443569
Conc: 520.96 ng/ml

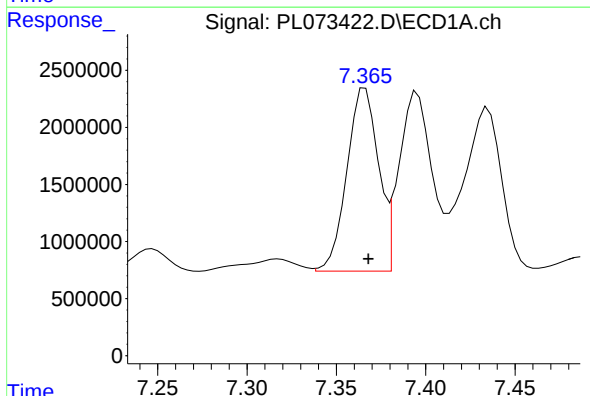


#25 Chlordane-3

R.T.: 7.366 min
Delta R.T.: -0.002 min
Response: 19622463
Conc: 480.54 ng/ml

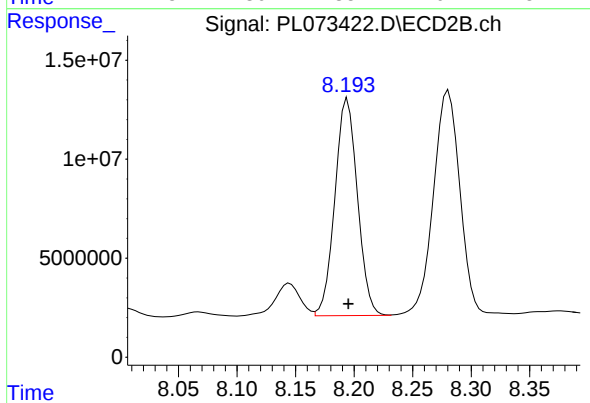

#25 Chlordane-3


R.T.: 8.194 min
Delta R.T.: 0.000 min
Response: 147064454
Conc: 542.41 ng/ml

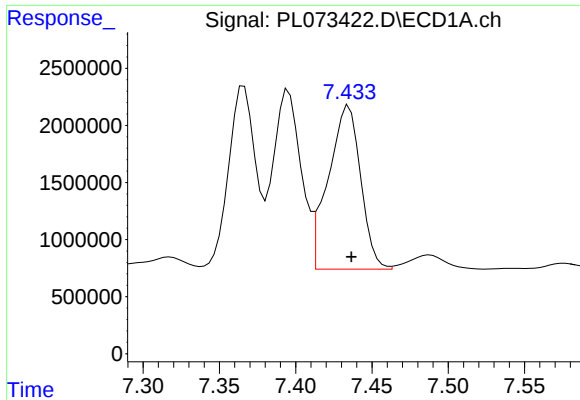

#26 Chlordane-4


R.T.: 7.435 min
Delta R.T.: -0.002 min
Response: 21139106
Conc: 476.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

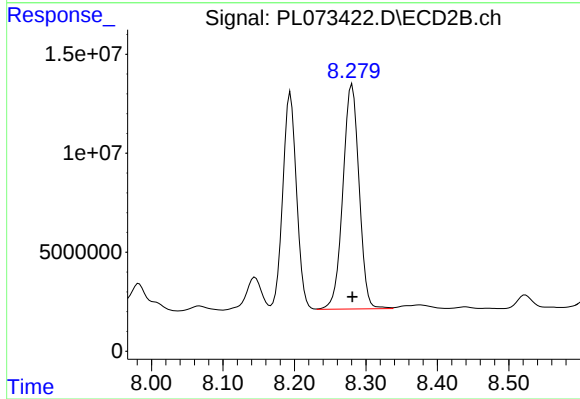


#26 Chlordane-4

R.T.: 8.281 min
Delta R.T.: 0.000 min
Response: 178790134
Conc: 539.74 ng/ml

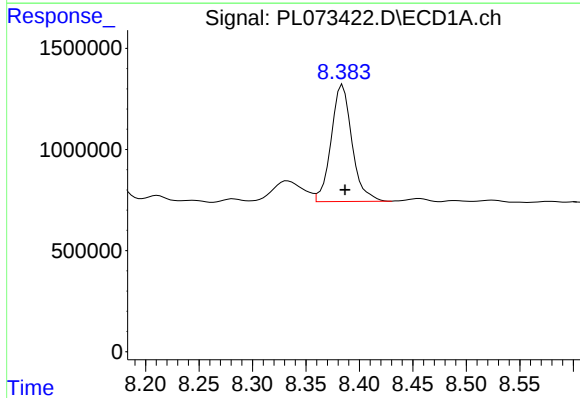


#27 Chlordane-5

R.T.: 8.384 min
Delta R.T.: -0.002 min
Response: 7811725
Conc: 477.04 ng/ml

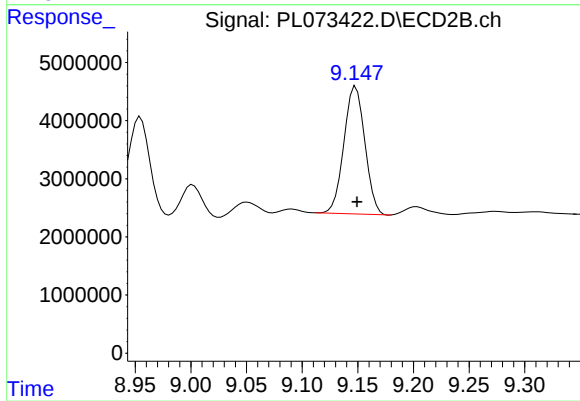

#27 Chlordane-5


R.T.: 9.148 min
Delta R.T.: -0.001 min
Response: 28702920
Conc: 528.82 ng/ml

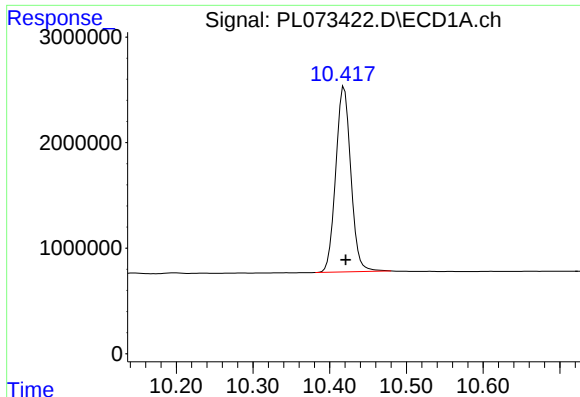

#28 Decachlorobiphenyl

R.T.: 10.419 min
Delta R.T.: -0.002 min
Response: 24024455
Conc: 47.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

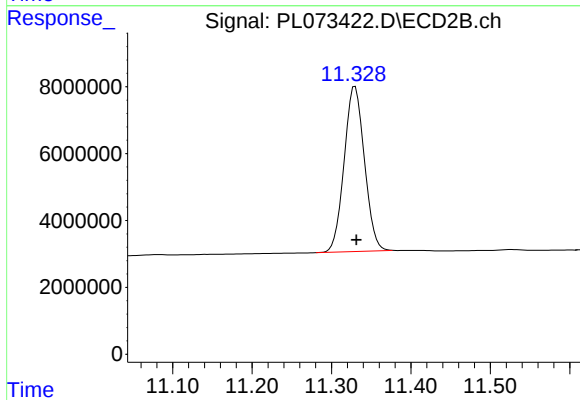

#28 Decachlorobiphenyl

R.T.: 11.330 min
Delta R.T.: -0.002 min
Response: 87708827
Conc: 49.05 ng/ml