

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031622\
 Data File : PL073433.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2022 19:46
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 01:57:28 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.642	5.492	19467419	87043920	60.781	53.035
28)	SA Decachlor...	10.416	11.329	23691796	87200028	46.592	48.765
Target Compounds							
23)	Chlordane-1	5.974	6.863	5650731	34574907	476.654	506.123
24)	Chlordane-2	6.664	7.445	7708015	36762845	472.510	511.492
25)	Chlordane-3	7.365	8.195	19254726	144.1E6	471.535	531.575
26)	Chlordane-4	7.434	8.281	20816966	174.7E6	469.688	527.316
27)	Chlordane-5	8.384	9.149	7466828	29085881	455.981	535.875



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031622\
Data File : PL073433.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2022 19:46
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 01:57:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

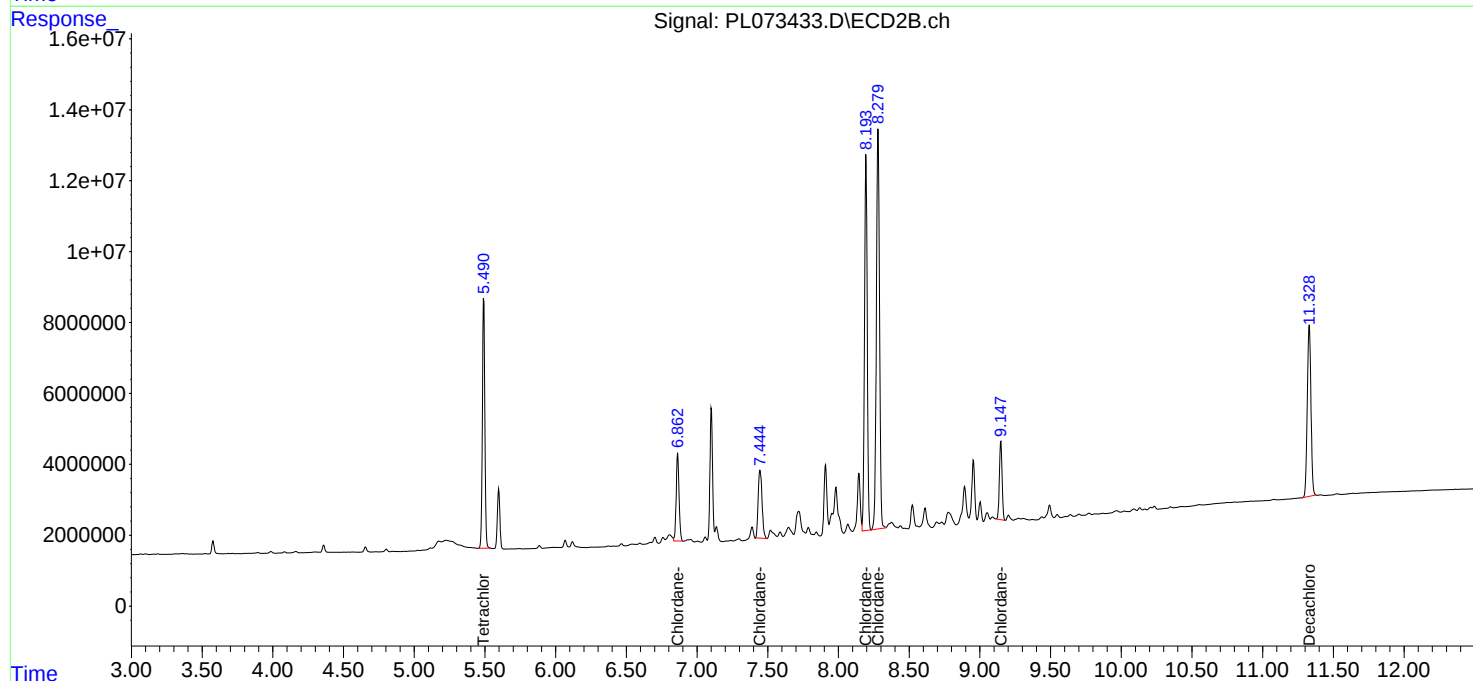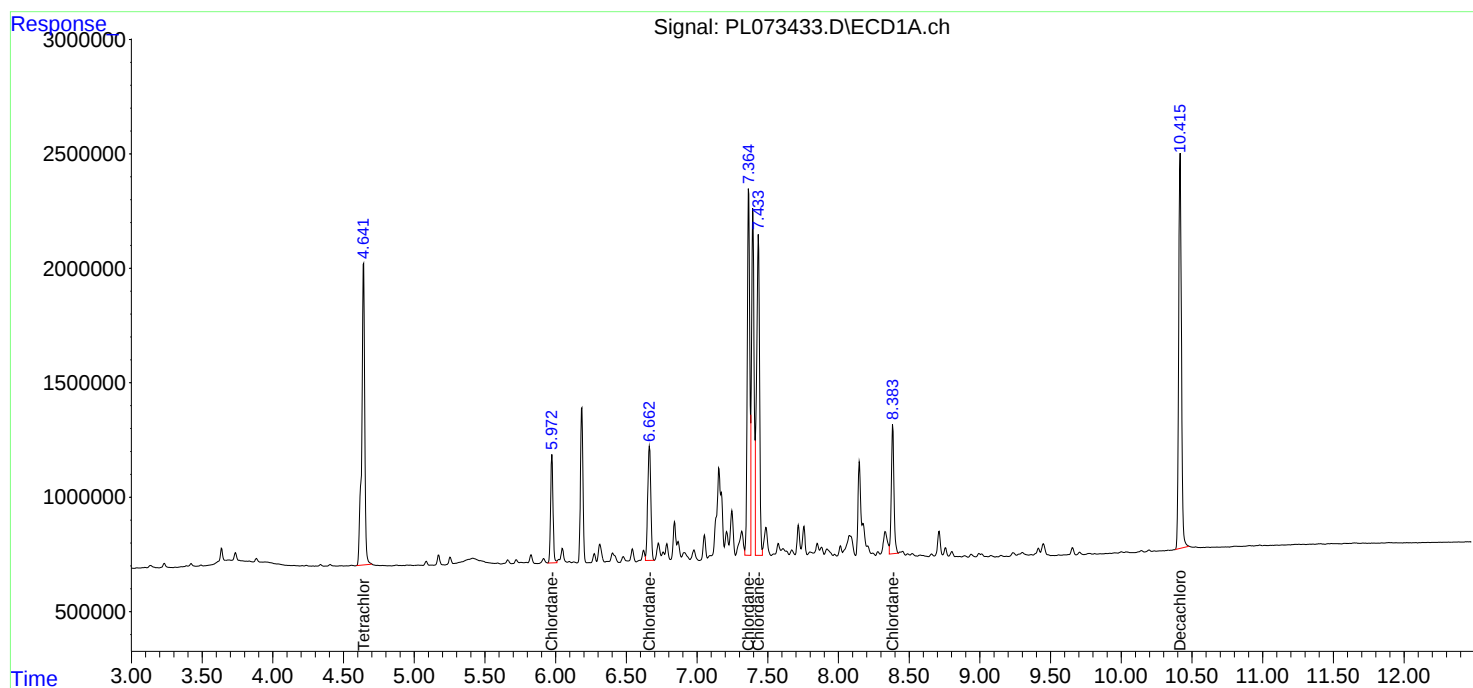


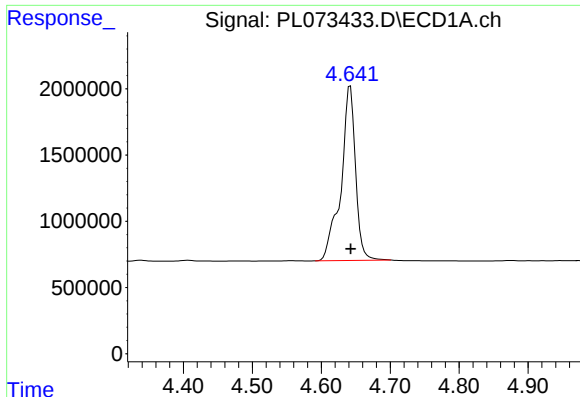

#1 Tetrachloro-m-xylene


R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 19467419
Conc: 60.78 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

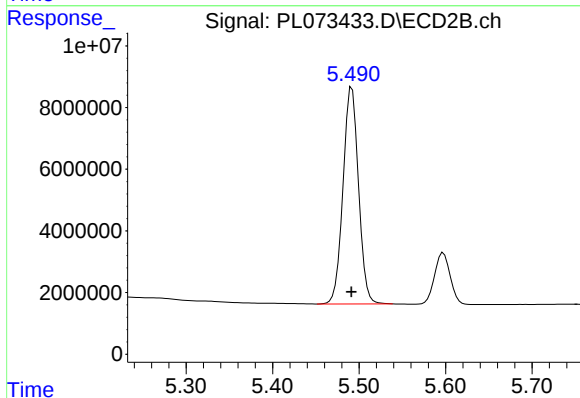


#1 Tetrachloro-m-xylene

R.T.: 5.492 min
Delta R.T.: 0.000 min
Response: 87043920
Conc: 53.04 ng/ml

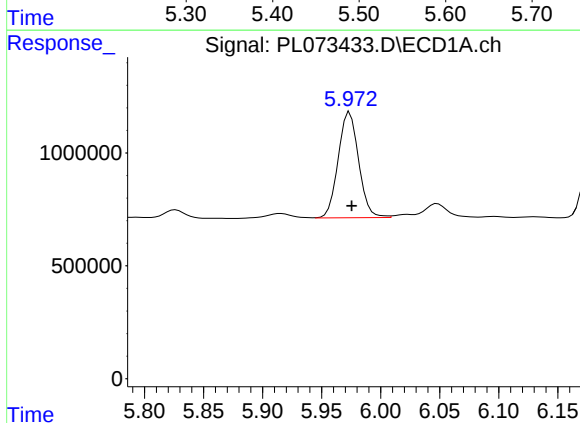


#23 Chlordane-1

R.T.: 5.974 min
Delta R.T.: -0.002 min
Response: 5650731
Conc: 476.65 ng/ml

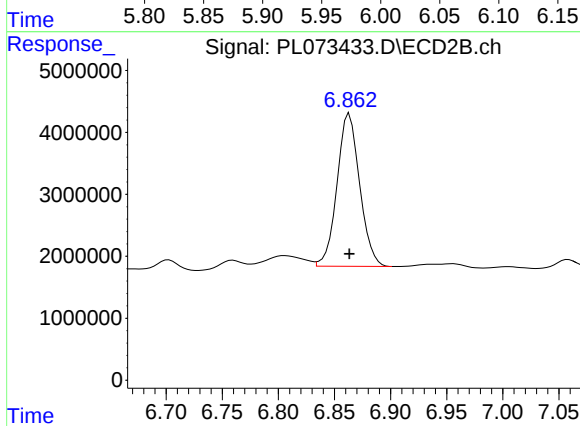

#23 Chlordane-1


R.T.: 6.863 min
Delta R.T.: 0.000 min
Response: 34574907
Conc: 506.12 ng/ml

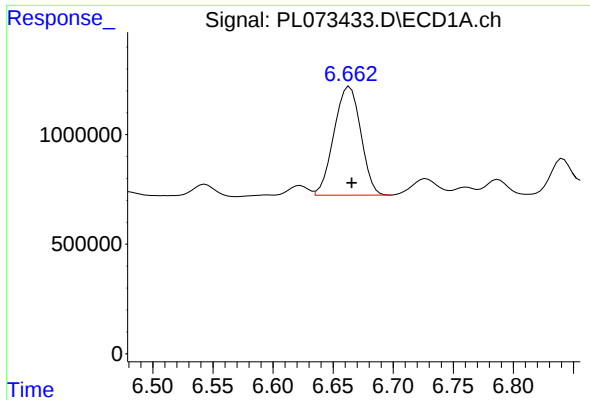

#24 Chlordane-2


R.T.: 6.664 min
Delta R.T.: -0.002 min
Response: 7708015
Conc: 472.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

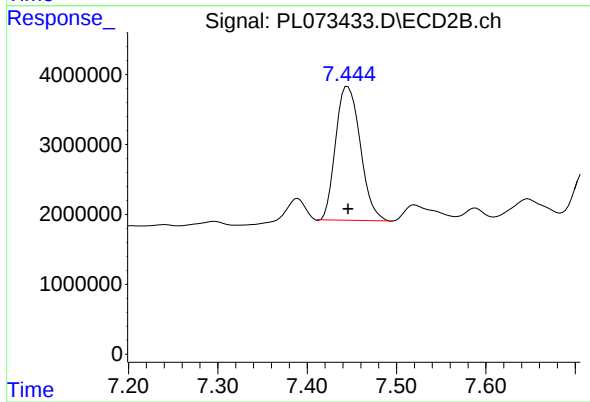


#24 Chlordane-2

R.T.: 7.445 min
Delta R.T.: 0.000 min
Response: 36762845
Conc: 511.49 ng/ml

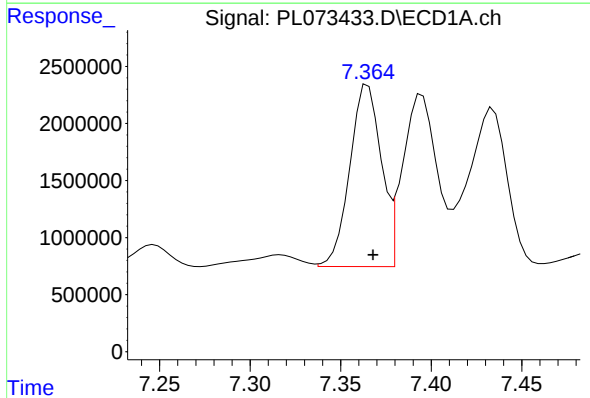


#25 Chlordane-3

R.T.: 7.365 min
Delta R.T.: -0.003 min
Response: 19254726
Conc: 471.53 ng/ml

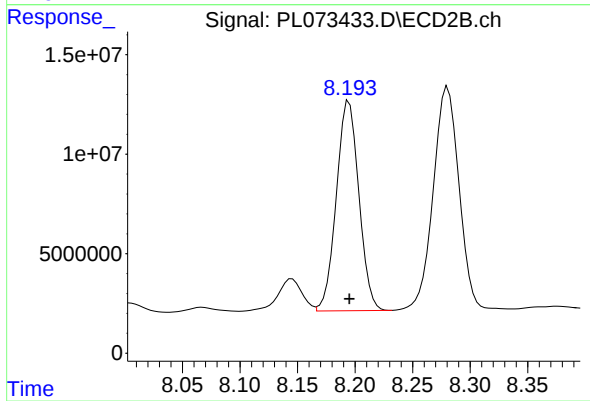

#25 Chlordane-3


R.T.: 8.195 min
Delta R.T.: 0.000 min
Response: 144127020
Conc: 531.57 ng/ml

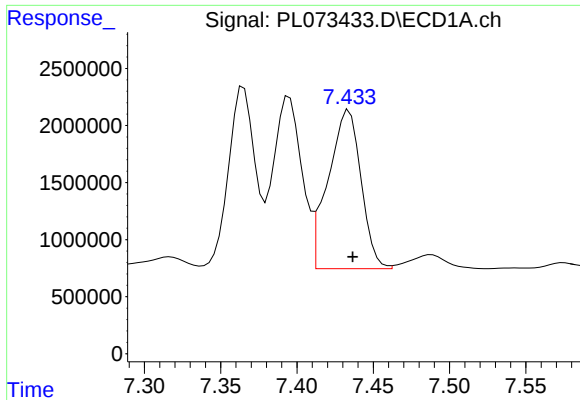

#26 Chlordane-4


R.T.: 7.434 min
Delta R.T.: -0.003 min
Response: 20816966
Conc: 469.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

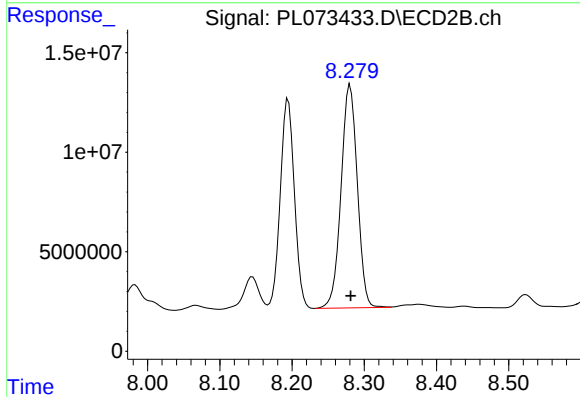


#26 Chlordane-4

R.T.: 8.281 min
Delta R.T.: 0.000 min
Response: 174674758
Conc: 527.32 ng/ml

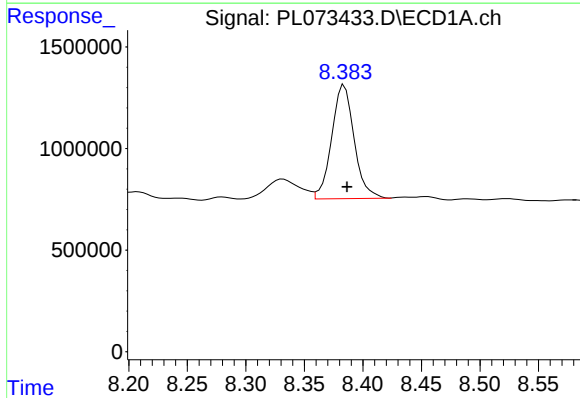


#27 Chlordane-5

R.T.: 8.384 min
Delta R.T.: -0.002 min
Response: 7466828
Conc: 455.98 ng/ml

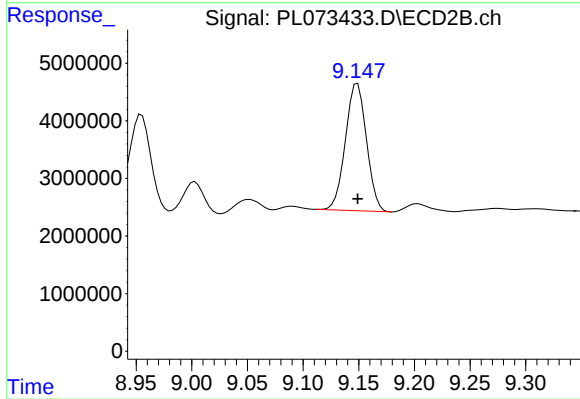

#27 Chlordane-5


R.T.: 9.149 min
Delta R.T.: 0.000 min
Response: 29085881
Conc: 535.87 ng/ml

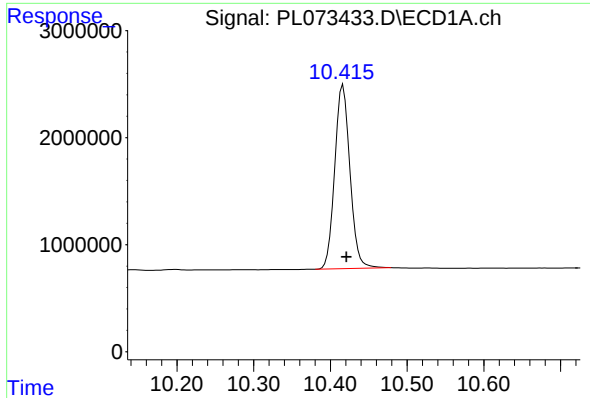

#28 Decachlorobiphenyl

R.T.: 10.416 min
Delta R.T.: -0.005 min
Response: 23691796
Conc: 46.59 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

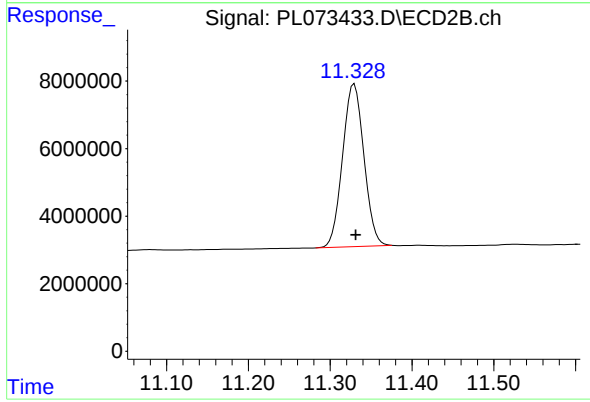

#28 Decachlorobiphenyl

R.T.: 11.329 min
Delta R.T.: -0.002 min
Response: 87200028
Conc: 48.76 ng/ml