

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031623\
 Data File : PL081488.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2023 09:24
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 21:44:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030223.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 03 01:48:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.332	2.661	106.5E6	112.0E6	49.278	55.347
28)	SA Decachlor...	8.757	7.783	71651589	90167078	46.999	47.071
Target Compounds							
23)	Chlordane-1	4.476	3.650	46858306	37195104	489.451	451.083
24)	Chlordane-2	5.003	4.225	48536732	45140701	484.980	440.960
25)	Chlordane-3	5.709	4.853	178.6E6	123.8E6	488.284	458.111
26)	Chlordane-4	5.790	4.914	214.2E6	124.7E6	487.432	443.941
27)	Chlordane-5	6.631	5.580	35654700	32228700	473.109	466.512



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031623\
Data File : PL081488.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2023 09:24
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 21:44:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030223.M
Quant Title : GC Extractables
QLast Update : Fri Mar 03 01:48:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

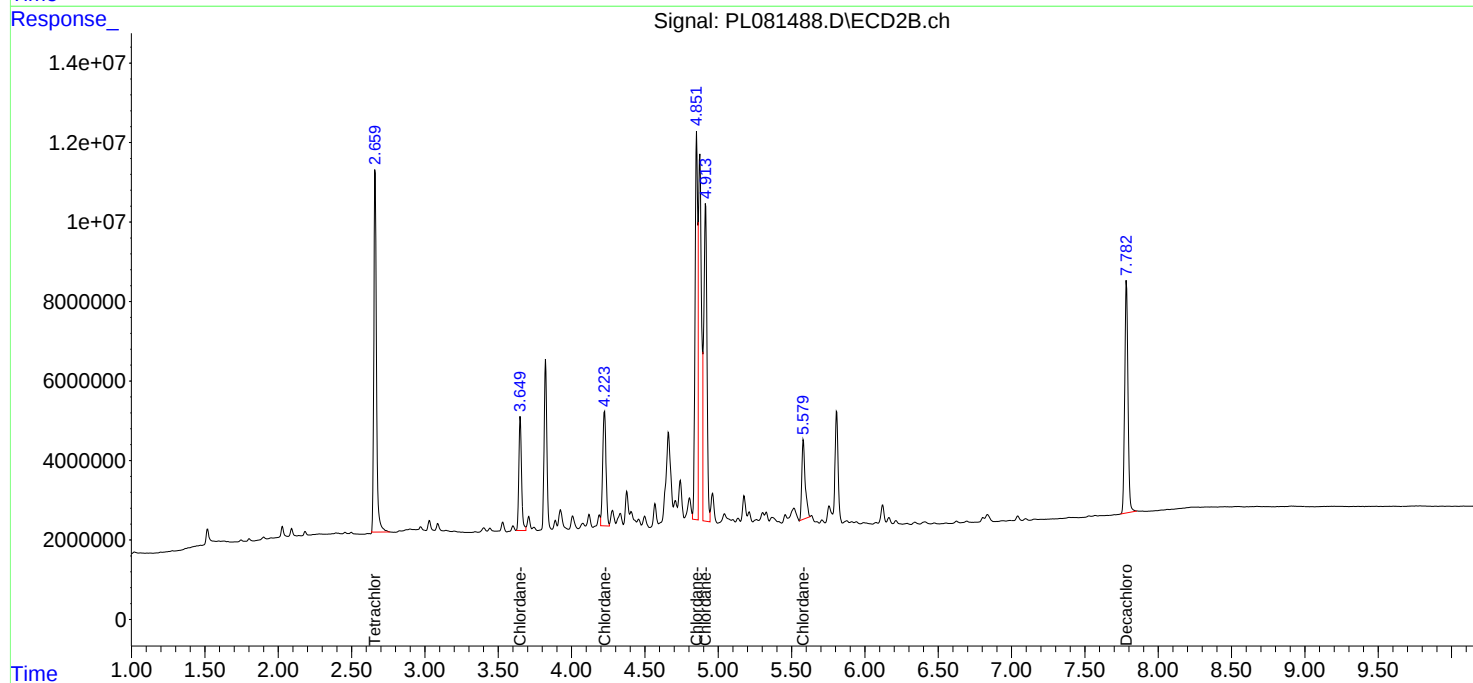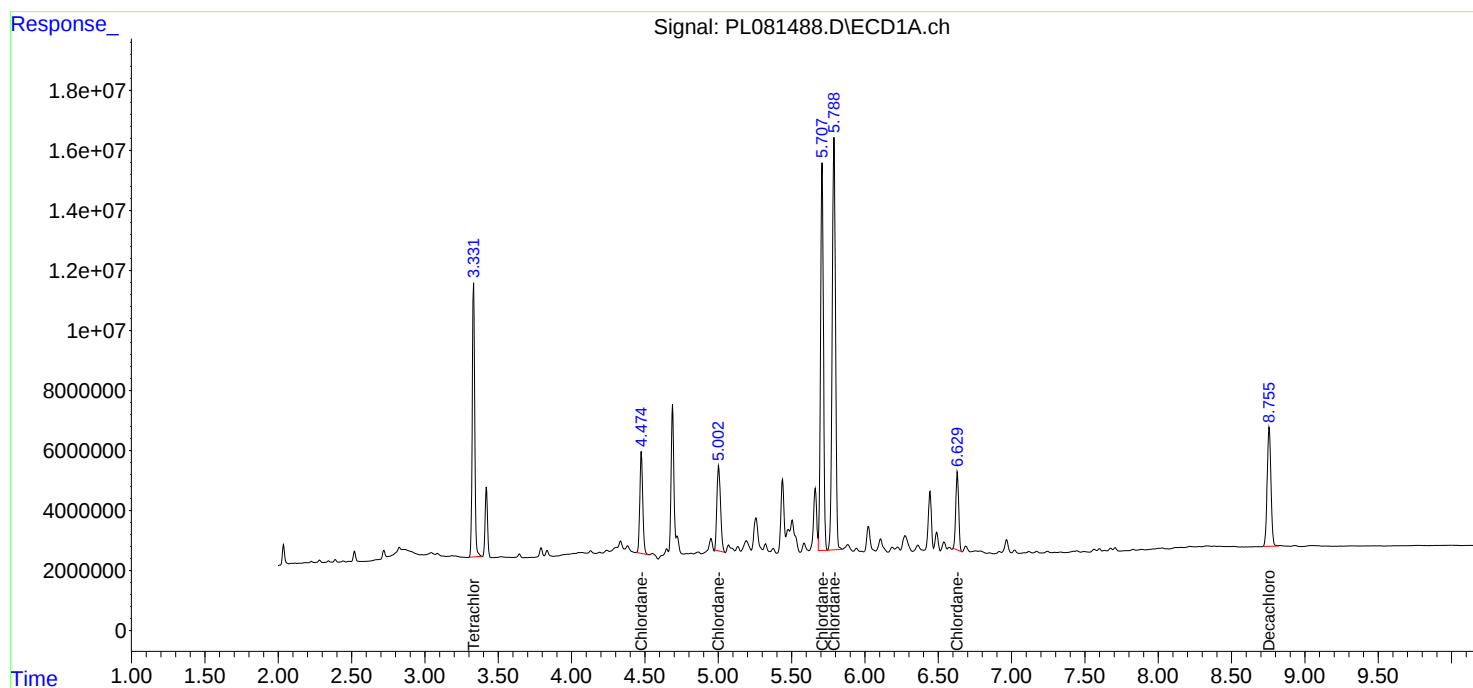


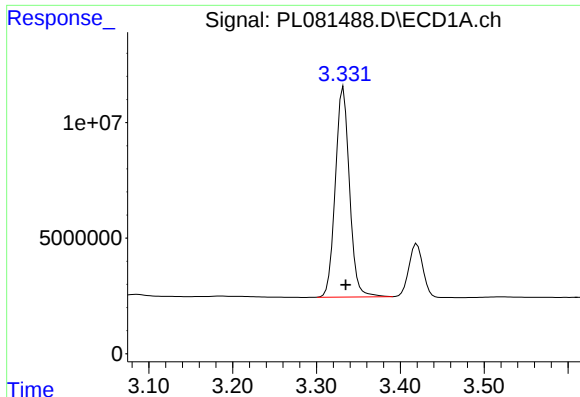

#1 Tetrachloro-m-xylene


R.T.: 3.332 min
Delta R.T.: -0.003 min
Response: 106468462
Conc: 49.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

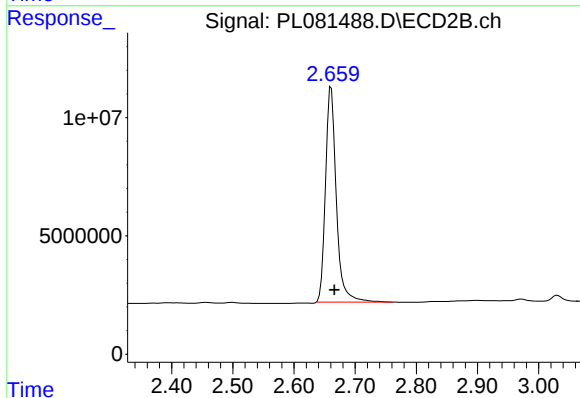


#1 Tetrachloro-m-xylene

R.T.: 2.661 min
Delta R.T.: -0.006 min
Response: 112012883
Conc: 55.35 ng/ml

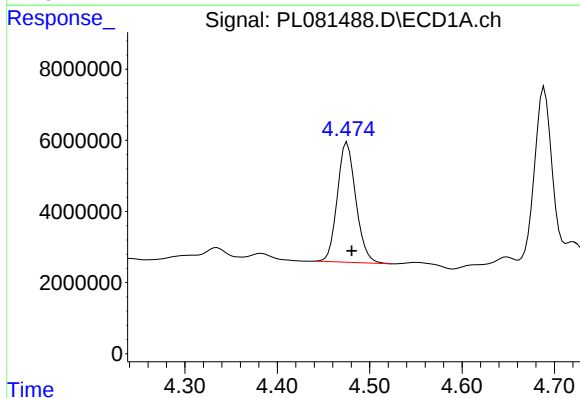


#23 Chlordane-1

R.T.: 4.476 min
Delta R.T.: -0.005 min
Response: 46858306
Conc: 489.45 ng/ml

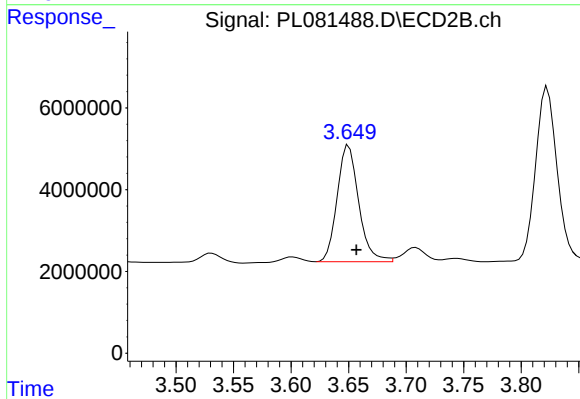

#23 Chlordane-1


R.T.: 3.650 min
Delta R.T.: -0.007 min
Response: 37195104
Conc: 451.08 ng/ml

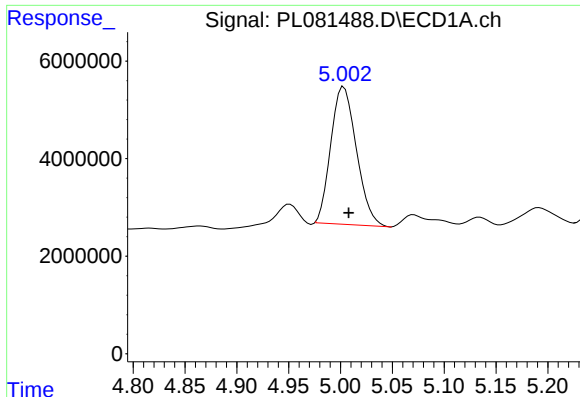

#24 Chlordane-2


R.T.: 5.003 min
Delta R.T.: -0.005 min
Response: 48536732
Conc: 484.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

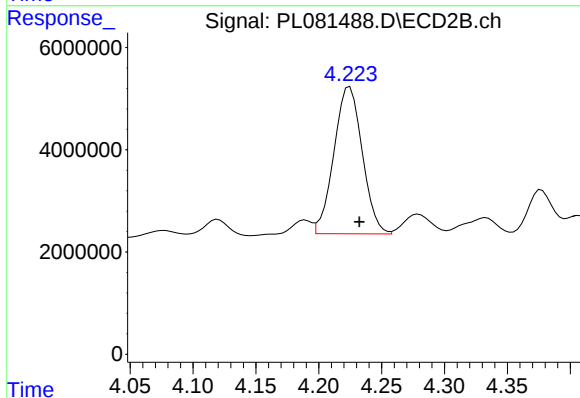


#24 Chlordane-2

R.T.: 4.225 min
Delta R.T.: -0.008 min
Response: 45140701
Conc: 440.96 ng/ml

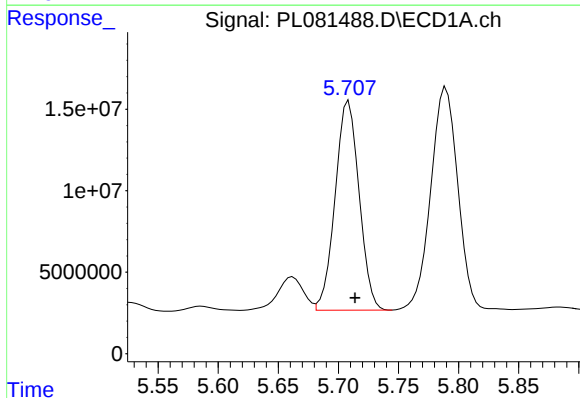


#25 Chlordane-3

R.T.: 5.709 min
Delta R.T.: -0.005 min
Response: 178603349
Conc: 488.28 ng/ml

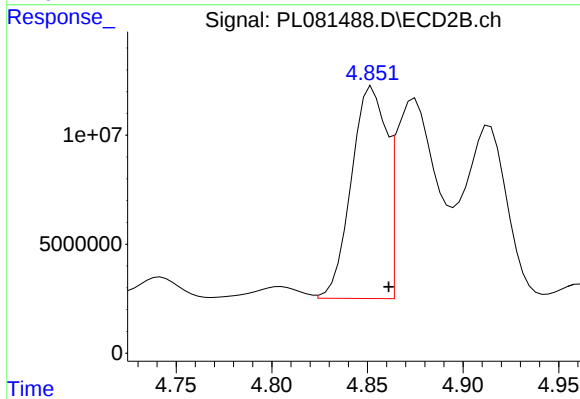

#25 Chlordane-3


R.T.: 4.853 min
Delta R.T.: -0.008 min
Response: 123809600
Conc: 458.11 ng/ml

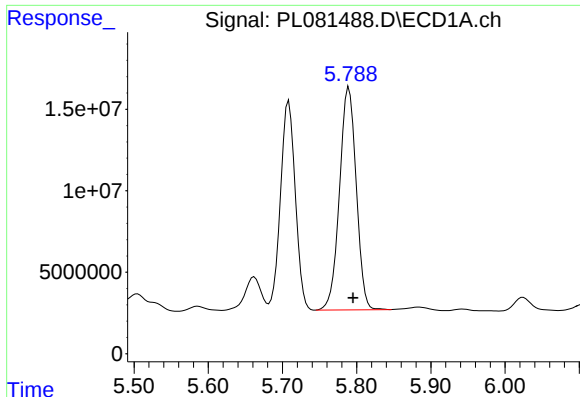

#26 Chlordane-4


R.T.: 5.790 min
Delta R.T.: -0.005 min
Response: 214242294
Conc: 487.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

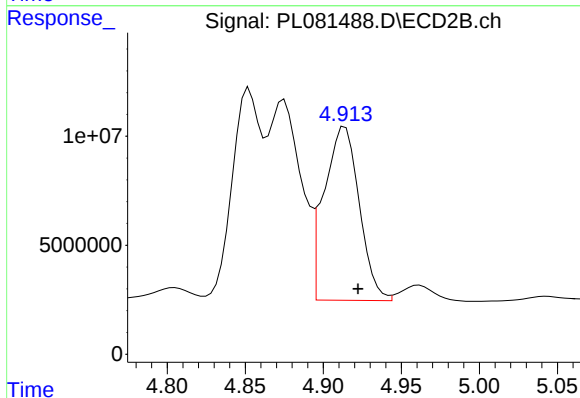


#26 Chlordane-4

R.T.: 4.914 min
Delta R.T.: -0.008 min
Response: 124675995
Conc: 443.94 ng/ml

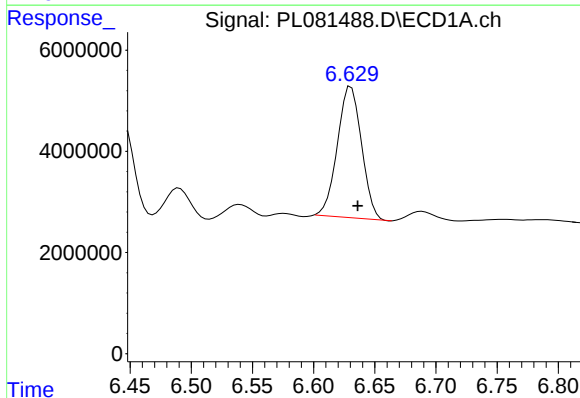


#27 Chlordane-5

R.T.: 6.631 min
Delta R.T.: -0.006 min
Response: 35654700
Conc: 473.11 ng/ml

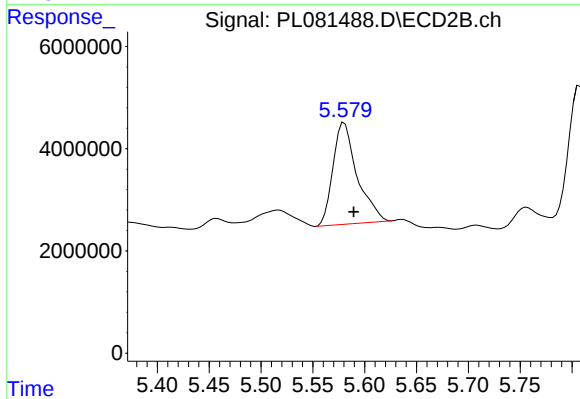

#27 Chlordane-5


R.T.: 5.580 min
Delta R.T.: -0.009 min
Response: 32228700
Conc: 466.51 ng/ml

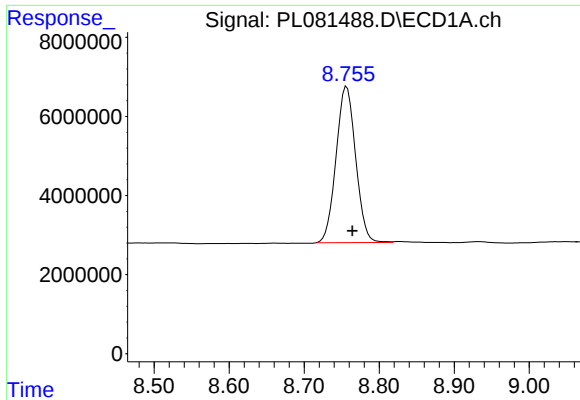

#28 Decachlorobiphenyl

R.T.: 8.757 min
Delta R.T.: -0.008 min
Response: 71651589
Conc: 47.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

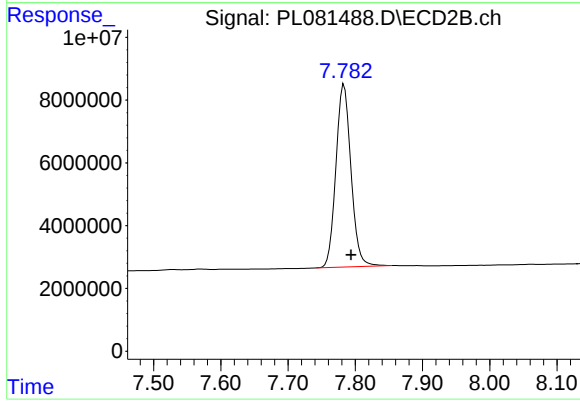

#28 Decachlorobiphenyl

R.T.: 7.783 min
Delta R.T.: -0.011 min
Response: 90167078
Conc: 47.07 ng/ml