

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031623\
 Data File : PL081501.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2023 14:41
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 21:52:20 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030223.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 03 01:48:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.332	2.661	94787672	105.4E6	43.872	52.100
28)	SA Decachlor...	8.755	7.782	66281518	85743614	43.476	44.762
Target Compounds							
23)	Chlordane-1	4.475	3.649	40811532	34547806	426.290	418.978
24)	Chlordane-2	5.002	4.224	42459817	41555353	424.259	405.936
25)	Chlordane-3	5.708	4.852	161.6E6	114.1E6	441.716	422.129
26)	Chlordane-4	5.789	4.913	194.1E6	116.4E6	441.574	414.600
27)	Chlordane-5	6.630	5.579	32330321	29994522	428.997	434.172



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031623\
Data File : PL081501.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2023 14:41
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 21:52:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030223.M
Quant Title : GC Extractables
QLast Update : Fri Mar 03 01:48:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

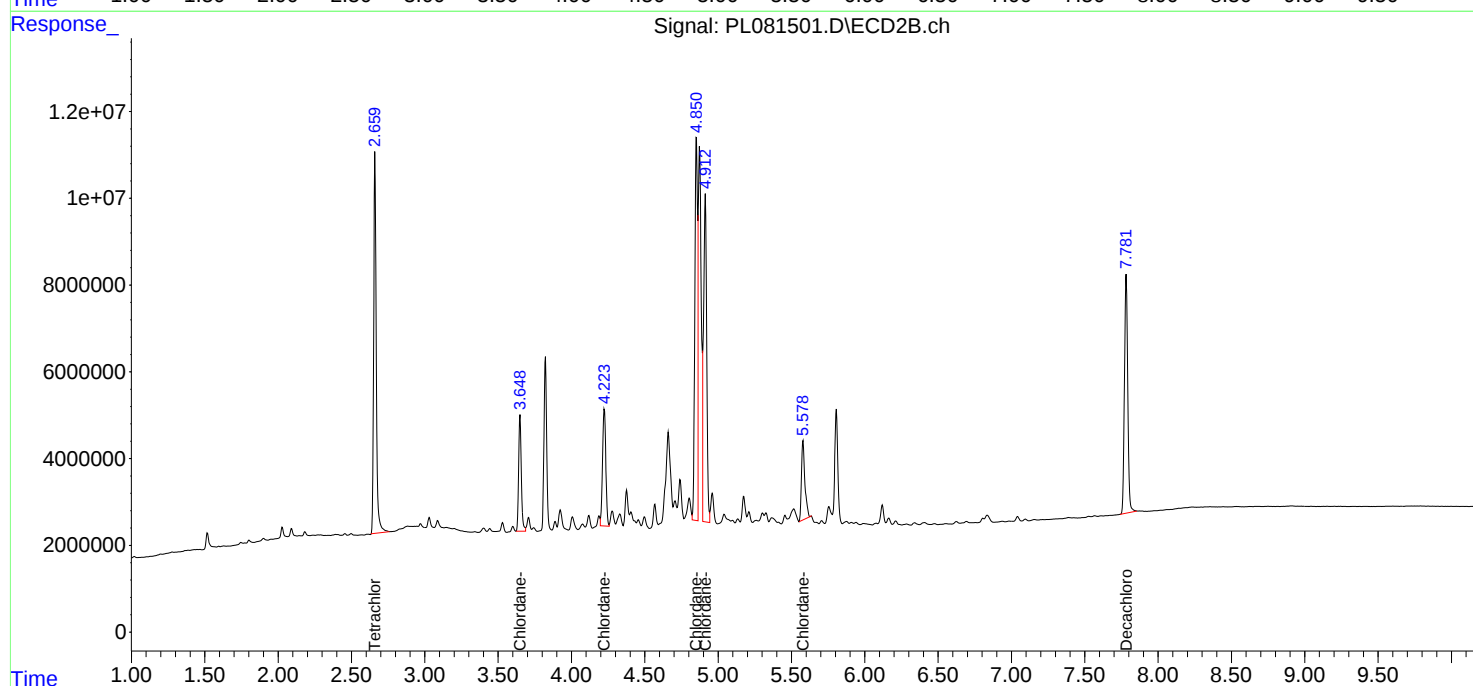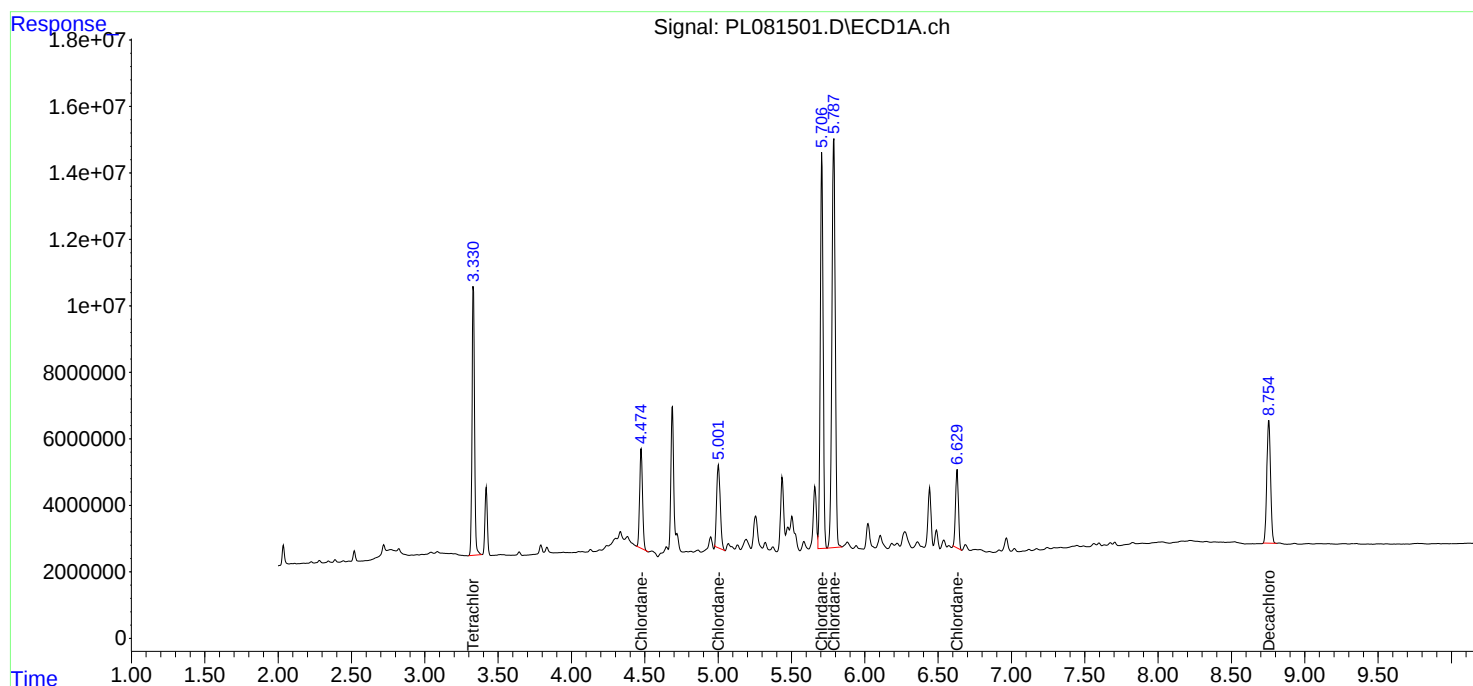


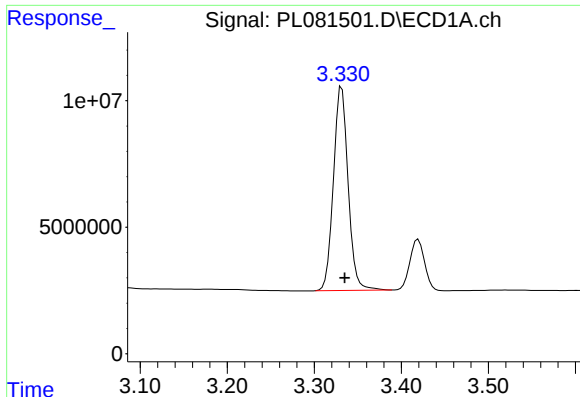

#1 Tetrachloro-m-xylene


R.T.: 3.332 min
Delta R.T.: -0.003 min
Response: 94787672
Conc: 43.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

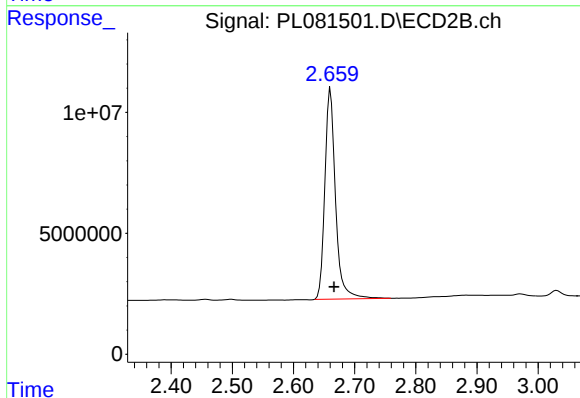


#1 Tetrachloro-m-xylene

R.T.: 2.661 min
Delta R.T.: -0.006 min
Response: 105442385
Conc: 52.10 ng/ml

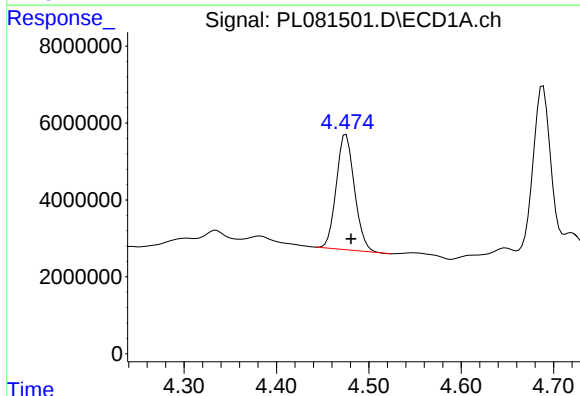


#23 Chlordane-1

R.T.: 4.475 min
Delta R.T.: -0.005 min
Response: 40811532
Conc: 426.29 ng/ml

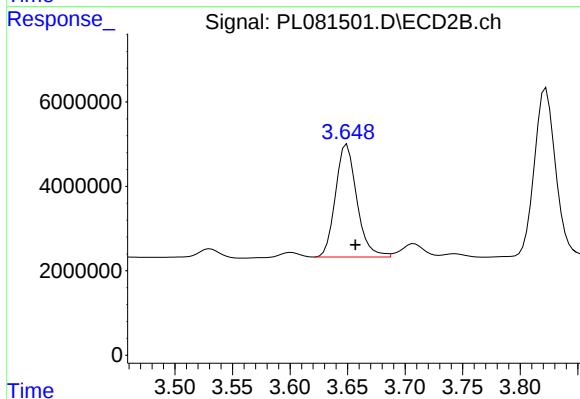

#23 Chlordane-1


R.T.: 3.649 min
Delta R.T.: -0.007 min
Response: 34547806
Conc: 418.98 ng/ml

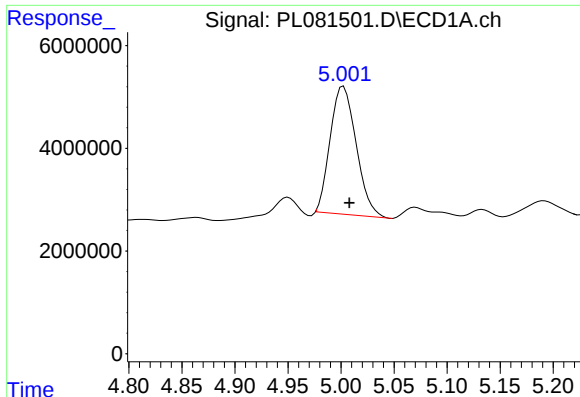

#24 Chlordane-2


R.T.: 5.002 min
Delta R.T.: -0.006 min
Response: 42459817
Conc: 424.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

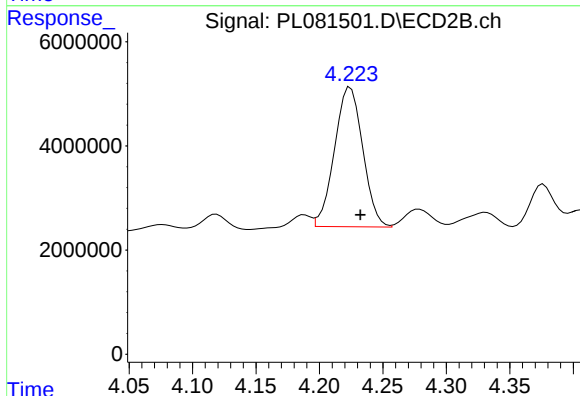


#24 Chlordane-2

R.T.: 4.224 min
Delta R.T.: -0.008 min
Response: 4155353
Conc: 405.94 ng/ml

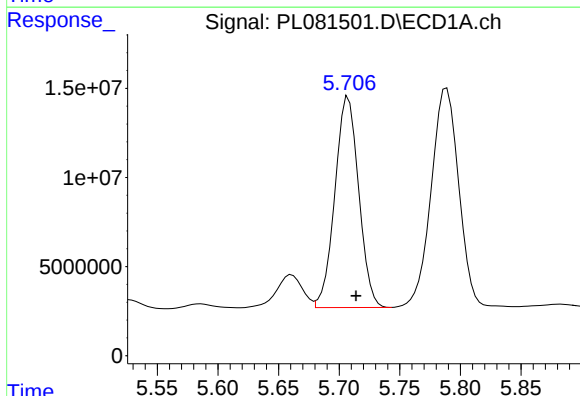


#25 Chlordane-3

R.T.: 5.708 min
Delta R.T.: -0.006 min
Response: 161569682
Conc: 441.72 ng/ml

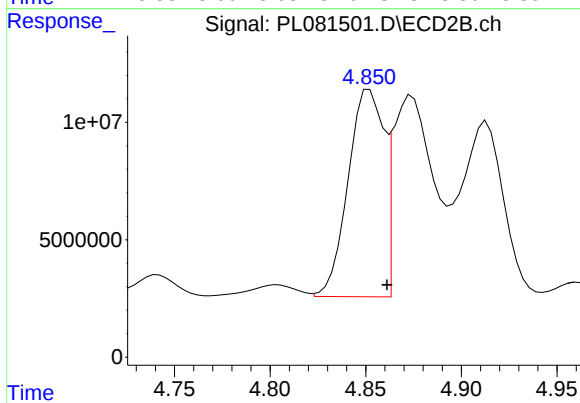

#25 Chlordane-3


R.T.: 4.852 min
Delta R.T.: -0.009 min
Response: 114084966
Conc: 422.13 ng/ml

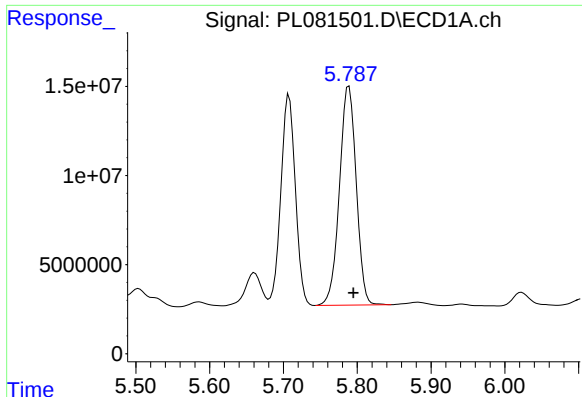

#26 Chlordane-4


R.T.: 5.789 min
Delta R.T.: -0.006 min
Response: 194086579
Conc: 441.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

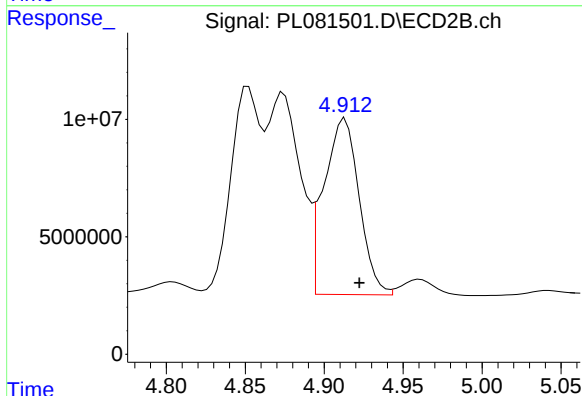


#26 Chlordane-4

R.T.: 4.913 min
Delta R.T.: -0.009 min
Response: 116435830
Conc: 414.60 ng/ml

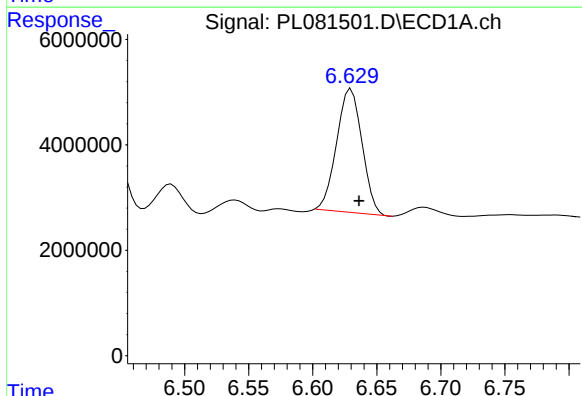


#27 Chlordane-5

R.T.: 6.630 min
Delta R.T.: -0.006 min
Response: 32330321
Conc: 429.00 ng/ml

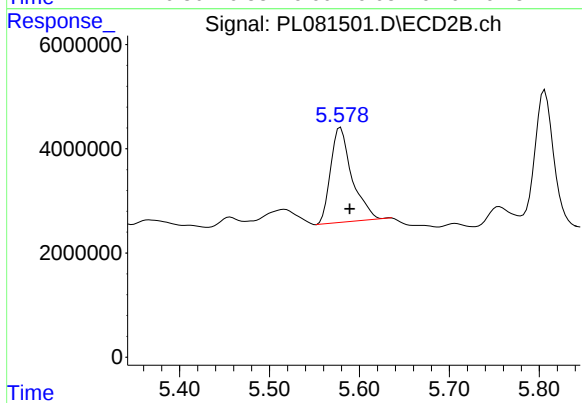

#27 Chlordane-5


R.T.: 5.579 min
Delta R.T.: -0.010 min
Response: 29994522
Conc: 434.17 ng/ml

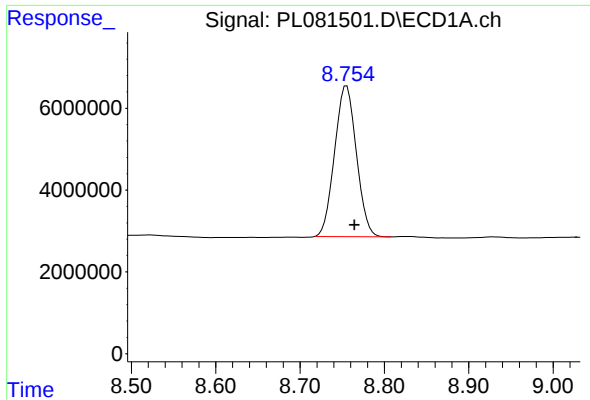

#28 Decachlorobiphenyl

R.T.: 8.755 min
Delta R.T.: -0.009 min
Response: 66281518
Conc: 43.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

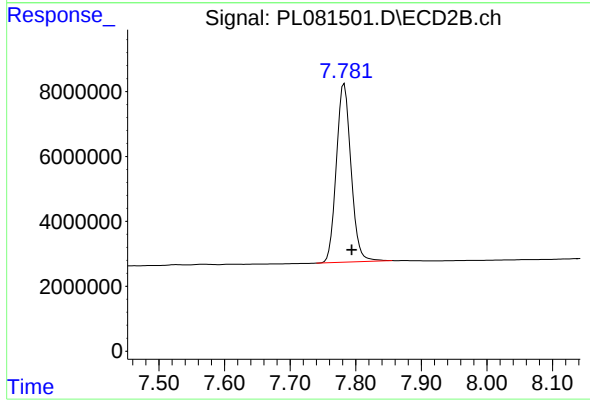

#28 Decachlorobiphenyl

R.T.: 7.782 min
Delta R.T.: -0.011 min
Response: 85743614
Conc: 44.76 ng/ml