

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031623\
 Data File : PL081505.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2023 15:59
 Operator : AR\AJ
 Sample : 01908-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HILLBOR-DRUMS-0314

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 21:55:06 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030223.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 03 01:48:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.332	2.661	50225921	46208187	23.247	22.832
28) SA Decachlor...	8.756	7.782	33153647	41709954	21.747	21.775

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031623\
Data File : PL081505.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2023 15:59
Operator : AR\AJ
Sample : 01908-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HILLBOR-DRUMS-0314

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 21:55:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030223.M
Quant Title : GC Extractables
QLast Update : Fri Mar 03 01:48:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

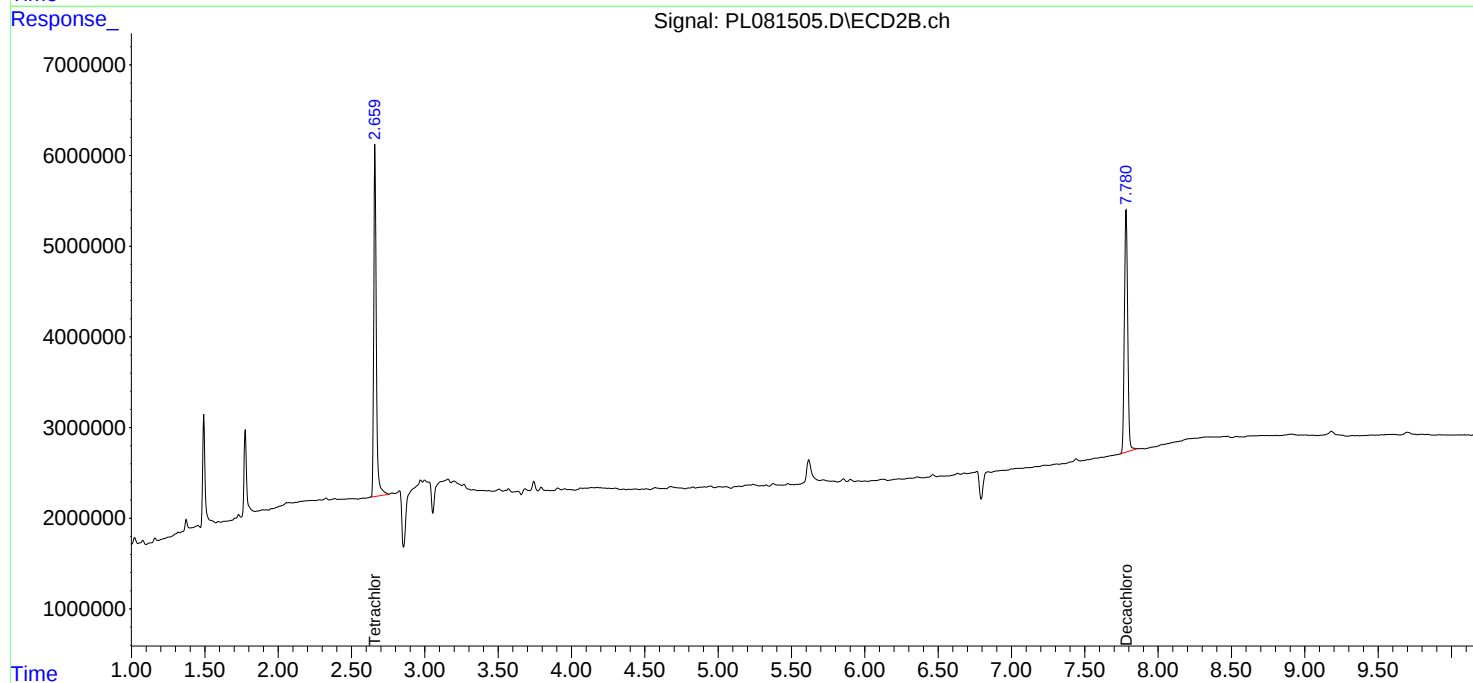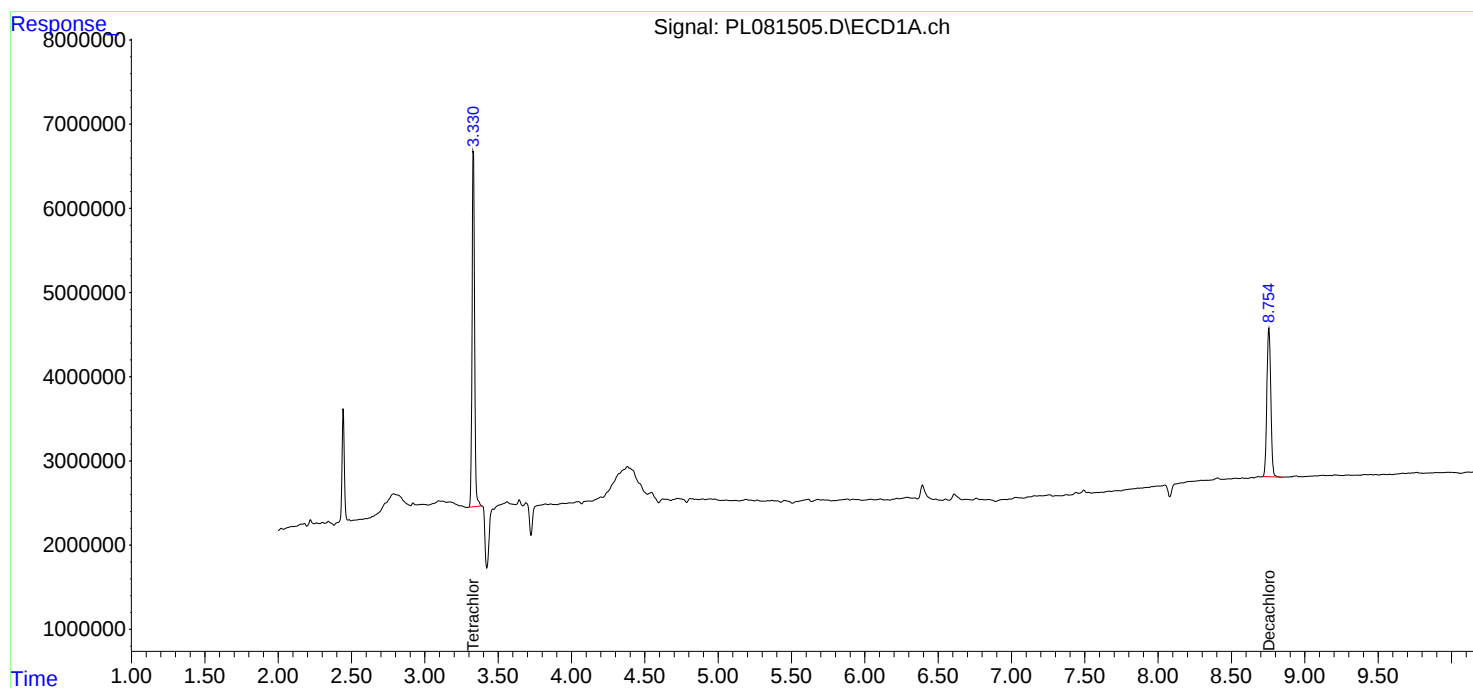


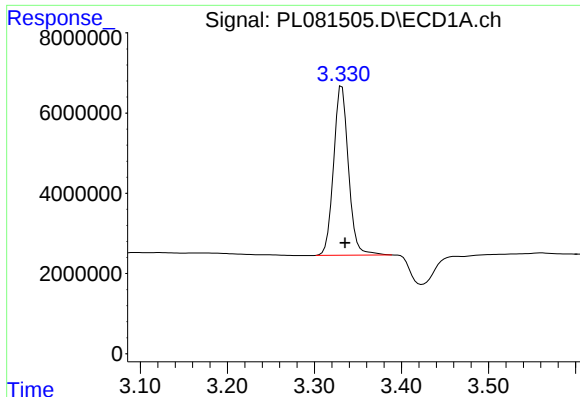

#1 Tetrachloro-m-xylene


R.T.: 3.332 min
Delta R.T.: -0.003 min
Response: 50225921
Conc: 23.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
HILLBOR-DRUMS-0314

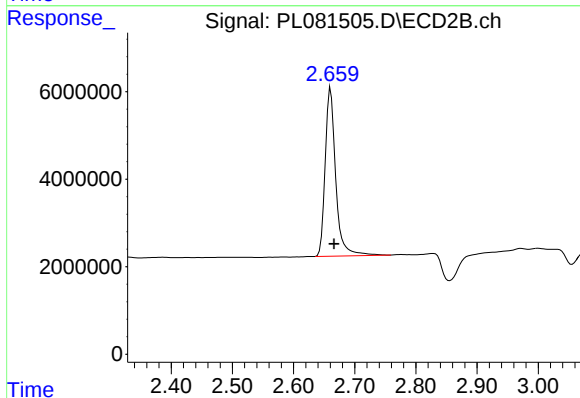


#1 Tetrachloro-m-xylene

R.T.: 2.661 min
Delta R.T.: -0.006 min
Response: 46208187
Conc: 22.83 ng/ml

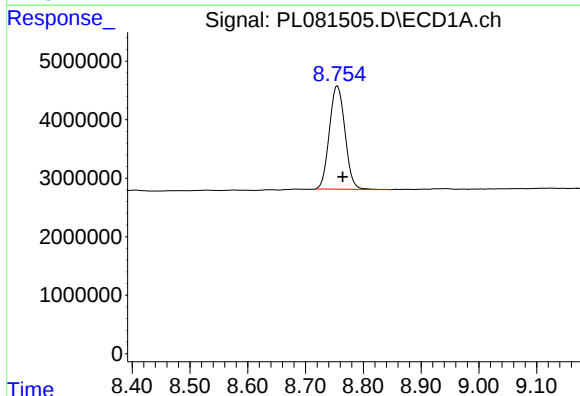

#28 Decachlorobiphenyl

R.T.: 8.756 min
Delta R.T.: -0.009 min
Response: 33153647
Conc: 21.75 ng/ml

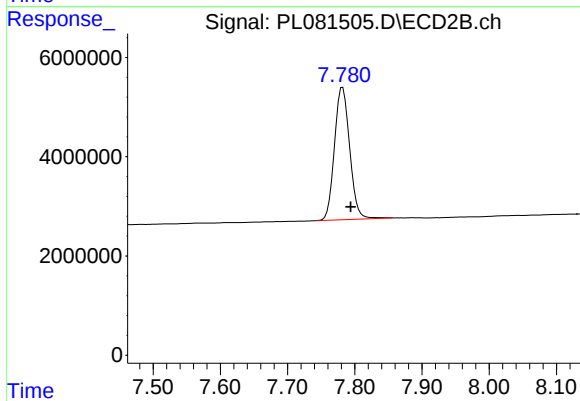

#28 Decachlorobiphenyl

R.T.: 7.782 min
Delta R.T.: -0.012 min
Response: 41709954
Conc: 21.77 ng/ml