

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031623\
 Data File : PL081521.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Mar 2023 20:53
 Operator : AR\AJ
 Sample : 01932-15
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 JPP-6A-031423

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 03/17/2023
 Supervised By :Ankita Jodhani 03/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 16 22:07:00 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030223.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 03 01:48:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.330	2.660	19143341	17308603	8.860	8.552
28)	SA Decachlor...	8.754	7.781	15174509	17913134	9.954	9.351
Target Compounds							
17)	MA 4,4'-DDT	6.786	5.905	1500544	2174281	0.945m	1.355 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031623\
Data File : PL081521.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Mar 2023 20:53
Operator : AR\AJ
Sample : 01932-15
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
JPP-6A-031423


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/17/2023
Supervised By : Ankita Jodhani 03/17/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 16 22:07:00 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030223.M
Quant Title : GC Extractables
QLast Update : Fri Mar 03 01:48:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

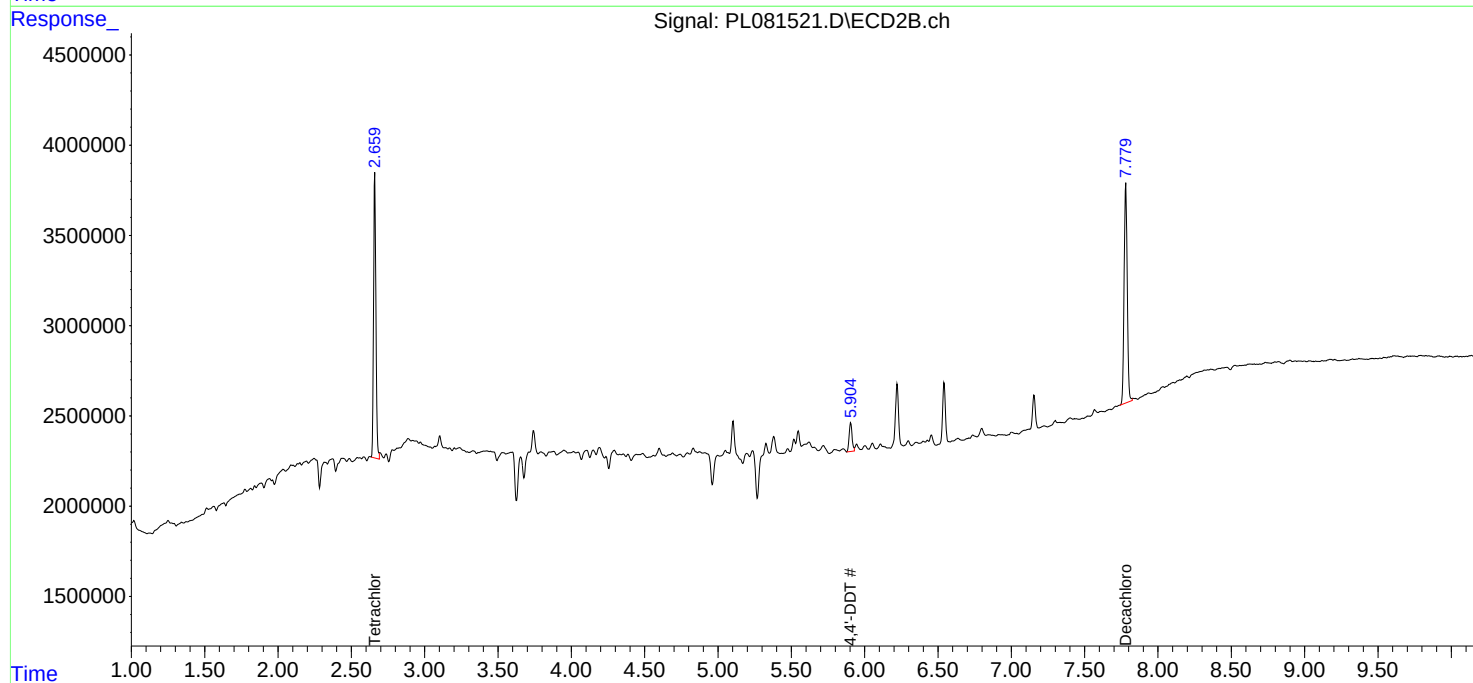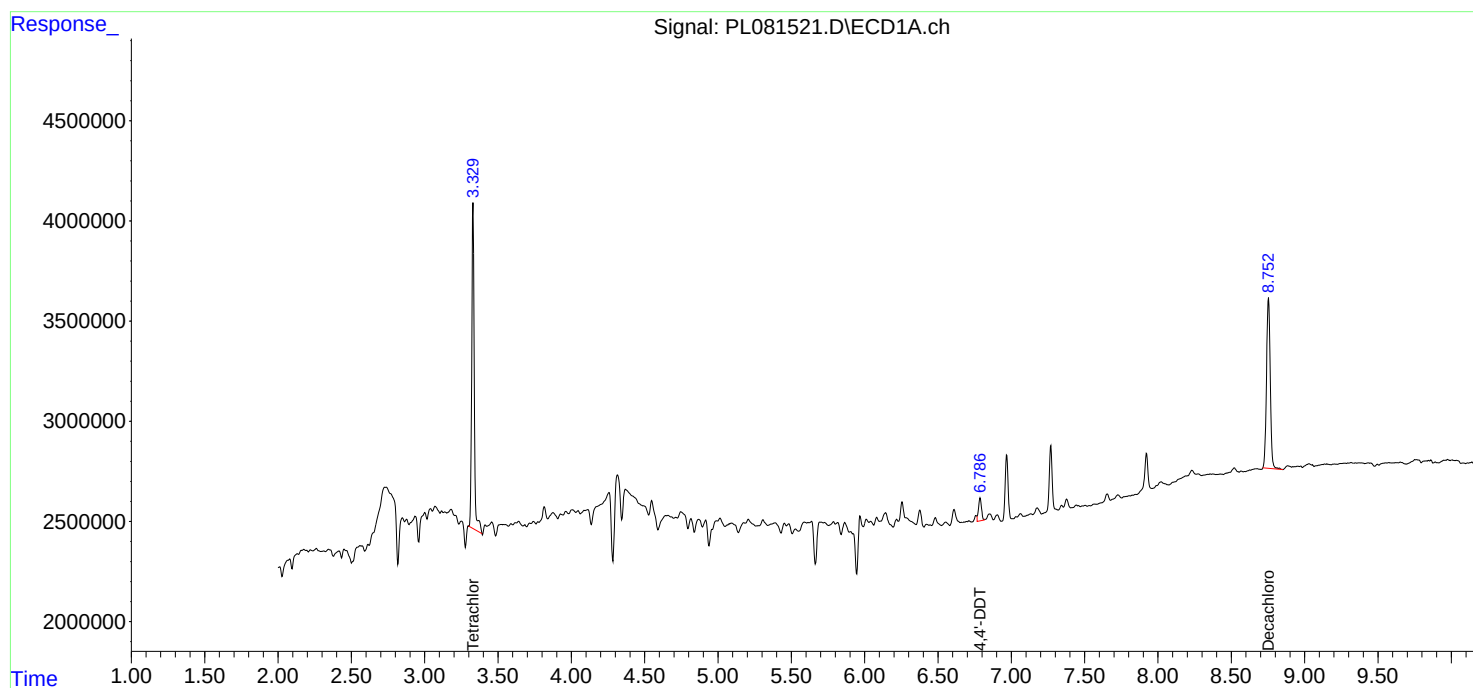

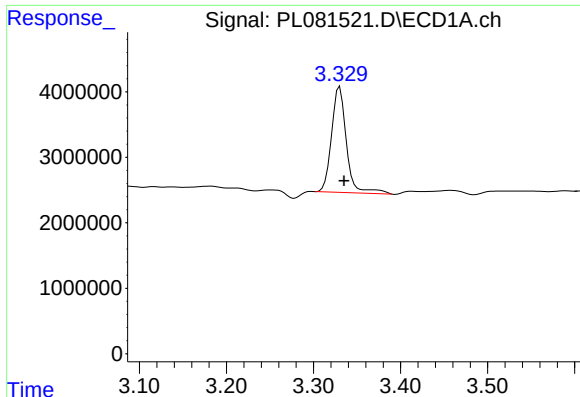

#1 Tetrachloro-m-xylene

R.T.: 3.330 min
Delta R.T.: -0.005 min
Response: 19143341
Conc: 8.86 ng/ml

Instrument :

ECD_L


ClientSampleId :

JPP-6A-031423

Manual Integrations


APPROVED

Reviewed By :Abdul Mirza 03/17/2023
Supervised By :Ankita Jodhani 03/17/2023

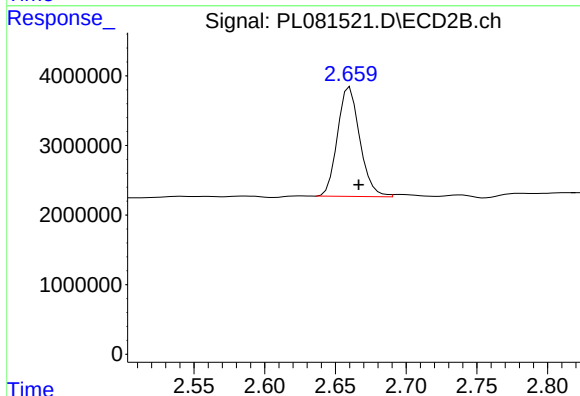


#1 Tetrachloro-m-xylene

R.T.: 2.660 min
Delta R.T.: -0.006 min
Response: 17308603
Conc: 8.55 ng/ml

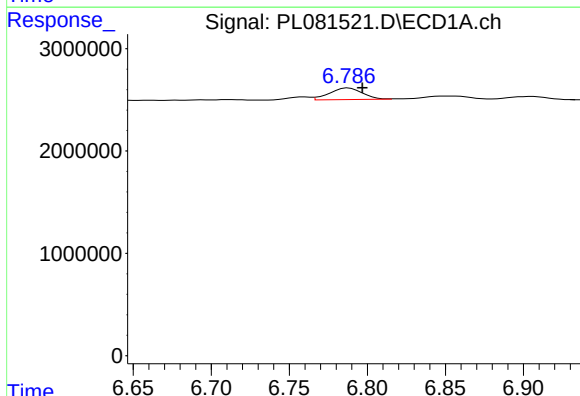


#17 4,4'-DDT

R.T.: 6.786 min
Delta R.T.: -0.010 min
Response: 1500544
Conc: 0.95 ng/ml m

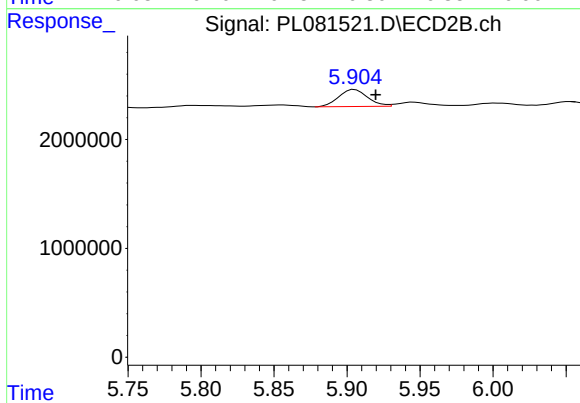

#17 4,4'-DDT

R.T.: 5.905 min
Delta R.T.: -0.014 min
Response: 2174281
Conc: 1.36 ng/ml

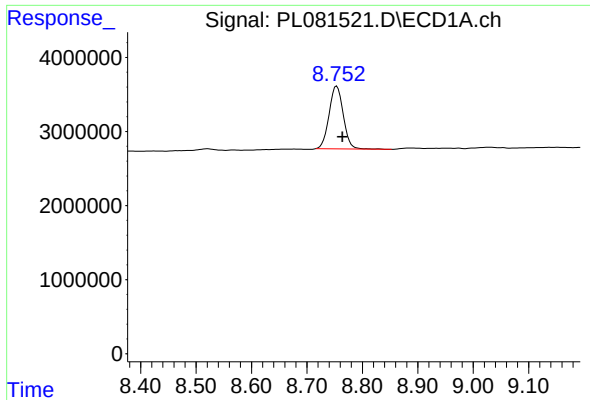

#28 Decachlorobiphenyl

R.T.: 8.754 min
Delta R.T.: -0.010 min
Response: 15174509
Conc: 9.95 ng/ml

Instrument :

ECD_L

ClientSampleId :


JPP-6A-031423

Manual Integrations

APPROVED

Reviewed By :Abdul Mirza 03/17/2023

Supervised By :Ankita Jodhani 03/17/2023

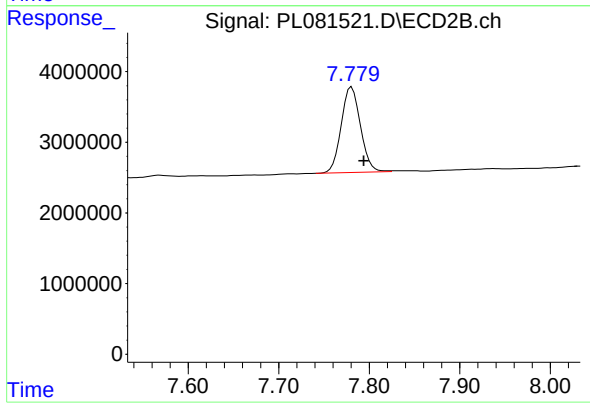

#28 Decachlorobiphenyl

R.T.: 7.781 min
Delta R.T.: -0.013 min
Response: 17913134
Conc: 9.35 ng/ml