

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL031624\  
Data File : PL088624.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 15 Mar 2024 08:22  
Operator : AR\AJ  
Sample : HEXANE  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampleId :  
HEXANE

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Mar 15 21:43:57 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL031324.M  
Quant Title : GC Extractables  
QLast Update : Wed Mar 13 15:45:55 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

-----  
System Monitoring Compounds

Target Compounds  
-----



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL031624\  
Data File : PL088624.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 15 Mar 2024 08:22  
Operator : AR\AJ  
Sample : HEXANE  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampleId :  
HEXANE

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Mar 15 21:43:57 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL031324.M  
Quant Title : GC Extractables  
QLast Update : Wed Mar 13 15:45:55 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1  $\mu$ l  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5 $\mu$ m

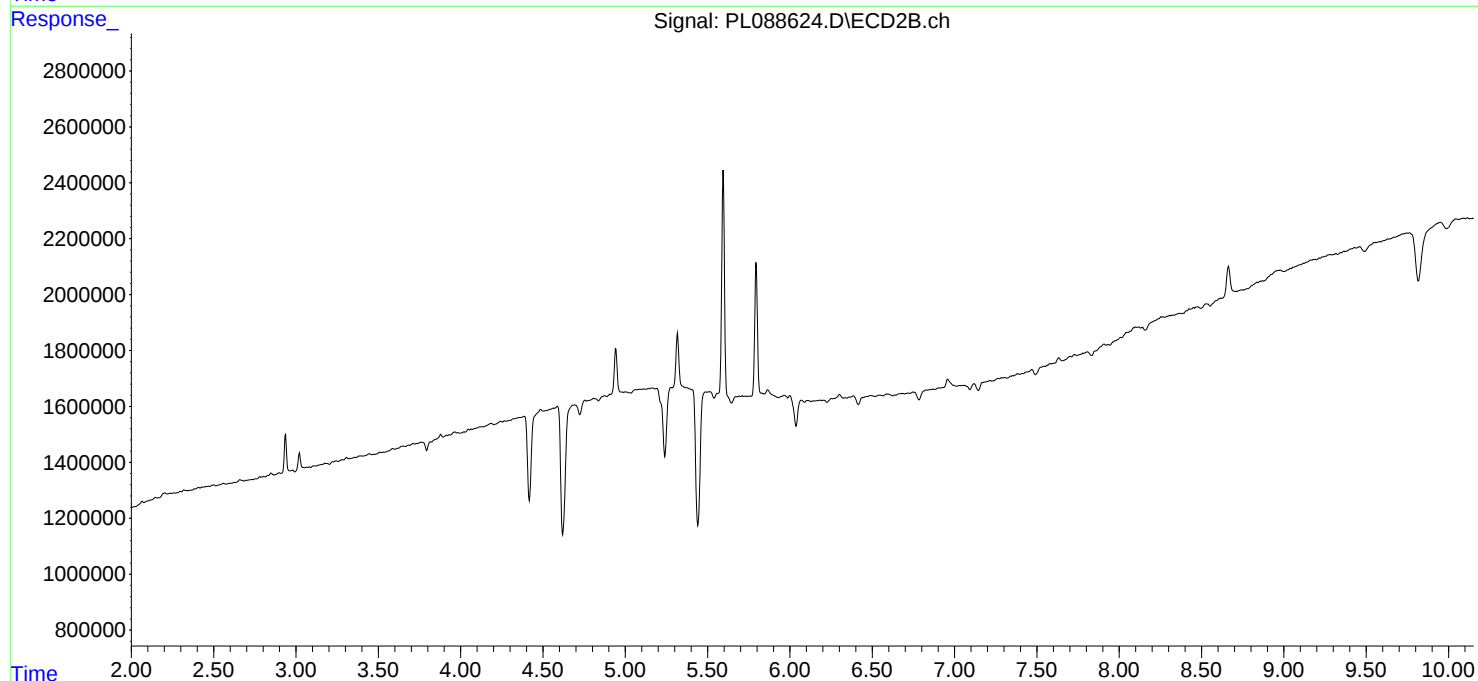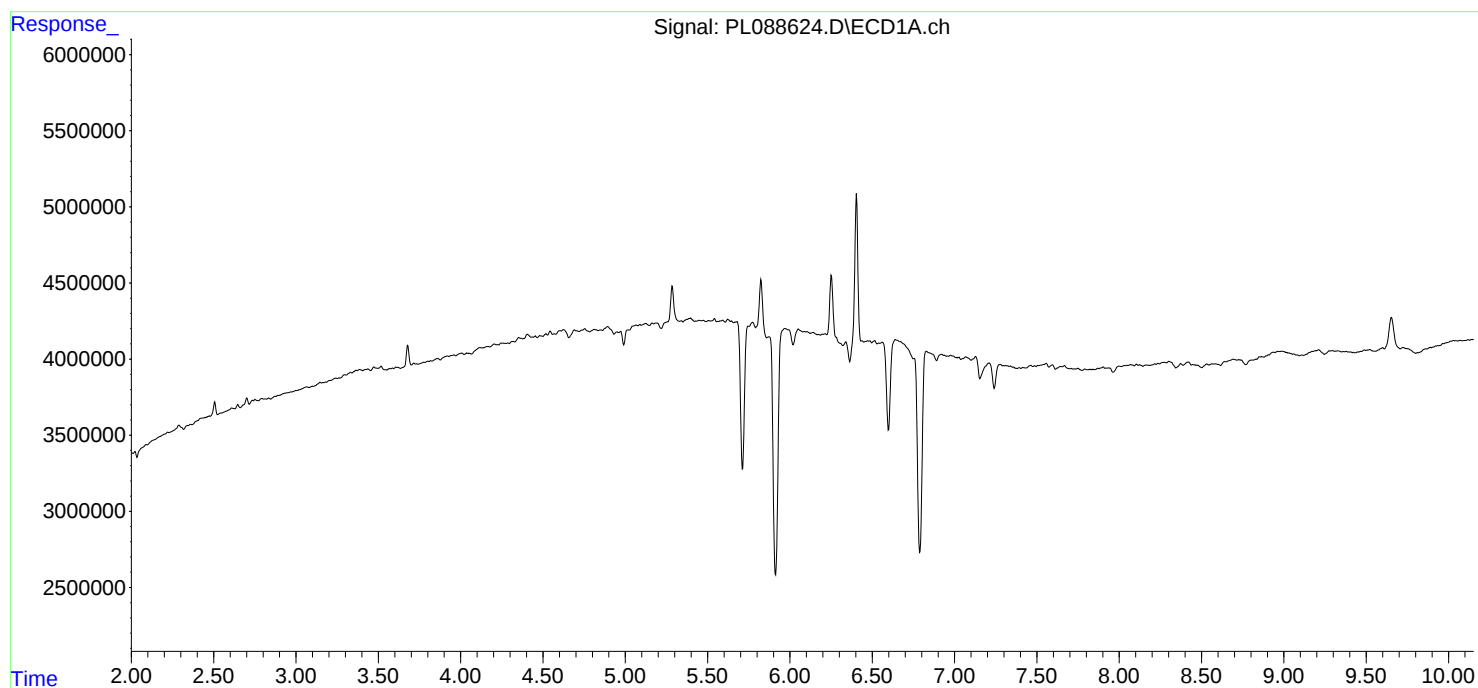


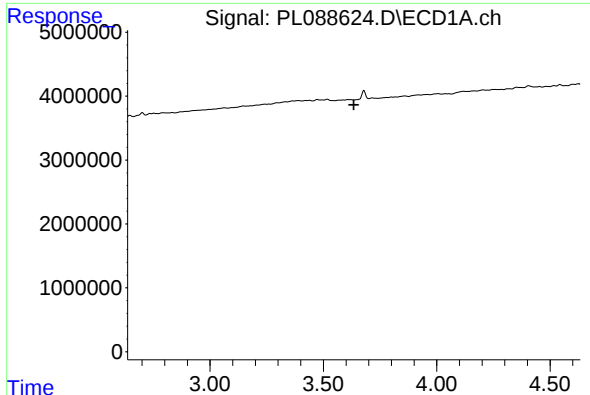

#1 Tetrachloro-m-xylene


R.T.: 0.000 min  
Exp R.T. : 3.634 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :  
HEXANE

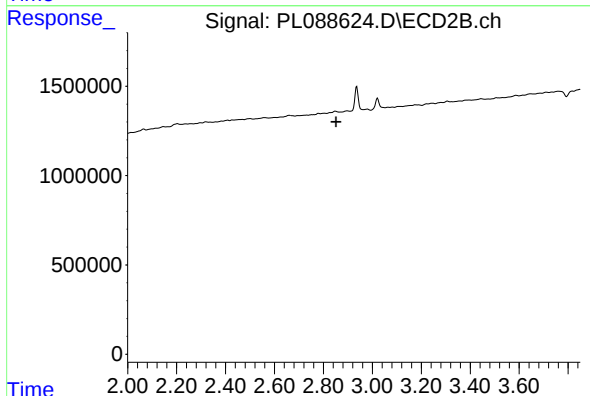


#1 Tetrachloro-m-xylene

R.T.: 0.000 min  
Exp R.T. : 2.852 min  
Response: 0  
Conc: N.D.

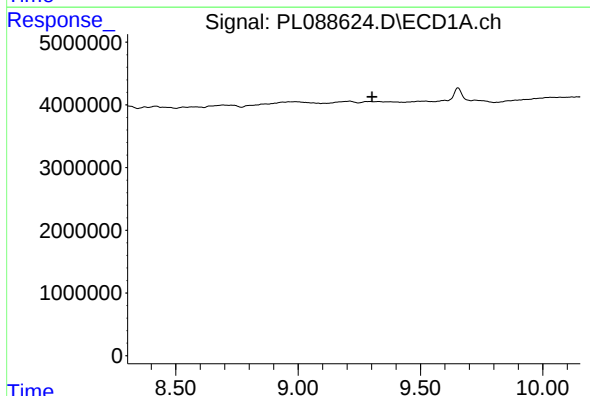

#28 Decachlorobiphenyl

R.T.: 0.000 min  
Exp R.T. : 9.303 min  
Response: 0  
Conc: N.D.

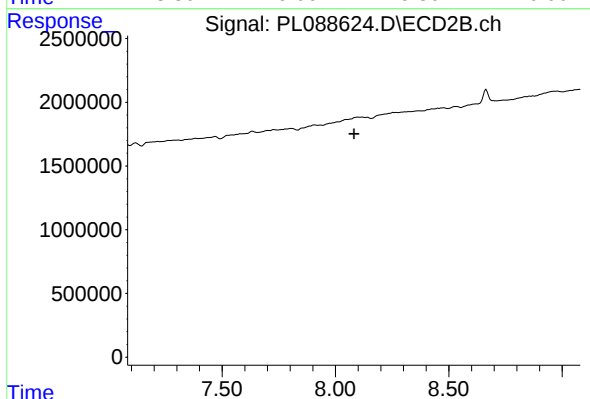

#28 Decachlorobiphenyl

R.T.: 0.000 min  
Exp R.T. : 8.082 min  
Response: 0  
Conc: N.D.