

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031624\
 Data File : PL088634.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2024 13:44
 Operator : AR\AJ
 Sample : P1767-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 NB-07-031424

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 03/18/2024
 Supervised By :Ankita Jodhani 03/18/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 15 21:49:22 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 13 15:45:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.633	2.850	31063889	15363519	11.722m	11.528m
28) SA Decachlor...	9.306	8.082	26331108	14499301	10.652	10.693

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031624\
Data File : PL088634.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2024 13:44
Operator : AR\AJ
Sample : P1767-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
NB-07-031424


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/18/2024
Supervised By : Ankita Jodhani 03/18/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 15 21:49:22 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
Quant Title : GC Extractables
QLast Update : Wed Mar 13 15:45:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

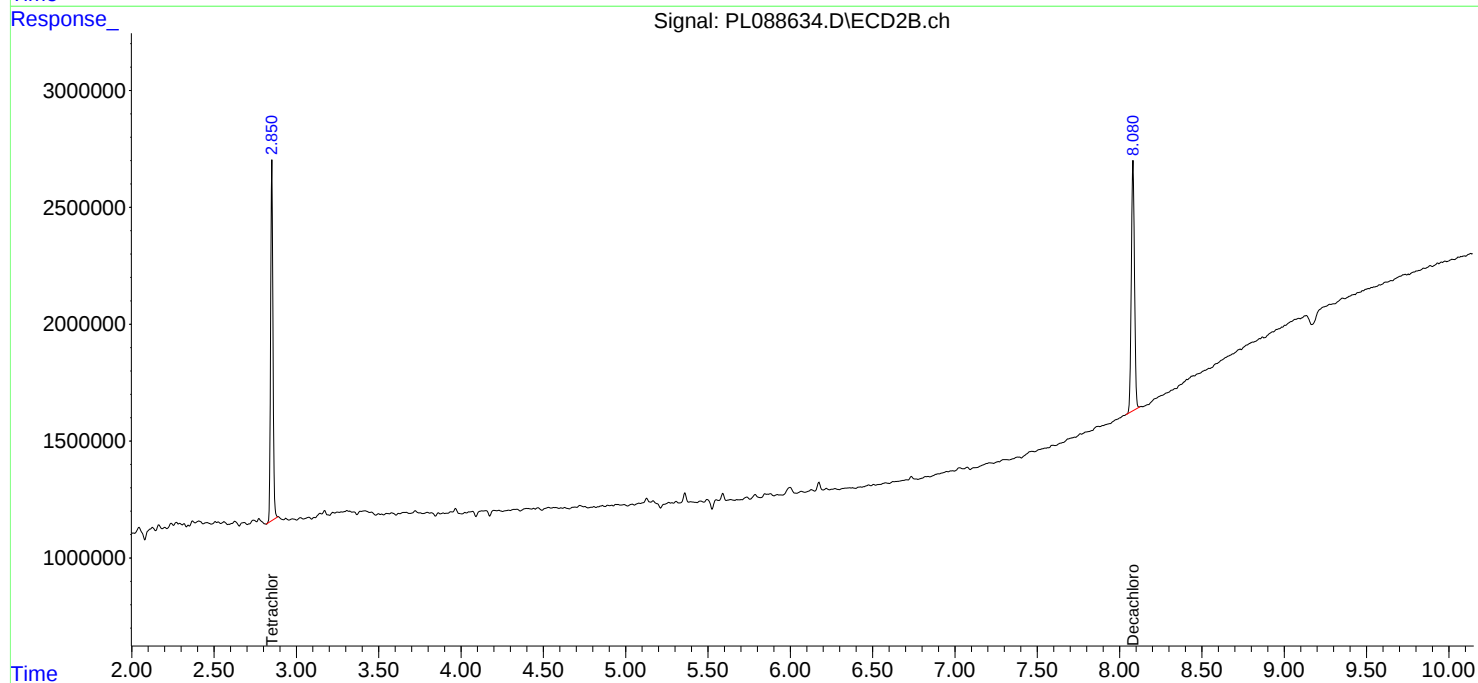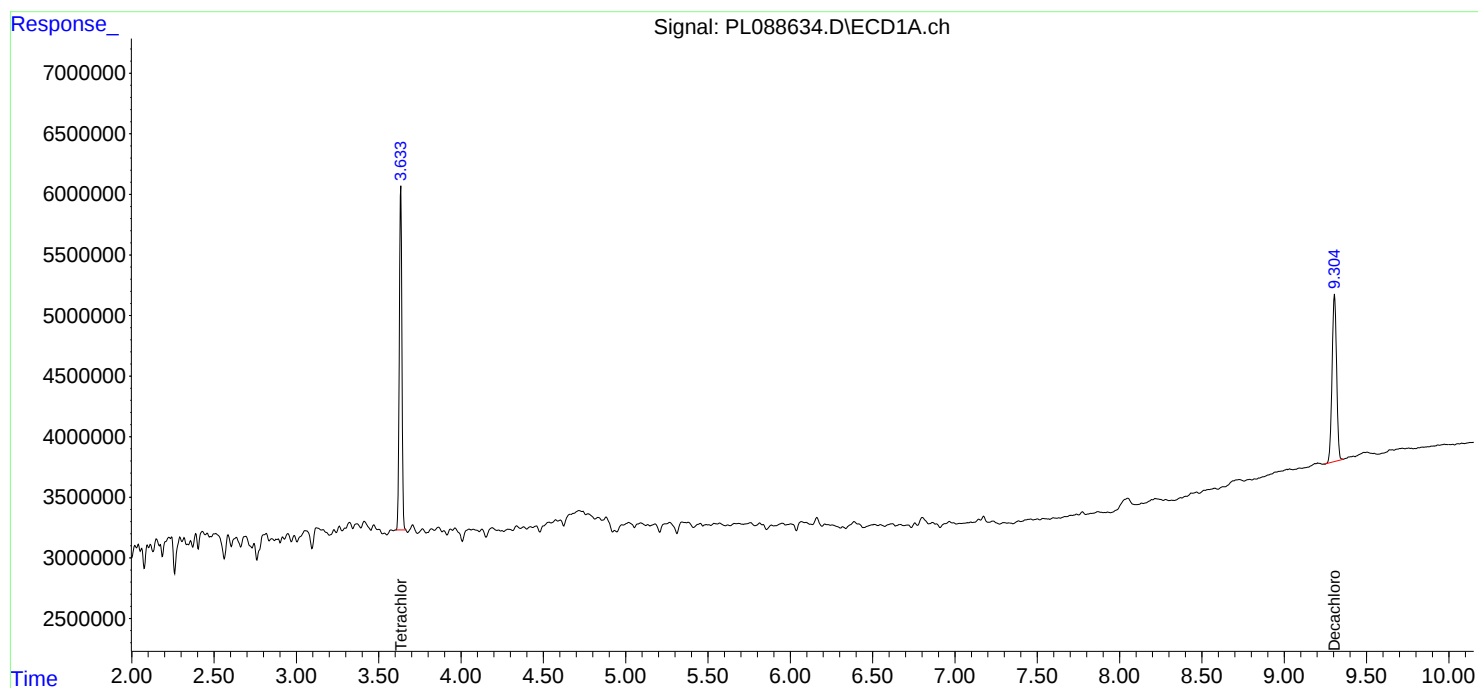

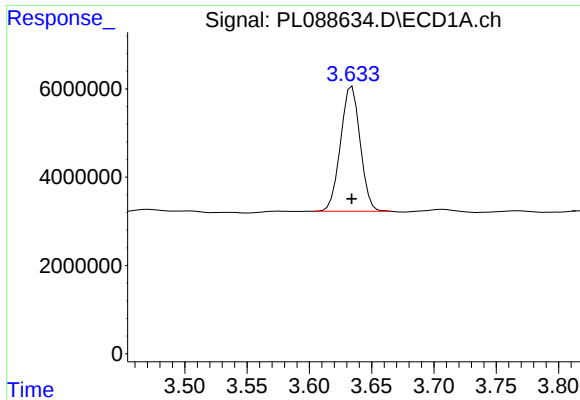


#1 Tetrachloro-m-xylene

R.T.: 3.633 min
Delta R.T.: -0.001 min
Response: 31063889
Conc: 11.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
NB-07-031424


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/18/2024
Supervised By :Ankita Jodhani 03/18/2024

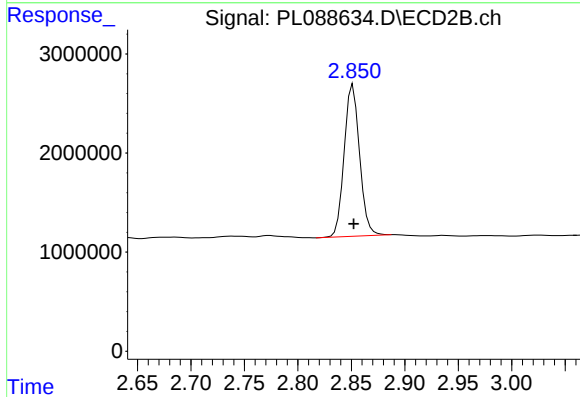


#1 Tetrachloro-m-xylene

R.T.: 2.850 min
Delta R.T.: -0.002 min
Response: 15363519
Conc: 11.53 ng/ml m

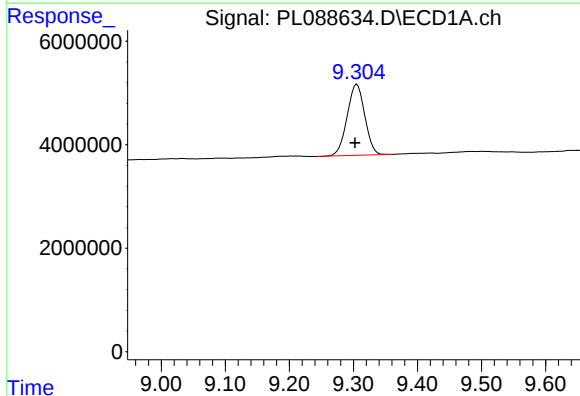

#28 Decachlorobiphenyl

R.T.: 9.306 min
Delta R.T.: 0.003 min
Response: 26331108
Conc: 10.65 ng/ml

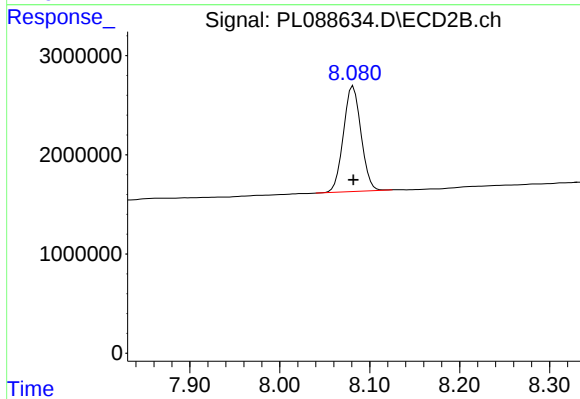

#28 Decachlorobiphenyl

R.T.: 8.082 min
Delta R.T.: 0.000 min
Response: 14499301
Conc: 10.69 ng/ml