

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031624\
 Data File : PL088638.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Mar 2024 14:39
 Operator : AR\AJ
 Sample : P1764-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 18 10:56:43 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 13 15:45:55 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.634	2.852	55384020	27485084	20.900m	20.623
2)	SA Decachlor...	9.303	8.082	37778856	21405784	15.283	15.787
Target Compounds							
11)	B alpha-Chl...	6.159	5.167	2618062	630625	0.788m	0.380 #
13)	MA Dieldrin	6.487	5.492	1495608	785275	0.461	0.483m



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031624\
Data File : PL088638.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Mar 2024 14:39
Operator : AR\AJ
Sample : P1764-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
COMP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 18 10:56:43 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031324.M
Quant Title : GC Extractables
QLast Update : Wed Mar 13 15:45:55 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

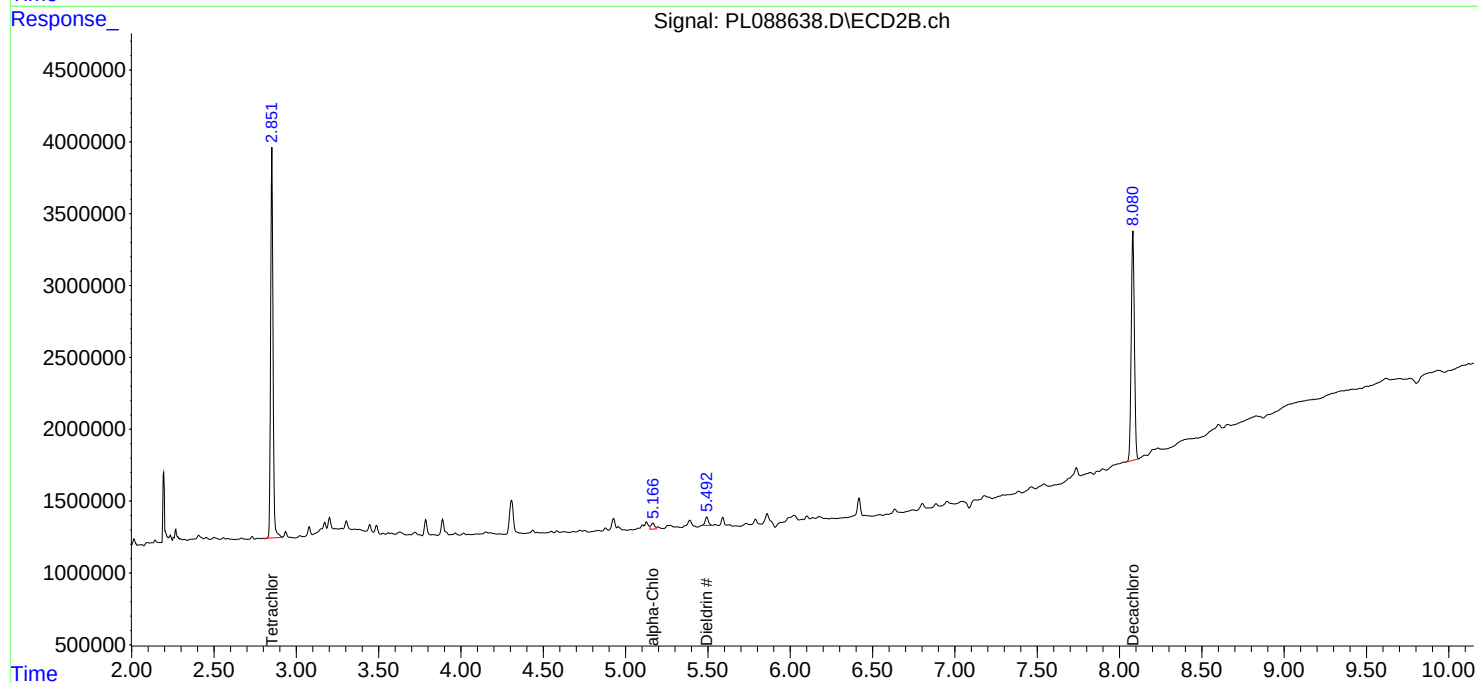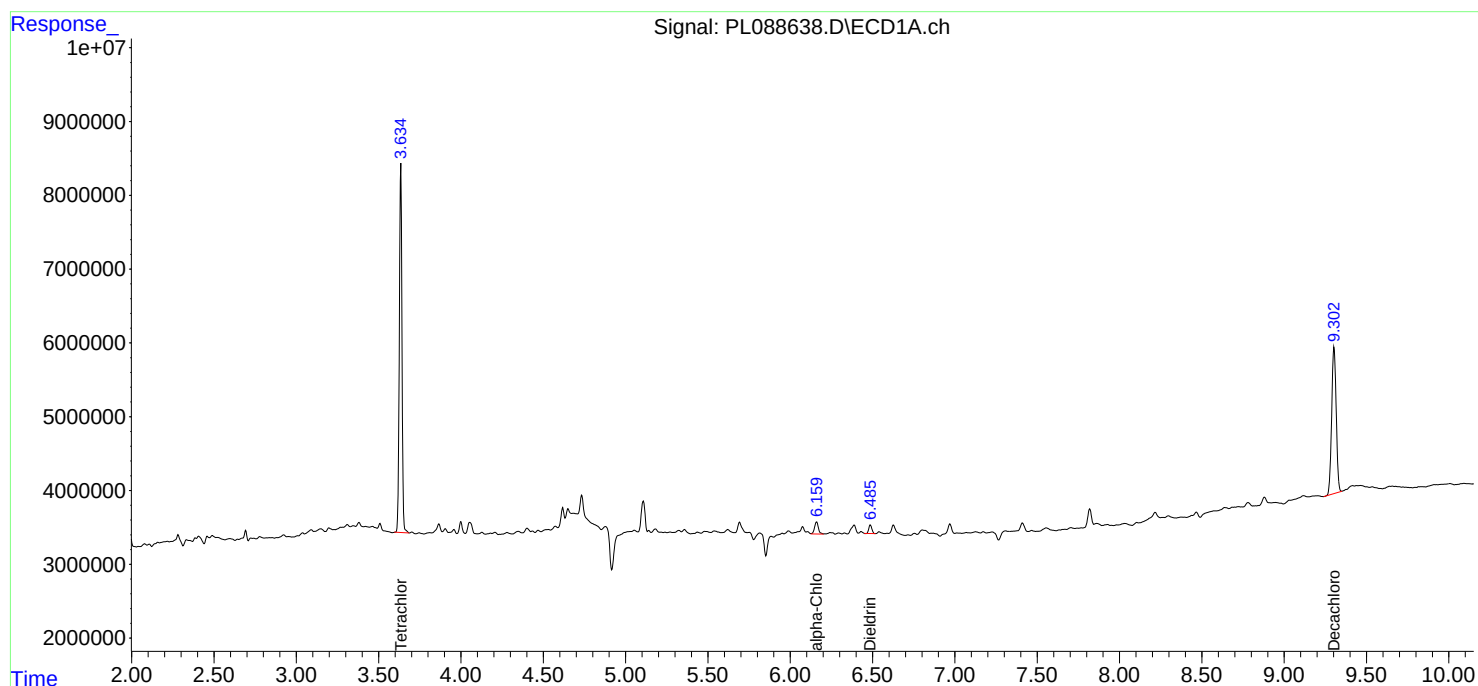


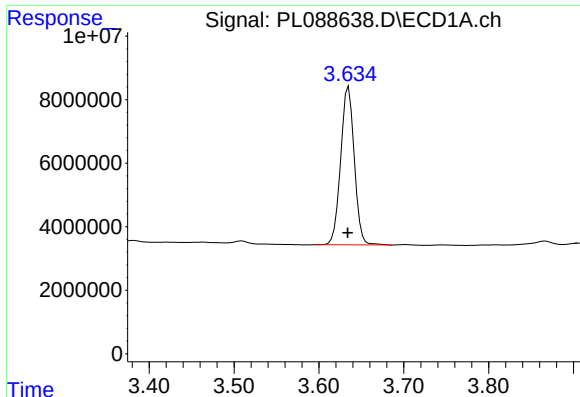

#1 Tetrachloro-m-xylene


R.T.: 3.634 min
Delta R.T.: 0.000 min
Response: 55384020
Conc: 20.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-2

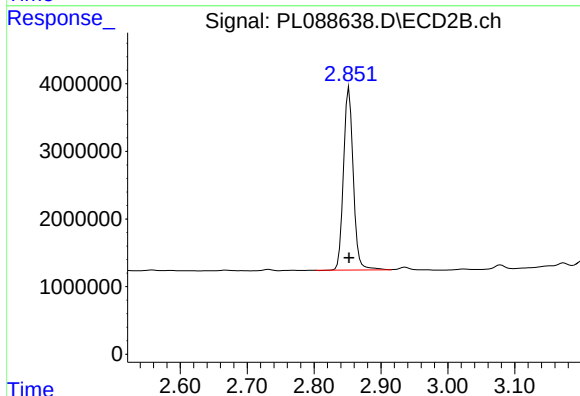


#1 Tetrachloro-m-xylene

R.T.: 2.852 min
Delta R.T.: 0.000 min
Response: 27485084
Conc: 20.62 ng/ml

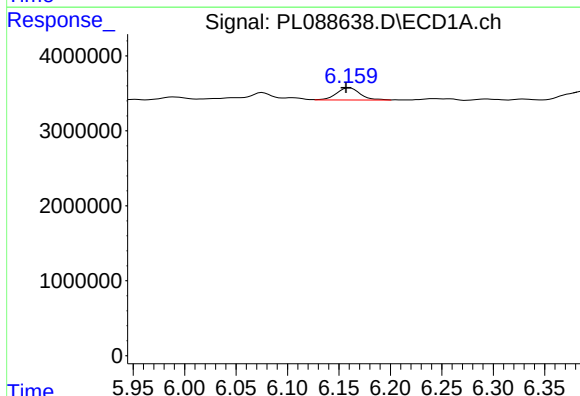


#11 alpha-Chlordane

R.T.: 6.159 min
Delta R.T.: 0.002 min
Response: 2618062
Conc: 0.79 ng/ml m

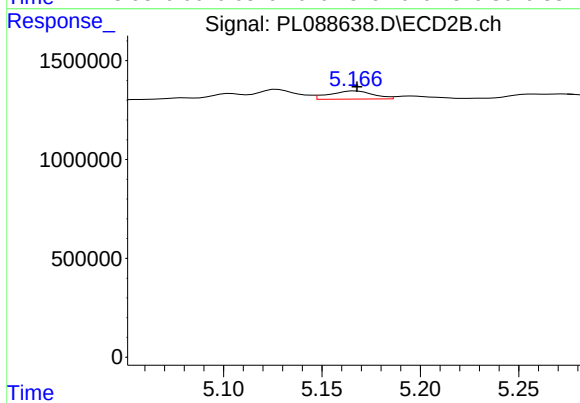

#11 alpha-Chlordane


R.T.: 5.167 min
Delta R.T.: 0.000 min
Response: 630625
Conc: 0.38 ng/ml

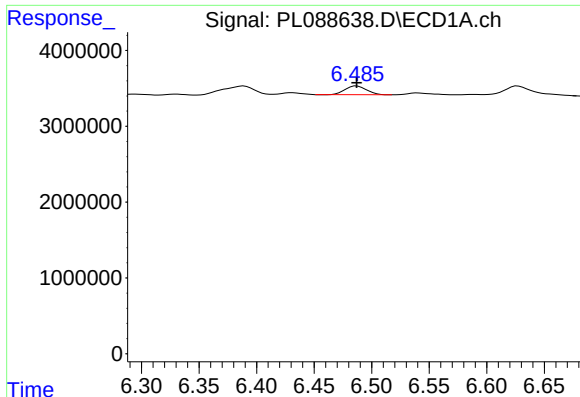

#13 Dieldrin


R.T.: 6.487 min
Delta R.T.: 0.000 min
Response: 1495608
Conc: 0.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-2

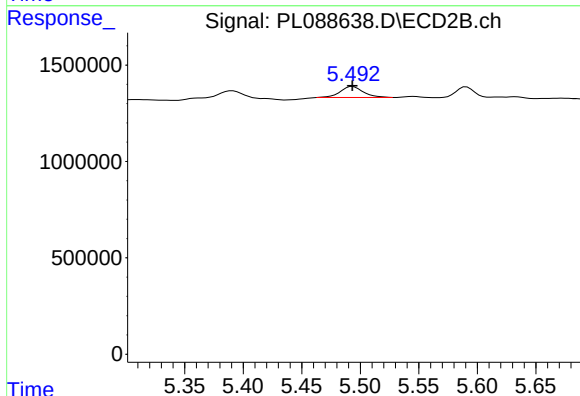


#13 Dieldrin

R.T.: 5.492 min
Delta R.T.: -0.001 min
Response: 785275
Conc: 0.48 ng/ml m

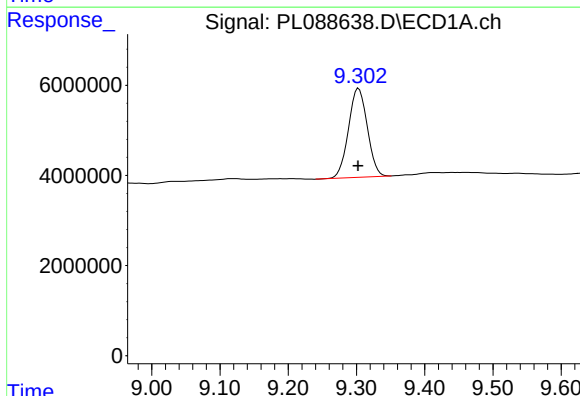

#28 Decachlorobiphenyl

R.T.: 9.303 min
Delta R.T.: 0.000 min
Response: 37778856
Conc: 15.28 ng/ml

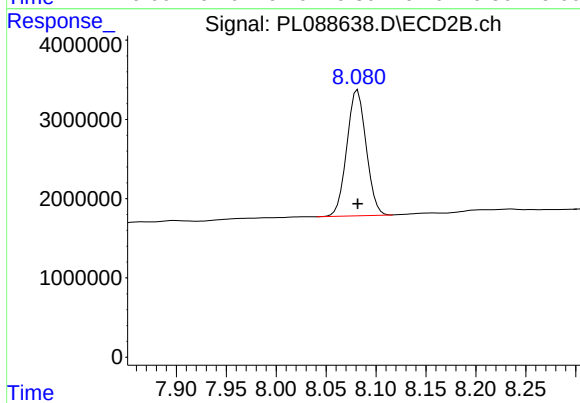

#28 Decachlorobiphenyl

R.T.: 8.082 min
Delta R.T.: 0.000 min
Response: 21405784
Conc: 15.79 ng/ml