

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031722\
 Data File : PL073442.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Mar 2022 12:35
 Operator : AR\AJ
 Sample : N1948-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 21:55:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.647	5.490	5864954	31588551	18.312	19.247
28)	SA Decachlor...	10.421	11.332	8822849	30555543	17.351	17.088
Target Compounds							
2)	A alpha-BHC	5.378f	0.000	93924	0	0.228	N.D. #
7)	B delta-BHC	0.000	6.920f	0	324146	N.D.	0.151 #
10)	B gamma-Chl...	0.000	8.199	0	769291	N.D.	0.377 #
13)	MA Dieldrin	7.788	0.000	39069	0	0.094	N.D. #
14)	MA Endrin	8.095f	8.852	67672	124107	0.174	0.081 #
15)	B Endosulfa...	8.379	0.000	36089	0	0.092	N.D. #
17)	MA 4,4'-DDT	8.494	9.283f	18302	156519	0.048	0.096 #
20)	A Methoxychlor	9.069f	0.000	29704	0	0.116	N.D. #
22)	Mirex	0.000	10.385f	0	333637	N.D.	0.246 #
25)	Chlordane-3	0.000	8.199	0	769291	N.D.	2.837 #
27)	Chlordane-5	8.379	0.000	36089	0	2.204	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031722\
Data File : PL073442.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Mar 2022 12:35
Operator : AR\AJ
Sample : N1948-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 21:55:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

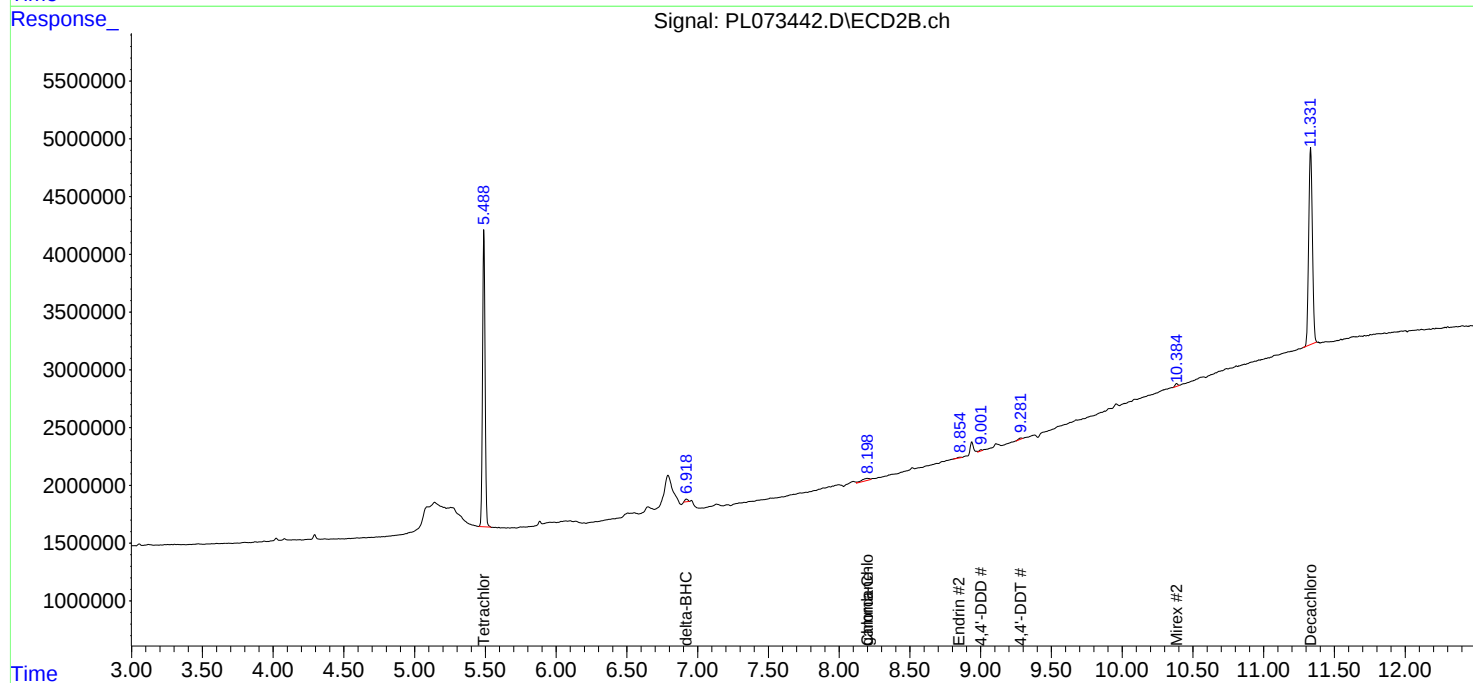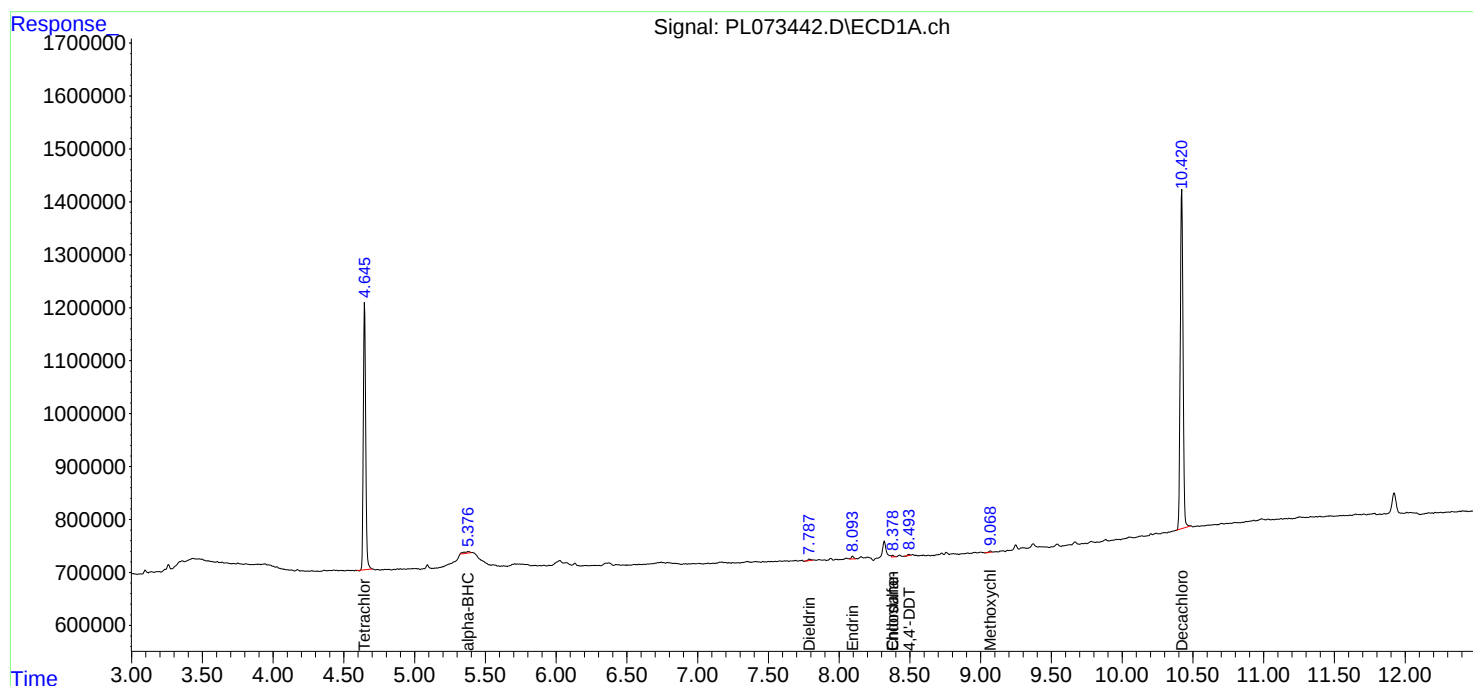


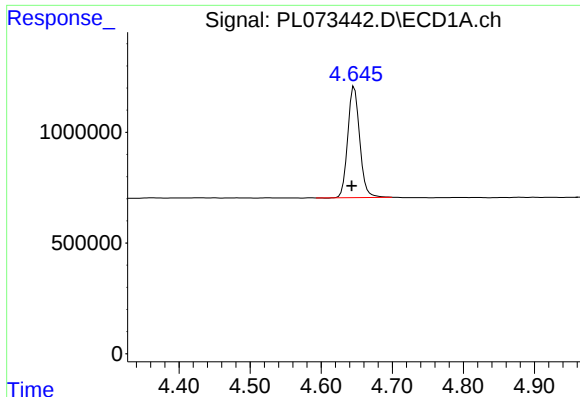

#1 Tetrachloro-m-xylene


R.T.: 4.647 min
Delta R.T.: 0.004 min
Response: 5864954
Conc: 18.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

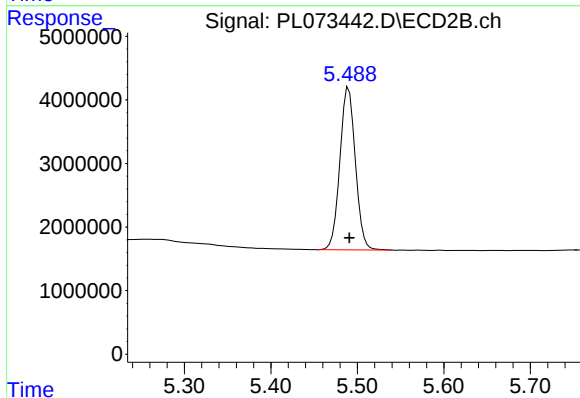


#1 Tetrachloro-m-xylene

R.T.: 5.490 min
Delta R.T.: -0.001 min
Response: 31588551
Conc: 19.25 ng/ml

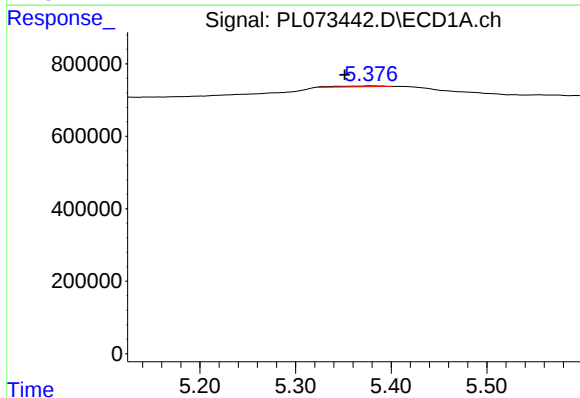


#2 alpha-BHC

R.T.: 5.378 min
Delta R.T.: 0.027 min
Response: 93924
Conc: 0.23 ng/ml

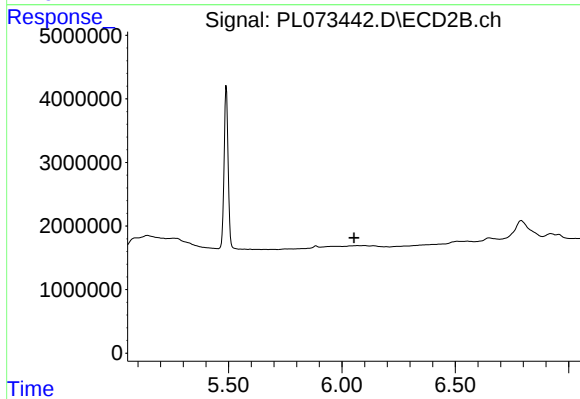

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.054 min
Response: 0
Conc: N.D.

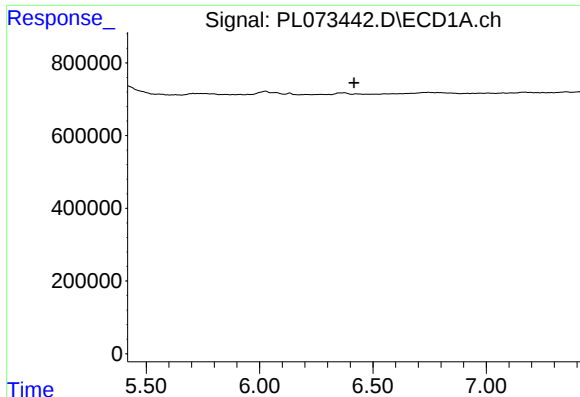

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.416 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

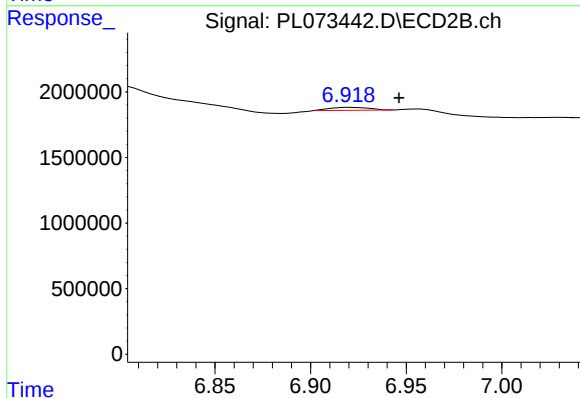


#7 delta-BHC

R.T.: 6.920 min
Delta R.T.: -0.026 min
Response: 324146
Conc: 0.15 ng/ml

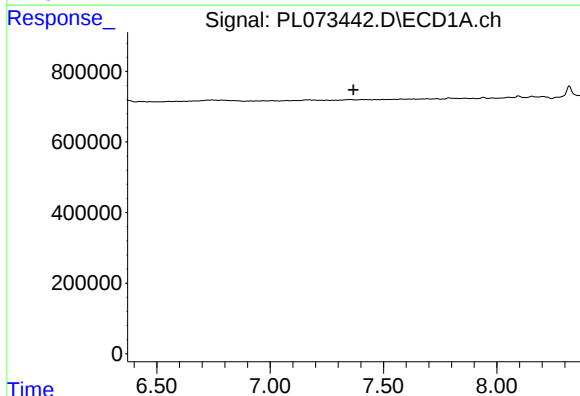


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

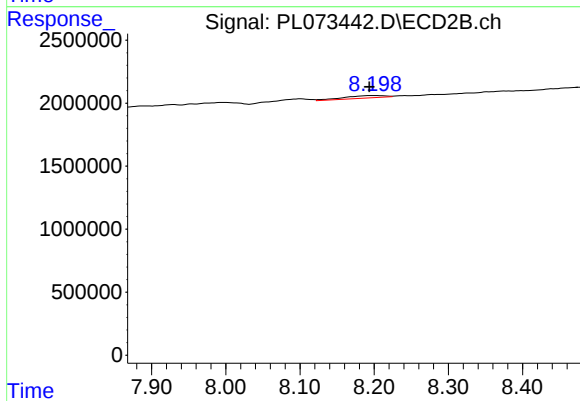

#10 gamma-Chlordane


R.T.: 8.199 min
Delta R.T.: 0.006 min
Response: 769291
Conc: 0.38 ng/ml

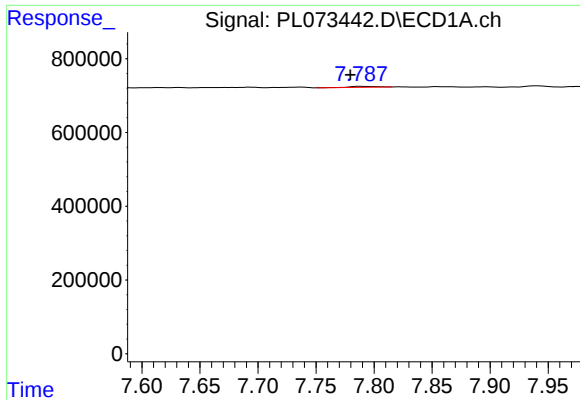

#13 Dieldrin


R.T.: 7.788 min
Delta R.T.: 0.008 min
Response: 39069
Conc: 0.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

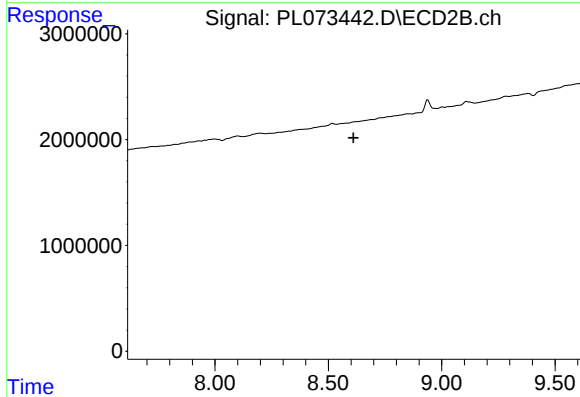


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.611 min
Response: 0
Conc: N.D.

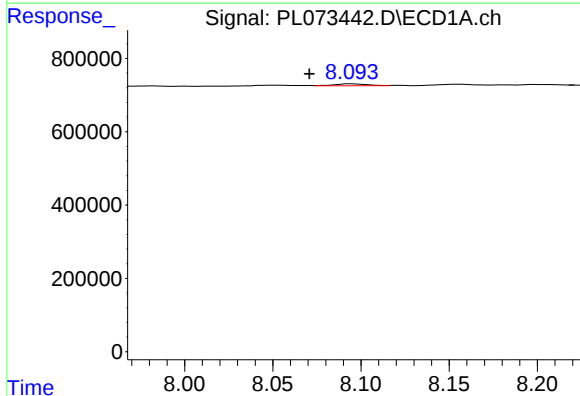


#14 Endrin

R.T.: 8.095 min
Delta R.T.: 0.024 min
Response: 67672
Conc: 0.17 ng/ml

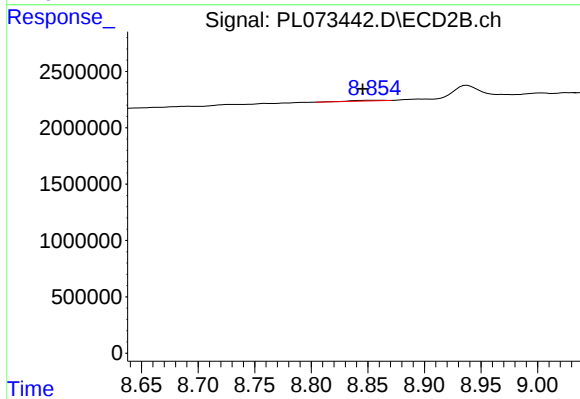

#14 Endrin


R.T.: 8.852 min
Delta R.T.: 0.007 min
Response: 124107
Conc: 0.08 ng/ml

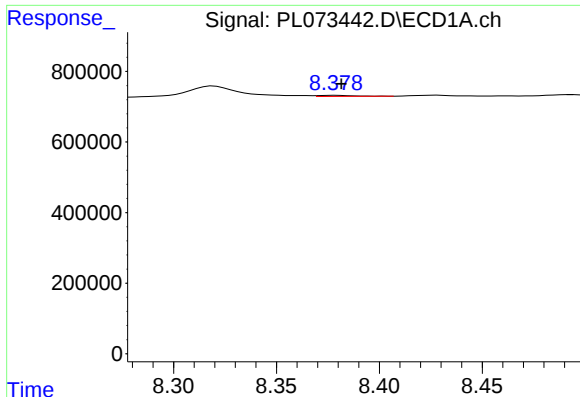

#15 Endosulfan II


R.T.: 8.379 min
Delta R.T.: -0.003 min
Response: 36089
Conc: 0.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

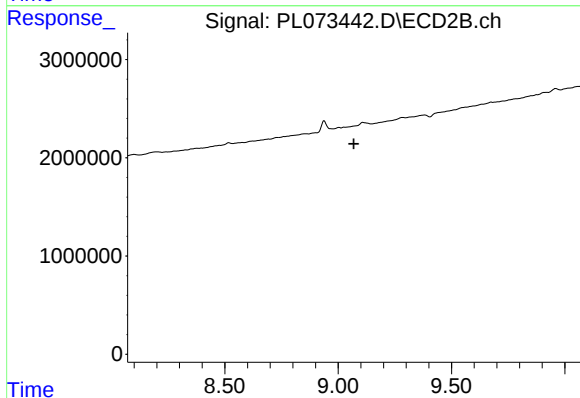


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 9.069 min
Response: 0
Conc: N.D.

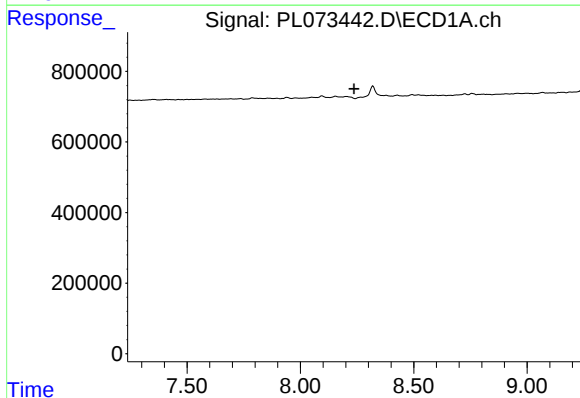


#16 4,4'-DDD

R.T.: 8.267 min
Delta R.T.: 0.030 min
Response: -35570
Conc: N.D.

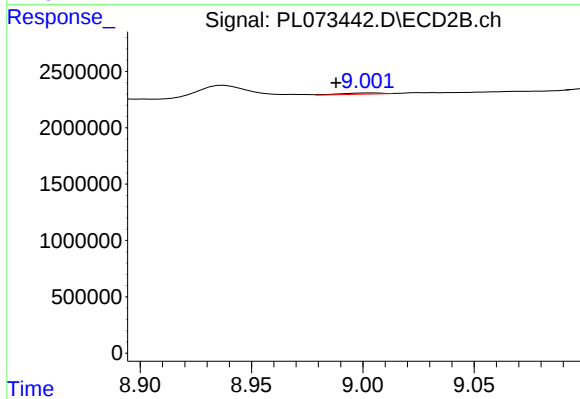

#16 4,4'-DDD


R.T.: 9.004 min
Delta R.T.: 0.016 min
Response: 136991
Conc: 0.09 ng/ml

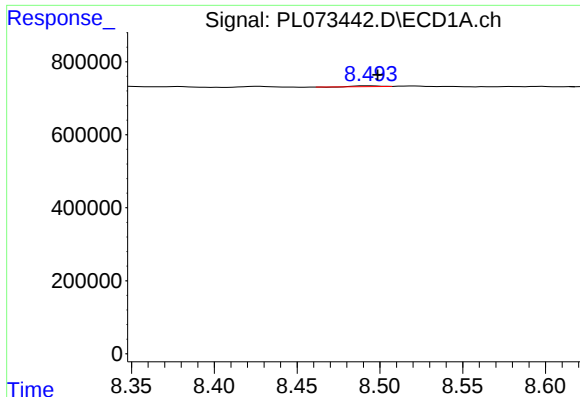

#17 4,4'-DDT


R.T.: 8.494 min
Delta R.T.: -0.005 min
Response: 18302
Conc: 0.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

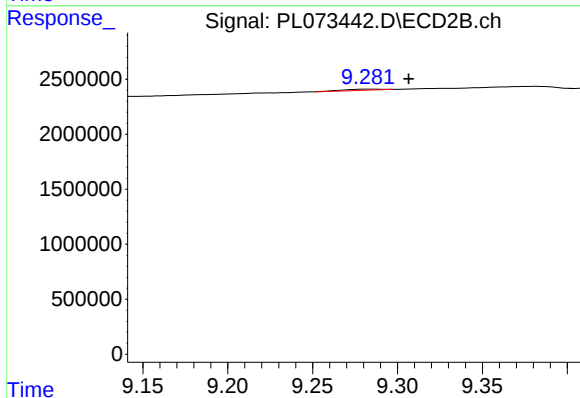


#17 4,4'-DDT

R.T.: 9.283 min
Delta R.T.: -0.023 min
Response: 156519
Conc: 0.10 ng/ml

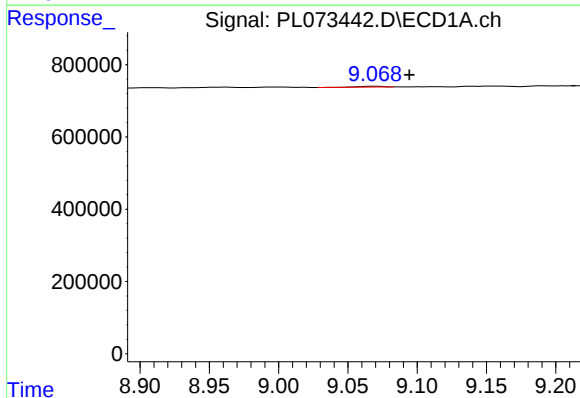


#20 Methoxychlor

R.T.: 9.069 min
Delta R.T.: -0.025 min
Response: 29704
Conc: 0.12 ng/ml

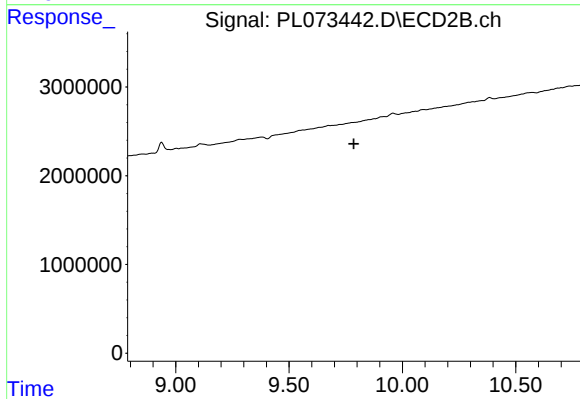

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.786 min
Response: 0
Conc: N.D.

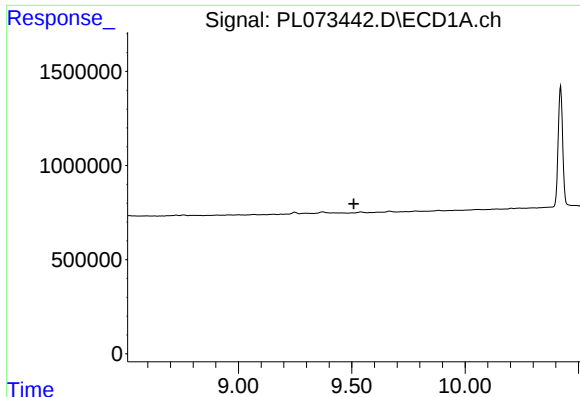

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 9.509 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

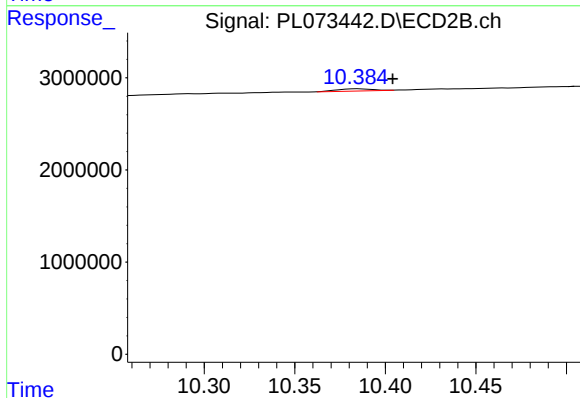


#22 Mirex

R.T.: 10.385 min
Delta R.T.: -0.019 min
Response: 333637
Conc: 0.25 ng/ml

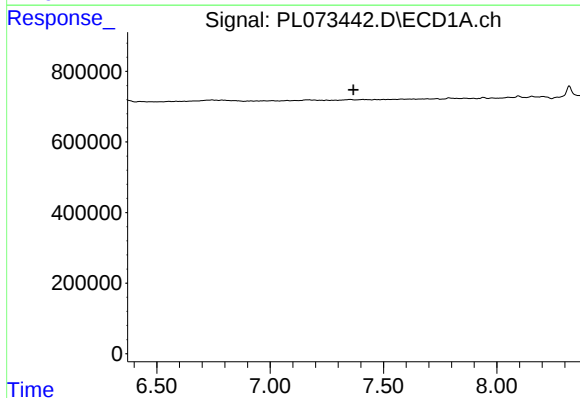


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.368 min
Response: 0
Conc: N.D.

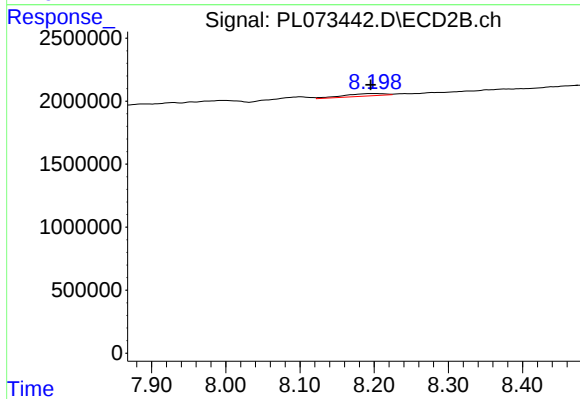

#25 Chlordane-3


R.T.: 8.199 min
Delta R.T.: 0.004 min
Response: 769291
Conc: 2.84 ng/ml

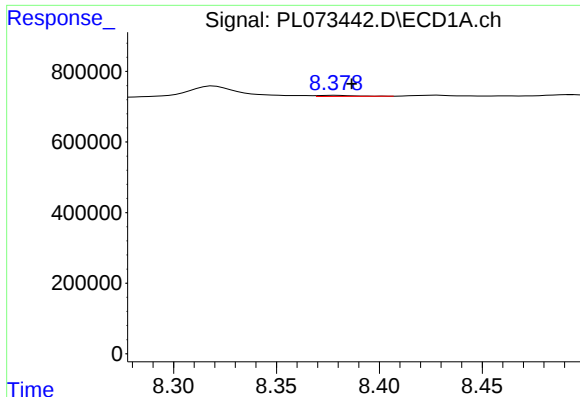

#27 Chlordane-5


R.T.: 8.379 min
Delta R.T.: -0.007 min
Response: 36089
Conc: 2.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

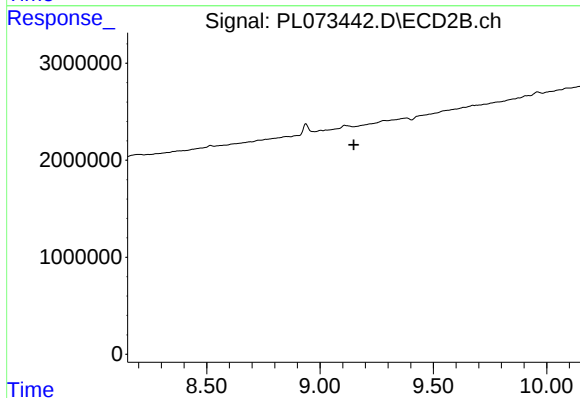


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 9.149 min
Response: 0
Conc: N.D.

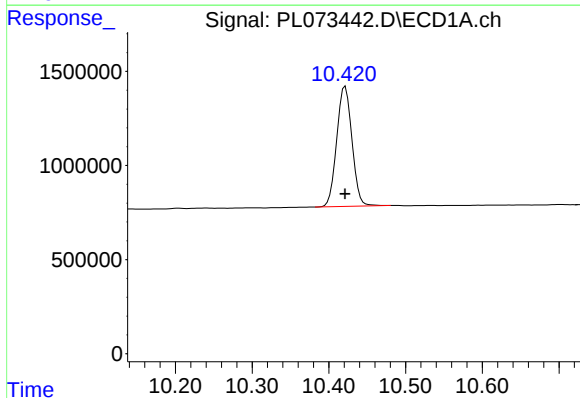

#28 Decachlorobiphenyl

R.T.: 10.421 min
Delta R.T.: 0.000 min
Response: 8822849
Conc: 17.35 ng/ml

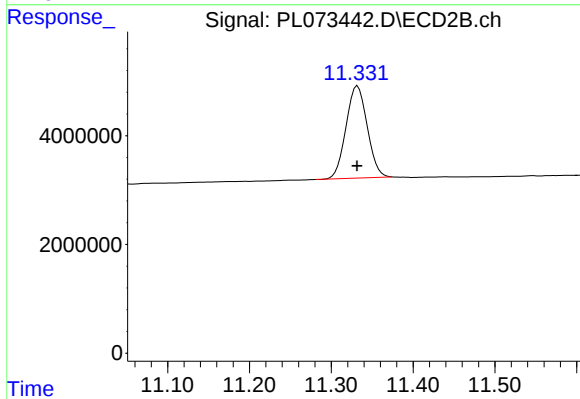

#28 Decachlorobiphenyl

R.T.: 11.332 min
Delta R.T.: 0.000 min
Response: 30555543
Conc: 17.09 ng/ml