

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031722\
 Data File : PL073439.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Mar 2022 10:29
 Operator : AR\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 21:54:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
 Quant Title : GC Extractables
 QLast Update : Mon Mar 14 04:12:46 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.650	5.488	18916176	85995239	59.060	52.396
28)	SA Decachlor...	10.422	11.331	23486070	83618015	46.187	46.762
Target Compounds							
23)	Chlordane-1	5.981	6.862	5633153	32608327	475.171	477.335
24)	Chlordane-2	6.670	7.444	7532338	35574440	461.741	494.958
25)	Chlordane-3	7.372	8.194	18598035	139.5E6	455.453	514.409
26)	Chlordane-4	7.440	8.280	19976123	169.4E6	450.717	511.328
27)	Chlordane-5	8.390	9.149	7361419	27053391	449.544	498.428



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031722\
Data File : PL073439.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Mar 2022 10:29
Operator : AR\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 21:54:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL031122.M
Quant Title : GC Extractables
QLast Update : Mon Mar 14 04:12:46 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

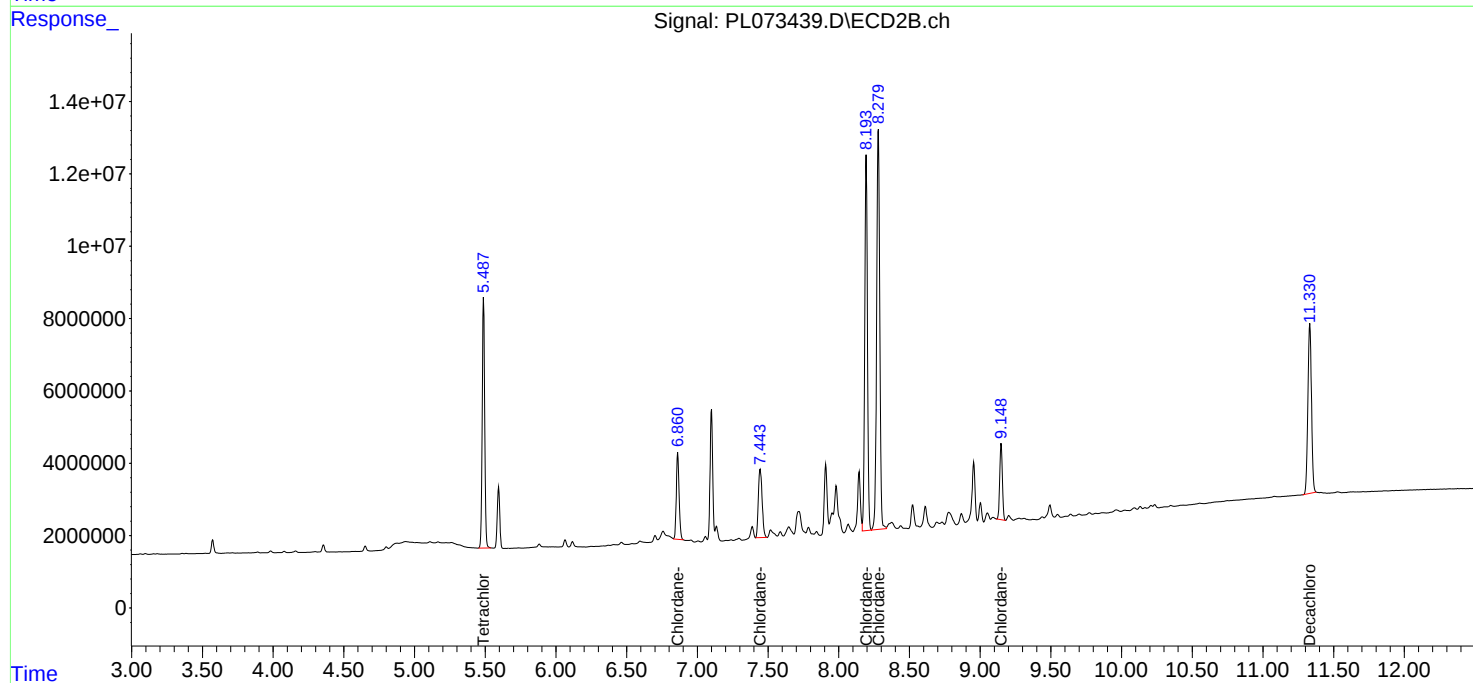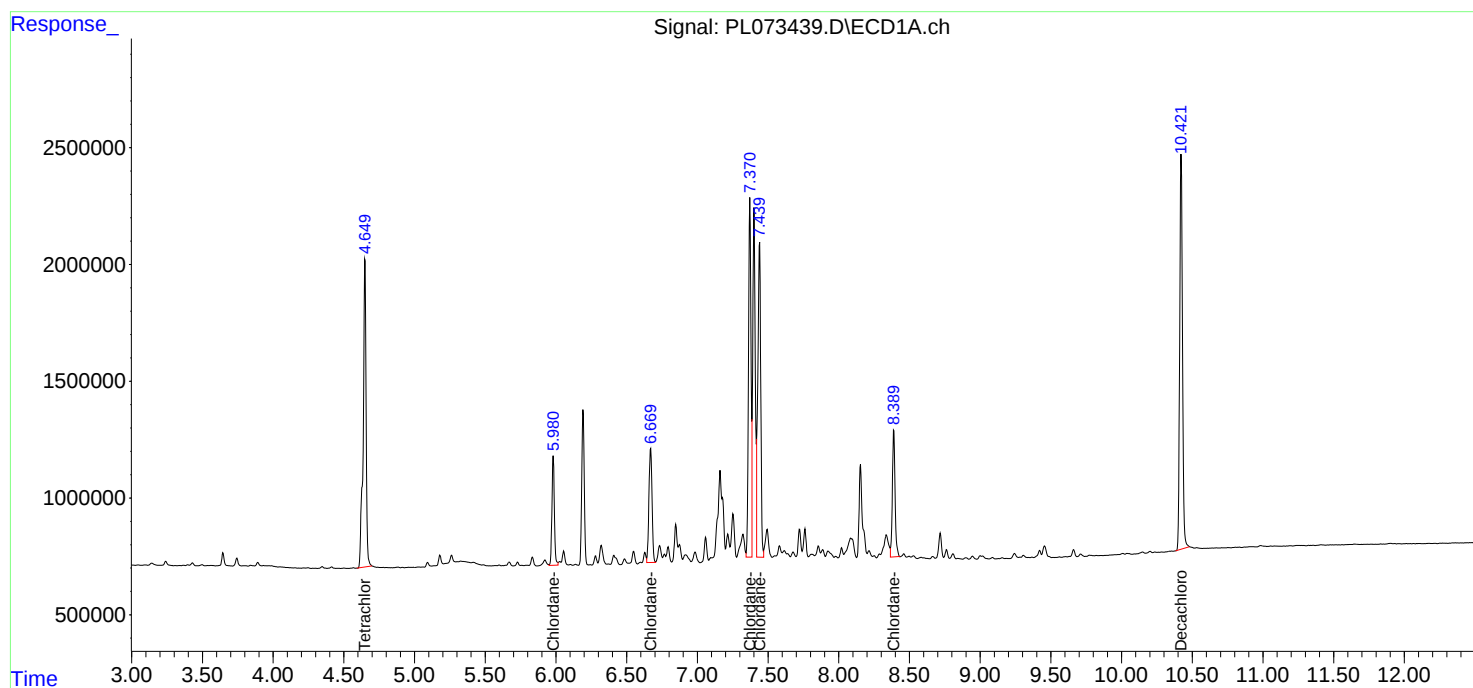


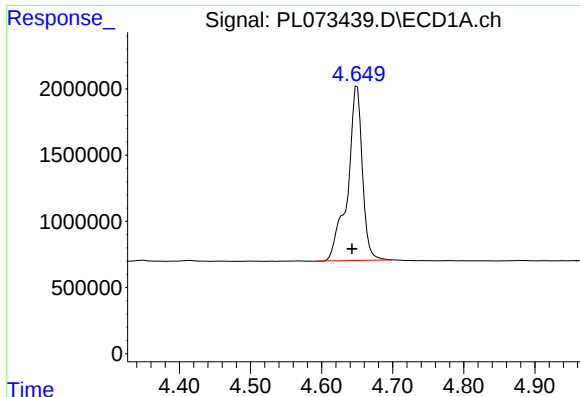

#1 Tetrachloro-m-xylene


R.T.: 4.650 min
Delta R.T.: 0.007 min
Response: 18916176
Conc: 59.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

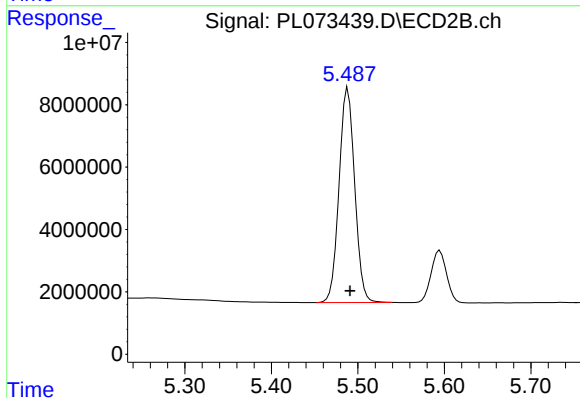


#1 Tetrachloro-m-xylene

R.T.: 5.488 min
Delta R.T.: -0.003 min
Response: 85995239
Conc: 52.40 ng/ml

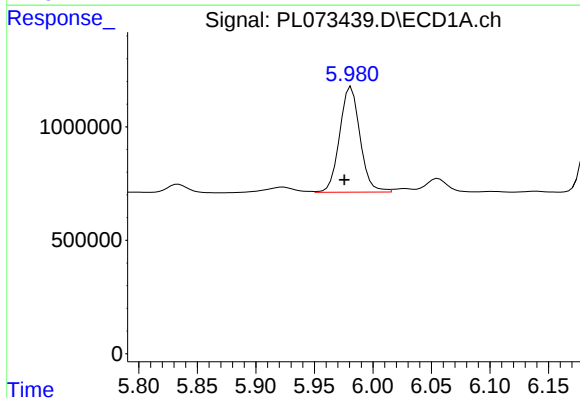


#23 Chlordane-1

R.T.: 5.981 min
Delta R.T.: 0.006 min
Response: 5633153
Conc: 475.17 ng/ml

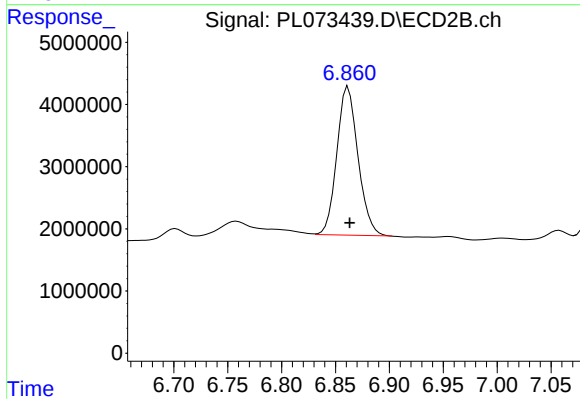

#23 Chlordane-1


R.T.: 6.862 min
Delta R.T.: -0.002 min
Response: 32608327
Conc: 477.34 ng/ml

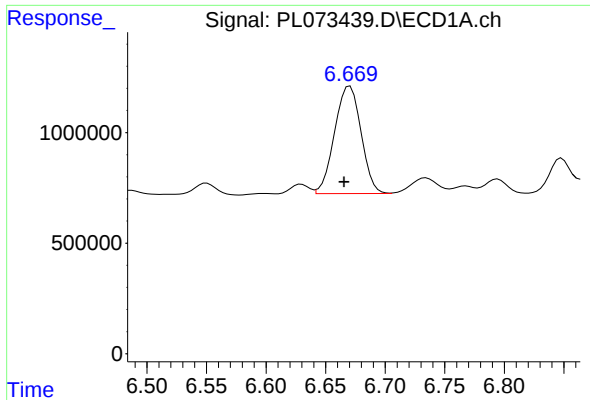

#24 Chlordane-2


R.T.: 6.670 min
Delta R.T.: 0.005 min
Response: 7532338
Conc: 461.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

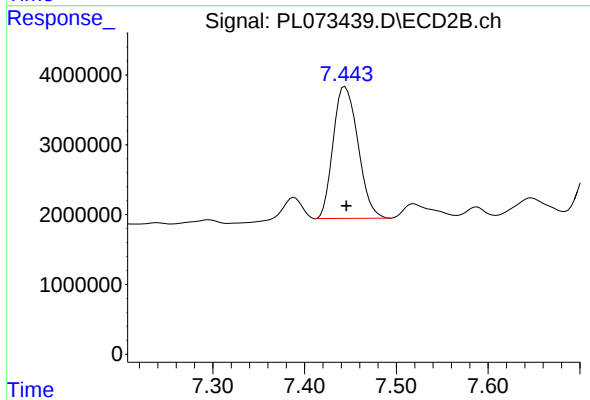


#24 Chlordane-2

R.T.: 7.444 min
Delta R.T.: -0.002 min
Response: 35574440
Conc: 494.96 ng/ml

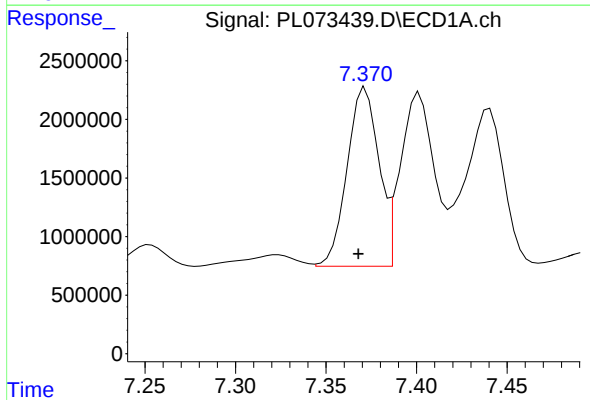


#25 Chlordane-3

R.T.: 7.372 min
Delta R.T.: 0.004 min
Response: 18598035
Conc: 455.45 ng/ml

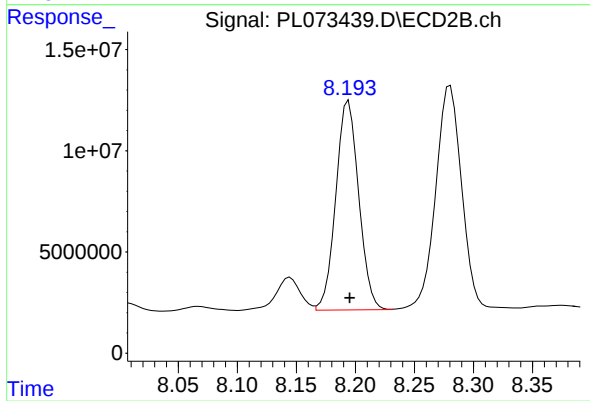

#25 Chlordane-3


R.T.: 8.194 min
Delta R.T.: -0.001 min
Response: 139472919
Conc: 514.41 ng/ml

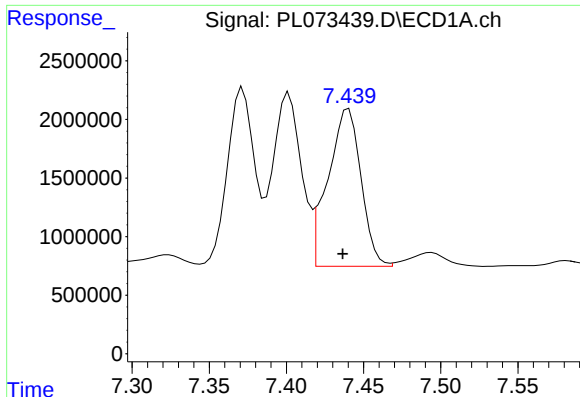

#26 Chlordane-4


R.T.: 7.440 min
Delta R.T.: 0.004 min
Response: 19976123
Conc: 450.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

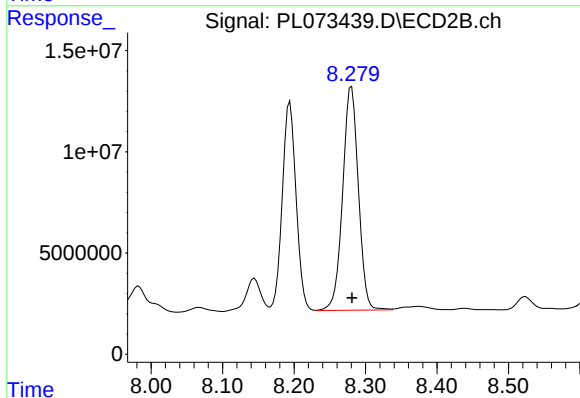


#26 Chlordane-4

R.T.: 8.280 min
Delta R.T.: 0.000 min
Response: 169378747
Conc: 511.33 ng/ml

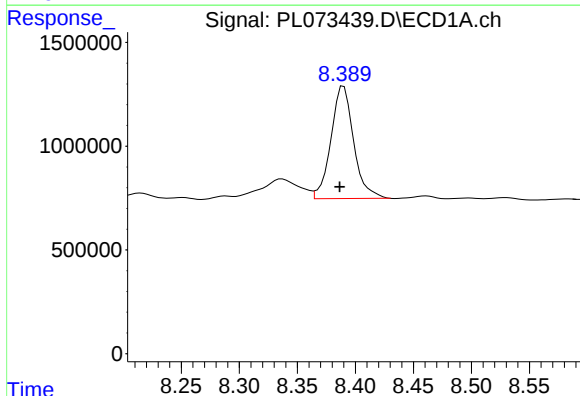


#27 Chlordane-5

R.T.: 8.390 min
Delta R.T.: 0.003 min
Response: 7361419
Conc: 449.54 ng/ml

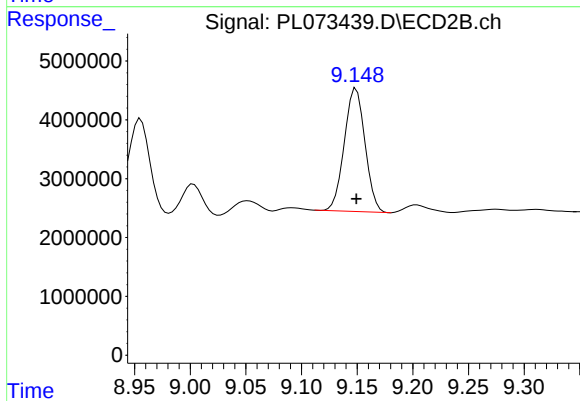

#27 Chlordane-5


R.T.: 9.149 min
Delta R.T.: 0.000 min
Response: 27053391
Conc: 498.43 ng/ml

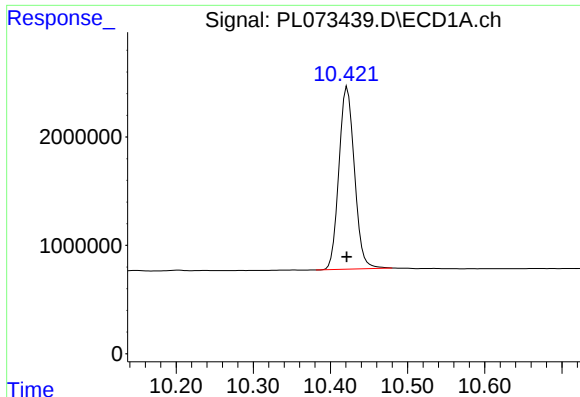

#28 Decachlorobiphenyl

R.T.: 10.422 min
Delta R.T.: 0.001 min
Response: 23486070
Conc: 46.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORCCC500

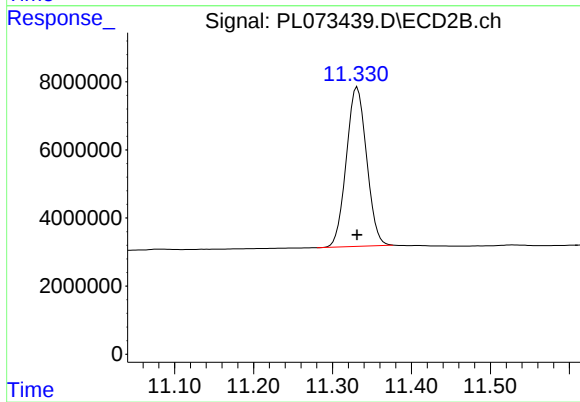

#28 Decachlorobiphenyl

R.T.: 11.331 min
Delta R.T.: 0.000 min
Response: 83618015
Conc: 46.76 ng/ml