

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031723\
 Data File : PL081539.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Mar 2023 13:21
 Operator : AR\AJ
 Sample : 01954-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SV-TP4-0316

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 17 22:17:55 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030223.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 03 01:48:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.332	2.661	20274691	18243087	9.384	9.014
28)	SA Decachlor...	8.761	7.785	13865609	17526646	9.095	9.150
Target Compounds							
10)	B gamma-Chl...	5.710	4.857	3958668	1488394	1.735m	0.608m#
11)	B alpha-Chl...	5.791	4.914	14693290	6791235	6.522m	2.774m#
12)	B 4,4'-DDE	5.964	5.107	2661024	2539248	1.360	1.294
17)	MA 4,4'-DDT	6.792	5.908	620462	1008295	0.391	0.628 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL031723\
Data File : PL081539.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Mar 2023 13:21
Operator : AR\AJ
Sample : 01954-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SV-TP4-0316

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 17 22:17:55 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030223.M
Quant Title : GC Extractables
QLast Update : Fri Mar 03 01:48:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

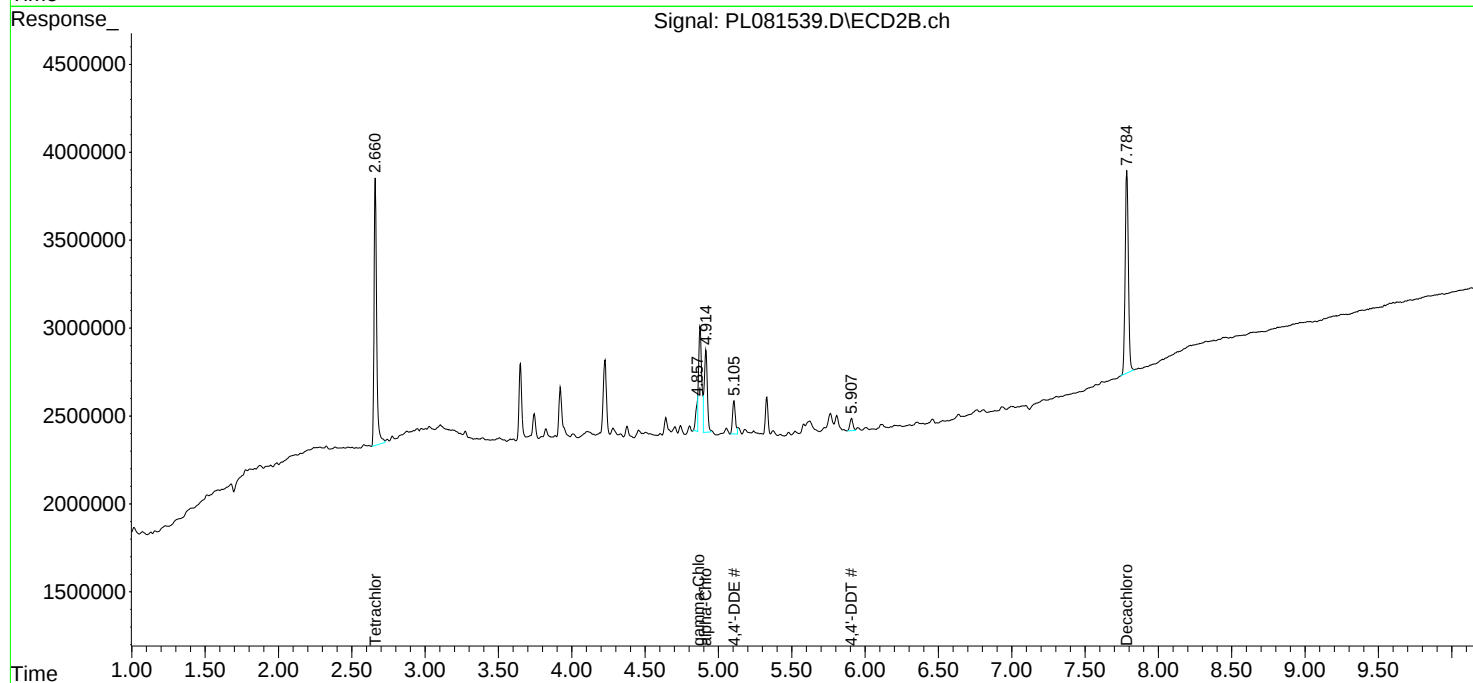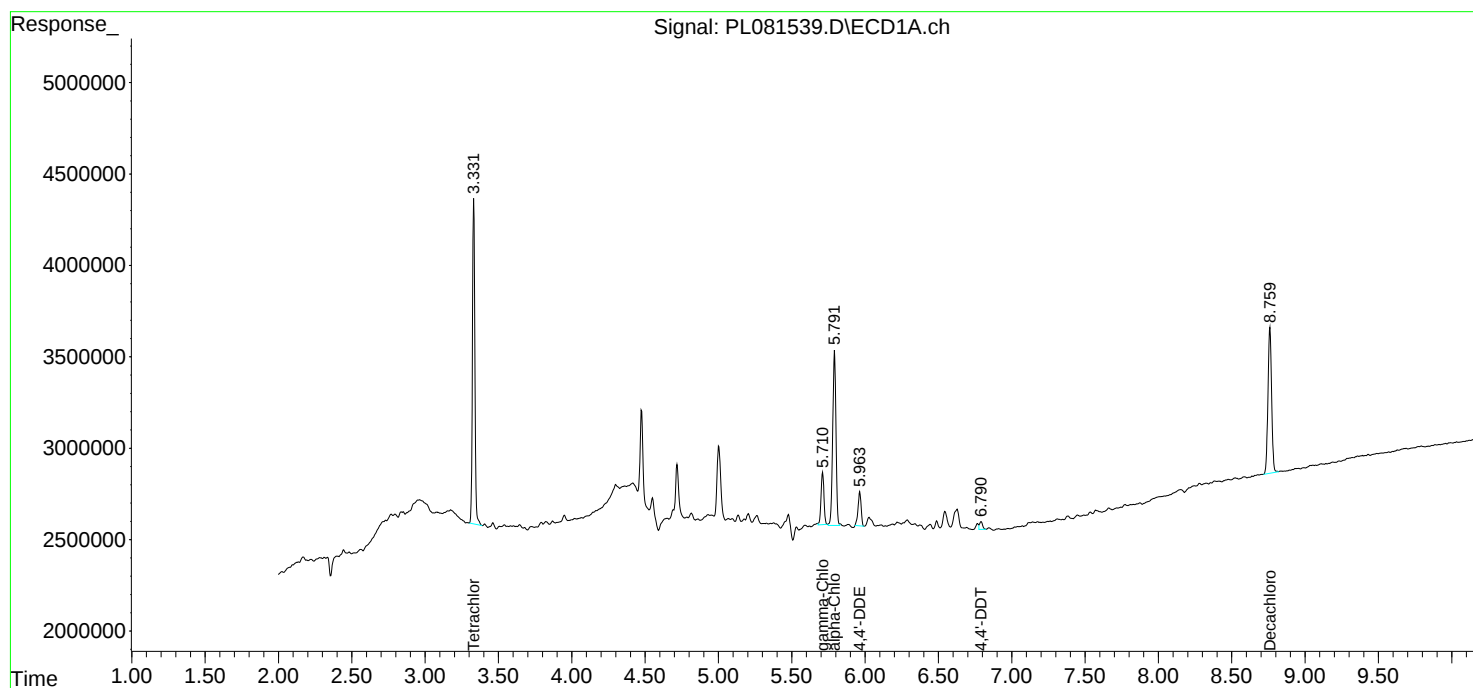


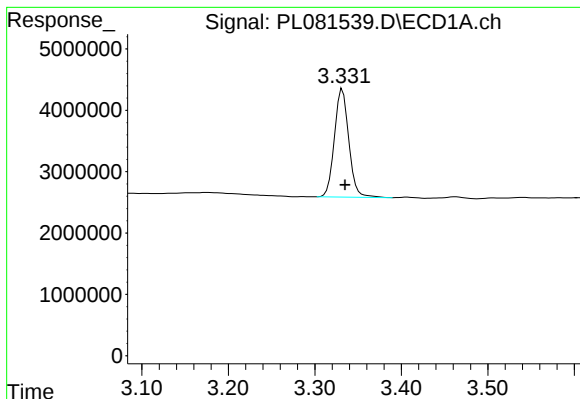

#1 Tetrachloro-m-xylene


R.T.: 3.332 min
Delta R.T.: -0.003 min
Response: 20274691
Conc: 9.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
SV-TP4-0316

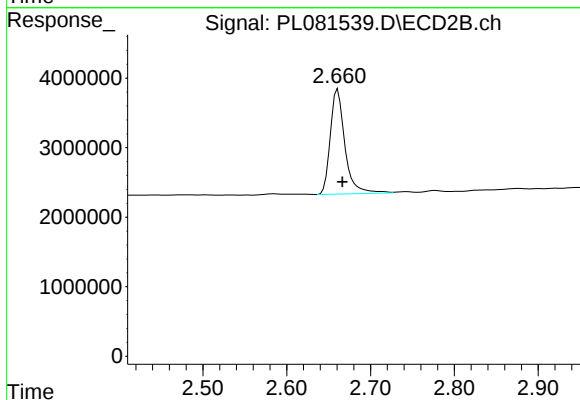


#1 Tetrachloro-m-xylene

R.T.: 2.661 min
Delta R.T.: -0.005 min
Response: 18243087
Conc: 9.01 ng/ml

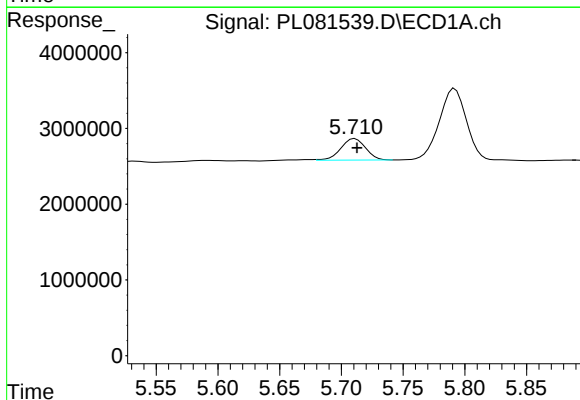


#10 gamma-Chlordane

R.T.: 5.710 min
Delta R.T.: -0.003 min
Response: 3958668
Conc: 1.73 ng/ml m

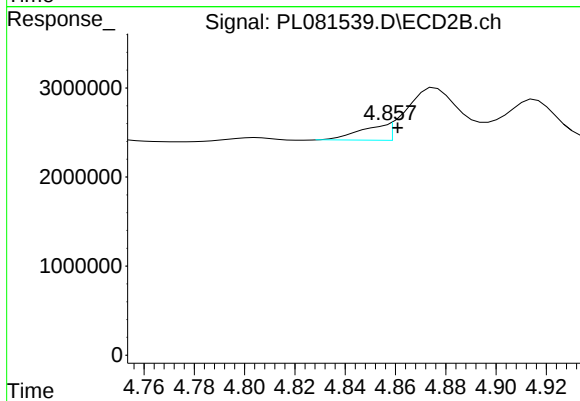

#10 gamma-Chlordane


R.T.: 4.857 min
Delta R.T.: -0.004 min
Response: 1488394
Conc: 0.61 ng/ml m

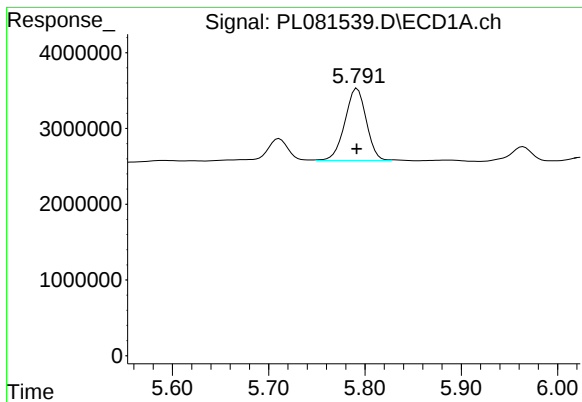

#11 alpha-Chlordane


R.T.: 5.791 min
Delta R.T.: 0.000 min
Response: 14693290
Conc: 6.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
SV-TP4-0316

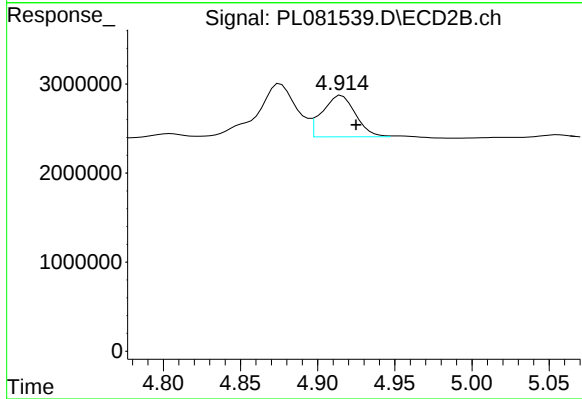


#11 alpha-Chlordane

R.T.: 4.914 min
Delta R.T.: -0.011 min
Response: 6791235
Conc: 2.77 ng/ml m

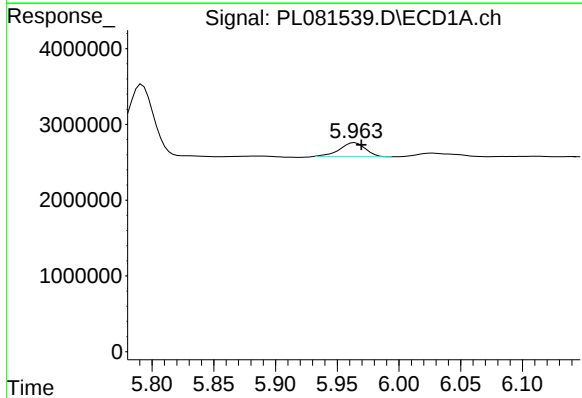


#12 4,4'-DDE

R.T.: 5.964 min
Delta R.T.: -0.005 min
Response: 2661024
Conc: 1.36 ng/ml

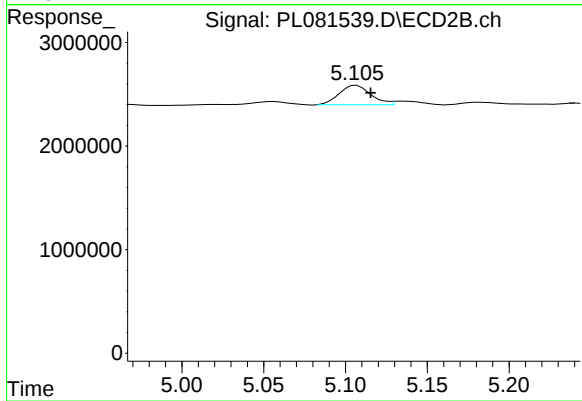

#12 4,4'-DDE


R.T.: 5.107 min
Delta R.T.: -0.009 min
Response: 2539248
Conc: 1.29 ng/ml

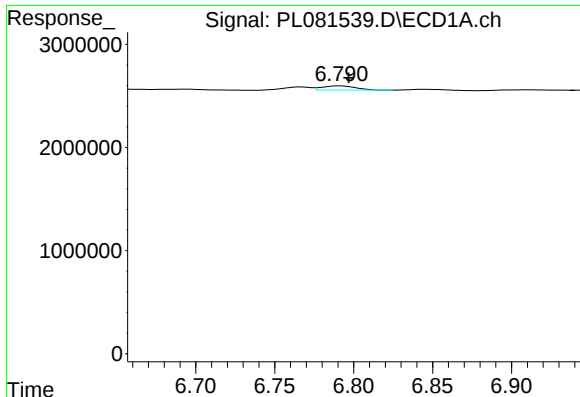

#17 4,4'-DDT


R.T.: 6.792 min
Delta R.T.: -0.005 min
Response: 620462
Conc: 0.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
SV-TP4-0316

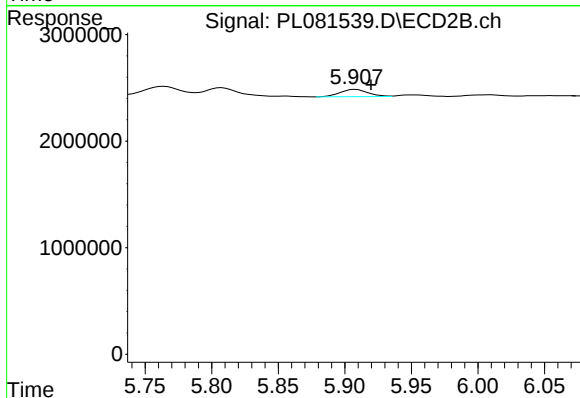


#17 4,4'-DDT

R.T.: 5.908 min
Delta R.T.: -0.012 min
Response: 1008295
Conc: 0.63 ng/ml

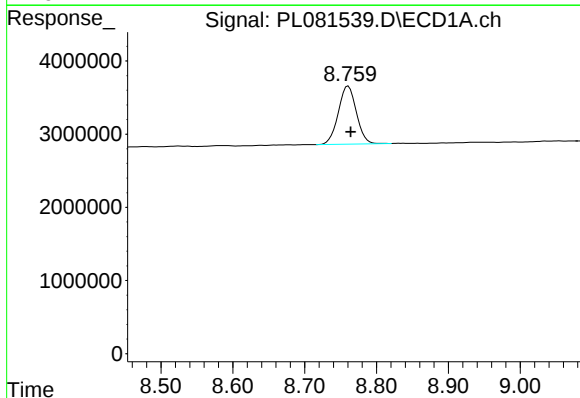

#28 Decachlorobiphenyl

R.T.: 8.761 min
Delta R.T.: -0.004 min
Response: 13865609
Conc: 9.09 ng/ml

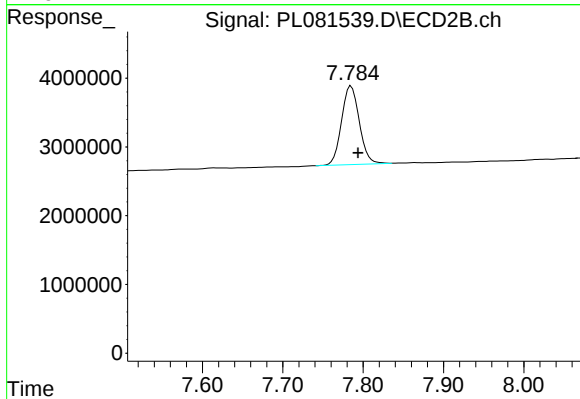

#28 Decachlorobiphenyl

R.T.: 7.785 min
Delta R.T.: -0.009 min
Response: 17526646
Conc: 9.15 ng/ml